

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
 Data File : PD056840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 17:27
 Operator : AJ\MA
 Sample : RESC01
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 06:32:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 03 06:06:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	16374124	29526035	19.156	19.020
27)	SA Decachlor...	7.959	8.999	37521210	55757449	38.500	38.388
Target Compounds							
2)	A alpha-BHC	3.712	4.347	11245050	19440250	9.064	8.914
3)	MA gamma-BHC...	3.987	4.629	11007164	18856739	9.035	9.005
4)	MA Heptachlor	4.272	5.136	10384419	19080374	9.325	8.987
5)	MB Aldrin	4.512	5.439	10332487	18139538	9.419	9.201
6)	B beta-BHC	4.238	4.799	5181649	9472325	9.804	9.721
7)	B delta-BHC	4.432	5.015	11015527	13674316	9.213	7.953
8)	B Heptachlo...	4.948	5.823	9662734	15806631	9.553	8.987
9)	A Endosulfan I	5.279	6.179	8547931	16367437	8.937	9.323
10)	B trans-Chl...	5.170	6.057	9794464	17792894	9.569	9.323
11)	B cis-Chlor...	5.228	6.129	9581855	18160050	9.267	9.462
12)	B 4,4'-DDE	5.396	6.286	19229370	32927503	18.747	18.351
13)	MA Dieldrin	5.519	6.435	19663665	34716363	18.328	18.243
14)	MA Endrin	5.773	6.652	17032115	28897252	18.999	18.658
15)	B Endosulfa...	6.046	6.860	17087229	30550685	18.979	18.604
16)	A 4,4'-DDD	5.907	6.774	14920500	26334447	18.480	18.103
17)	MA 4,4'-DDT	6.142	7.072	12698742	25299138	17.291	17.834
18)	B Endrin al...	6.214	6.984	15480481	26616802	19.733	19.218
19)	B Endosulfa...	6.425	7.206	17413658	31267961	19.320	19.153
20)	A Methoxychlor	6.691	7.529	38195342	74831221	95.839	95.284
21)	B Endrin ke...	6.910	7.675	19375081	32539163	20.209	19.488

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 17:27
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 06:32:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 06:06:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

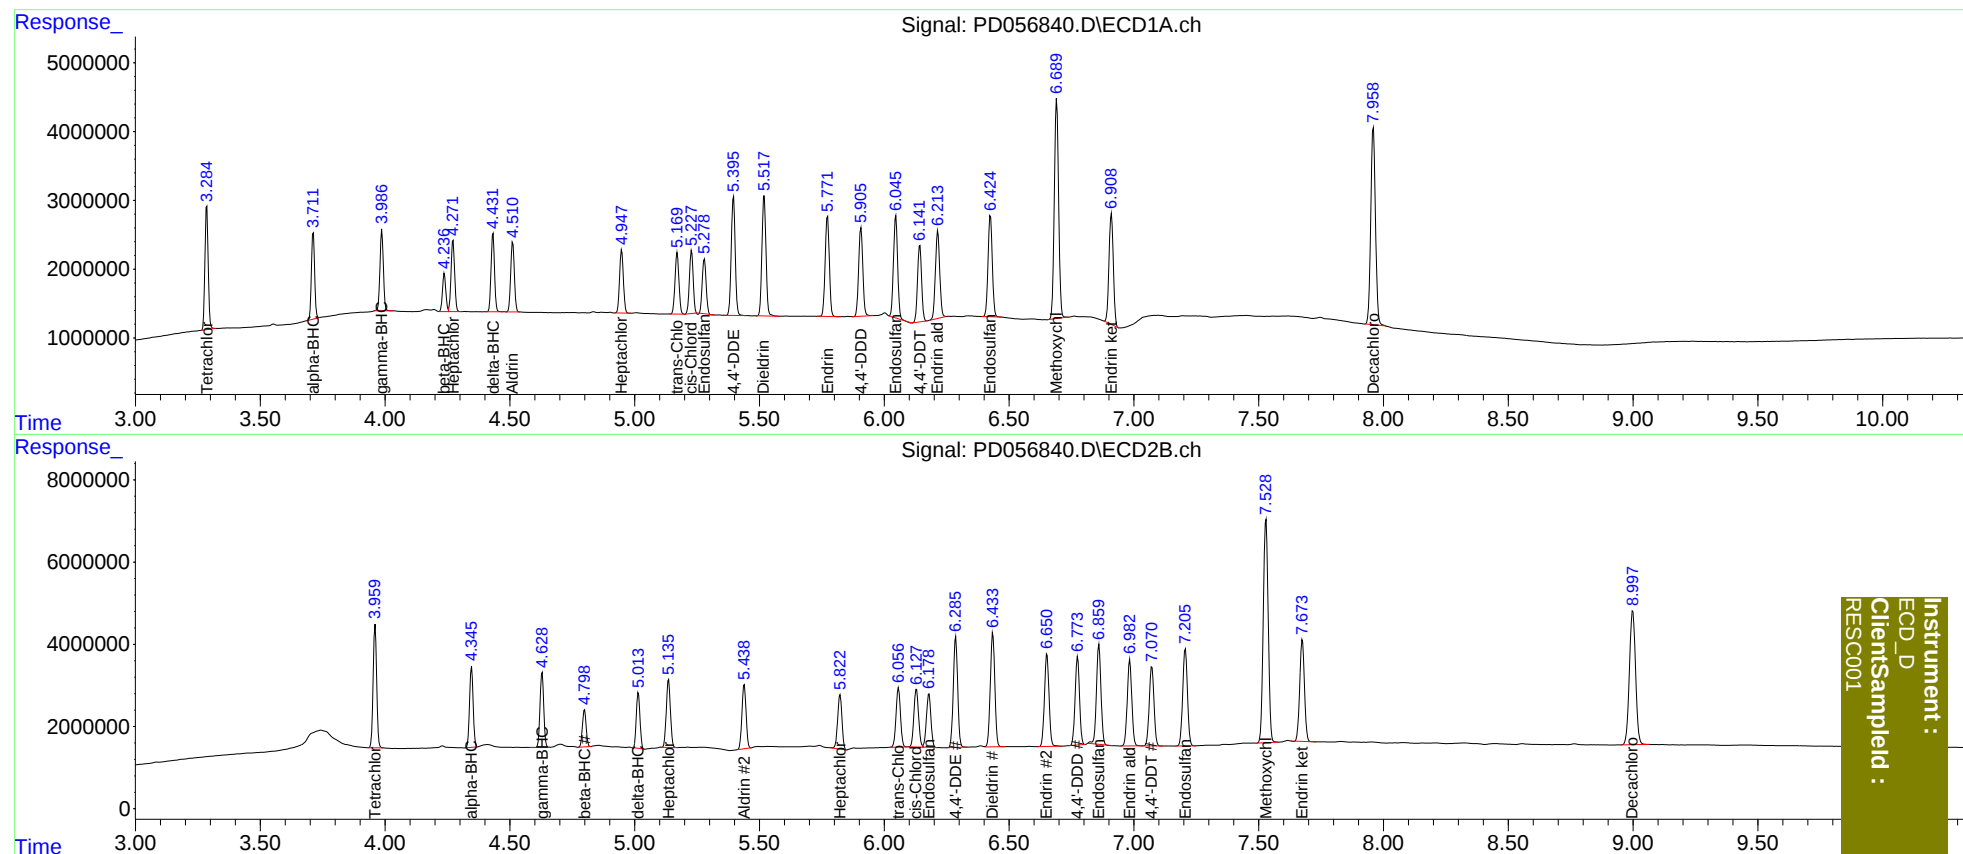

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056840.D
Acq On : 02 Jan 2020 17:27
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Title : GC Extractables
Last Update : Fri Jan 03 06:06:42 2020
Integrator: ChemStation

RT#1	RT#2	Resolution
3.286	3.712	100.00%
3.712	3.987	100.00%
3.987	4.238	100.00%
4.238	4.272	96.00%
4.272	4.432	100.00%
4.432	4.512	100.00%
4.512	4.948	100.00%
4.948	5.170	100.00%
5.170	5.228	100.00%
5.228	5.279	100.00%
5.279	5.396	100.00%
5.396	5.519	100.00%
5.519	5.773	100.00%
5.773	5.907	100.00%
5.907	6.046	100.00%
6.046	6.142	100.00%
6.142	6.214	100.00%
6.214	6.425	100.00%
6.425	6.691	100.00%
6.691	6.910	100.00%
6.910	7.959	100.00%

Signal #2


3.960	4.347	100.00%
4.347	4.629	100.00%
4.629	4.799	100.00%
4.799	5.015	100.00%
5.015	5.136	100.00%
5.136	5.439	100.00%
5.439	5.823	100.00%
5.823	6.057	100.00%
6.057	6.129	100.00%
6.129	6.179	96.42%
6.179	6.286	100.00%
6.286	6.435	100.00%
6.435	6.652	100.00%
6.652	6.774	100.00%
6.774	6.860	100.00%
6.860	6.984	100.00%
6.984	7.072	100.00%
7.072	7.206	100.00%
7.206	7.529	100.00%
7.529	7.675	100.00%
7.675	8.999	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 17:27
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 06:32:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 06:06:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

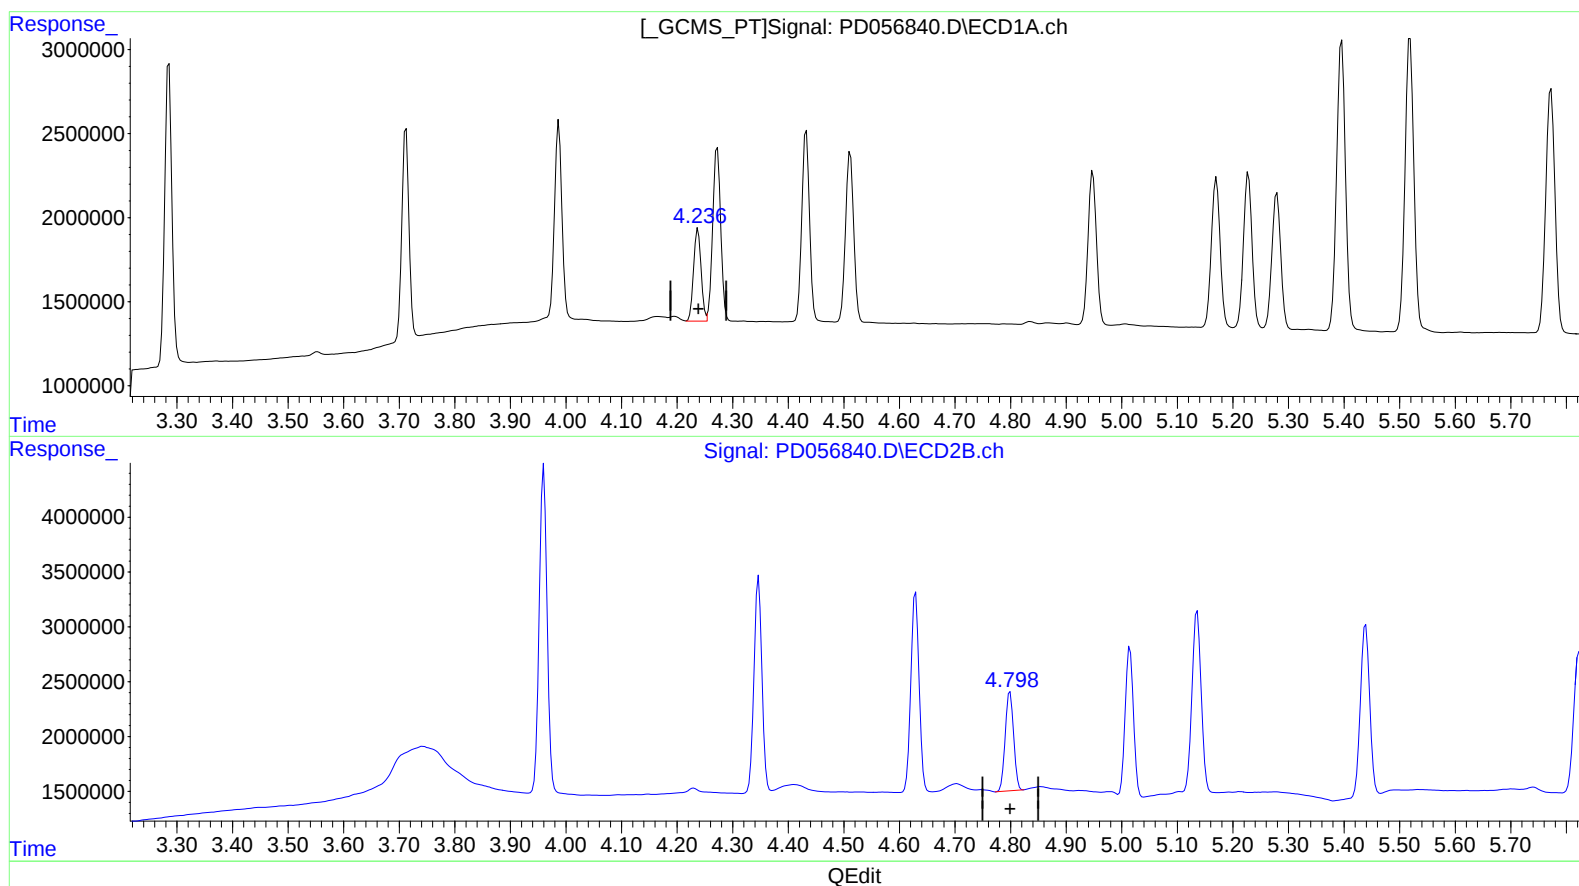

(6) beta-BHC (B)
4.238min 9.804 ng/ml
response 5181649


(6) beta-BHC #2 (B)
4.799min 9.721 ng/ml
response 9472325

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 17:27
Operator : AJ\MA
Sample : RESC01
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC001

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 06:32:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 06:06:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

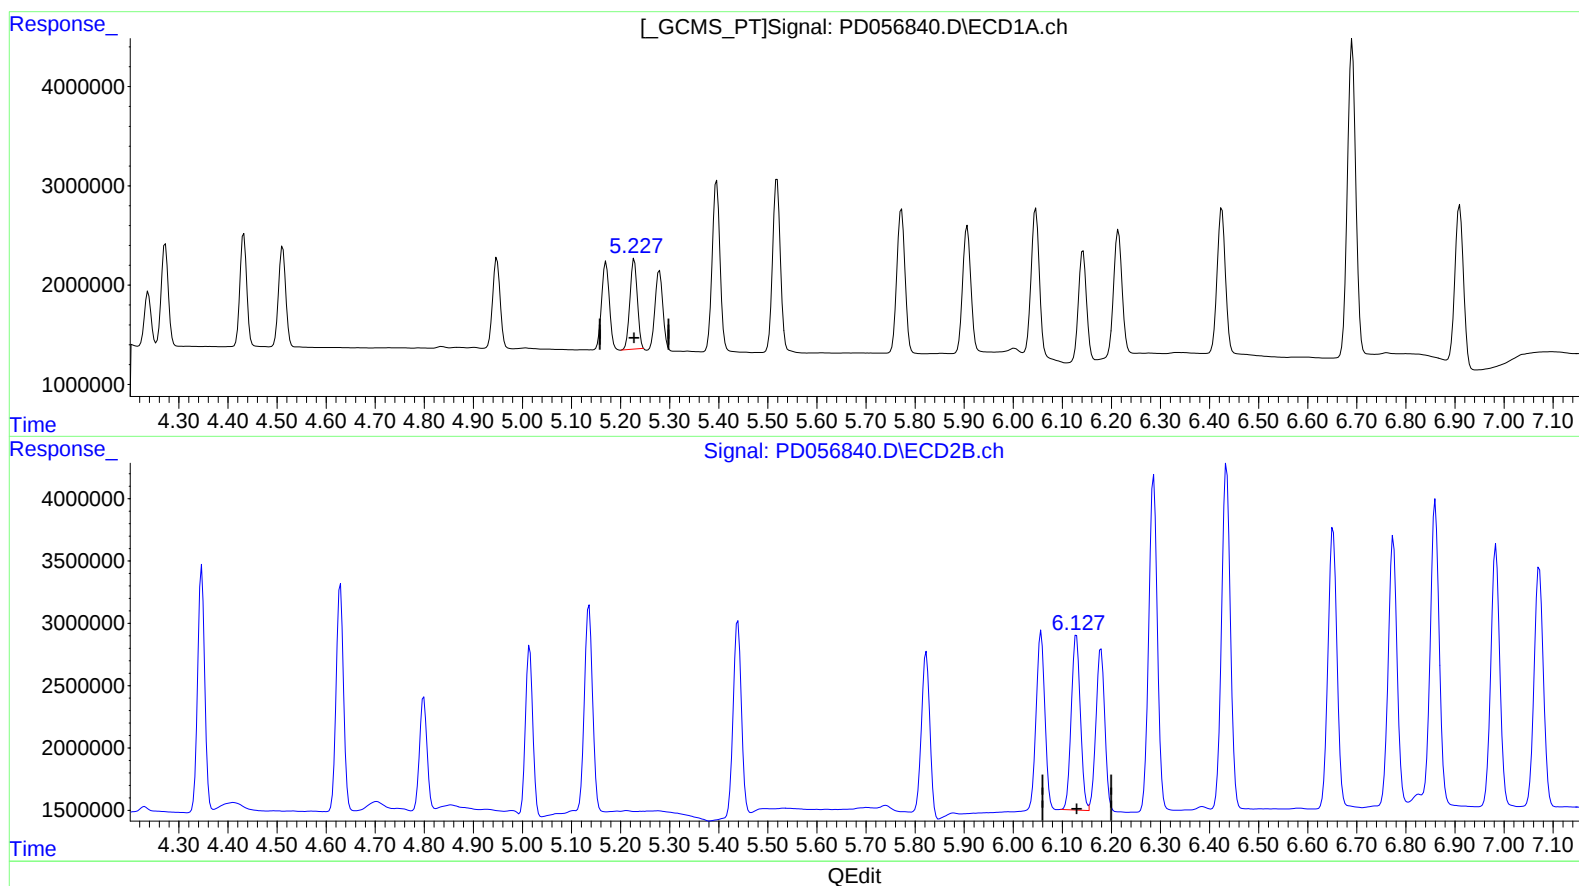

(11) cis-Chlordane (B)

5.228min 9.267 ng/ml

response 9581855

(11) cis-Chlordane #2 (B)

6.129min 9.462 ng/ml

response 18160050