

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
 Data File : PD056853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:30
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4001

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 05:54:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 03 05:45:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.961	33752920	61637480	39.721	39.653
27)	SA Decachlor...	7.959	8.998	74480831	110.8E6	76.634	76.150
Target Compounds							
2)	A alpha-BHC	3.713	4.347	50892231	91111043	41.388	41.857
3)	MA gamma-BHC...	3.987	4.630	48041190	85903273	40.612	41.125
4)	MA Heptachlor	4.273	5.136	44693088	85322234	40.511	40.503
9)	A Endosulfan I	5.279	6.179	38288745	69908414	40.052	40.065
13)	MA Dieldrin	5.520	6.435	88046560	155.7E6	82.158	81.814
14)	MA Endrin	5.772	6.652	71958455	124.4E6	80.351	80.694
16)	A 4,4'-DDD	5.907	6.775	66184151	119.6E6	81.721	81.910
17)	MA 4,4'-DDT	6.142	7.073	64795763	119.6E6	87.128	84.113
20)	A Methoxychlor	6.691	7.530	159.2E6	310.4E6	393.508	391.130

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010220\
Data File : PD056853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:30
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 05:54:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010220CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 03 05:45:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

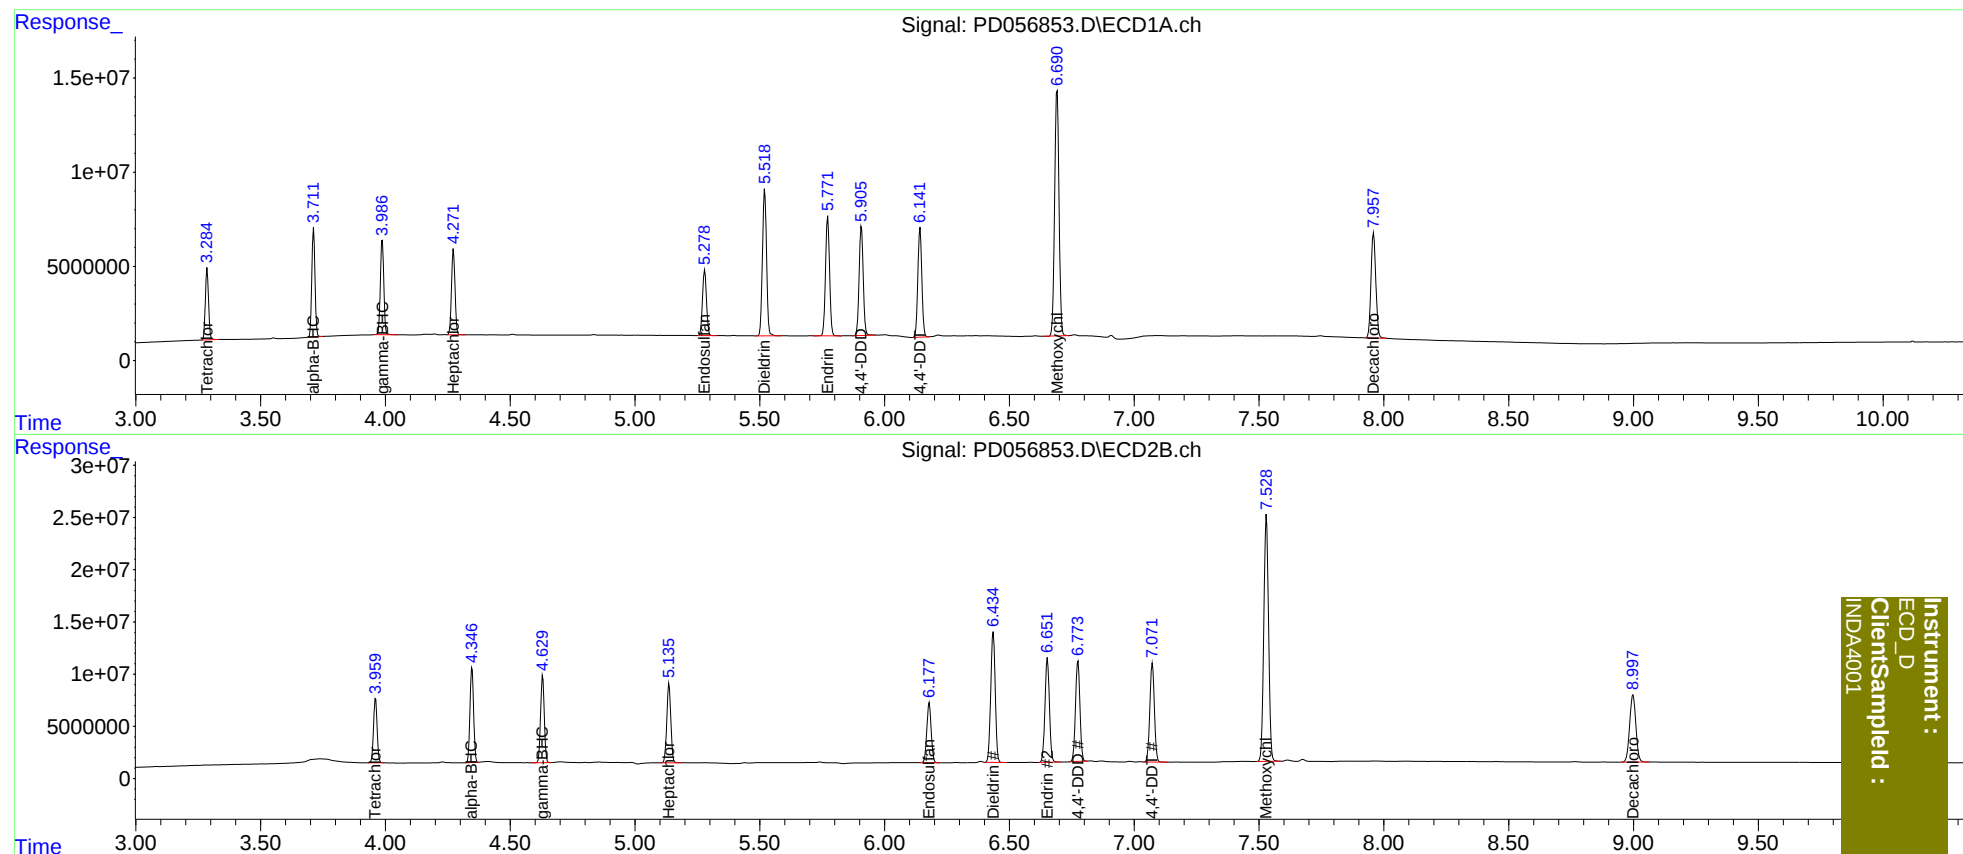

Instrument :
ECD_D
ClientSampled :
INDA4001