

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010224\
 Data File : PD080638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 16:00
 Operator : AR\AJ
 Sample : PB158130BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK130

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 20:40:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.798	27823772	47450926	21.792	21.340
27) SA Decachlor...	9.115	7.938	44569973	59226692	27.722	24.675
Target Compounds						
2) A alpha-BHC	0.000	3.289	0	112605	N.D.	<MDL
3) MA gamma-BHC...	0.000	3.647	0	157610	N.D.	<MDL
6) B beta-BHC	0.000	3.887f	0	236439	N.D.	0.138
13) MA Dieldrin	0.000	5.436f	0	116030	N.D.	<MDL
17) MA 4,4'-DDT	0.000	6.108f	0	136478	N.D.	<MDL
18) B Endrin al...	0.000	6.150	0	54346	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010224\
Data File : PD080638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 16:00
Operator : AR\AJ
Sample : PB158130BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 20:40:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

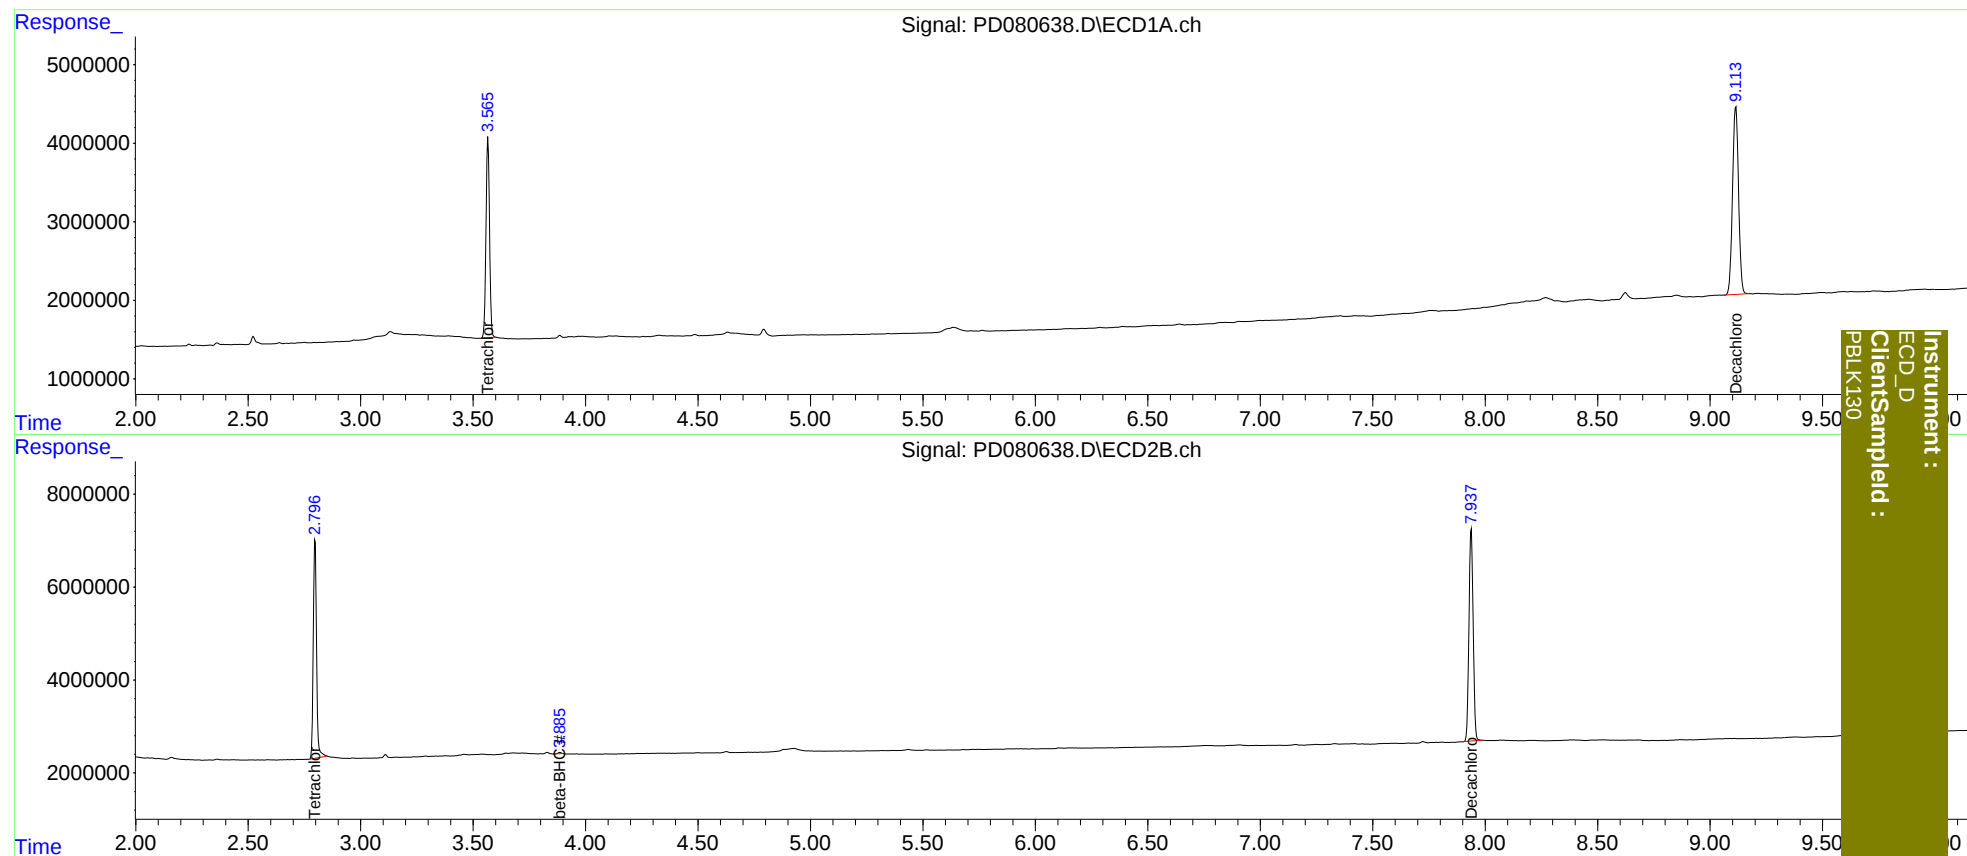


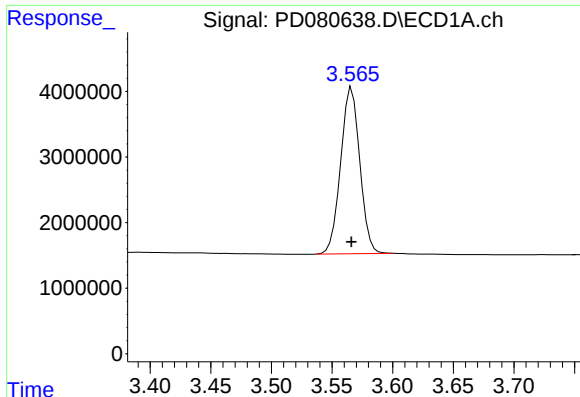

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 27823772
Conc: 21.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK130

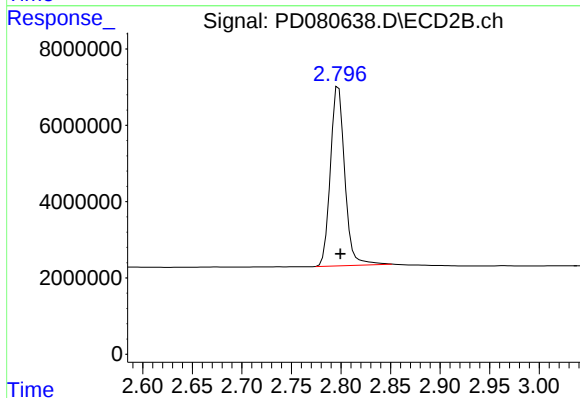


#1 Tetrachloro-m-xylene

R.T.: 2.798 min
Delta R.T.: -0.002 min
Response: 47450926
Conc: 21.34 ng/ml

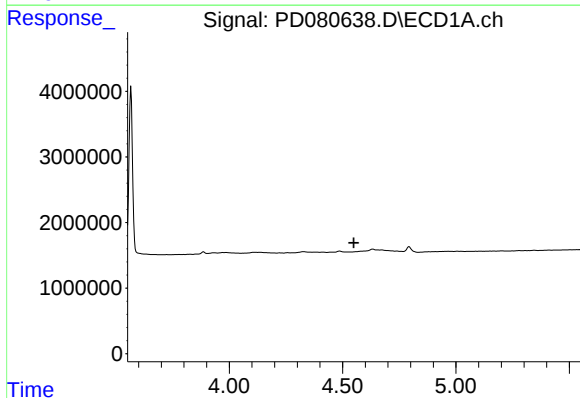


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.550 min
Response: 0
Conc: N.D.

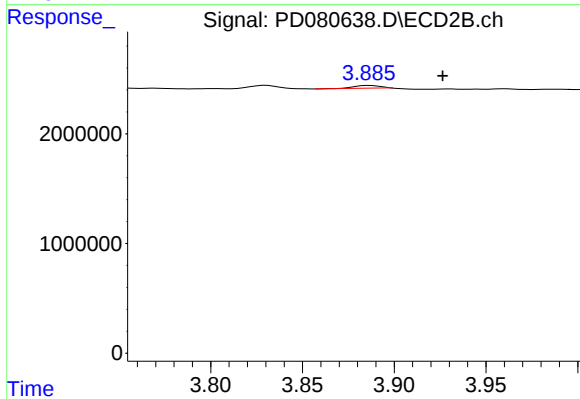

#6 beta-BHC


R.T.: 3.887 min
Delta R.T.: -0.040 min
Response: 236439
Conc: 0.14 ng/ml

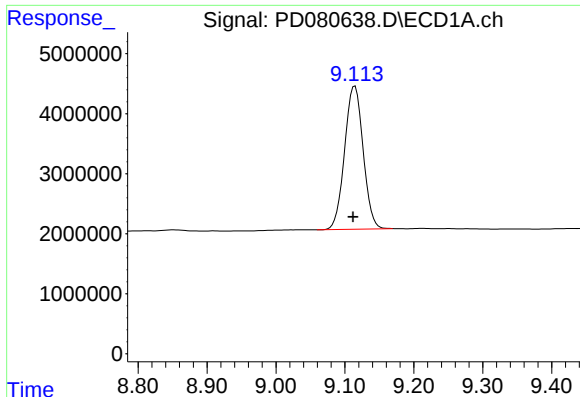

#27 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: 0.003 min
Response: 44569973
Conc: 27.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK130

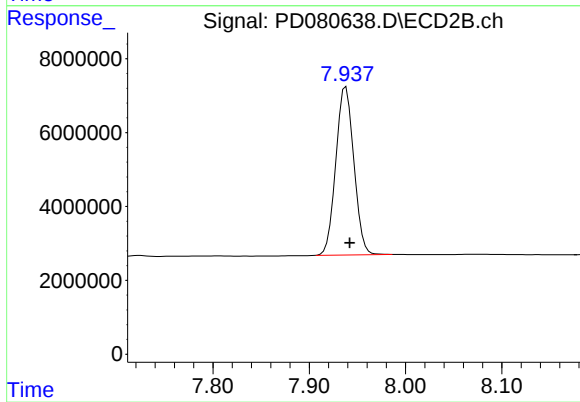

#27 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.004 min
Response: 59226692
Conc: 24.68 ng/ml