

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010224\
 Data File : PD080654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2024 19:38
 Operator : AR\AJ
 Sample : 05984-13MSD
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSN4MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 20:45:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.797	24313387	41883749	19.043	18.836
2)	SA Decachlor...	9.113	7.938	40068180	52800314	24.922	21.998
Target Compounds							
2)	A alpha-BHC	4.022	3.299	122.8E6	200.0E6	59.592	58.673
3)	MA gamma-BHC...	4.356	3.629	114.1E6	185.7E6	57.451	57.702
4)	MA Heptachlor	4.949	3.970	115.8E6	182.4E6	55.462	56.943
5)	MB Aldrin	5.293	4.251	112.0E6	179.1E6	50.055	50.699
6)	B beta-BHC	4.550	3.924	49496042	79068257	47.684	46.049
7)	B delta-BHC	4.800	4.155	119.1E6	190.9E6	51.870	49.102
8)	B Heptachlo...	5.719	4.752	103.3E6	166.9E6	48.101	49.239
9)	A Endosulfan I	6.106	5.122	98293195	155.0E6	55.178	56.549
10)	B trans-Chl...	5.975	5.003	101.4E6	164.1E6	49.434	49.854
11)	B cis-Chlor...	6.055	5.067	104.6E6	166.1E6	49.848	49.395
12)	B 4,4'-DDE	6.226	5.256	197.7E6	321.0E6	102.332	102.201
13)	MA Dieldrin	6.381	5.387	214.3E6	346.5E6	115.129	115.610
14)	MA Endrin	6.612	5.662	174.8E6	297.7E6	111.575	113.141
15)	B Endosulfa...	6.831	5.955	182.8E6	293.6E6	97.487	101.260
16)	A 4,4'-DDD	6.743	5.809	162.4E6	264.8E6	117.106	115.185
17)	MA 4,4'-DDT	7.059	6.060	170.6E6	269.1E6	115.473	111.592
18)	B Endrin al...	6.960	6.134	130.6E6	207.6E6	87.532	90.042
19)	B Endosulfa...	7.194	6.357	177.3E6	277.3E6	96.685	98.860
20)	A Methoxychlor	7.533	6.635	425.4E6	637.3E6	537.252	506.251
21)	B Endrin ke...	7.681	6.863	198.1E6	322.3E6	101.795	100.710

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010224\
Data File : PD080654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2024 19:38
Operator : AR\AJ
Sample : 05984-13MSD
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 20:45:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

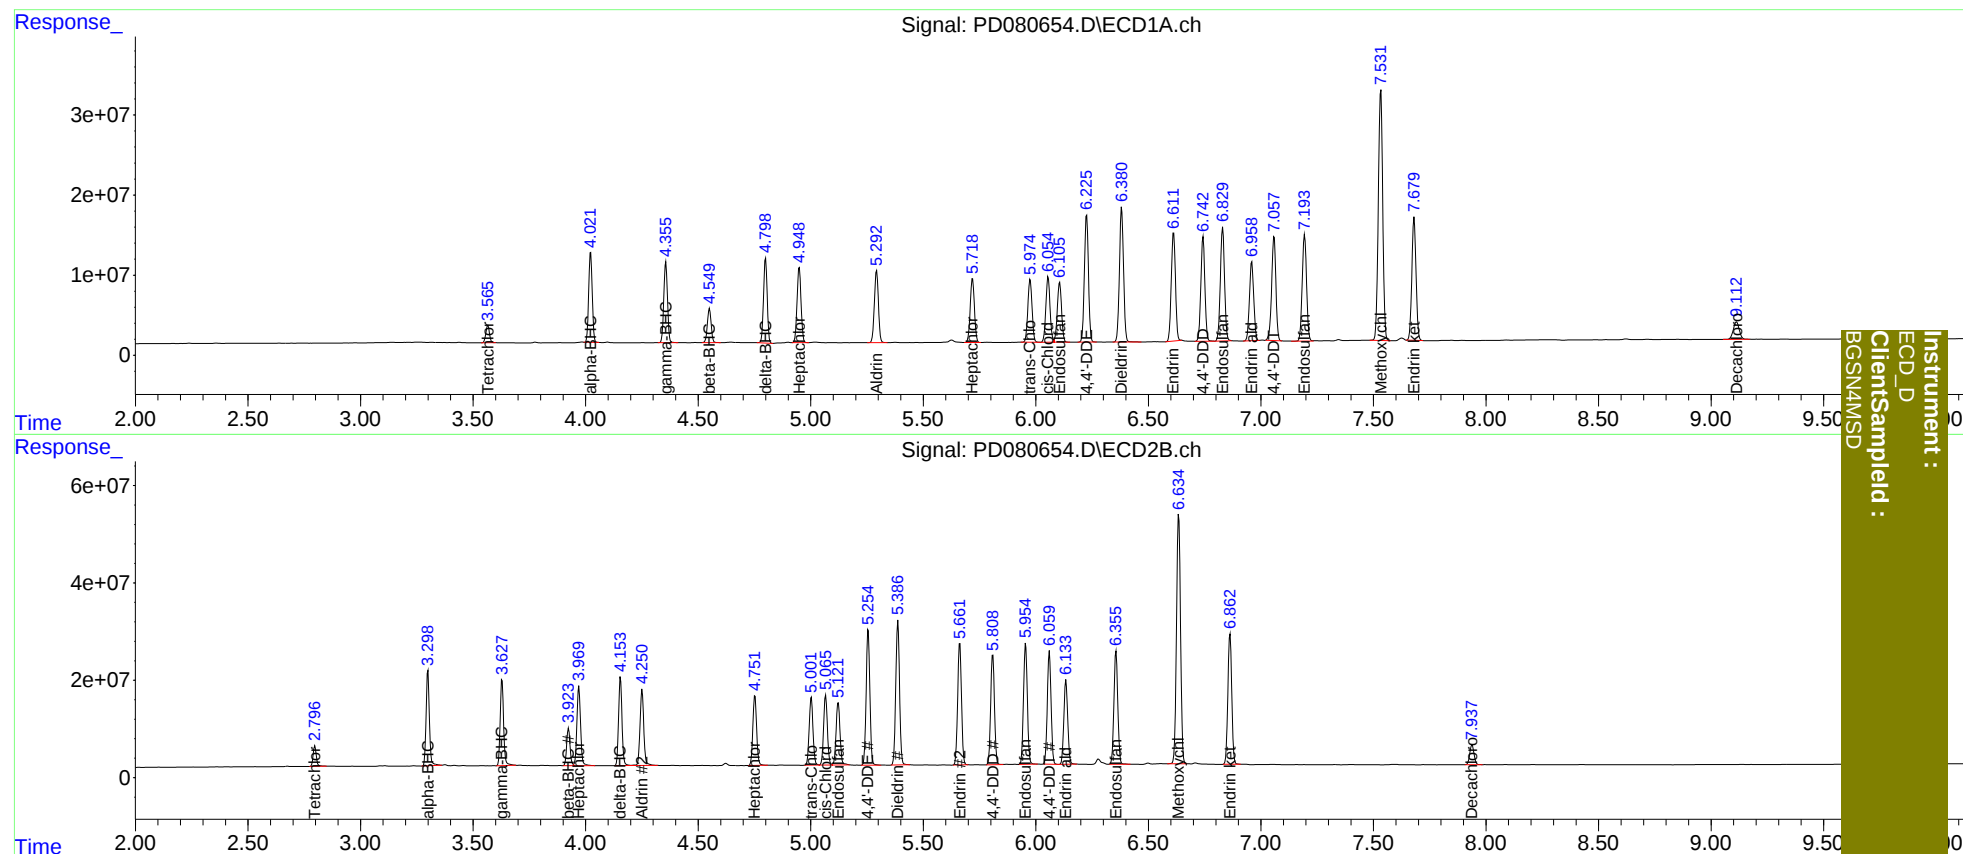

Instrument :
ECD_D
ClientSampled :
BGSN4MSD