

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010319\
 Data File : PD050916.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2019 13:13
 Operator : AJ\SJ
 Sample : PIBLK30
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK30

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 06:05:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122718CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 03 08:35:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.230	4.048	30741628	577.9E6	19.927	21.432
27) SA Decachlor...	7.836	9.163	41376752	692.2E6	36.725	37.221
Target Compounds						
6) B beta-BHC	0.000	4.926f	0	69941530	N.D.	4.172


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010319\
Data File : PD050916.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 13:13
Operator : AJ\SJ
Sample : PIBLK30
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK30

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 06:05:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122718CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 03 08:35:31 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

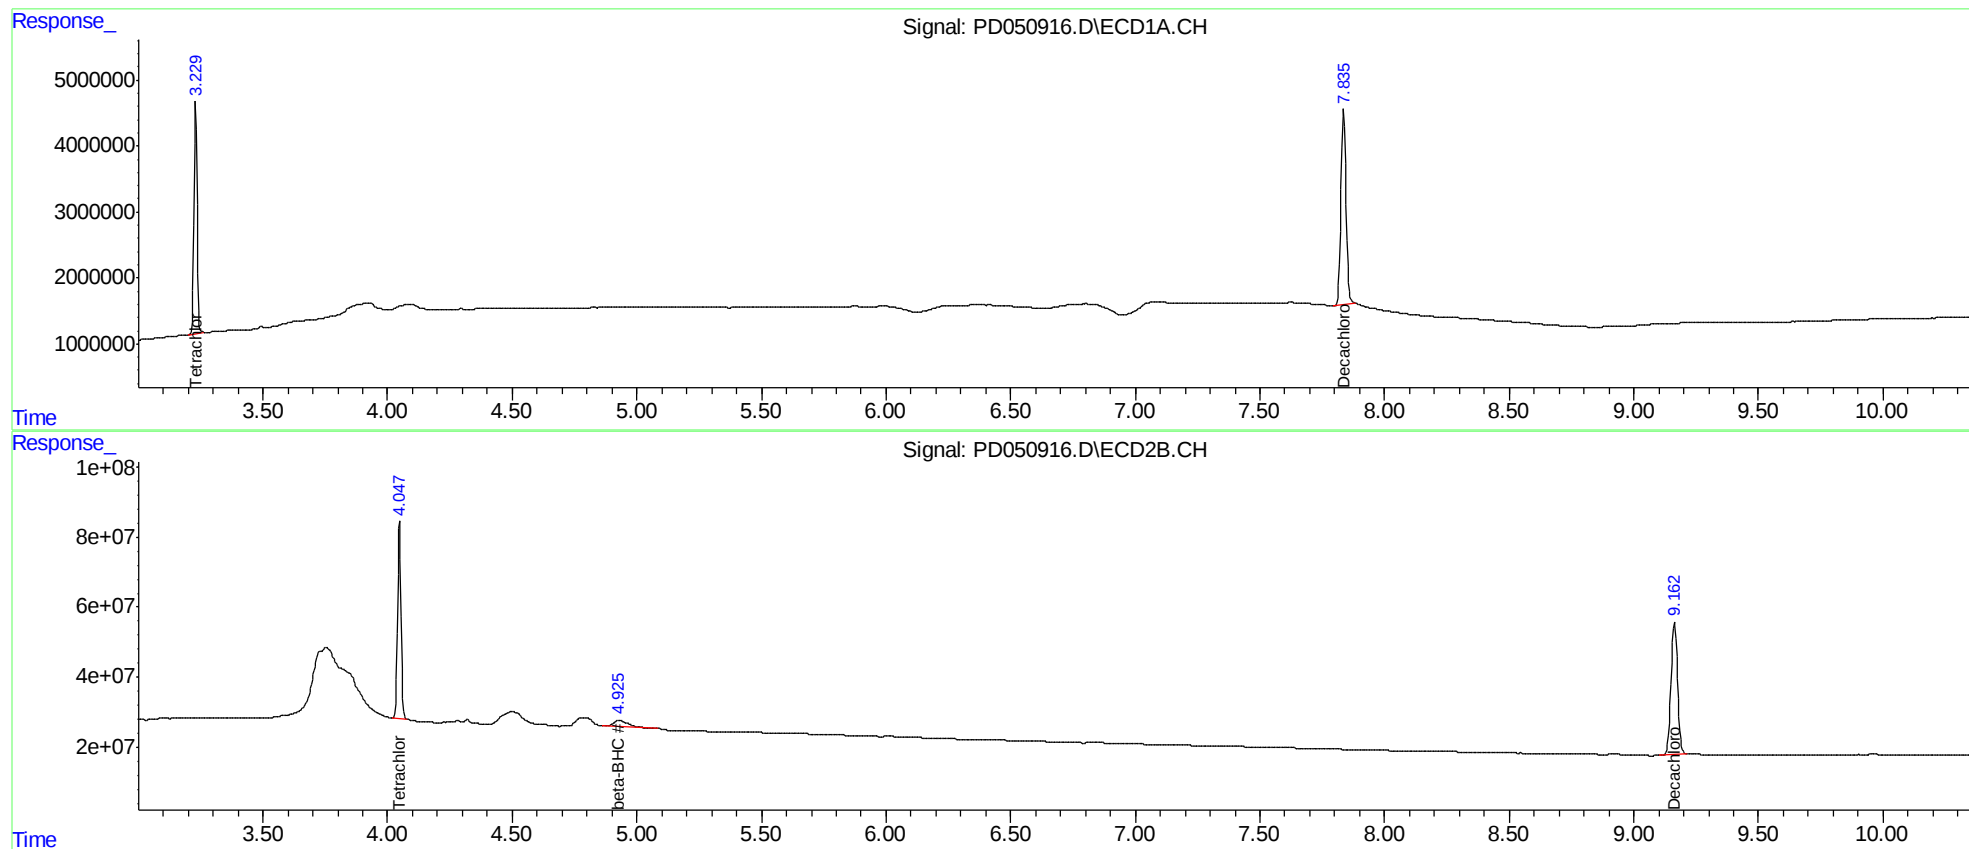


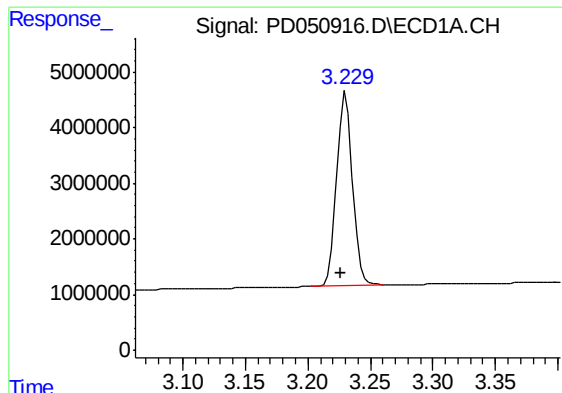

#1 Tetrachloro-m-xylene


R.T.: 3.230 min
Delta R.T.: 0.004 min
Response: 30741628
Conc: 19.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK30

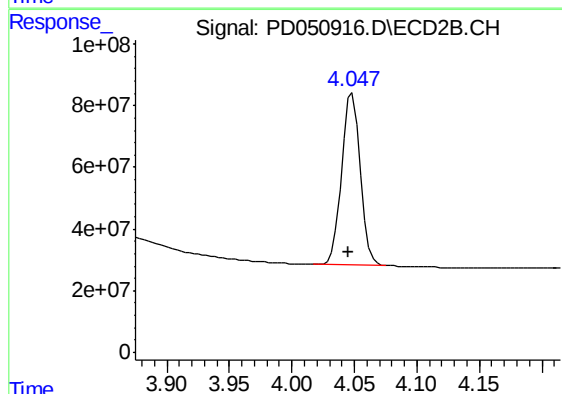


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.003 min
Response: 577886823
Conc: 21.43 ng/ml

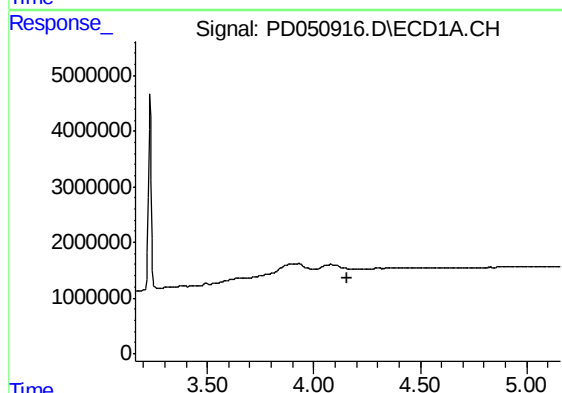


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

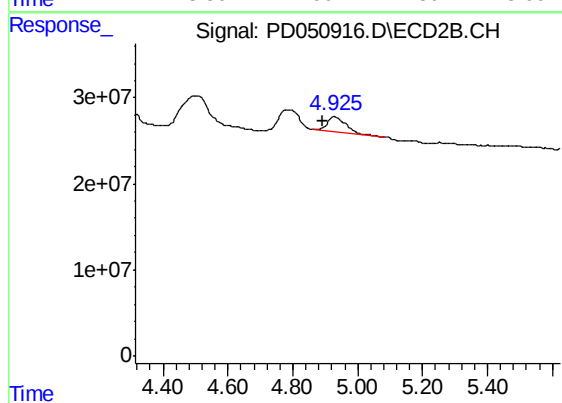

#6 beta-BHC


R.T.: 4.926 min
Delta R.T.: 0.033 min
Response: 69941530
Conc: 4.17 ng/ml

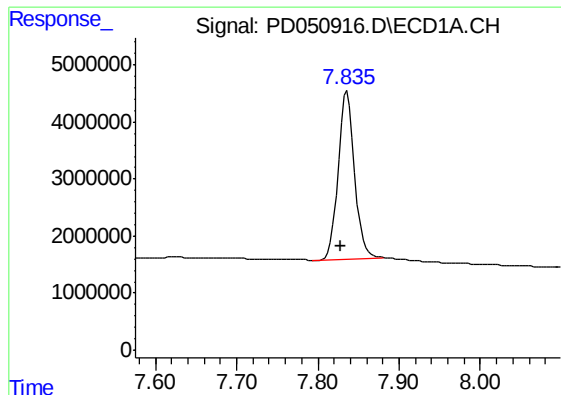

#27 Decachlorobiphenyl

R.T.: 7.836 min
Delta R.T.: 0.008 min
Response: 41376752
Conc: 36.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK30

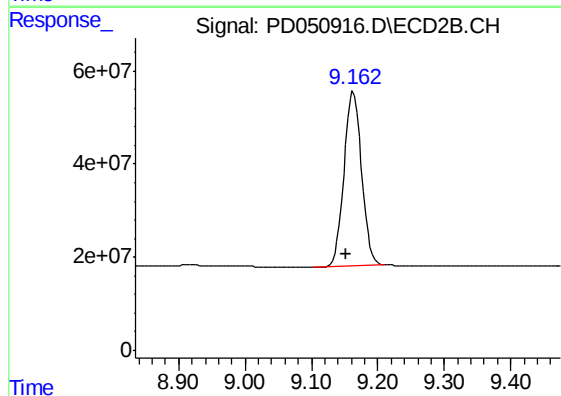

#27 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.012 min
Response: 692171660
Conc: 37.22 ng/ml