

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010322\
 Data File : PD067567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2022 14:20
 Operator : AR\AJ
 Sample : PB141792BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB141792BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/04/2022
 Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:36:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	3.962	34398428	138.7E6	18.929	21.014
2) SA Decachlor...	8.162	9.020	15734779	88306916	17.714m	18.581

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010322\
Data File : PD067567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2022 14:20
Operator : AR\AJ
Sample : PB141792BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PB141792BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/04/2022
Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:36:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

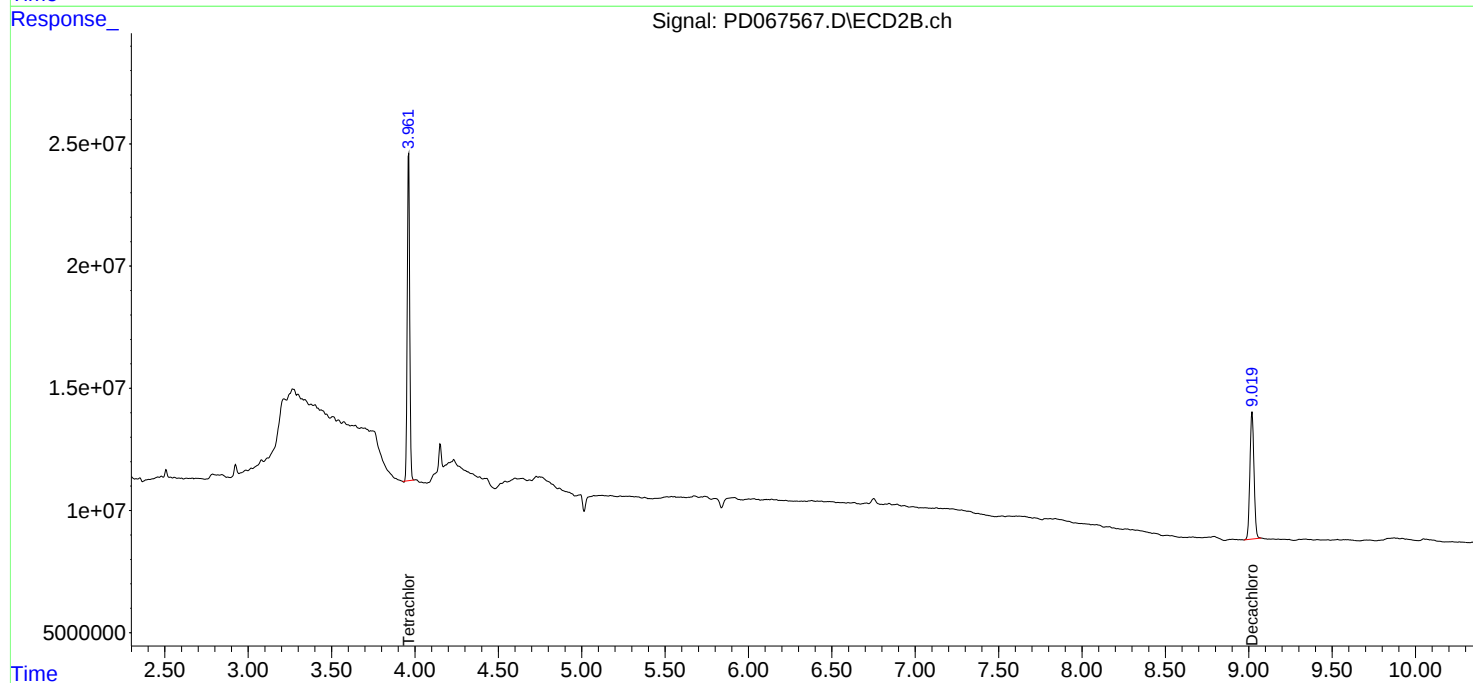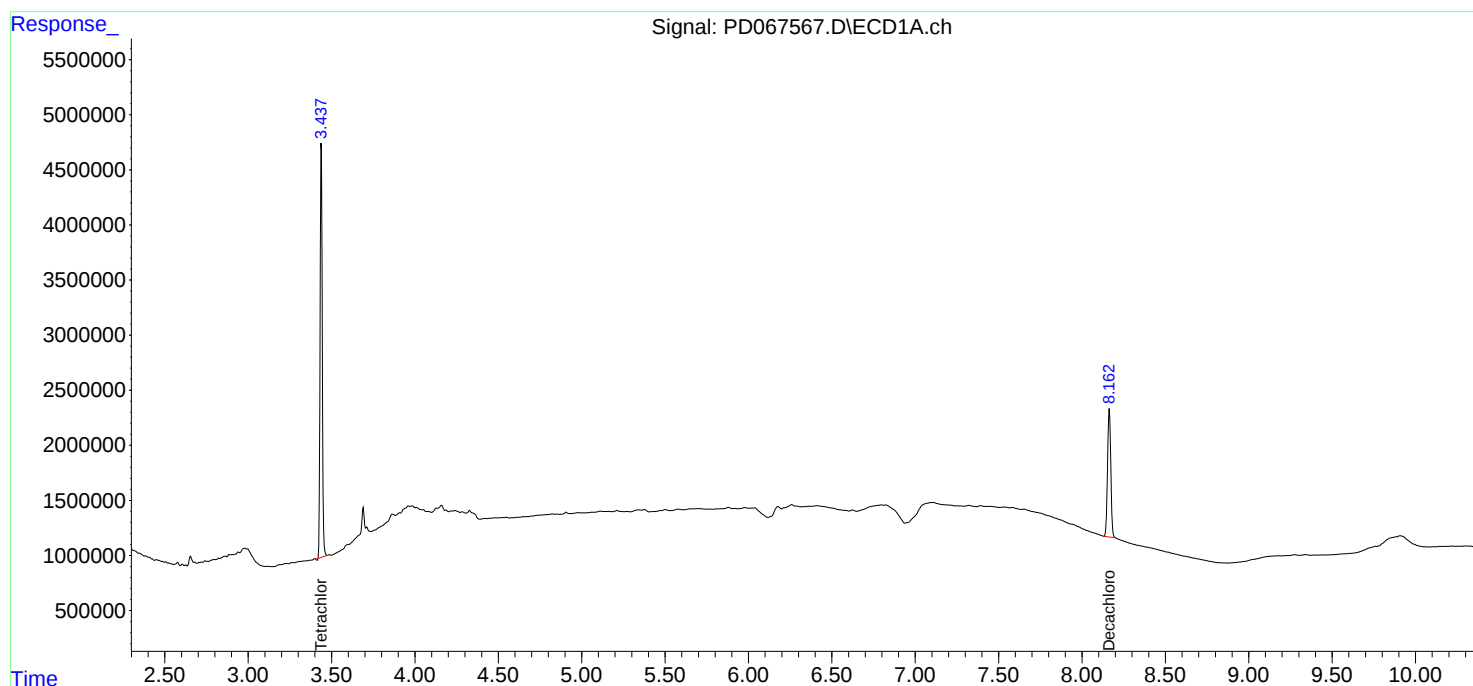

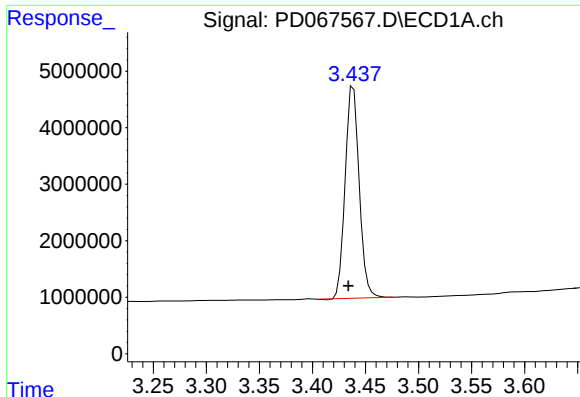


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.005 min
Response: 34398428
Conc: 18.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB141792BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/04/2022
Supervised By :mohammad ahmed 01/05/2022

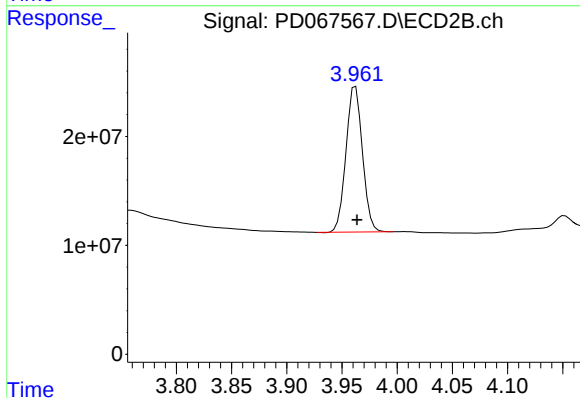


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.002 min
Response: 138654099
Conc: 21.01 ng/ml

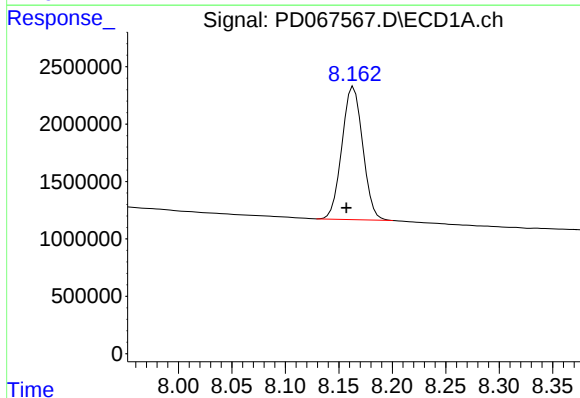

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.005 min
Response: 15734779
Conc: 17.71 ng/ml m

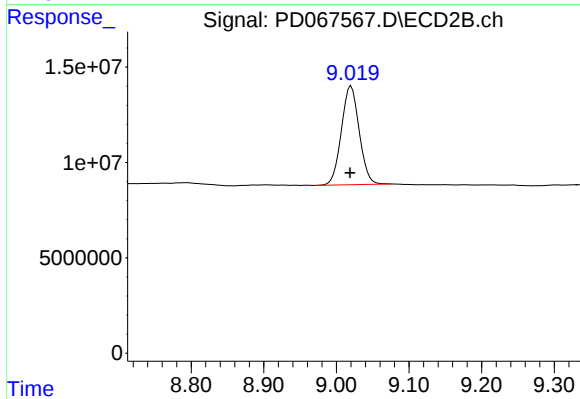

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.002 min
Response: 88306916
Conc: 18.58 ng/ml