

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010324\
 Data File : PD080668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 16:06
 Operator : AR\AJ
 Sample : PIBLK155
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK909

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 21:39:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.797	30972073	52985679	24.258	23.829
27)	SA Decachlor...	9.113	7.938	50525506	66510994	31.426	27.710
Target Compounds							
2)	A alpha-BHC	0.000	3.287	0	113342	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.648	0	150355	N.D.	<MDL
4)	MA Heptachlor	0.000	3.936 ^f	0	174682	N.D.	<MDL
5)	MB Aldrin	0.000	4.269	0	2724132	N.D.	0.771
6)	B beta-BHC	0.000	3.936	0	174682	N.D.	0.102
8)	B Heptachlo...	0.000	4.777	0	148509	N.D.	<MDL
9)	A Endosulfan I	0.000	5.156	0	180333	N.D.	<MDL
14)	MA Endrin	0.000	5.680	0	901059	N.D.	0.342
15)	B Endosulfa...	0.000	5.915 ^f	0	291994	N.D.	0.101
18)	B Endrin al...	0.000	6.150	0	381964	N.D.	0.166


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010324\
Data File : PD080668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 16:06
Operator : AR\AJ
Sample : PIBLK155
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 21:39:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

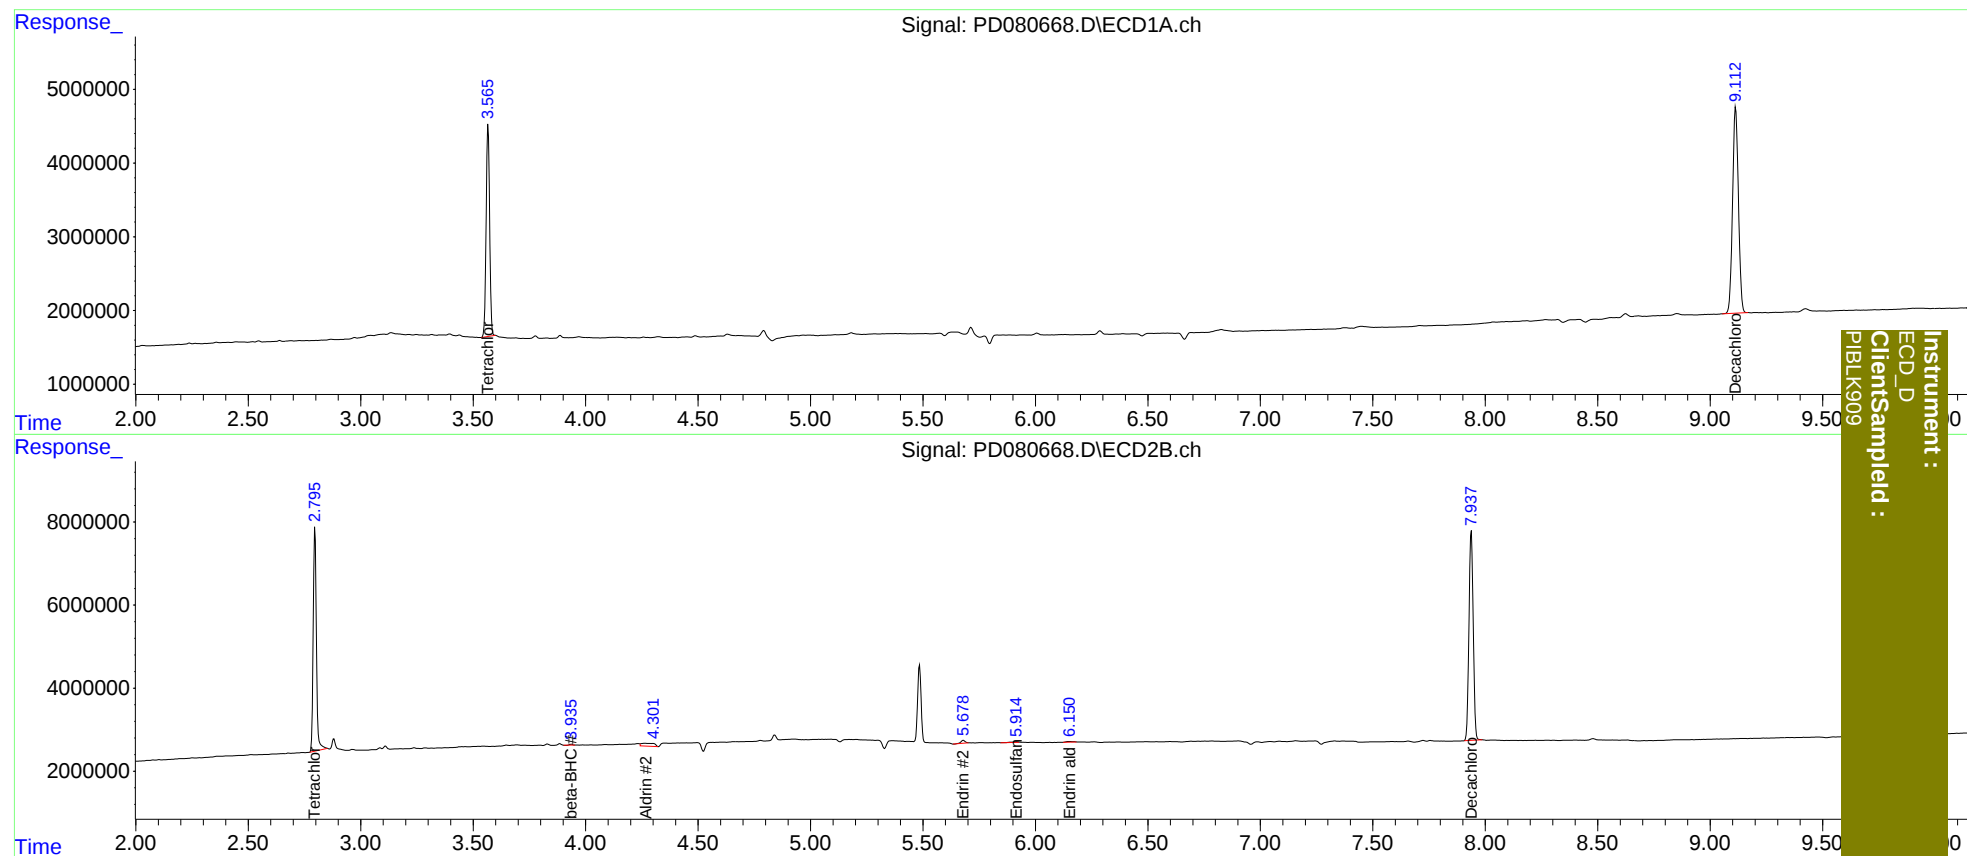


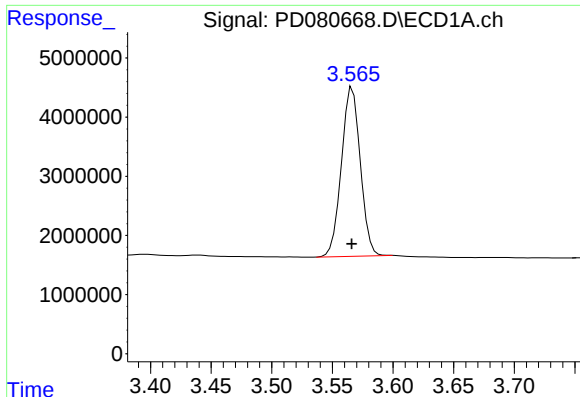

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 30972073
Conc: 24.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK909

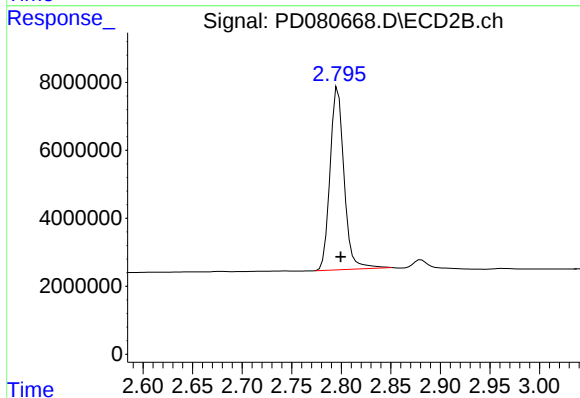


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: -0.003 min
Response: 52985679
Conc: 23.83 ng/ml

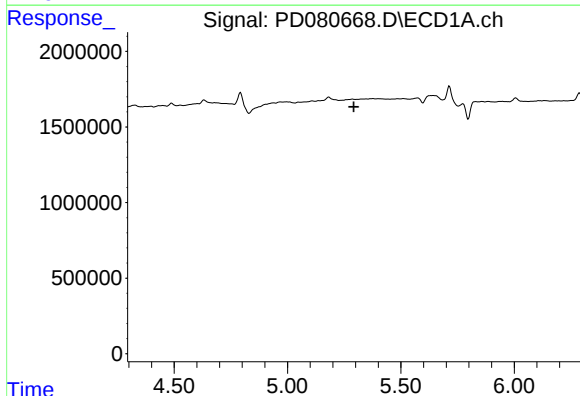


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

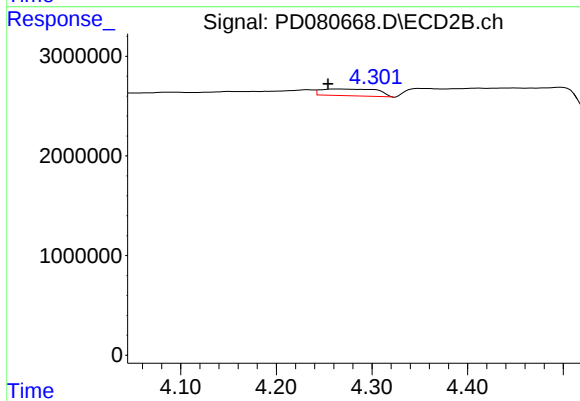

#5 Aldrin


R.T.: 4.269 min
Delta R.T.: 0.015 min
Response: 2724132
Conc: 0.77 ng/ml

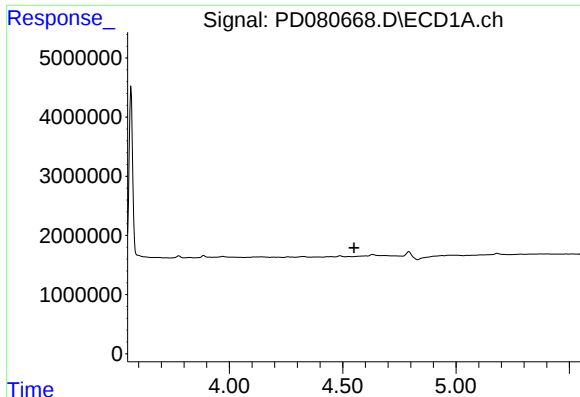

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK909

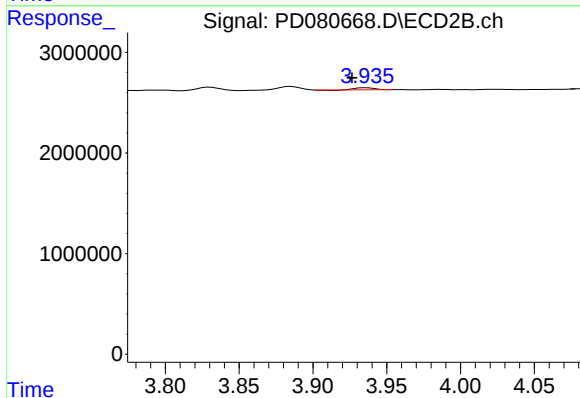


#6 beta-BHC

R.T.: 3.936 min
Delta R.T.: 0.010 min
Response: 174682
Conc: 0.10 ng/ml

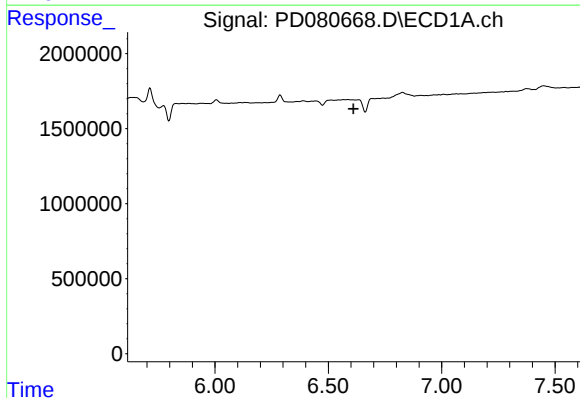


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

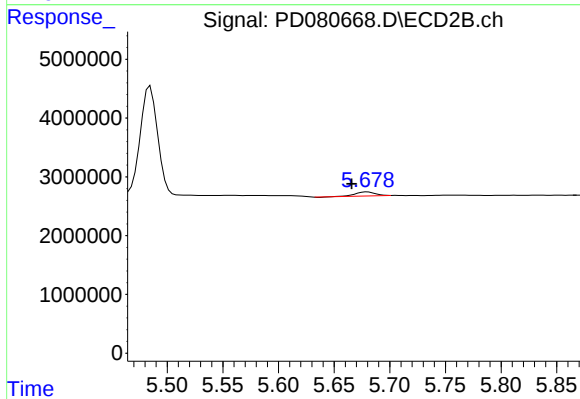

#14 Endrin


R.T.: 5.680 min
Delta R.T.: 0.014 min
Response: 901059
Conc: 0.34 ng/ml

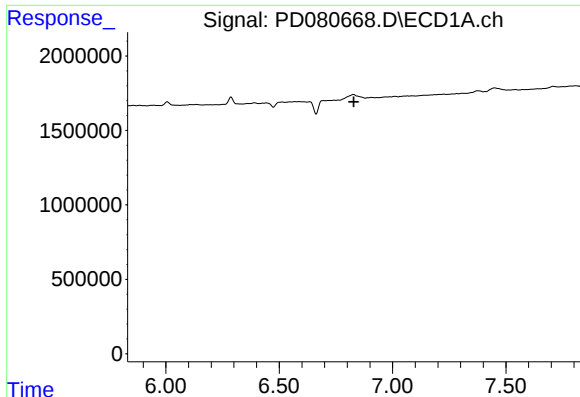

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK909

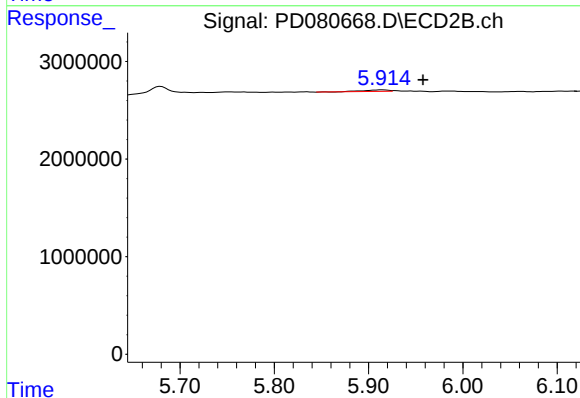


#15 Endosulfan II

R.T.: 5.915 min
Delta R.T.: -0.043 min
Response: 291994
Conc: 0.10 ng/ml

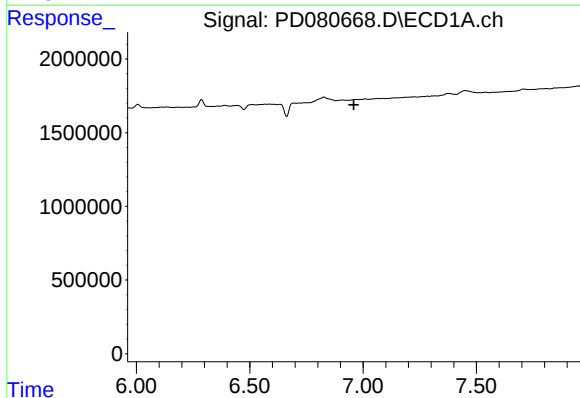


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

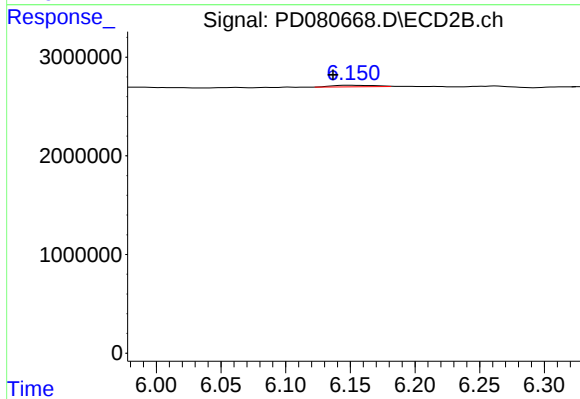

#18 Endrin aldehyde


R.T.: 6.150 min
Delta R.T.: 0.013 min
Response: 381964
Conc: 0.17 ng/ml

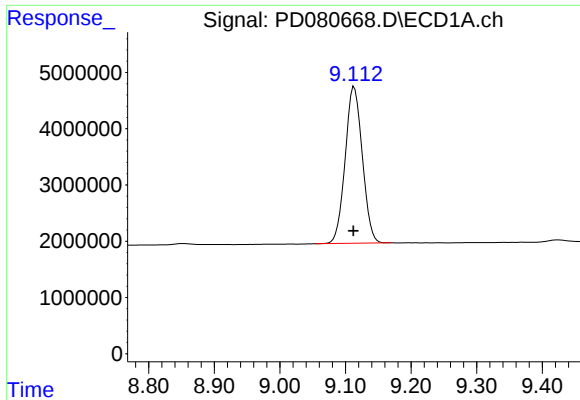

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.001 min
Response: 50525506
Conc: 31.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK909

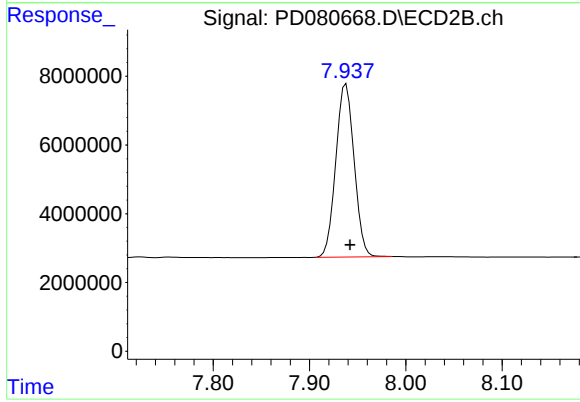

#27 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.004 min
Response: 66510994
Conc: 27.71 ng/ml