

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010422\
 Data File : PD067578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 11:07
 Operator : AR\AJ
 Sample : PIBLK197
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 00:14:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.433	3.962	38039562	147.7E6	16.790	18.229
27) SA Decachlor...	8.153	9.012	32314113	170.5E6	33.739	33.747
Target Compounds						
6) B beta-BHC	0.000	4.835	0	2411897	N.D.	0.522
7) B delta-BHC	0.000	5.050	0	975187	N.D.	0.104


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010422\
Data File : PD067578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 11:07
Operator : AR\AJ
Sample : PIBLK197
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 00:14:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

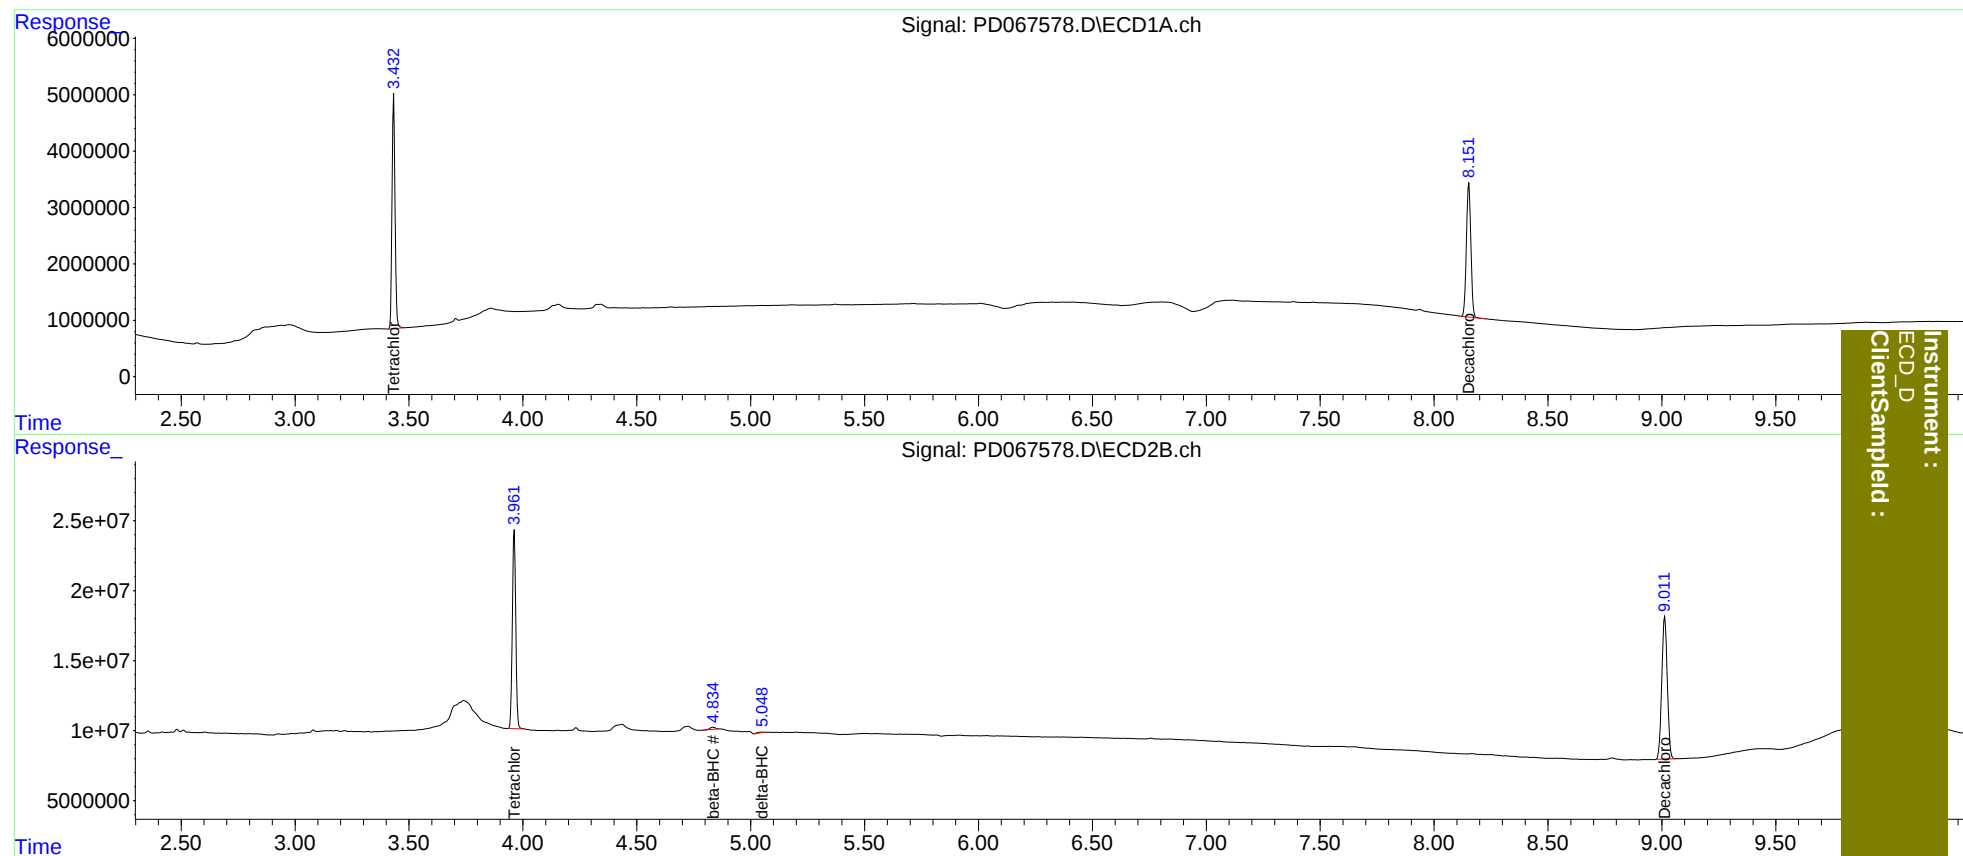


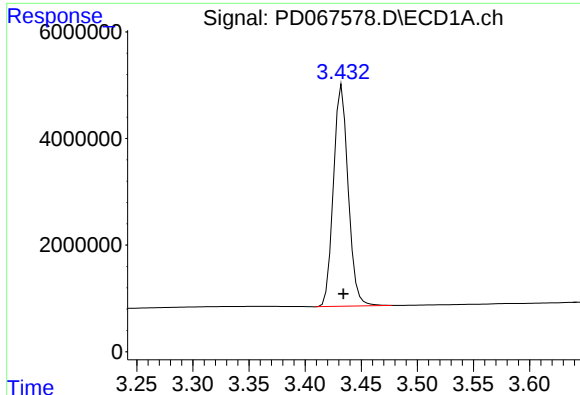

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: -0.001 min
Response: 38039562
Conc: 16.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

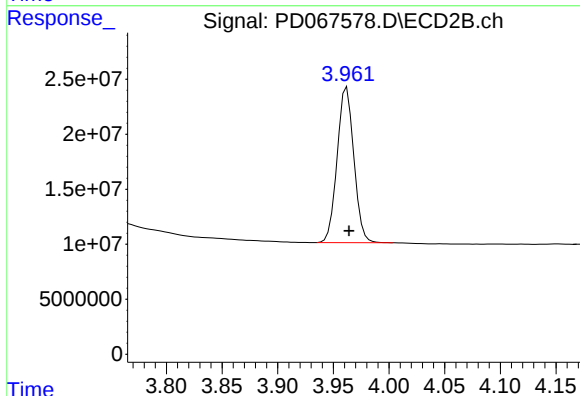


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.002 min
Response: 147737985
Conc: 18.23 ng/ml

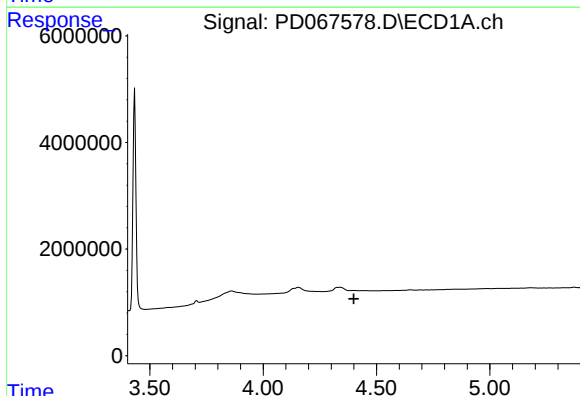


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.400 min
Response: 0
Conc: N.D.

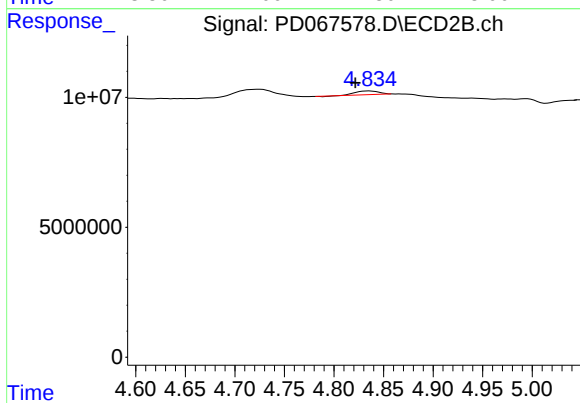

#6 beta-BHC


R.T.: 4.835 min
Delta R.T.: 0.013 min
Response: 2411897
Conc: 0.52 ng/ml

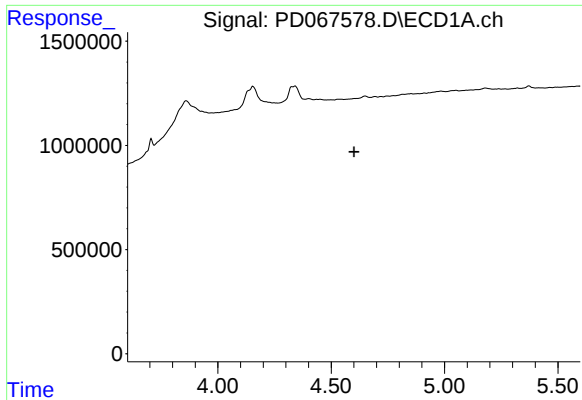

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

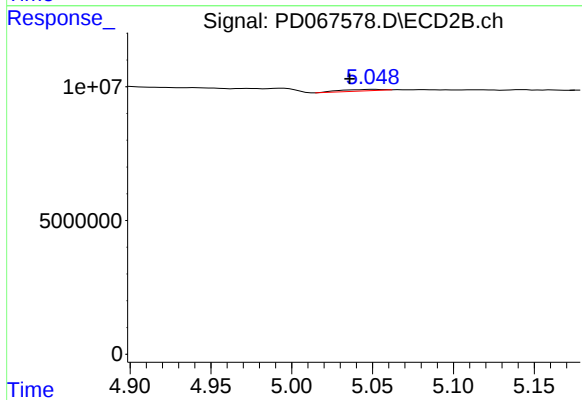


#7 delta-BHC

R.T.: 5.050 min
Delta R.T.: 0.014 min
Response: 975187
Conc: 0.10 ng/ml

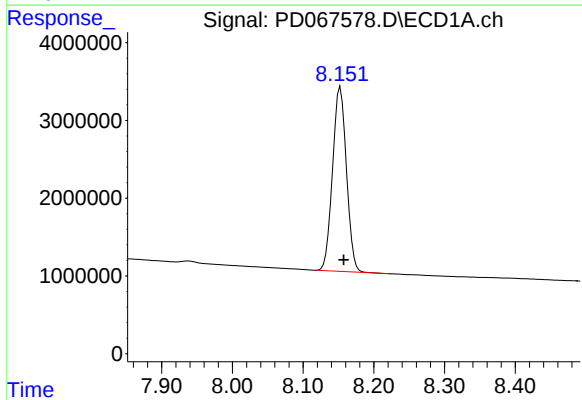

#27 Decachlorobiphenyl

R.T.: 8.153 min
Delta R.T.: -0.005 min
Response: 32314113
Conc: 33.74 ng/ml

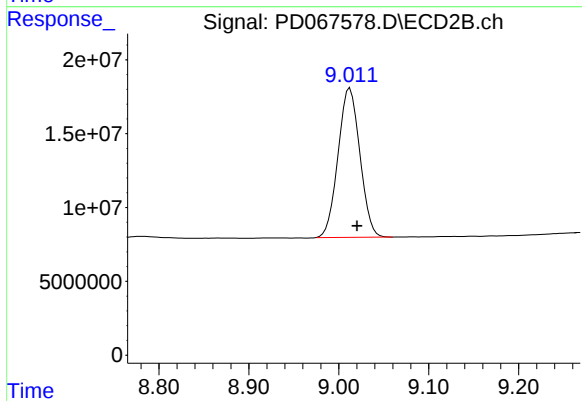

#27 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: -0.008 min
Response: 170526671
Conc: 33.75 ng/ml