

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010422\
 Data File : PD067586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 14:48
 Operator : AR\AJ
 Sample : PB141820BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS820

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
 Supervised By :mohammad ahmed 01/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 00:17:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.962	38665325	147.3E6	17.066	18.180
27)	SA Decachlor...	8.155	9.014	32569733	177.4E6	34.006	35.102
Target Compounds							
2)	A alpha-BHC	3.870	4.356	9129326	28224015	2.754	2.693
3)	MA gamma-BHC...	4.151	4.640	11397929	33694239	3.603	3.415
4)	MA Heptachlor	4.444	5.138	11821333	39821081	3.814	4.453m
5)	MB Aldrin	4.689	5.443	11937263	36557833	3.818	4.359
6)	B beta-BHC	4.400	4.818	5555826	23552687	4.134	5.093m
7)	B delta-BHC	4.602	5.033	14379511	54053085	4.862	5.765
8)	B Heptachlo...	5.128	5.830	11398339	33128217	4.100m	3.949m
9)	A Endosulfan I	5.465	6.187	10531031	31267781	3.979	4.352m
10)	B trans-Chl...	5.353	6.066	11792946	32858625	4.177	4.394
11)	B cis-Chlor...	5.411	6.137	11328815	32948615	4.133	4.471
12)	B 4,4'-DDE	5.575	6.298	21317216	63292336	8.487	9.374
13)	MA Dieldrin	5.707	6.447	21716441	64916525	7.705	8.633
14)	MA Endrin	5.964	6.665	16780737	41998077	7.532	7.529
15)	B Endosulfa...	6.237	6.880	18349865	58125486	8.483	9.201
16)	A 4,4'-DDD	6.089	6.792	15793031	50607688	7.927	8.610
17)	MA 4,4'-DDT	6.328	7.089	13344604	42567654	6.480	7.327
18)	B Endrin al...	6.406	7.005	16418449	50483556	10.541	10.682
19)	B Endosulfa...	6.617	7.228	10928293	36953185	6.015	6.334
20)	A Methoxychlor	6.876	7.552	35456556	117.0E6	40.201	42.443
21)	B Endrin ke...	7.110	7.701	18389408	64765761	9.665	9.781

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010422\
Data File : PD067586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 14:48
Operator : AR\AJ
Sample : PB141820BS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 00:17:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

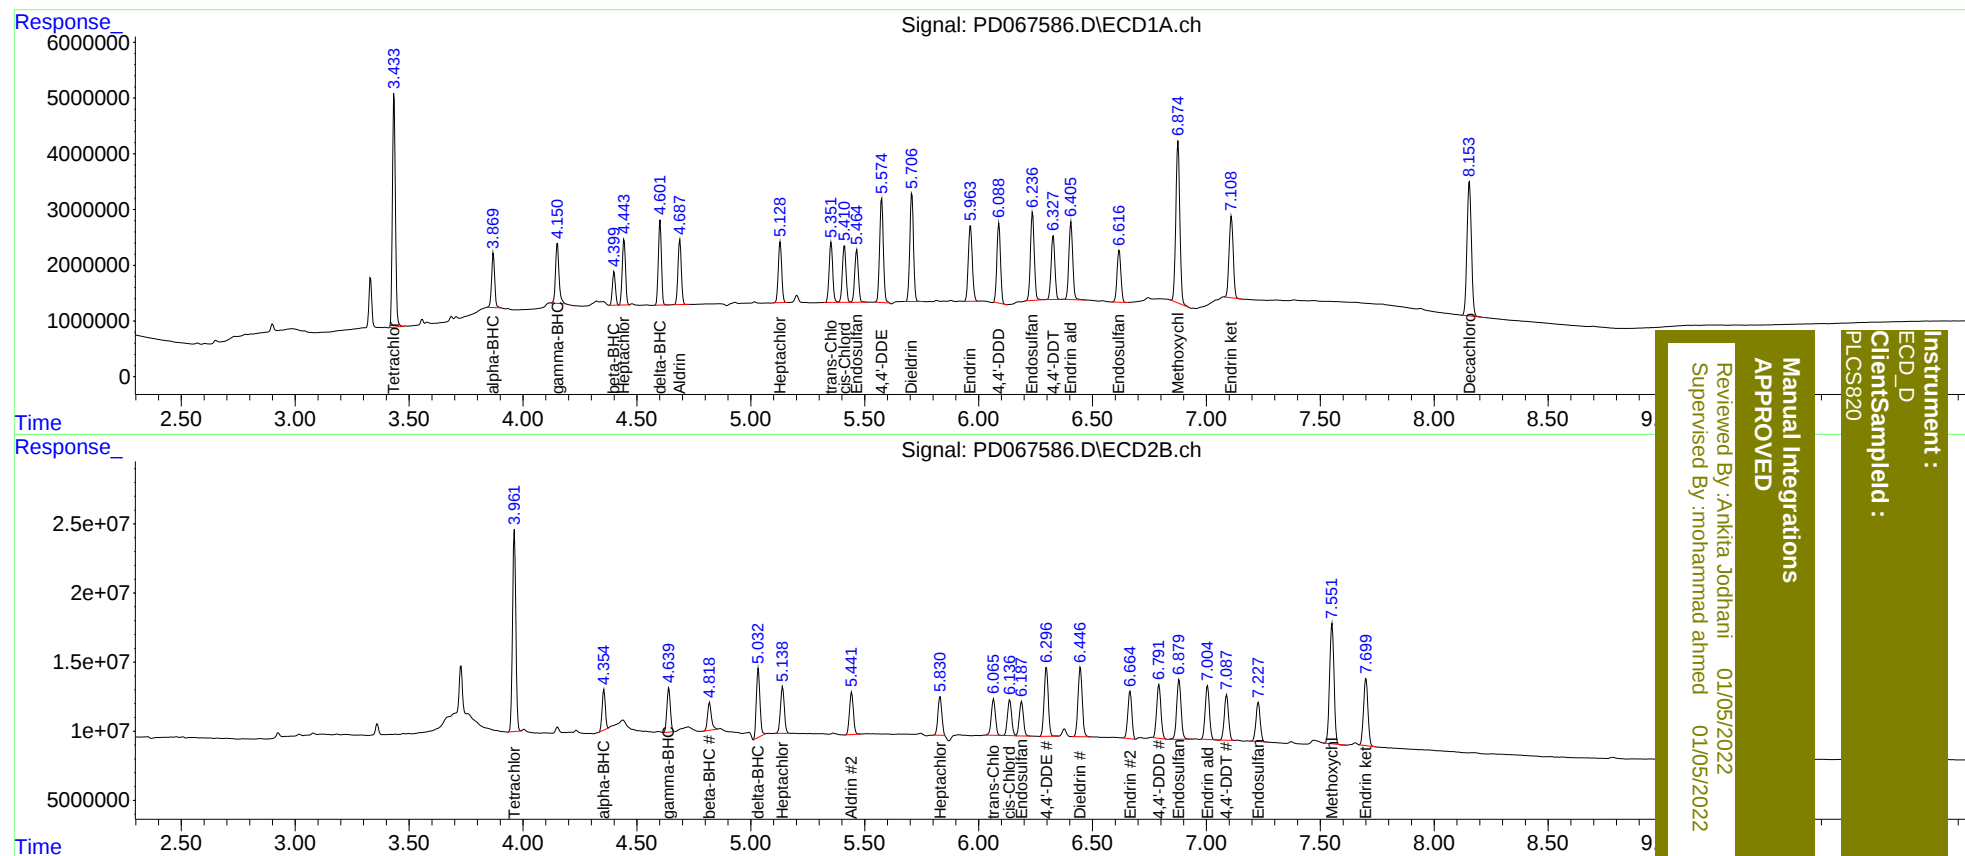

Instrument :
ECD_D
ClientSampled :
PLCS820

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/05/2022
Supervised By :mohammad ahmed 01/05/2022