

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010424\
 Data File : PD080713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2024 14:32
 Operator : AR\AJ
 Sample : 05961-21MS
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGSM2MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/05/2024
 Supervised By :Ankita Jodhani 01/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 22:23:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:52:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.796	25716285	44897439	20.141	20.192
2)	SA Decachlor...	9.115	7.938	41509412	56152357	25.818	23.394
Target Compounds							
2)	A alpha-BHC	4.023	3.299	132.2E6	214.8E6	64.126	62.998
3)	MA gamma-BHC...	4.354	3.628	122.2E6	199.0E6	61.524m	61.815
4)	MA Heptachlor	4.949	3.969	127.0E6	239.9E6	60.795	74.898
5)	MB Aldrin	5.293	4.251	121.3E6	193.7E6	54.228	54.819
6)	B beta-BHC	4.550	3.924	52792656	84570743	50.860	49.254
7)	B delta-BHC	4.800	4.154	153.8E6	206.4E6	66.960	53.101
8)	B Heptachlo...	5.719	4.752	112.9E6	181.8E6	52.564	53.638
9)	A Endosulfan I	6.106	5.122	106.6E6	170.2E6	59.859	62.101
10)	B trans-Chl...	5.975	5.002	110.3E6	180.2E6	53.771	54.729
11)	B cis-Chlor...	6.056	5.066	114.4E6	182.2E6	54.498	54.185
12)	B 4,4'-DDE	6.227	5.255	216.6E6	352.9E6	112.132	112.359
13)	MA Dieldrin	6.382	5.387	238.9E6	386.8E6	128.362	129.072
14)	MA Endrin	6.613	5.662	200.0E6	342.3E6	127.711	130.085
15)	B Endosulfa...	6.831	5.955	197.8E6	319.1E6	105.511	110.057
16)	A 4,4'-DDD	6.743	5.808	175.6E6	284.6E6	126.603	123.788
17)	MA 4,4'-DDT	7.060	6.060	192.4E6	303.8E6	130.197	125.994
18)	B Endrin al...	6.960	6.134	133.9E6	212.0E6	89.760	91.958
19)	B Endosulfa...	7.195	6.356	192.8E6	304.7E6	105.107	108.624
20)	A Methoxychlor	7.533	6.634	473.5E6	716.6E6	598.060	569.233
21)	B Endrin ke...	7.682	6.863	210.5E6	345.8E6	108.173	108.058

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010424\
Data File : PD080713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2024 14:32
Operator : AR\AJ
Sample : 05961-21MS
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 22:23:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:52:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

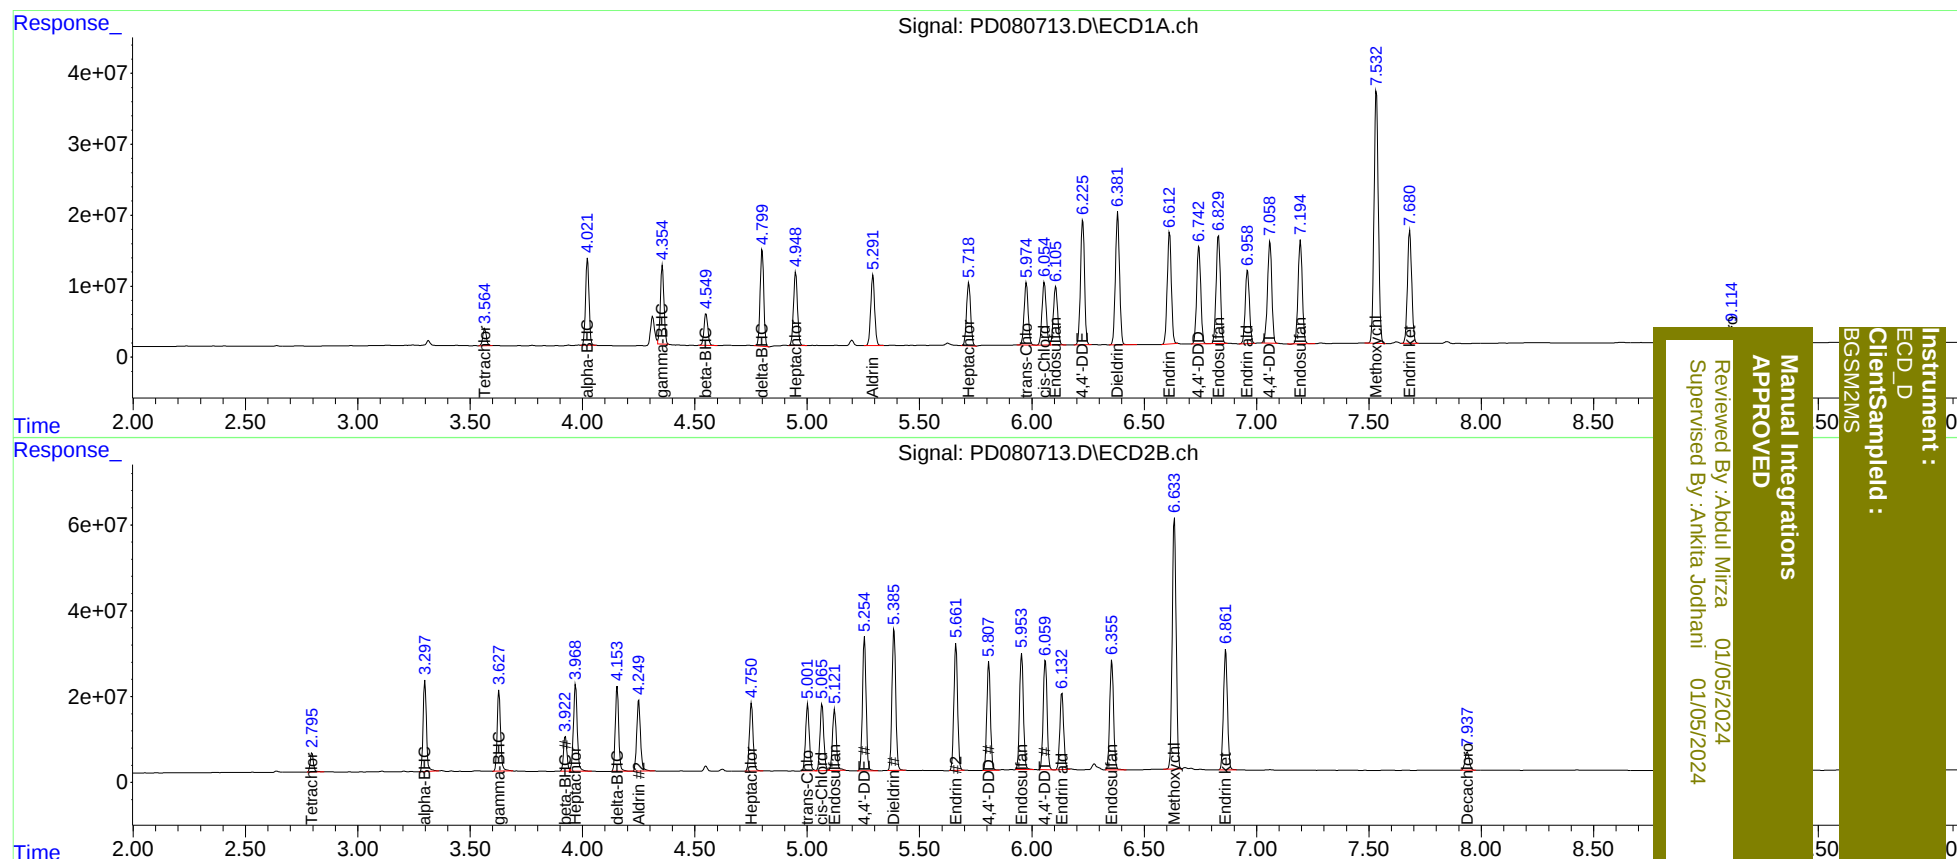

Instrument :
ECD_D
ClientSampled :
BGSIMZMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/05/2024
Supervised By: Ankita Jodhani 01/05/2024