

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010522\
 Data File : PD067611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 21:32
 Operator : AR\AJ
 Sample : N1010-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20211307-CAPE-1-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 03:30:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.963	38815015	144.2E6	21.359	21.856
28)	SA Decachlor...	8.153	9.014	15534250	82830904	17.488	17.429

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010522\
Data File : PD067611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 21:32
Operator : AR\AJ
Sample : N1010-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20211307-CAPE-1-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 03:30:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

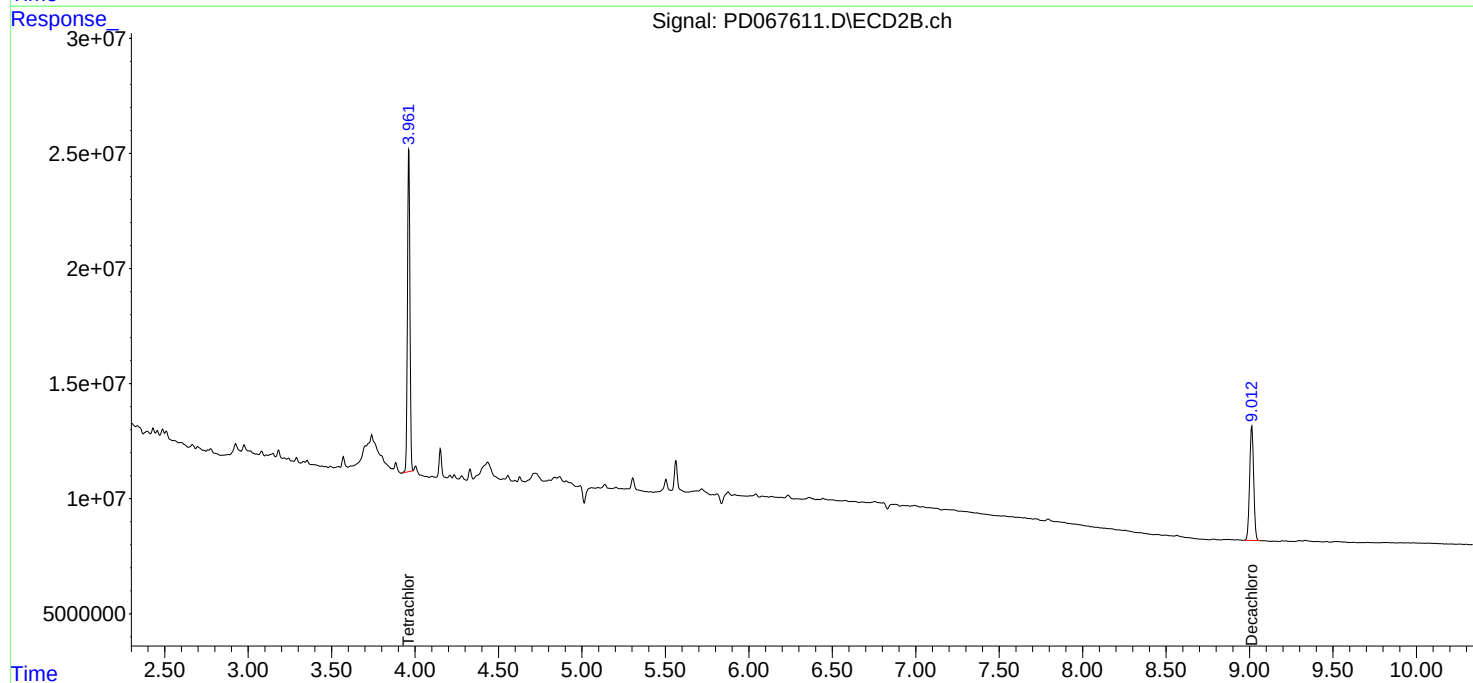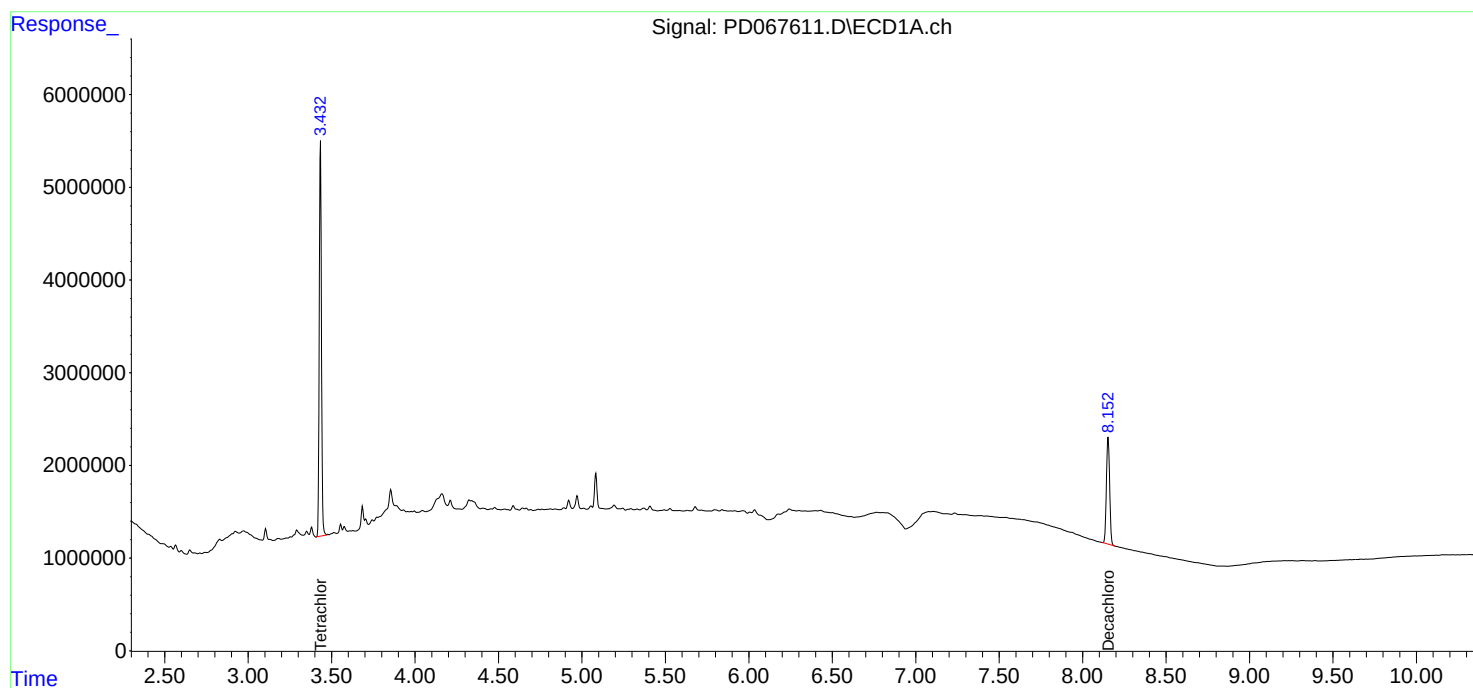


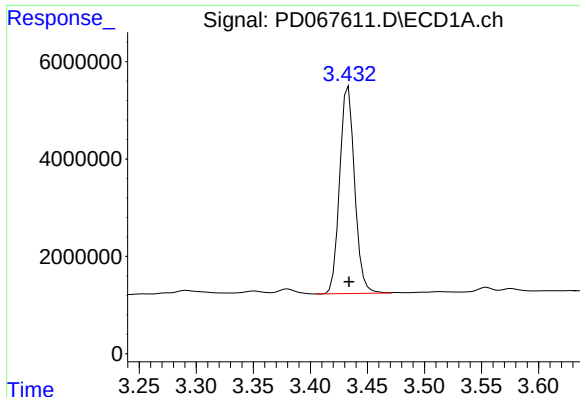

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 38815015
Conc: 21.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
20211307-CAPE-1-SITE-WATER

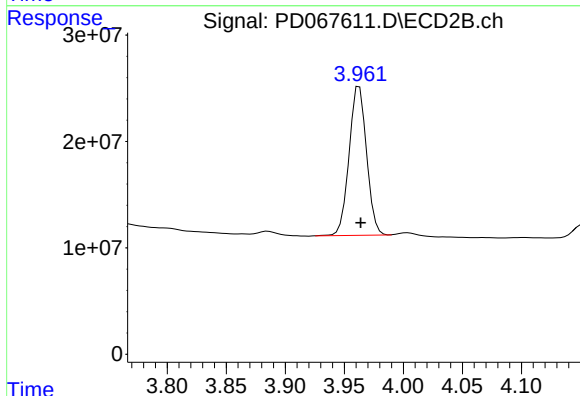


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: 0.000 min
Response: 144208558
Conc: 21.86 ng/ml

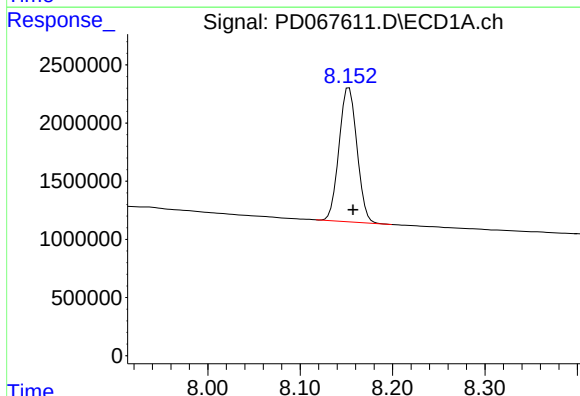

#28 Decachlorobiphenyl

R.T.: 8.153 min
Delta R.T.: -0.004 min
Response: 15534250
Conc: 17.49 ng/ml

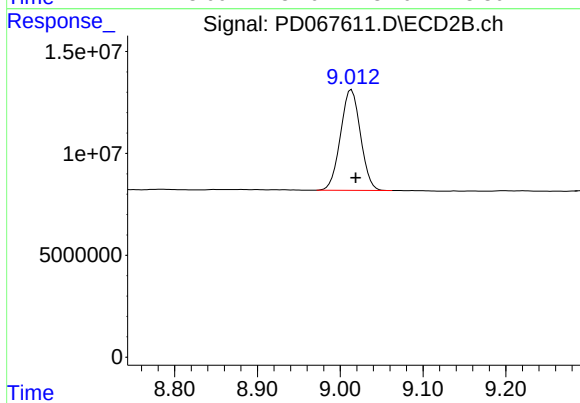

#28 Decachlorobiphenyl

R.T.: 9.014 min
Delta R.T.: -0.005 min
Response: 82830904
Conc: 17.43 ng/ml