

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010522\
 Data File : PD067613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 22:00
 Operator : AR\AJ
 Sample : N1010-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20211309-CAPE-3-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 03:31:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	3.962	38260621	142.5E6	21.054	21.596
28)	SA Decachlor...	8.154	9.014	15223408	81743012	17.138	17.200

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010522\
Data File : PD067613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 22:00
Operator : AR\AJ
Sample : N1010-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20211309-CAPE-3-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 03:31:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

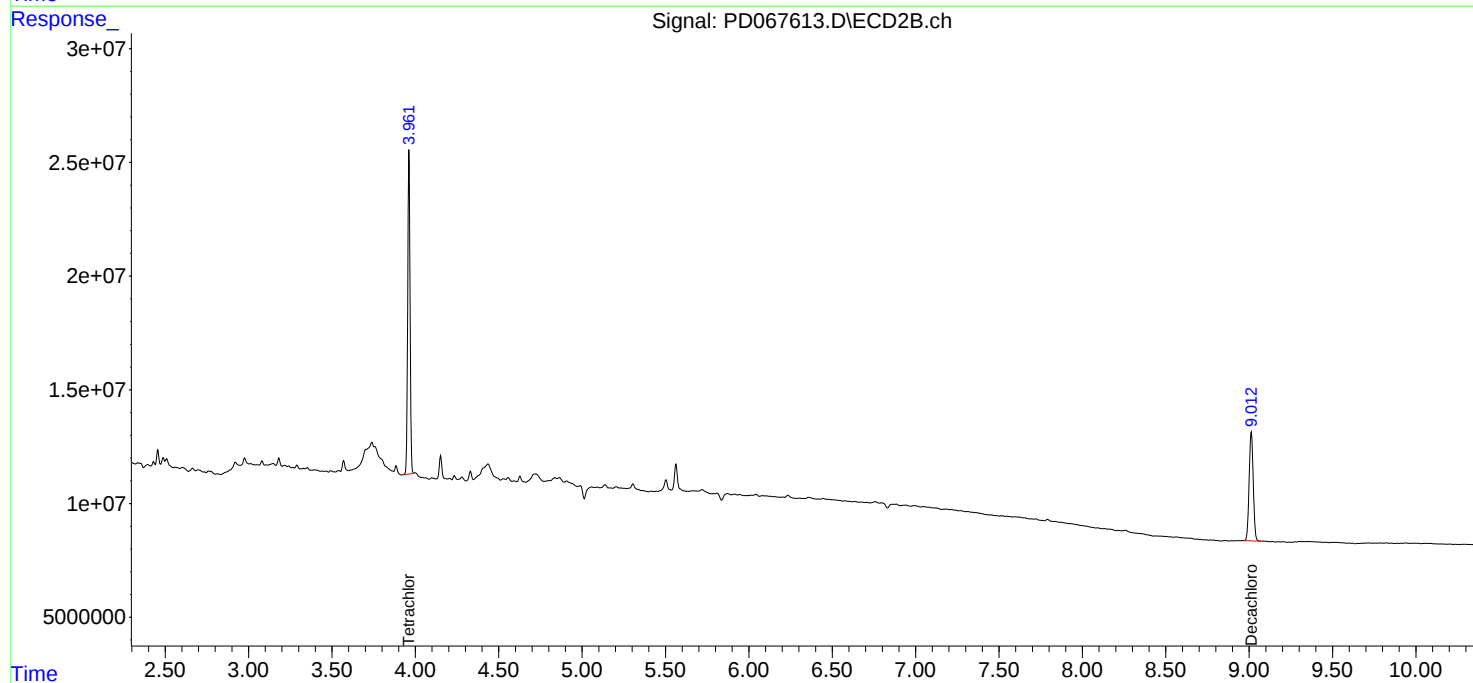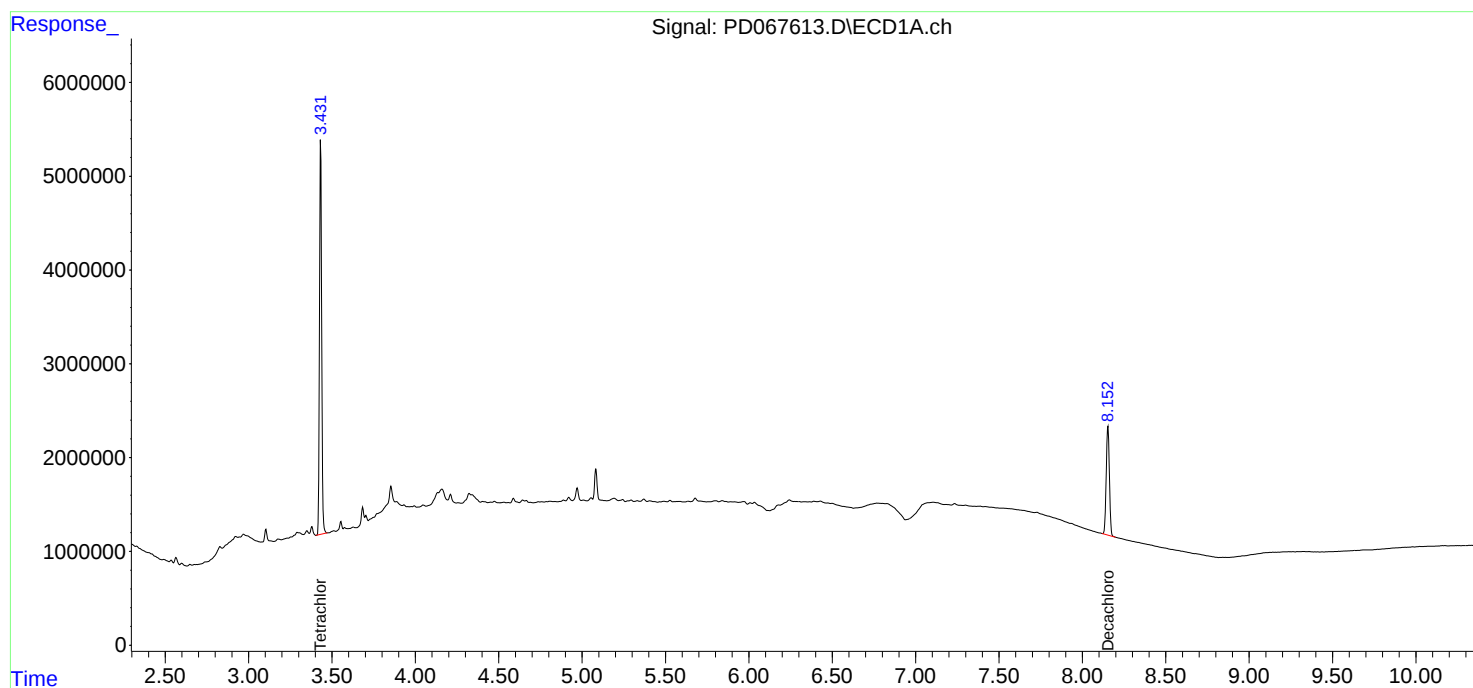


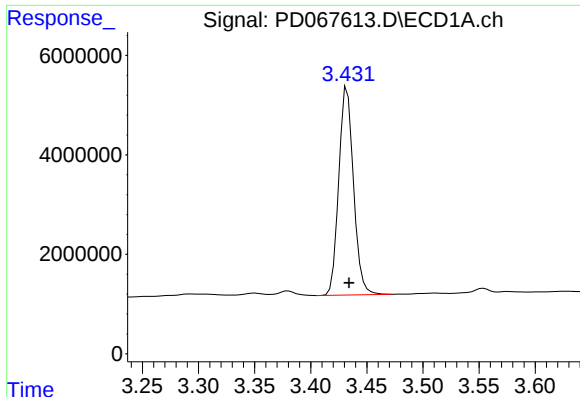

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: -0.001 min
Response: 38260621
Conc: 21.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
20211309-CAPE-3-SITE-WATER

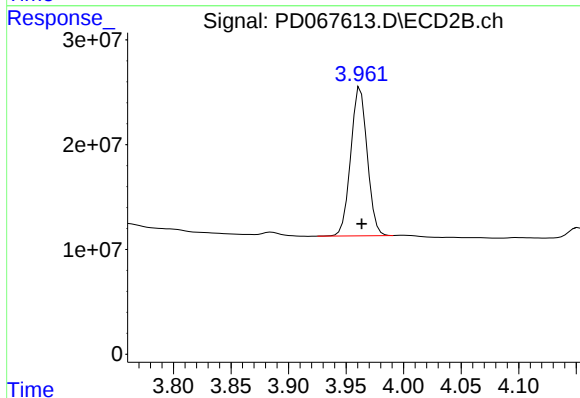


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.001 min
Response: 142497145
Conc: 21.60 ng/ml

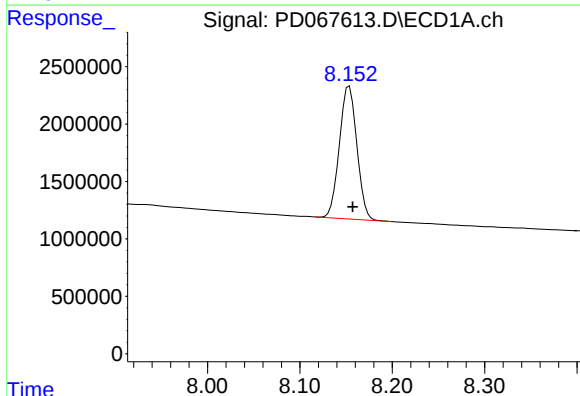

#28 Decachlorobiphenyl

R.T.: 8.154 min
Delta R.T.: -0.004 min
Response: 15223408
Conc: 17.14 ng/ml

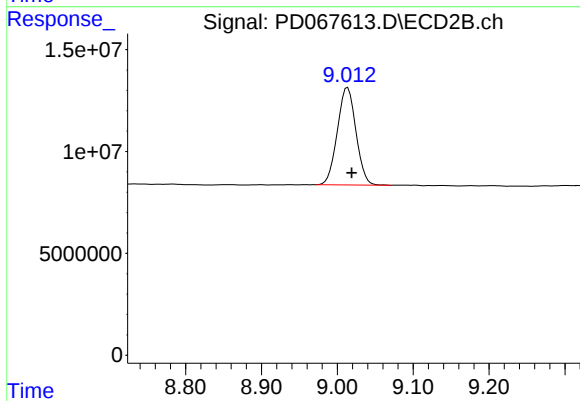

#28 Decachlorobiphenyl

R.T.: 9.014 min
Delta R.T.: -0.005 min
Response: 81743012
Conc: 17.20 ng/ml