

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 10:18
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 11:29:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 11:28:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	7430468	36964420	5.653	5.286
27)	SA Decachlor...	8.280	9.104	17788531	68581034	11.006	10.990
Target Compounds							
2)	A alpha-BHC	3.937	4.411	10070042	54683224	5.200	5.118
3)	MA gamma-BHC...	4.223	4.697	9894077	51202571	5.329	5.206
4)	MA Heptachlor	4.528	5.208	10646614	51108455	5.263	5.150
9)	A Endosulfan I	5.565	6.260	9296623	41220175	5.278	5.190
13)	MA Dieldrin	5.810	6.517	19498524	87038378	9.984	10.154
14)	MA Endrin	6.068	6.735	16408353	67539481	10.268	10.167
16)	A 4,4'-DDD	6.193	6.855	14209309	59883534	10.074	10.032
17)	MA 4,4'-DDT	6.436	7.154	15547204	64185618	9.873	10.311
20)	A Methoxychlor	6.982	7.611	40848957	155.9E6	52.682	53.280

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 10:18
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 11:29:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 11:28:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

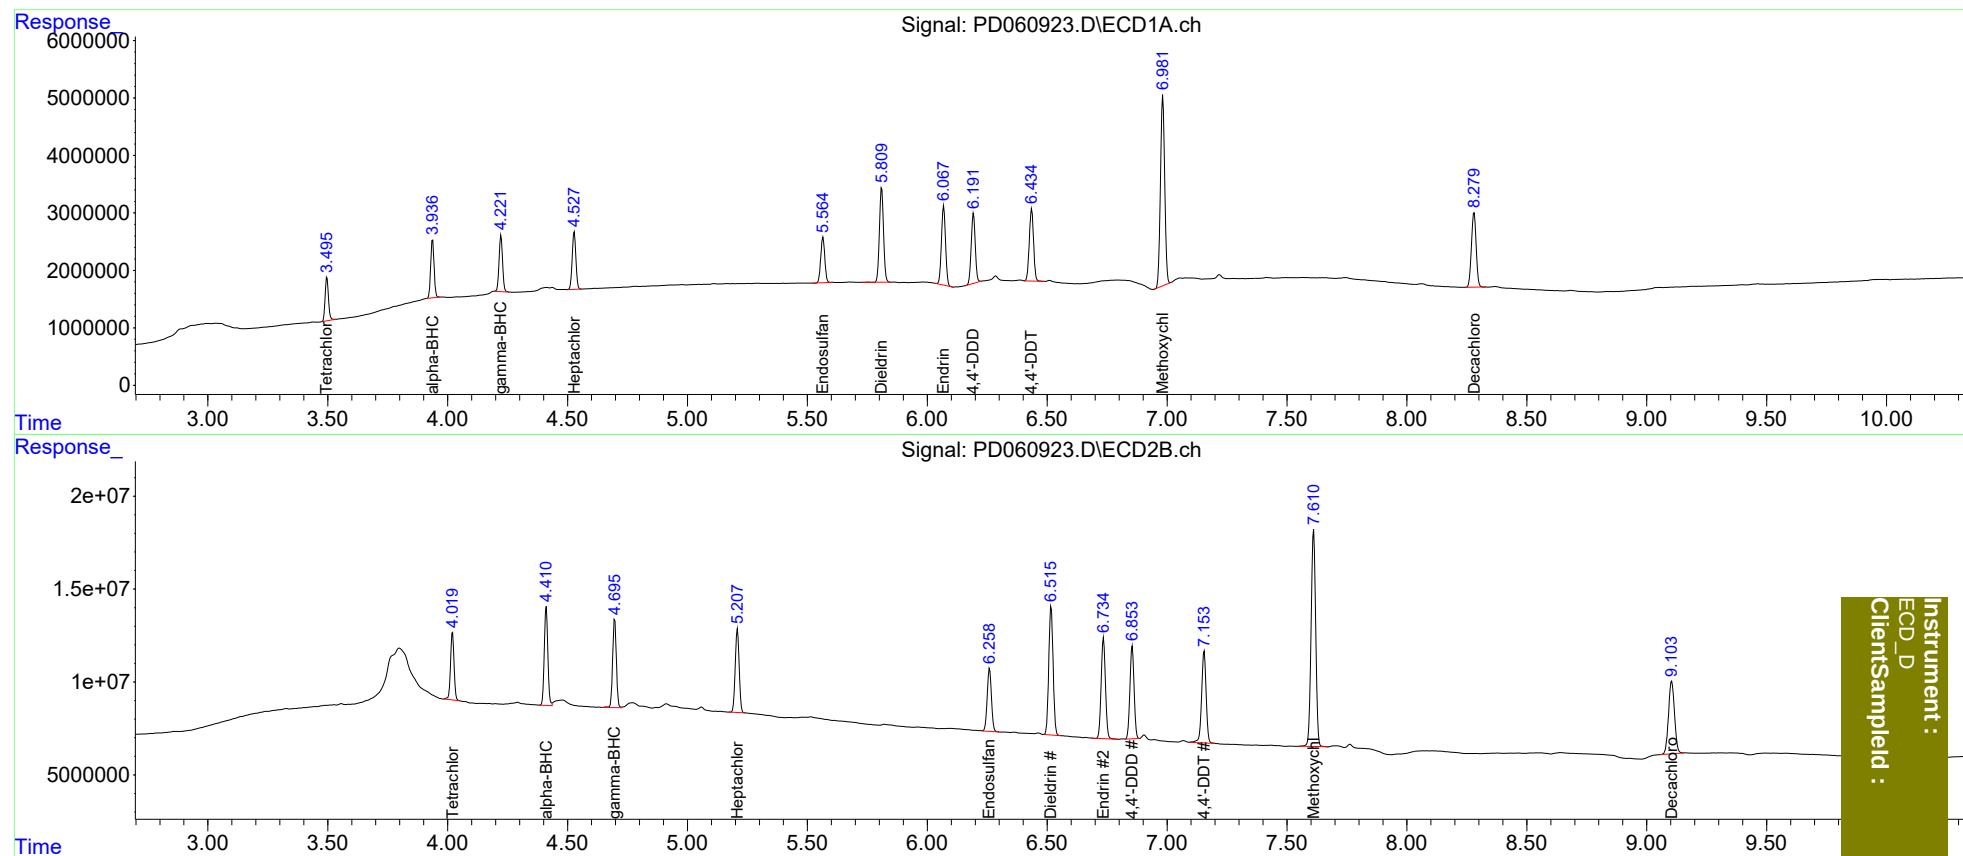


Instrument :
ECD_D
ClientSampled :

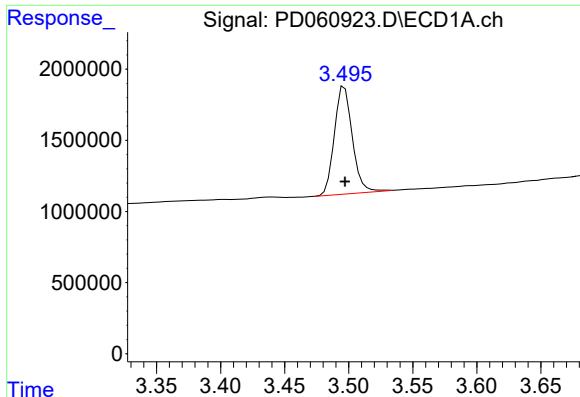

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 7430468
Conc: 5.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

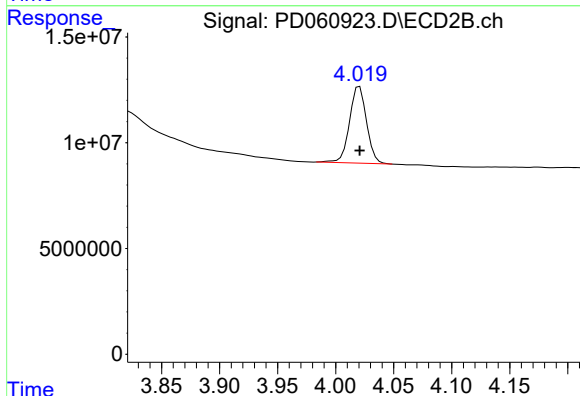


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 36964420
Conc: 5.29 ng/ml

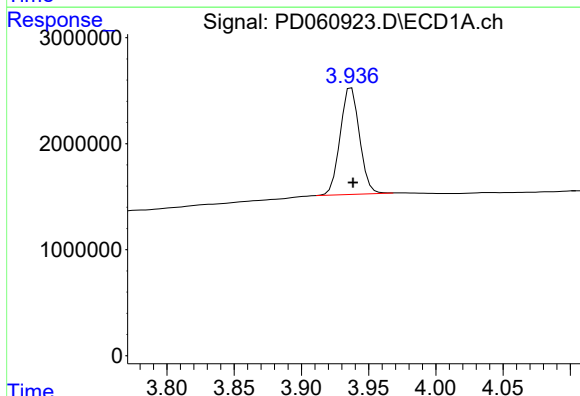


#2 alpha-BHC

R.T.: 3.937 min
Delta R.T.: -0.001 min
Response: 10070042
Conc: 5.20 ng/ml

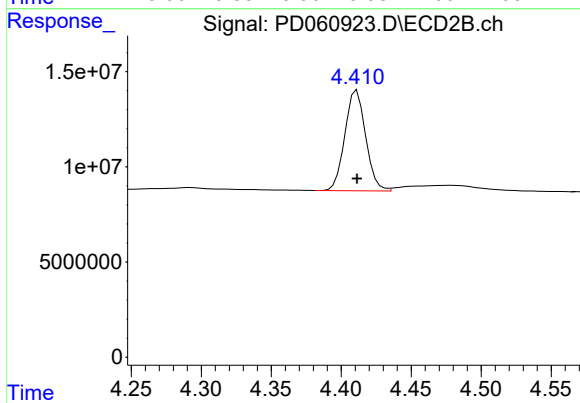

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 54683224
Conc: 5.12 ng/ml

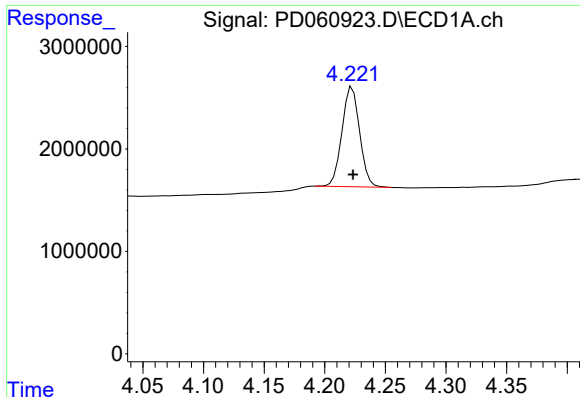

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 9894077
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

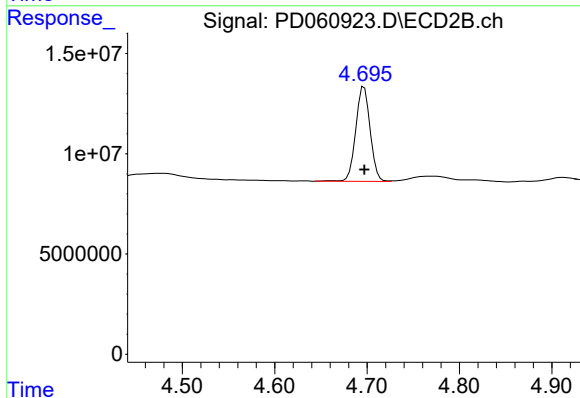


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 51202571
Conc: 5.21 ng/ml

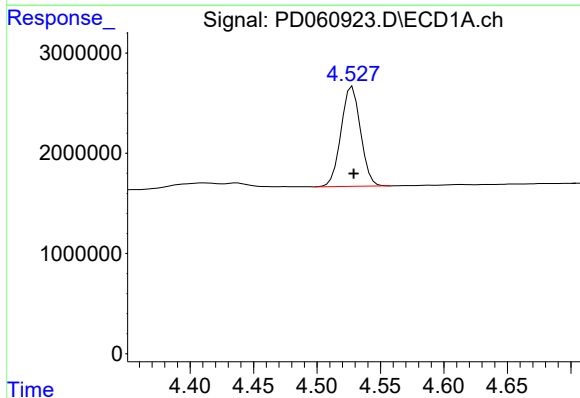


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 10646614
Conc: 5.26 ng/ml

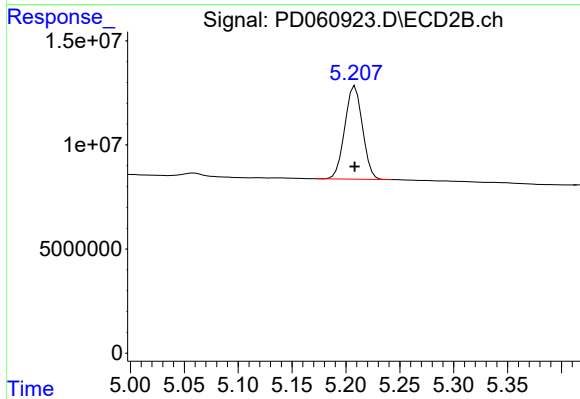

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 51108455
Conc: 5.15 ng/ml

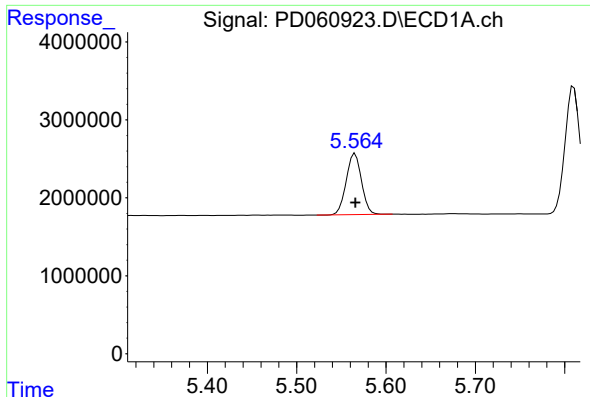

#9 Endosulfan I


R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 9296623
Conc: 5.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

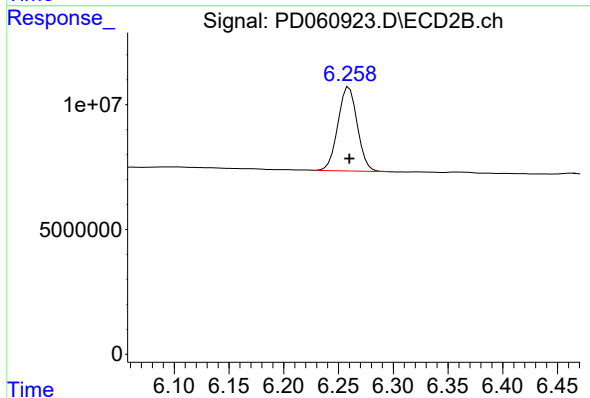


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 41220175
Conc: 5.19 ng/ml

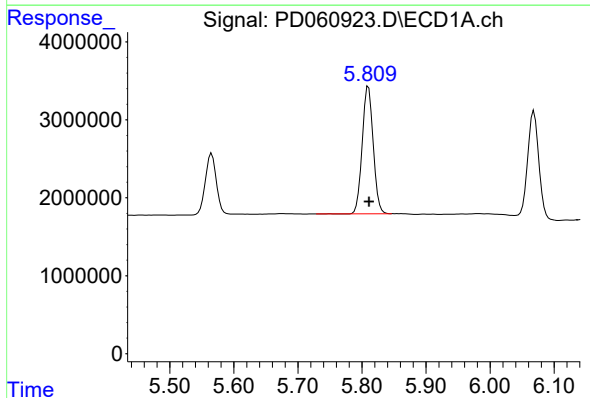


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 19498524
Conc: 9.98 ng/ml

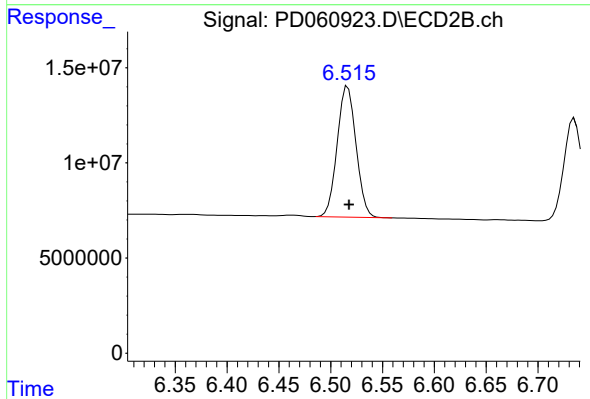

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: -0.001 min
Response: 87038378
Conc: 10.15 ng/ml

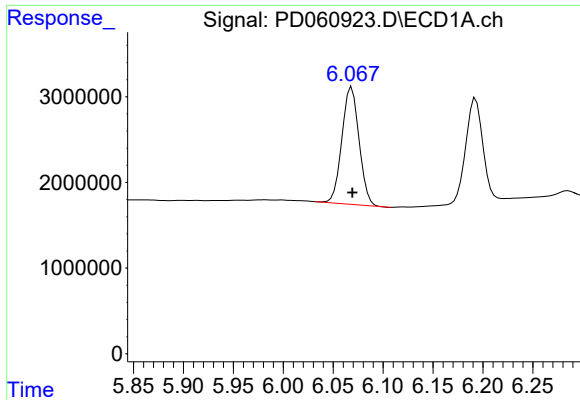

#14 Endrin


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 16408353
Conc: 10.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

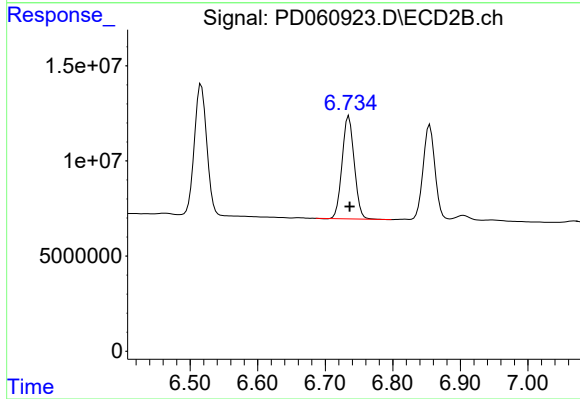


#14 Endrin

R.T.: 6.735 min
Delta R.T.: -0.001 min
Response: 67539481
Conc: 10.17 ng/ml

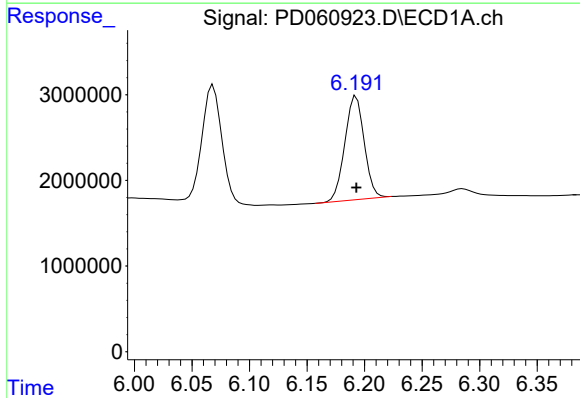


#16 4,4'-DDD

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 14209309
Conc: 10.07 ng/ml

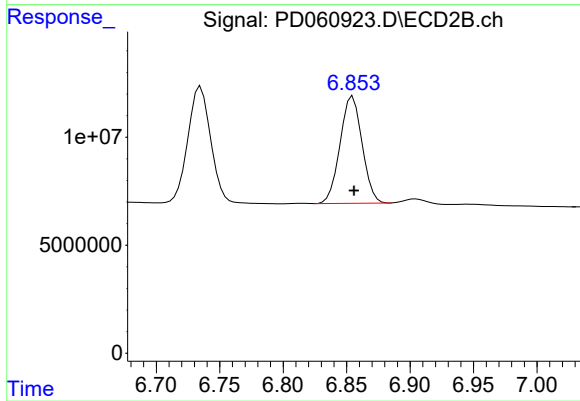

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: 0.000 min
Response: 59883534
Conc: 10.03 ng/ml

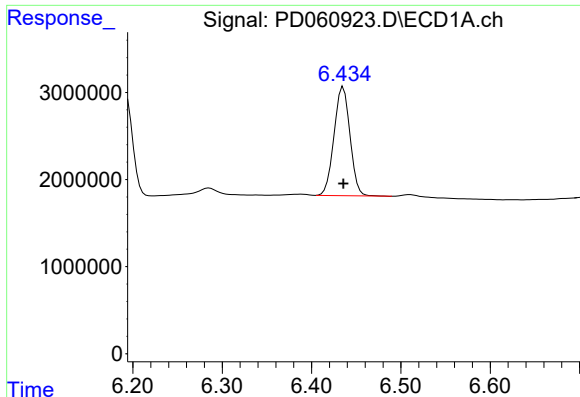

#17 4,4'-DDT


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 15547204
Conc: 9.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

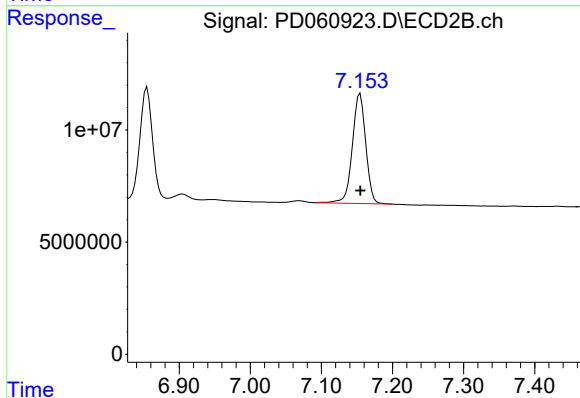


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 64185618
Conc: 10.31 ng/ml

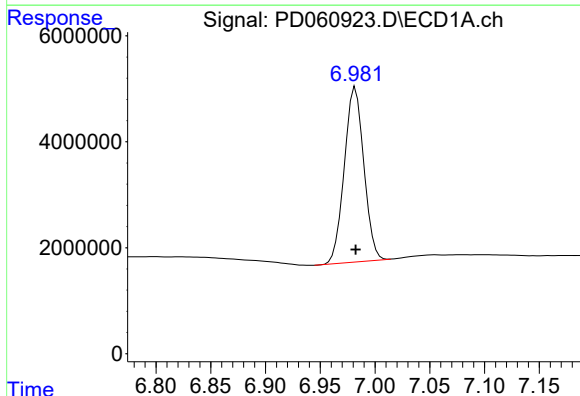


#20 Methoxychlor

R.T.: 6.982 min
Delta R.T.: 0.000 min
Response: 40848957
Conc: 52.68 ng/ml

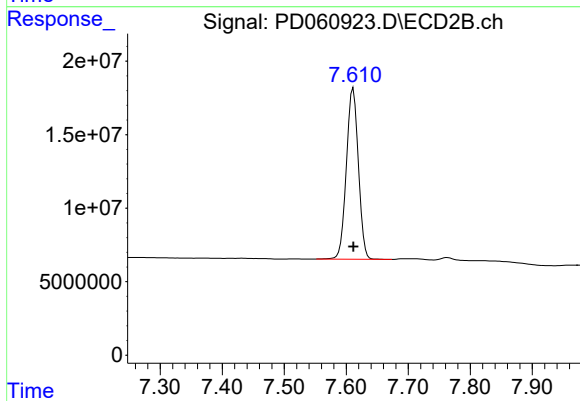

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 155877285
Conc: 53.28 ng/ml

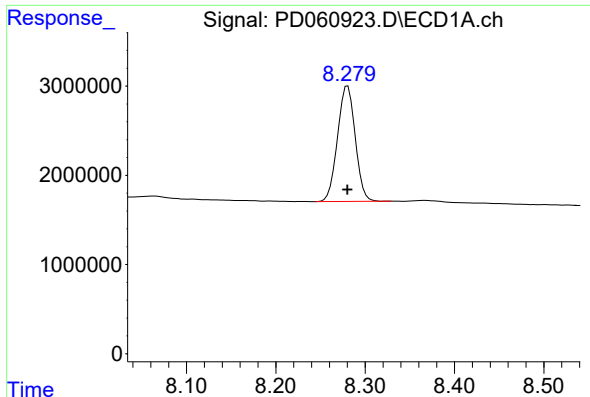

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 17788531
Conc: 11.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

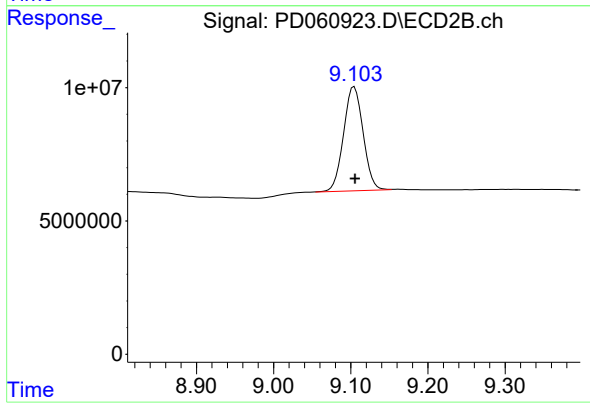

#27 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: -0.001 min
Response: 68581034
Conc: 10.99 ng/ml