

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 10:46
 Operator : DD\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 11:29:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 11:28:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	13907726	71583339	10.580	10.237
27)	SA Decachlor...	8.280	9.105	34352950	131.7E6	21.254	21.108
Target Compounds							
2)	A alpha-BHC	3.938	4.411	19576555	108.6E6	10.110	10.165
3)	MA gamma-BHC...	4.223	4.697	18939437	99540030	10.201	10.120
4)	MA Heptachlor	4.528	5.208	20574867	101.7E6	10.171	10.245
9)	A Endosulfan I	5.566	6.259	18005351	80974198	10.223	10.196
13)	MA Dieldrin	5.810	6.517	38776292	173.3E6	19.855	20.222
14)	MA Endrin	6.069	6.735	32221996	134.2E6	20.163	20.203
16)	A 4,4'-DDD	6.192	6.854	28237447	120.3E6	20.020	20.155
17)	MA 4,4'-DDT	6.436	7.154	31202047	128.1E6	19.814	20.583
20)	A Methoxychlor	6.983	7.611	79764010	307.5E6	102.871	105.097

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 10:46
Operator : DD\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 11:29:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 11:28:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

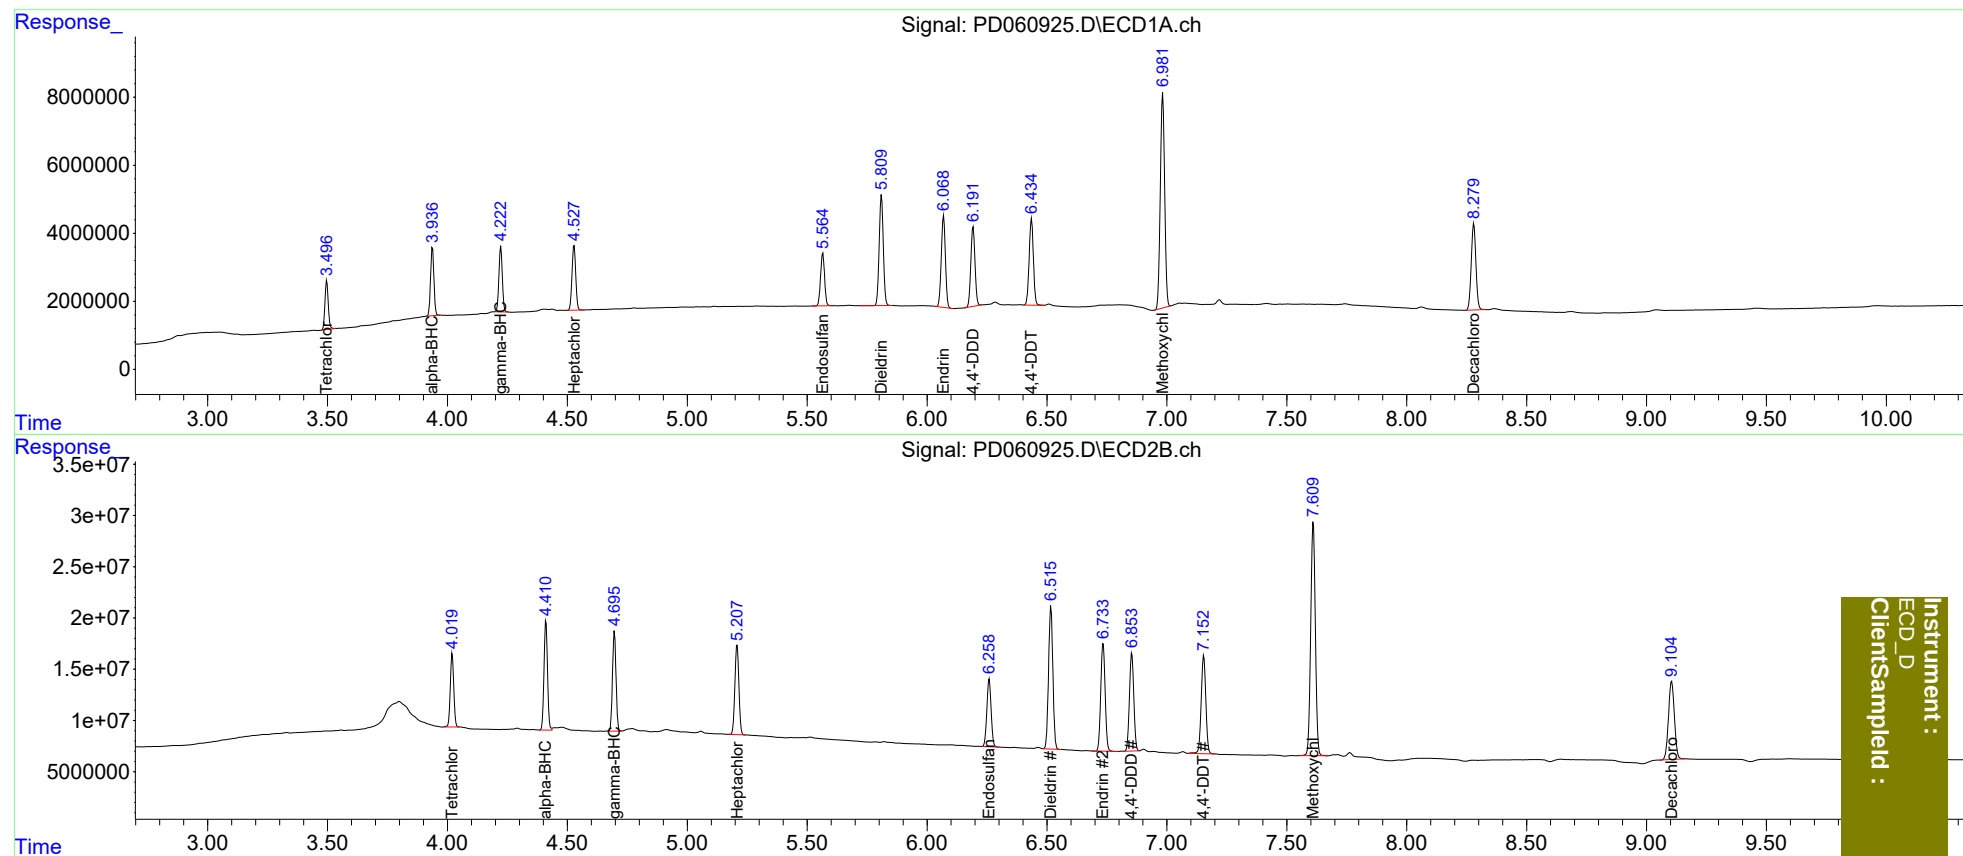


Instrument :
ECD_D
ClientSampled :

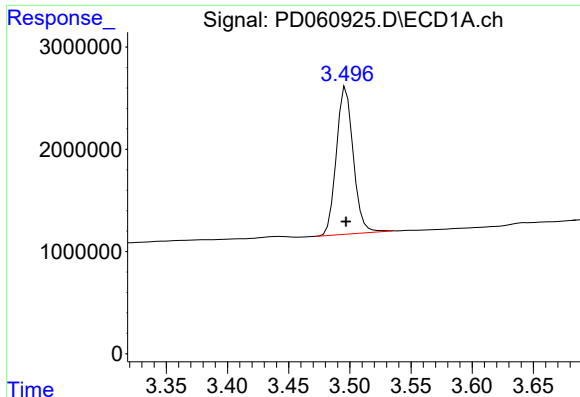

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 13907726
Conc: 10.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

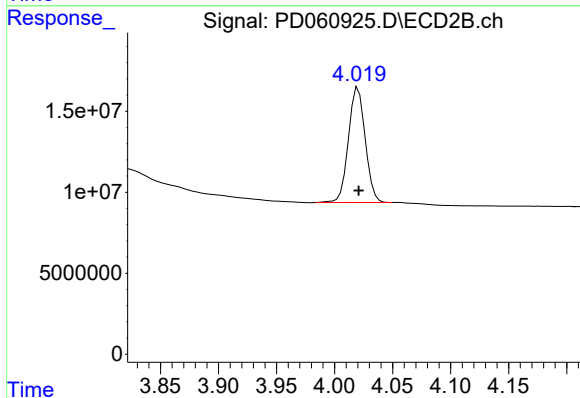


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 71583339
Conc: 10.24 ng/ml

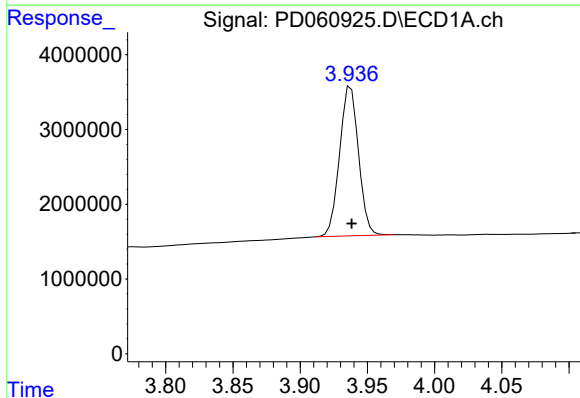


#2 alpha-BHC

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 19576555
Conc: 10.11 ng/ml

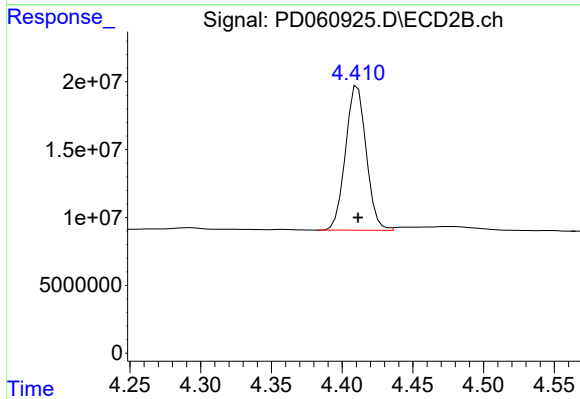

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 108594935
Conc: 10.16 ng/ml

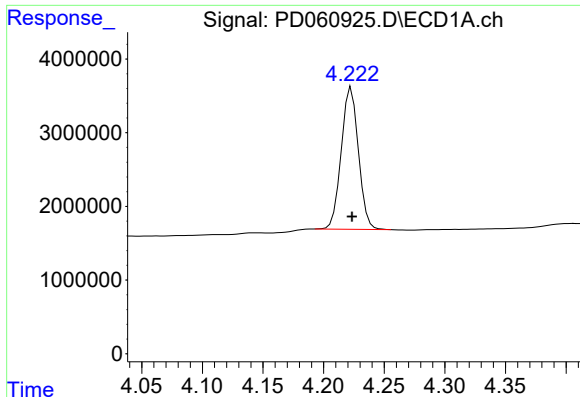

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 18939437
Conc: 10.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

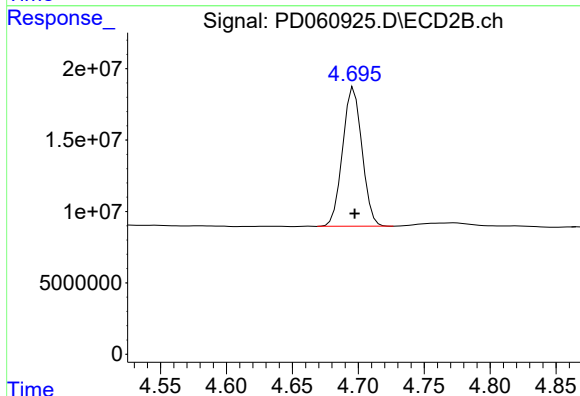


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 99540030
Conc: 10.12 ng/ml

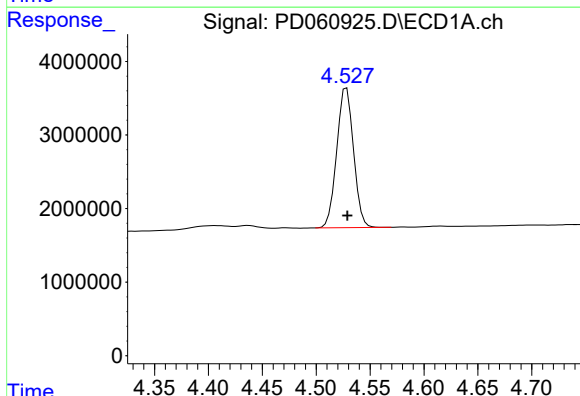


#4 Heptachlor

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 20574867
Conc: 10.17 ng/ml

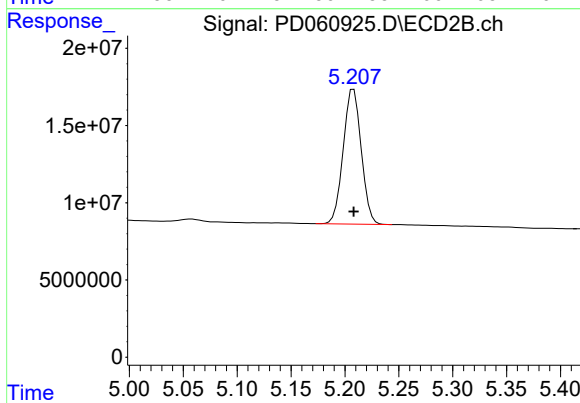

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 101680113
Conc: 10.25 ng/ml

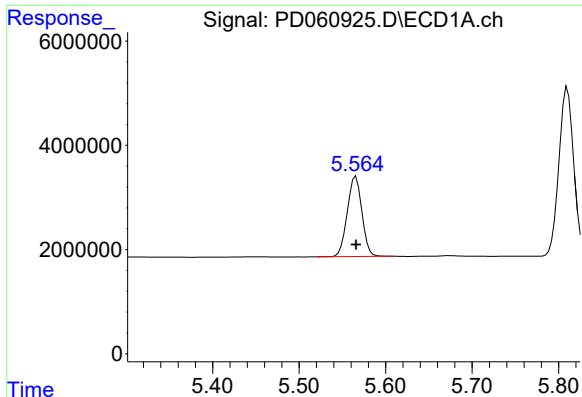

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 18005351
Conc: 10.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

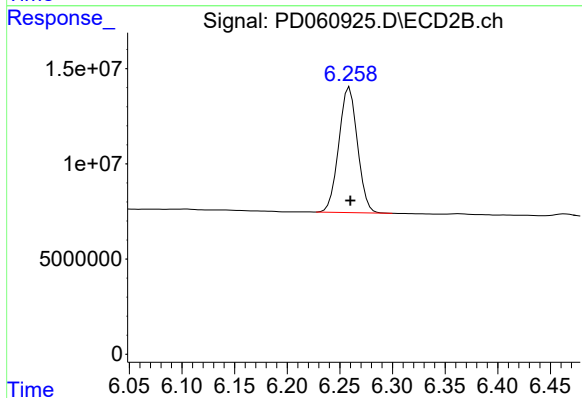


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 80974198
Conc: 10.20 ng/ml

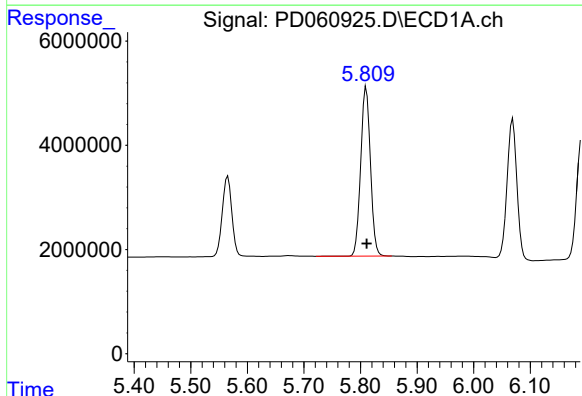


#13 Dieldrin

R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 38776292
Conc: 19.86 ng/ml

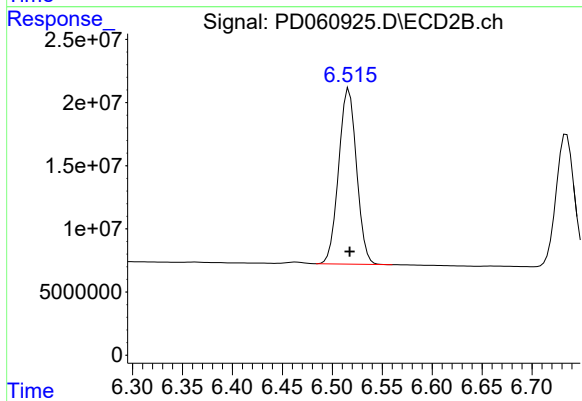

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 173341554
Conc: 20.22 ng/ml

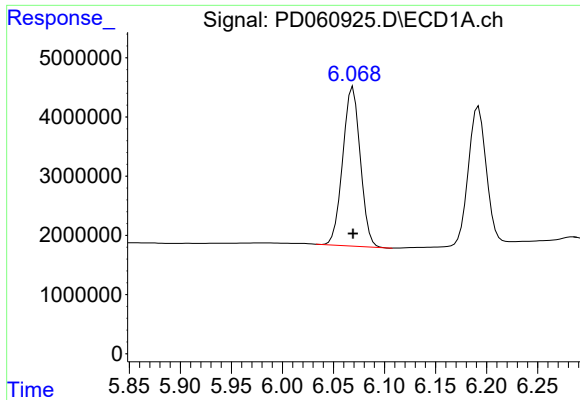

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 32221996
Conc: 20.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

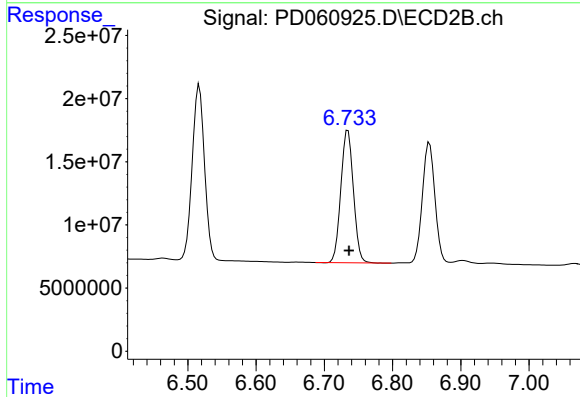


#14 Endrin

R.T.: 6.735 min
Delta R.T.: -0.002 min
Response: 134212430
Conc: 20.20 ng/ml

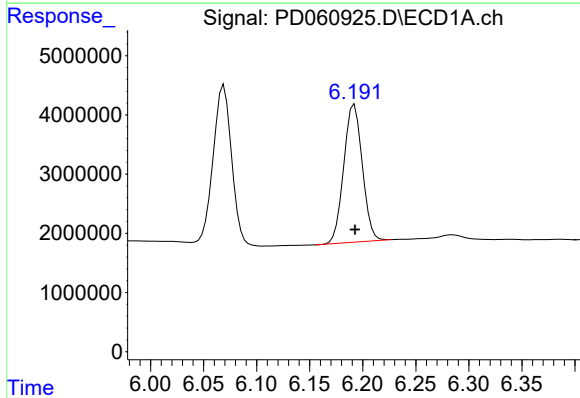


#16 4,4'-DDD

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 28237447
Conc: 20.02 ng/ml

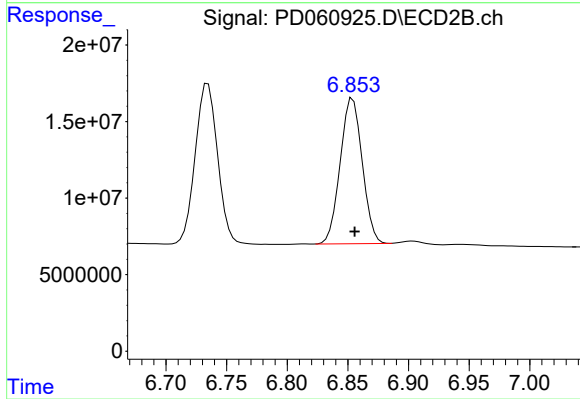

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: -0.002 min
Response: 120305792
Conc: 20.16 ng/ml

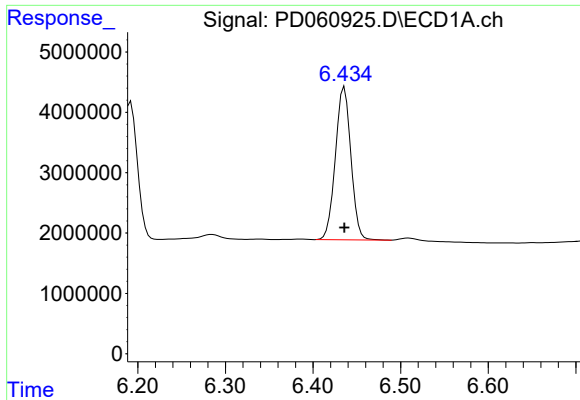

#17 4,4'-DDT


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 31202047
Conc: 19.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

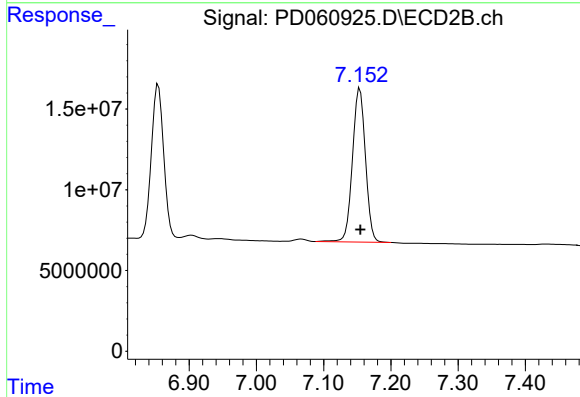


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 128122814
Conc: 20.58 ng/ml

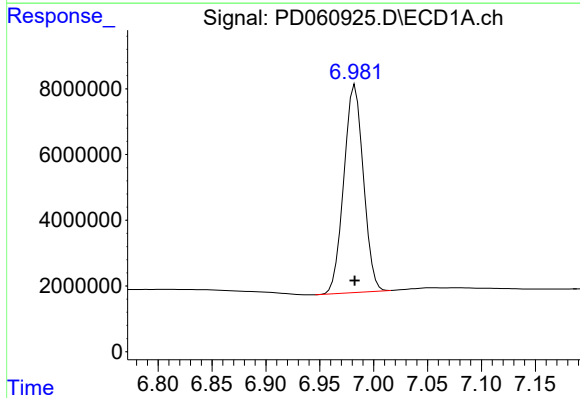


#20 Methoxychlor

R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 79764010
Conc: 102.87 ng/ml

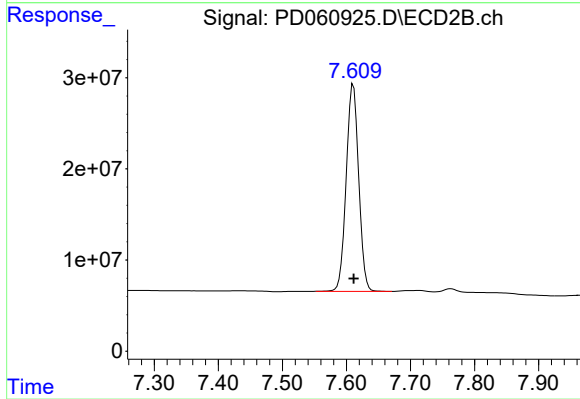

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 307472611
Conc: 105.10 ng/ml

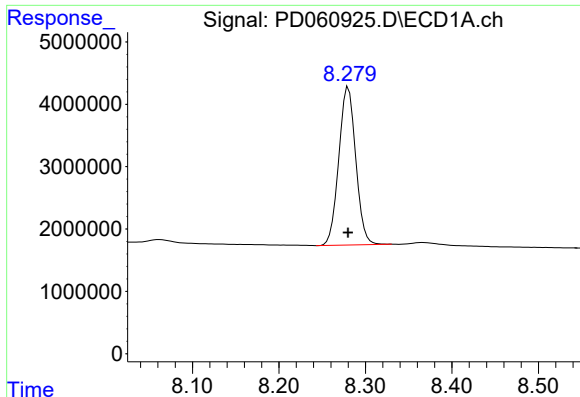

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 34352950
Conc: 21.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

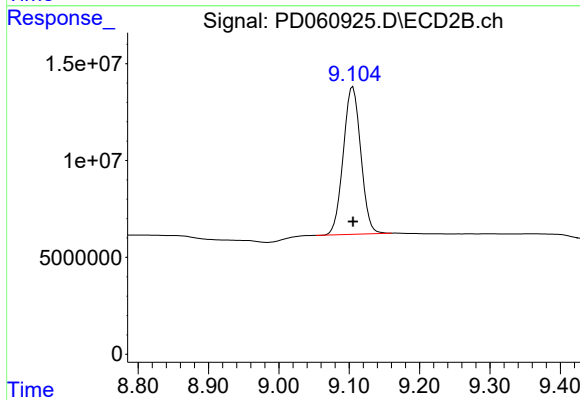

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 131720365
Conc: 21.11 ng/ml