

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 11:14
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 11:28:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 11:28:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	26289367	139.9E6	20.000	20.000
27)	SA Decachlor...	8.280	9.105	64652018	249.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.938	4.411	38727329	213.7E6	20.000	20.000
3)	MA gamma-BHC...	4.223	4.697	37130772	196.7E6	20.000	20.000
4)	MA Heptachlor	4.529	5.208	40458449	198.5E6	20.000	20.000
9)	A Endosulfan I	5.566	6.260	35225448	158.8E6	20.000	20.000
13)	MA Dieldrin	5.811	6.518	78117442	342.9E6	40.000	40.000
14)	MA Endrin	6.069	6.736	63923453	265.7E6	40.000	40.000
16)	A 4,4'-DDD	6.193	6.856	56417695	238.8E6	40.000	40.000
17)	MA 4,4'-DDT	6.436	7.155	62989828	249.0E6	40.000	40.000
20)	A Methoxychlor	6.983	7.612	155.1E6	585.1E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 11:14
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 11:28:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 11:28:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

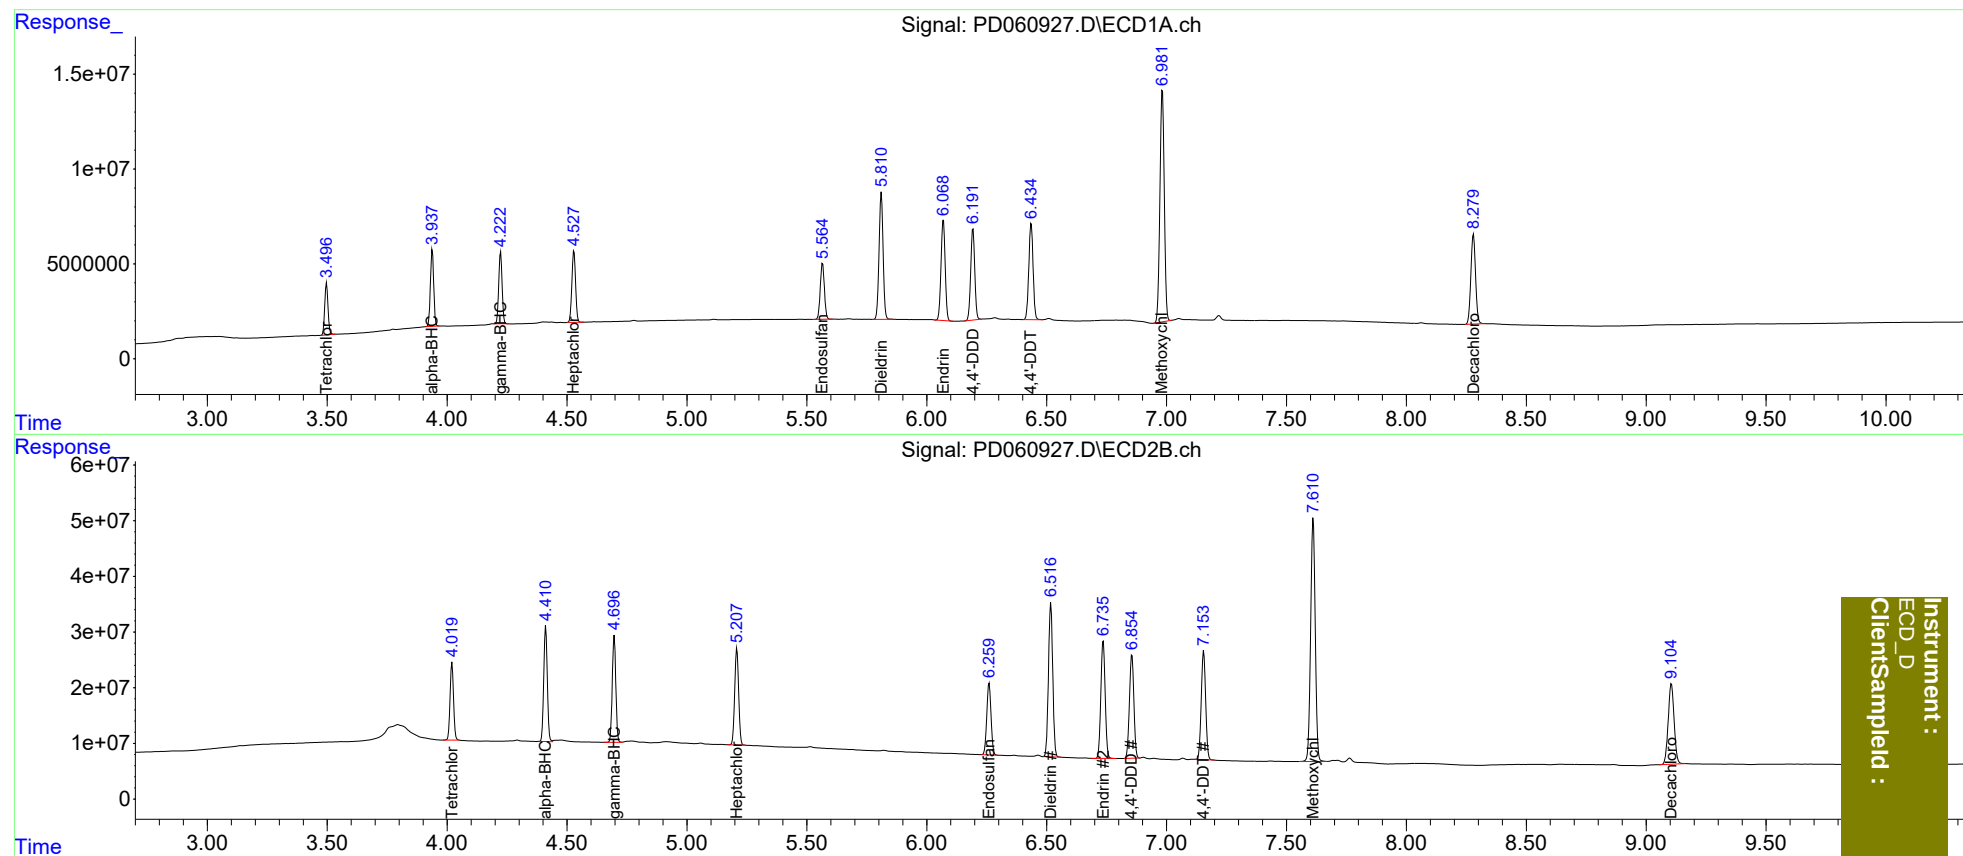


Instrument :
ECD_D
ClientSampled :

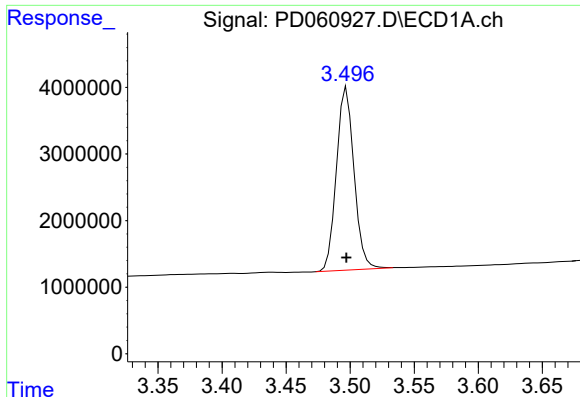

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 26289367
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

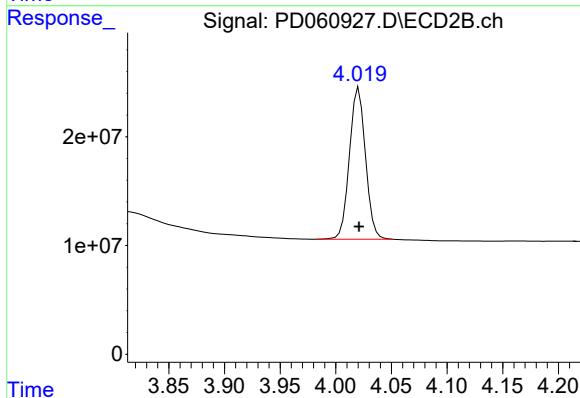


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 139852756
Conc: 20.00 ng/ml

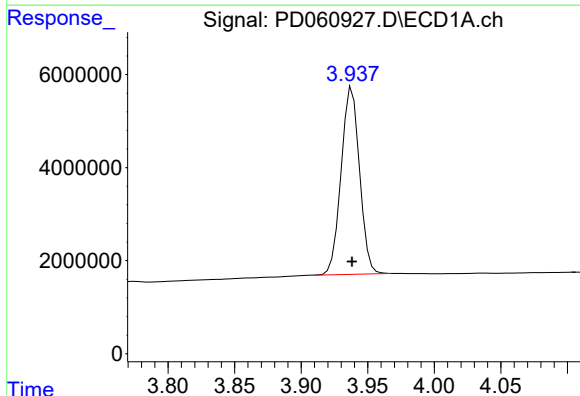


#2 alpha-BHC

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 38727329
Conc: 20.00 ng/ml

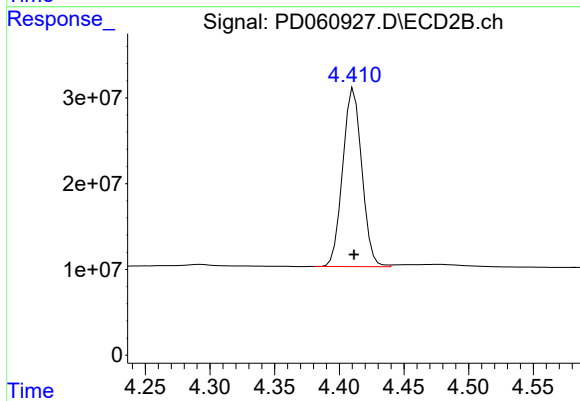

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 213674104
Conc: 20.00 ng/ml

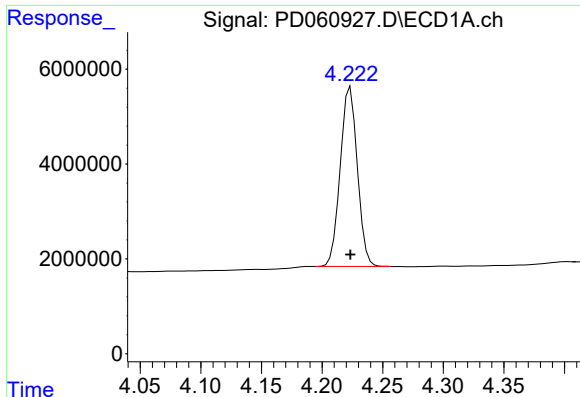

#3 gamma-BHC (Lindane)


R.T.: 4.223 min
Delta R.T.: 0.000 min
Response: 37130772
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

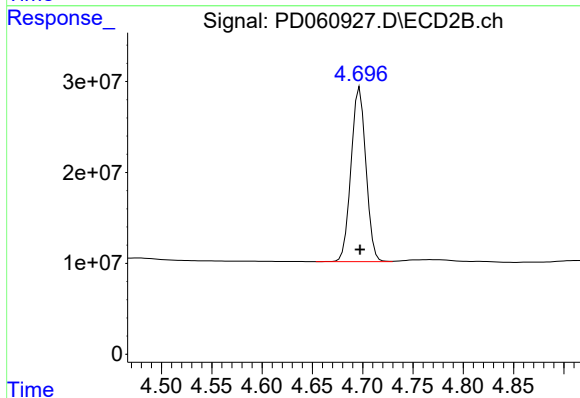


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 196717926
Conc: 20.00 ng/ml

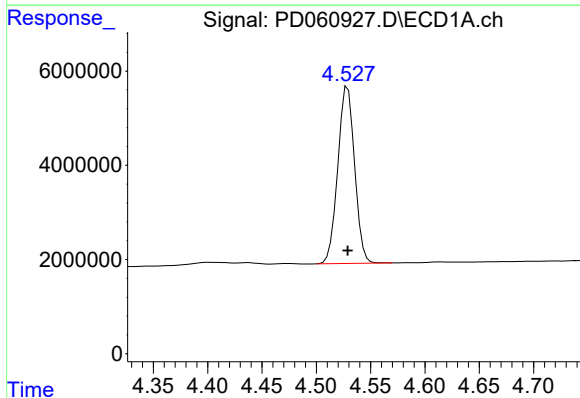


#4 Heptachlor

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 40458449
Conc: 20.00 ng/ml

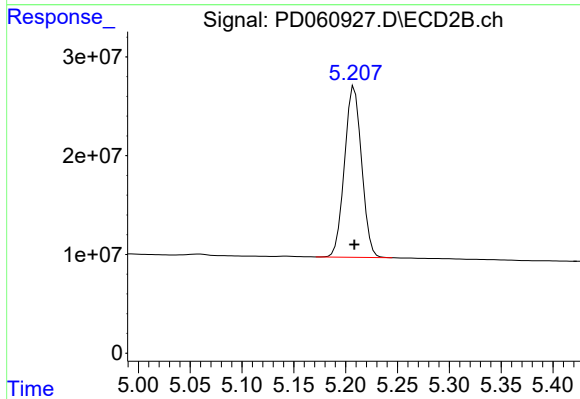

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 198492486
Conc: 20.00 ng/ml

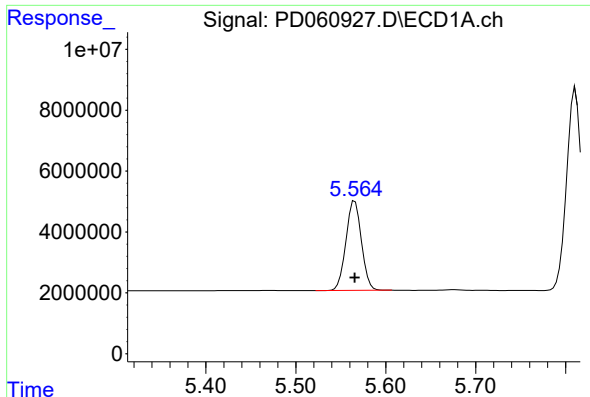

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 35225448
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

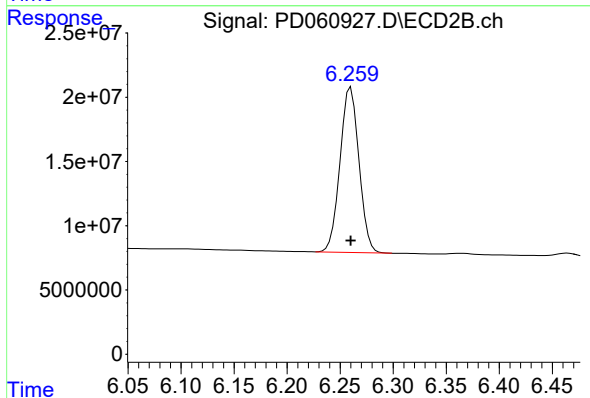


#9 Endosulfan I

R.T.: 6.260 min
Delta R.T.: 0.000 min
Response: 158830951
Conc: 20.00 ng/ml

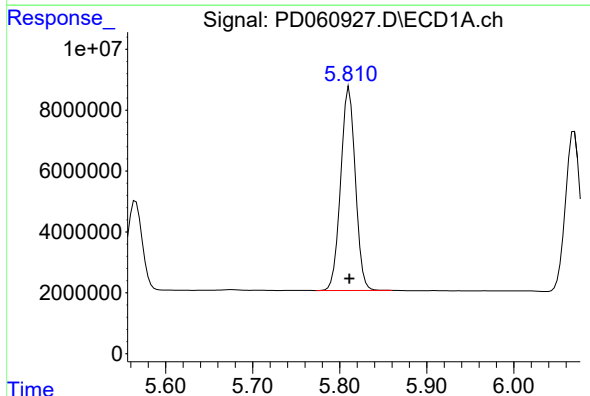


#13 Dieldrin

R.T.: 5.811 min
Delta R.T.: 0.000 min
Response: 78117442
Conc: 40.00 ng/ml

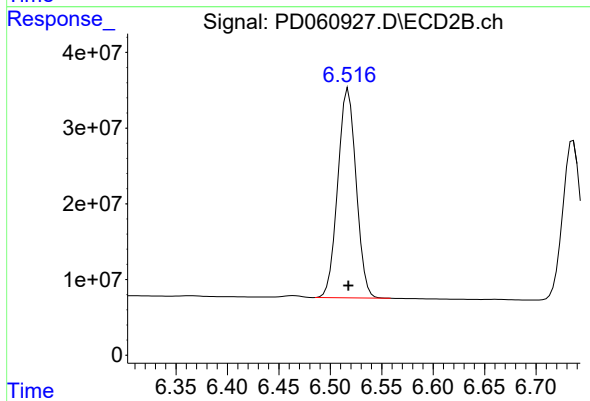

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 342871118
Conc: 40.00 ng/ml

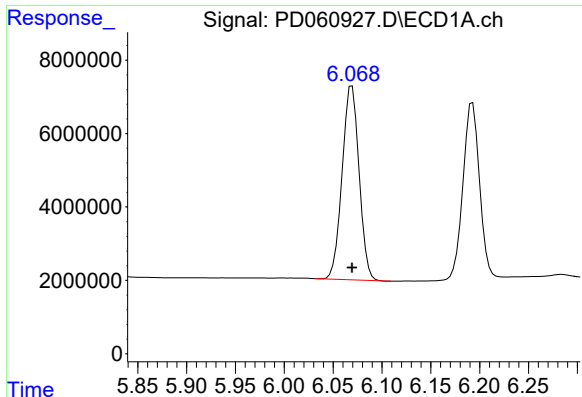

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 63923453
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

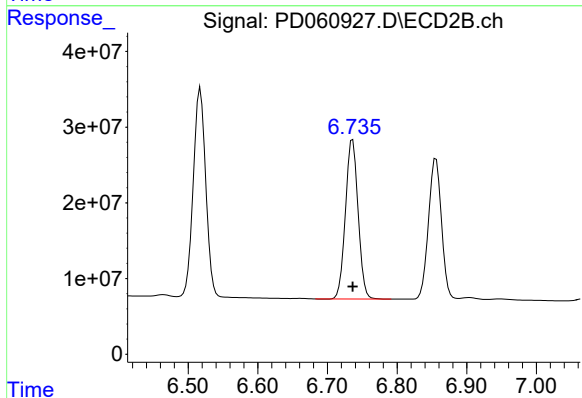


#14 Endrin

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 265723683
Conc: 40.00 ng/ml

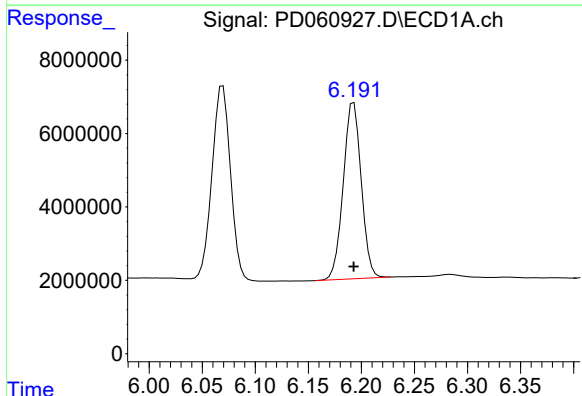


#16 4,4'-DDD

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 56417695
Conc: 40.00 ng/ml

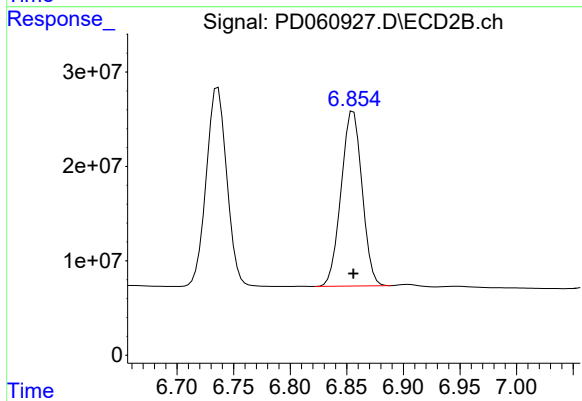

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 238759400
Conc: 40.00 ng/ml

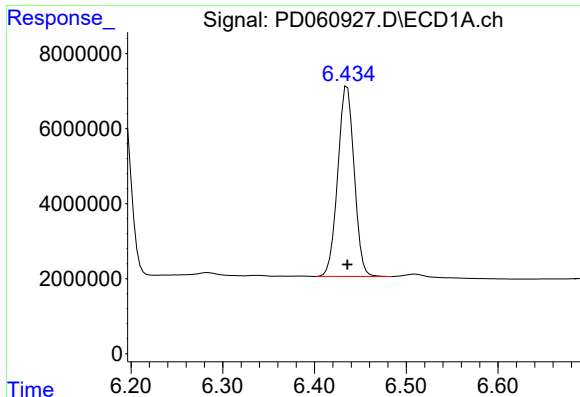

#17 4,4'-DDT


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 62989828
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

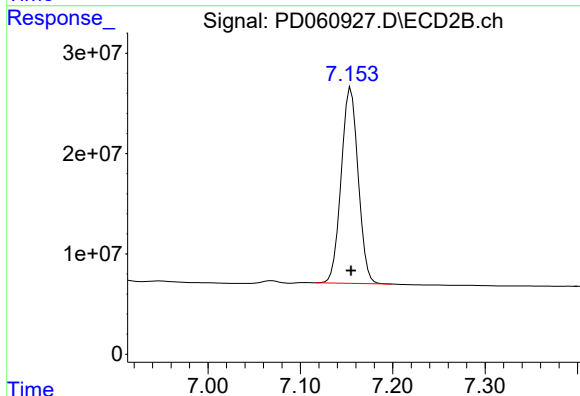


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 248986641
Conc: 40.00 ng/ml

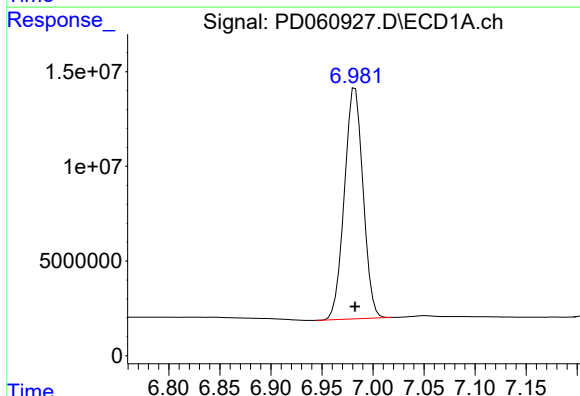


#20 Methoxychlor

R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 155076508
Conc: 200.00 ng/ml

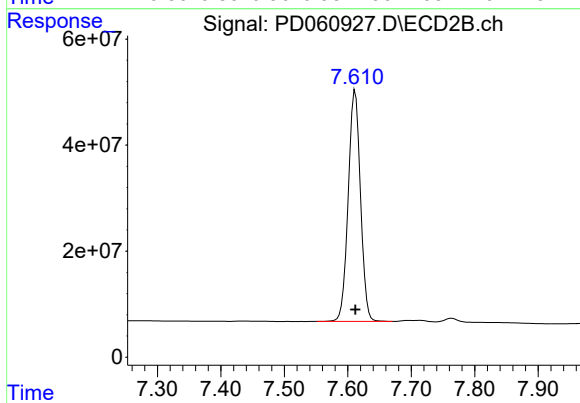

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 585120588
Conc: 200.00 ng/ml

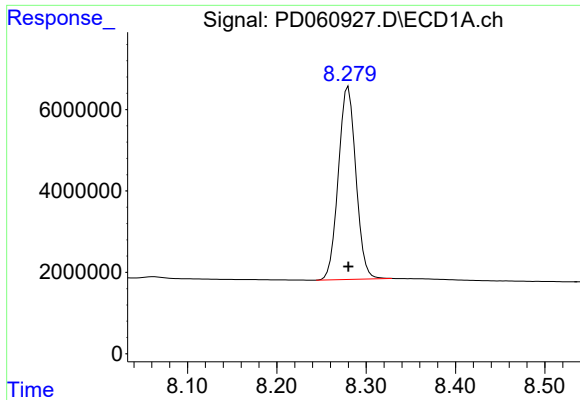

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 64652018
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

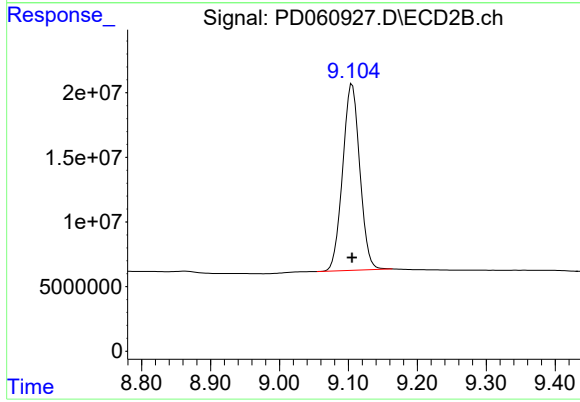

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 249616784
Conc: 40.00 ng/ml