

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 11:42
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 11:52:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 11:31:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	50079979	269.3E6	35.845	37.495
27)	SA Decachlor...	8.280	9.105	120.9E6	459.0E6	70.950	69.953
Target Compounds							
2)	A alpha-BHC	3.938	4.411	77003390	421.8E6	39.101	38.955
3)	MA gamma-BHC...	4.224	4.697	72945368	385.9E6	38.196	38.548
4)	MA Heptachlor	4.529	5.209	79174672	385.5E6	38.250	38.151
9)	A Endosulfan I	5.566	6.259	67686808	297.0E6	37.457	36.696
13)	MA Dieldrin	5.811	6.517	152.9E6	650.0E6	78.519	75.165
14)	MA Endrin	6.069	6.735	123.8E6	501.4E6	76.559	74.806
16)	A 4,4'-DDD	6.193	6.855	110.6E6	449.9E6	78.163	75.103
17)	MA 4,4'-DDT	6.435	7.155	124.0E6	474.3E6	79.331	74.692
20)	A Methoxychlor	6.983	7.612	295.1E6	1057.9E6	370.359	348.082

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 11:42
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 11:52:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 11:31:42 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

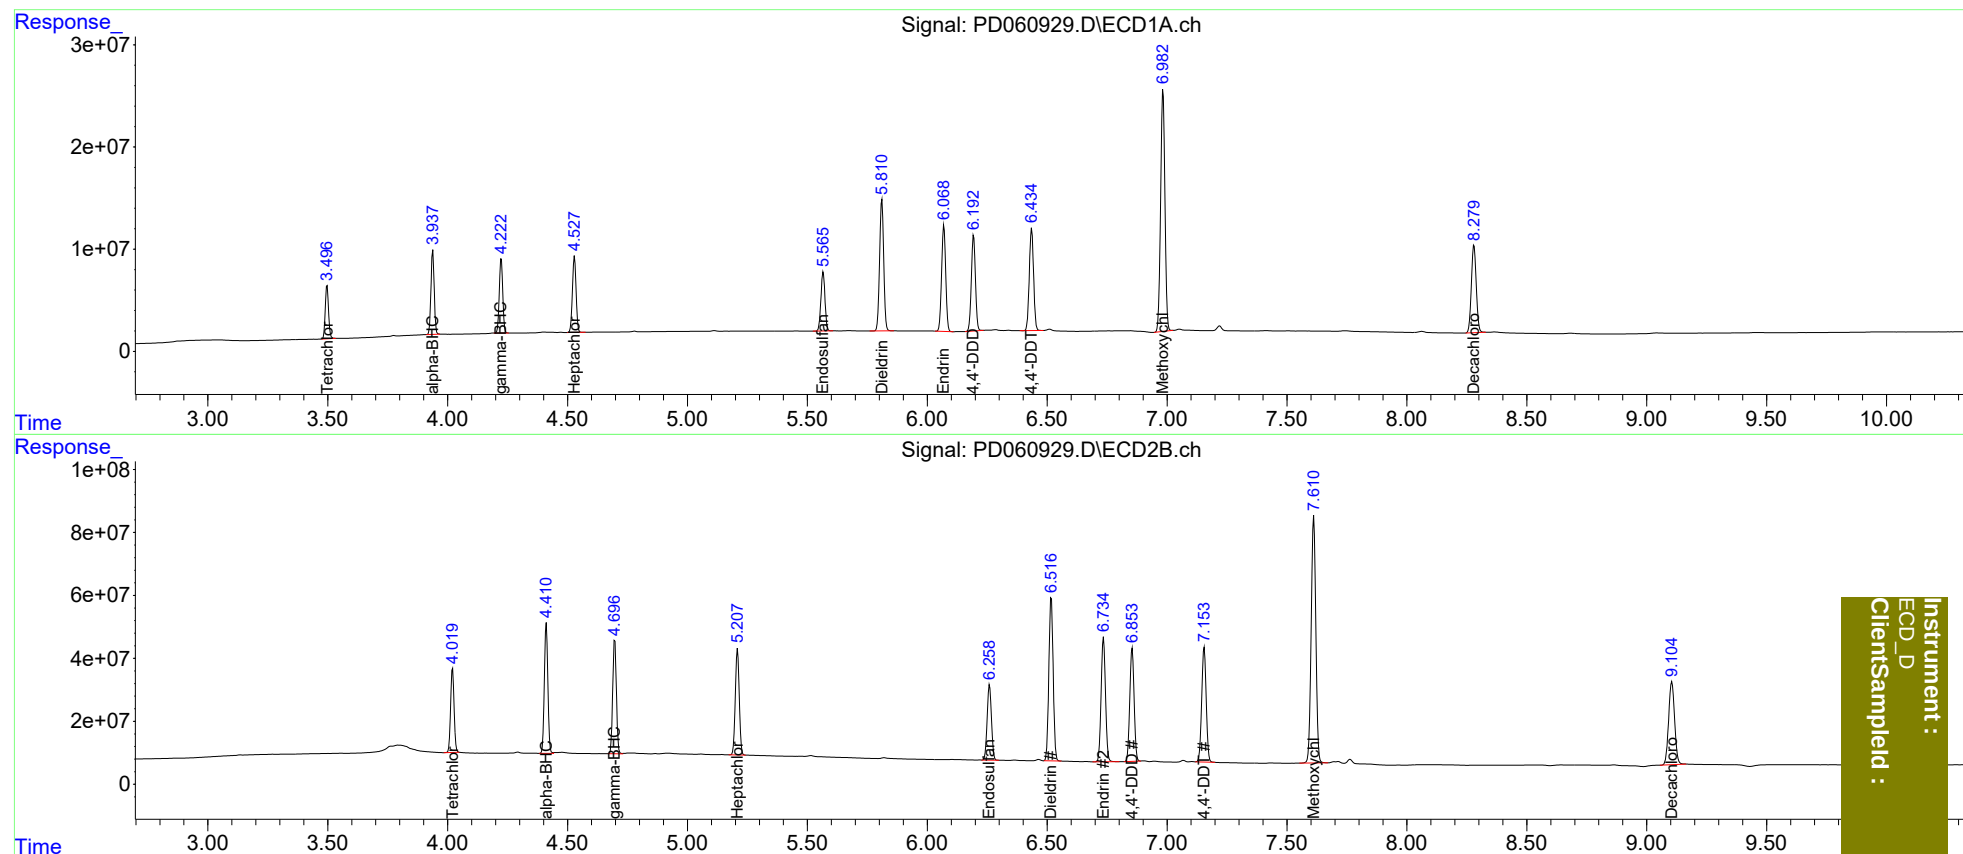


Instrument :
ECD_D
ClientSampled :

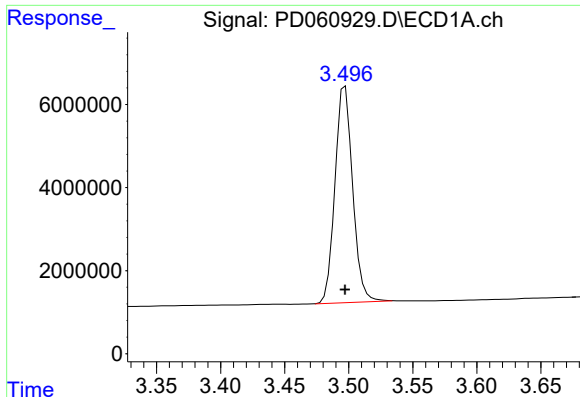

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 50079979
Conc: 35.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

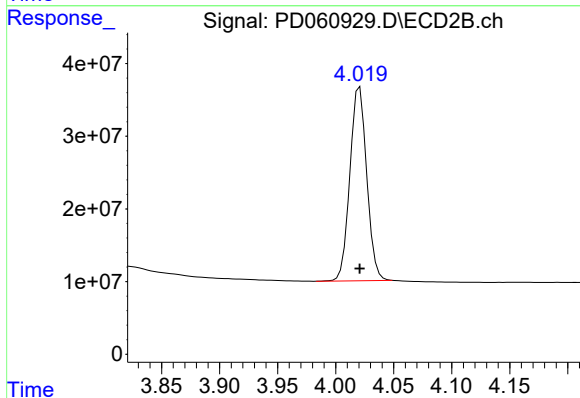


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 269258926
Conc: 37.49 ng/ml

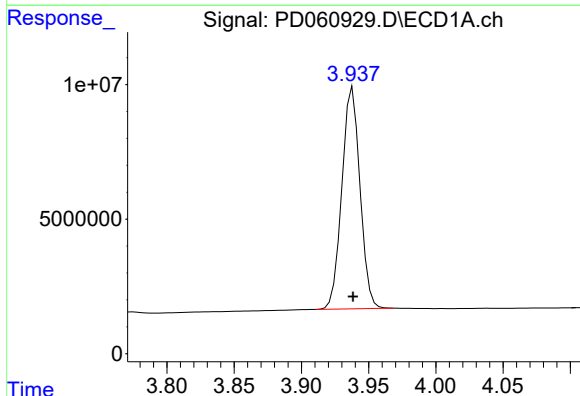


#2 alpha-BHC

R.T.: 3.938 min
Delta R.T.: 0.000 min
Response: 77003390
Conc: 39.10 ng/ml

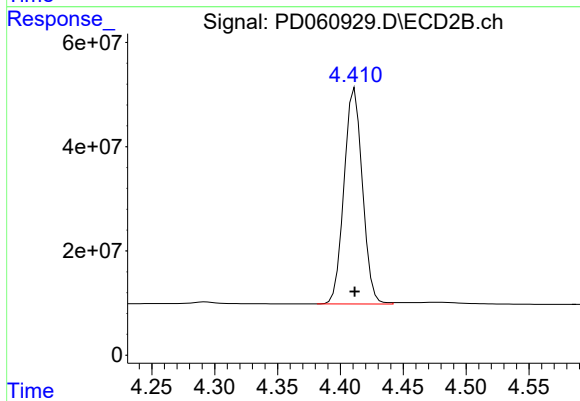

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 421752623
Conc: 38.96 ng/ml

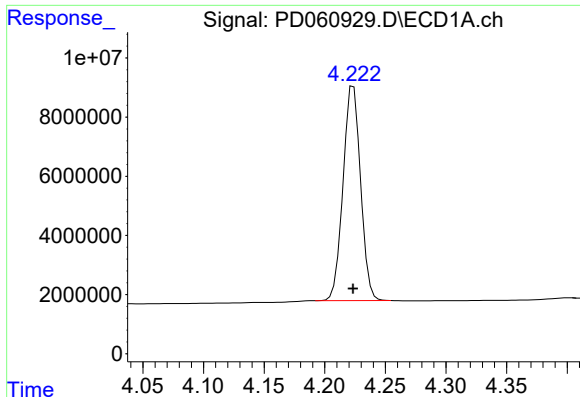

#3 gamma-BHC (Lindane)


R.T.: 4.224 min
Delta R.T.: 0.000 min
Response: 72945368
Conc: 38.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

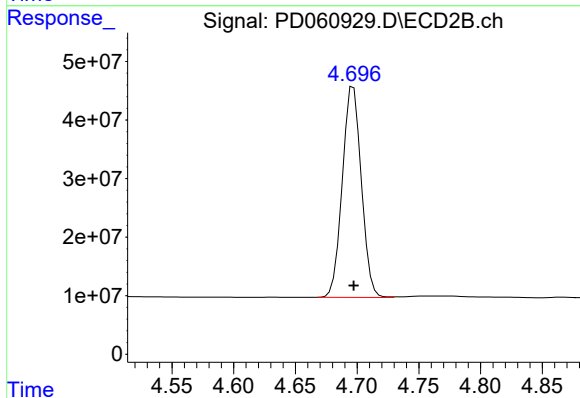


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 385866821
Conc: 38.55 ng/ml

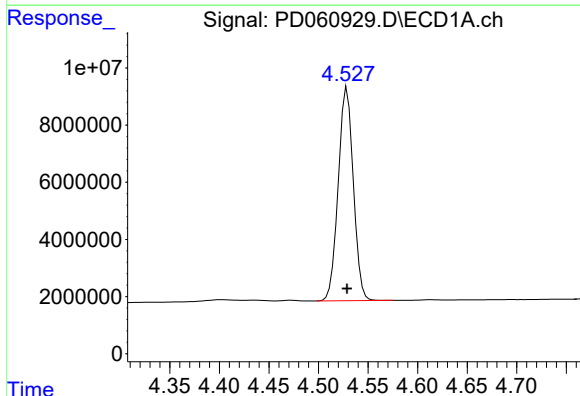


#4 Heptachlor

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 79174672
Conc: 38.25 ng/ml

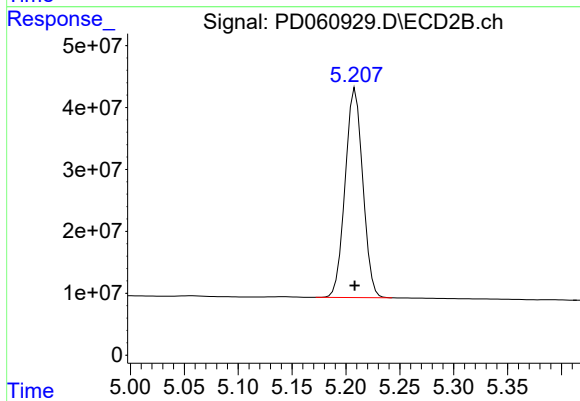

#4 Heptachlor


R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 385511003
Conc: 38.15 ng/ml

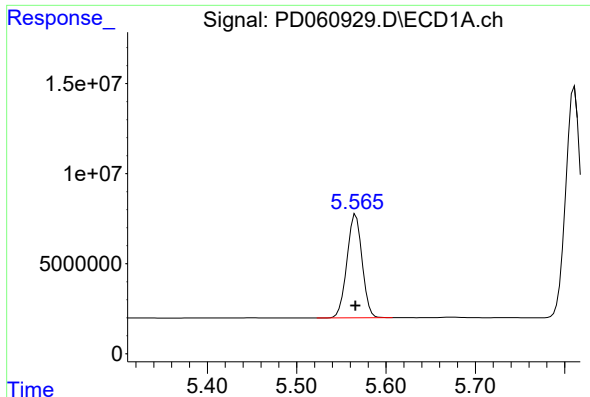

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 67686808
Conc: 37.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

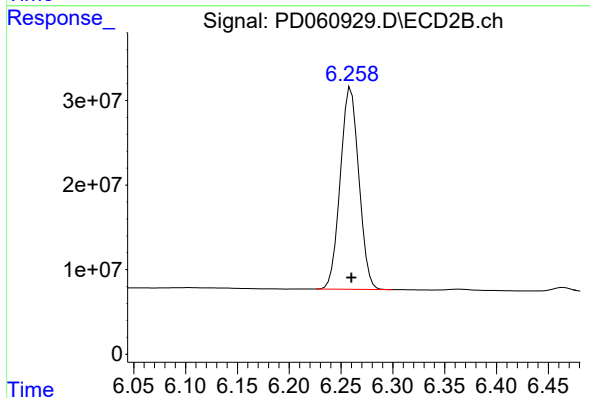


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 297033165
Conc: 36.70 ng/ml

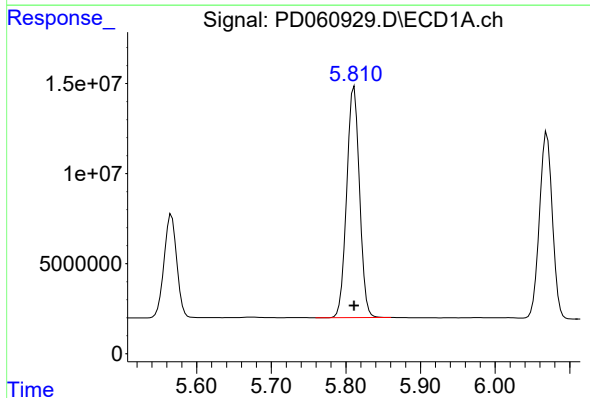


#13 Dieldrin

R.T.: 5.811 min
Delta R.T.: 0.000 min
Response: 152891593
Conc: 78.52 ng/ml

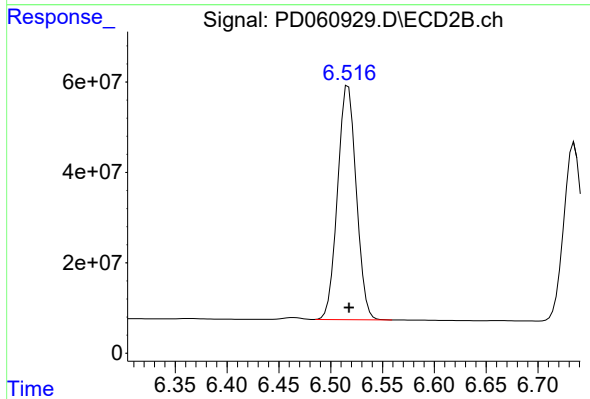

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 649995658
Conc: 75.17 ng/ml

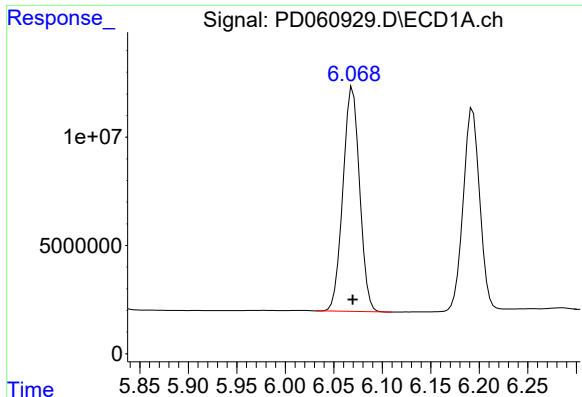

#14 Endrin


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 123771009
Conc: 76.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

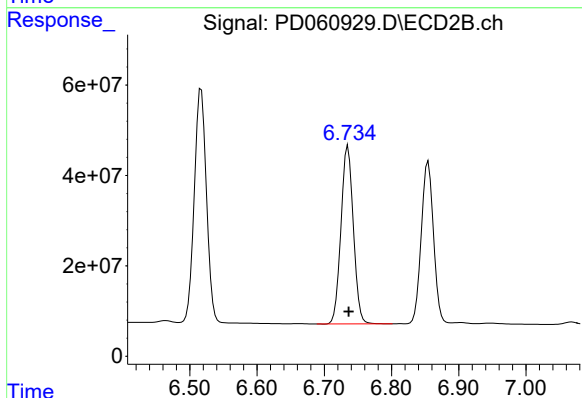


#14 Endrin

R.T.: 6.735 min
Delta R.T.: -0.001 min
Response: 501387910
Conc: 74.81 ng/ml

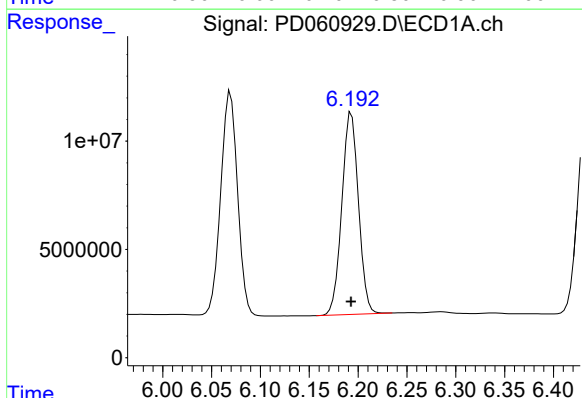


#16 4,4'-DDD

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 110554386
Conc: 78.16 ng/ml

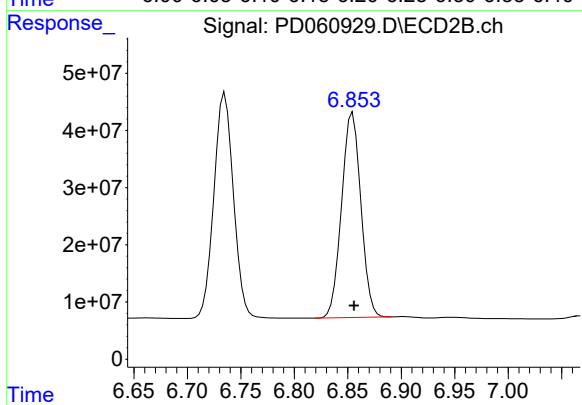

#16 4,4'-DDD


R.T.: 6.855 min
Delta R.T.: -0.001 min
Response: 449933511
Conc: 75.10 ng/ml

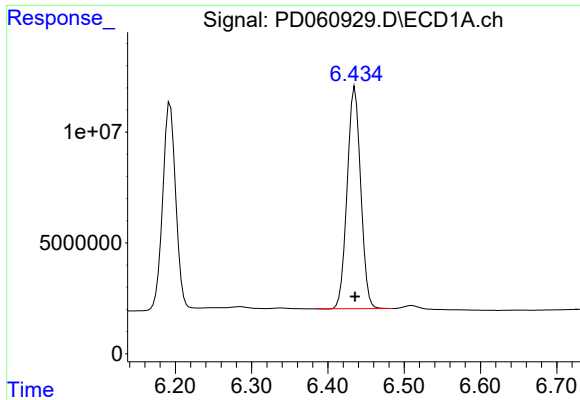

#17 4,4'-DDT


R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 124009667
Conc: 79.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

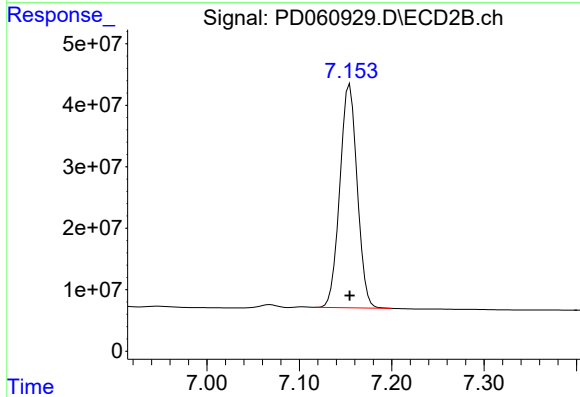


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 474279419
Conc: 74.69 ng/ml

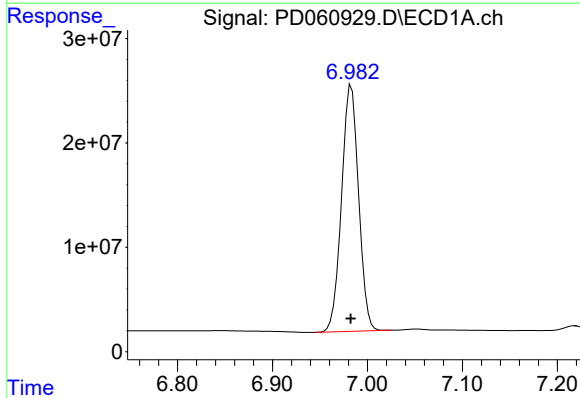


#20 Methoxychlor

R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 295053066
Conc: 370.36 ng/ml

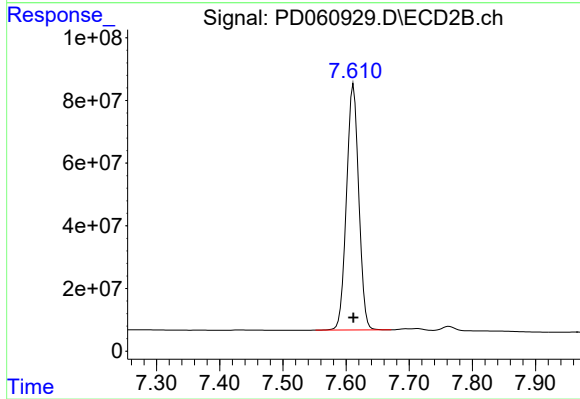

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: 0.000 min
Response: 1057923545
Conc: 348.08 ng/ml

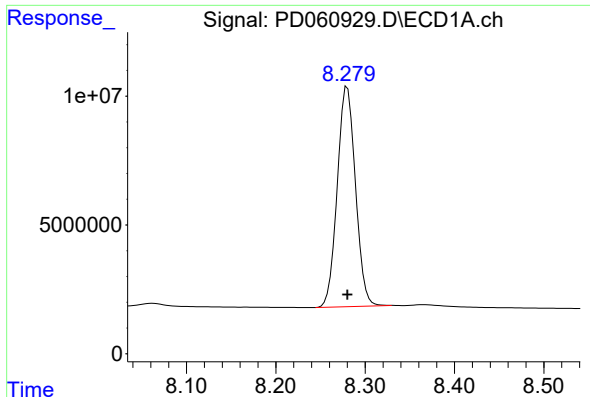

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 120918592
Conc: 70.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

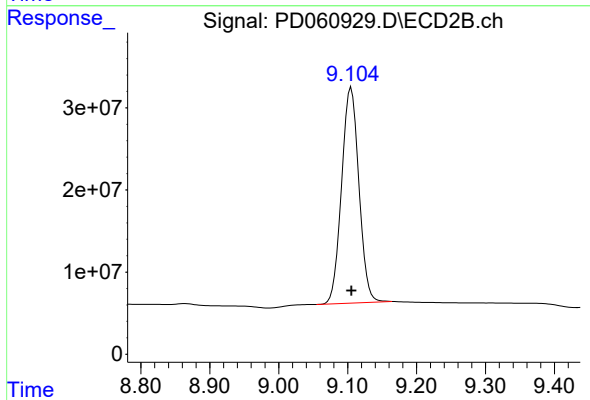

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 458996567
Conc: 69.95 ng/ml