

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 12:10
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 12:27:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 11:54:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.021	95475689	515.7E6	70.160	72.957
27)	SA Decachlor...	8.280	9.104	227.4E6	866.4E6	137.310	136.318
Target Compounds							
2)	A alpha-BHC	3.939	4.411	153.1E6	820.5E6	78.204	76.285
3)	MA gamma-BHC...	4.224	4.697	143.8E6	745.4E6	76.138	75.149
4)	MA Heptachlor	4.530	5.208	154.8E6	737.7E6	75.637	73.856
9)	A Endosulfan I	5.566	6.259	131.6E6	579.5E6	73.988	73.105
13)	MA Dieldrin	5.812	6.517	302.8E6	1261.5E6	156.249	148.112
14)	MA Endrin	6.070	6.735	241.3E6	975.3E6	150.877	147.907
16)	A 4,4'-DDD	6.194	6.854	218.9E6	890.5E6	155.681	150.957
17)	MA 4,4'-DDT	6.436	7.154	247.7E6	943.3E6	158.816	151.067
20)	A Methoxychlor	6.983	7.611	555.2E6	1981.0E6	709.996	673.663


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 12:10
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 12:27:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 11:54:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

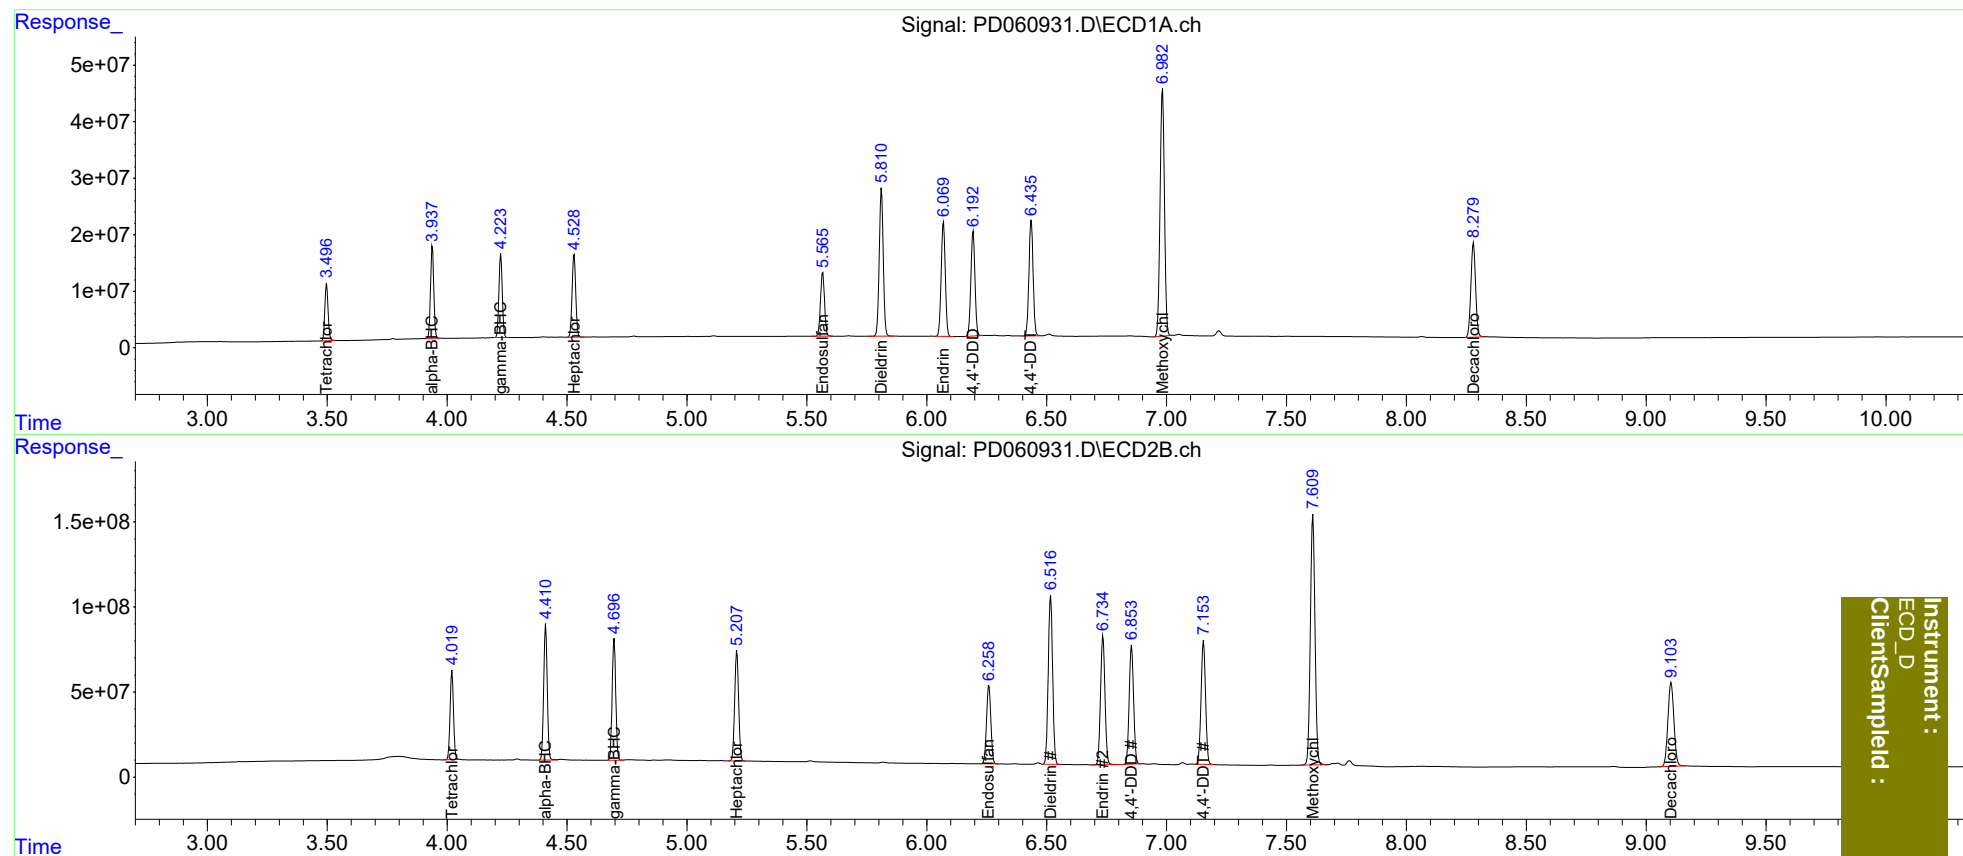


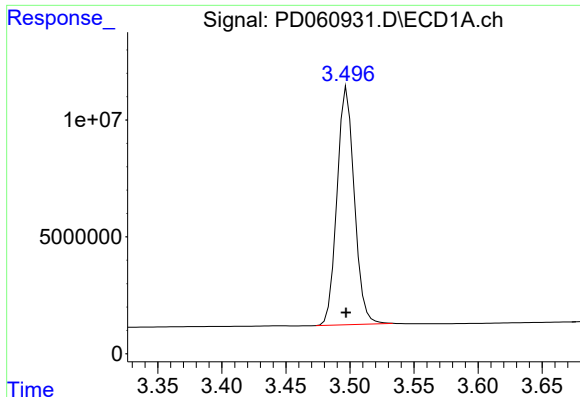

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 95475689
Conc: 70.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

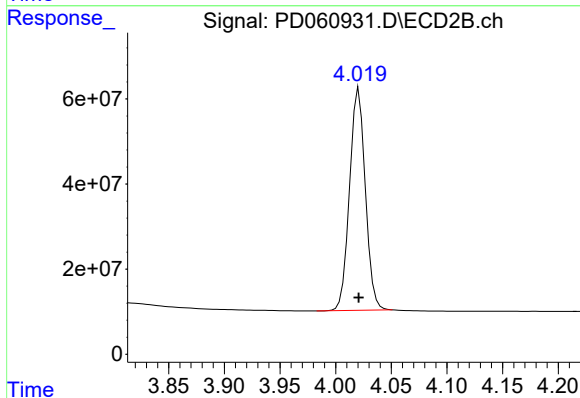


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 515719456
Conc: 72.96 ng/ml

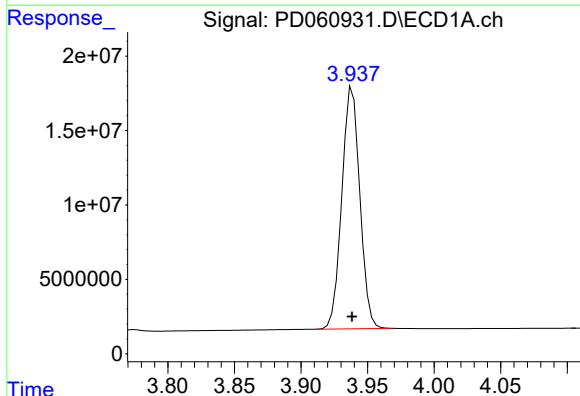


#2 alpha-BHC

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 153144812
Conc: 78.20 ng/ml

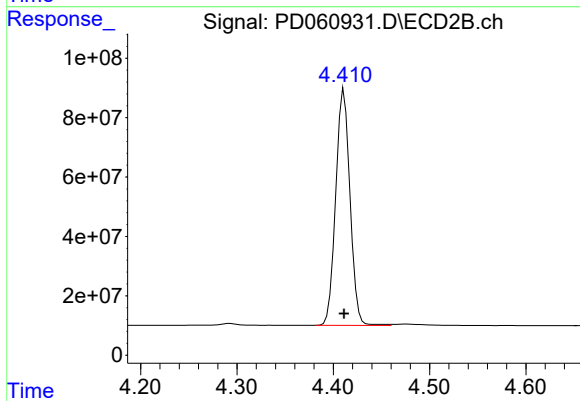

#2 alpha-BHC


R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 820519519
Conc: 76.29 ng/ml

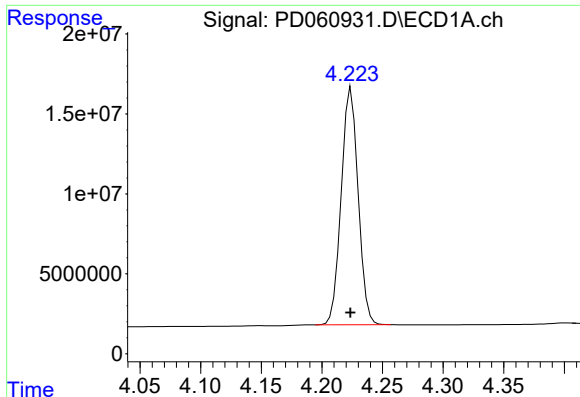

#3 gamma-BHC (Lindane)


R.T.: 4.224 min
Delta R.T.: 0.000 min
Response: 143766029
Conc: 76.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

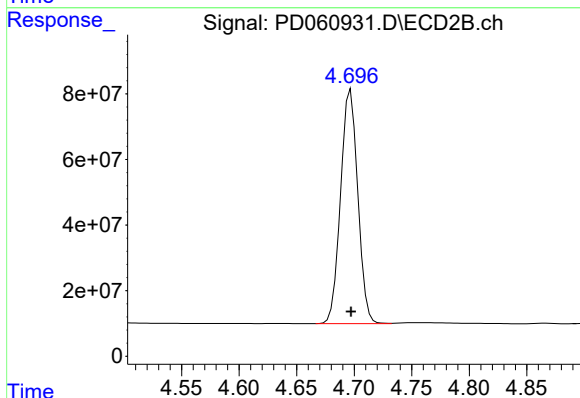


#3 gamma-BHC (Lindane)

R.T.: 4.697 min
Delta R.T.: 0.000 min
Response: 745420757
Conc: 75.15 ng/ml

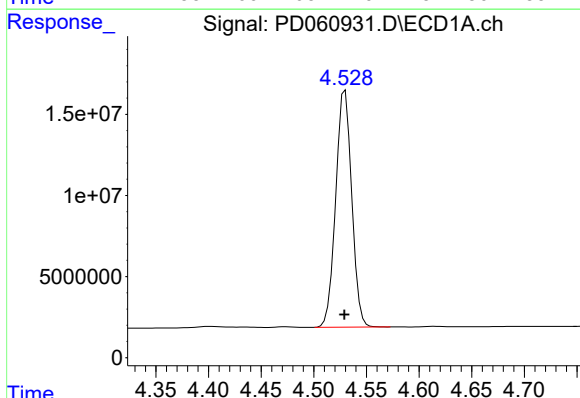


#4 Heptachlor

R.T.: 4.530 min
Delta R.T.: 0.000 min
Response: 154849888
Conc: 75.64 ng/ml

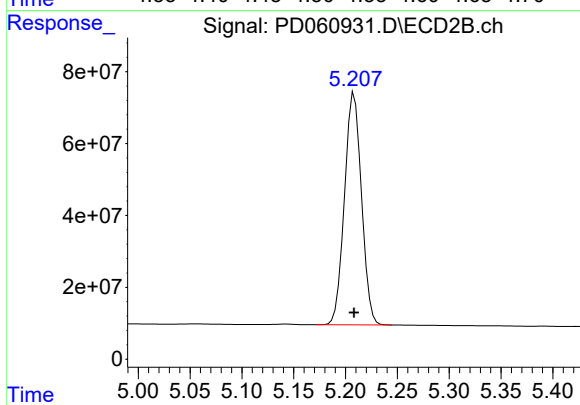

#4 Heptachlor


R.T.: 5.208 min
Delta R.T.: 0.000 min
Response: 737679189
Conc: 73.86 ng/ml

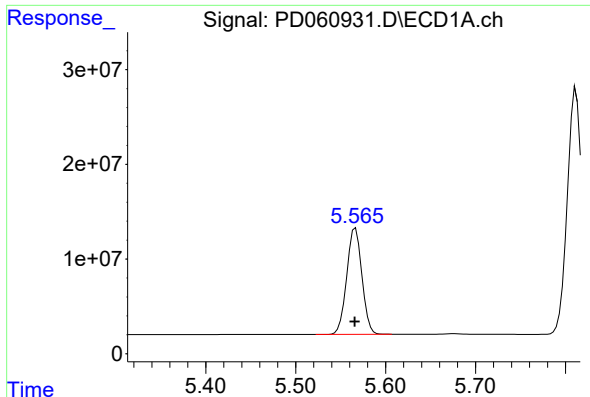

#9 Endosulfan I


R.T.: 5.566 min
Delta R.T.: 0.000 min
Response: 131575237
Conc: 73.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

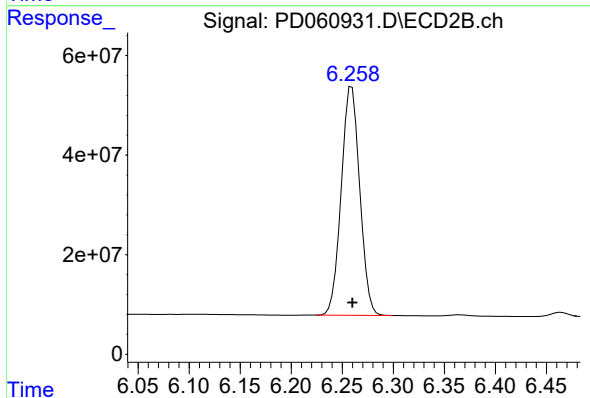


#9 Endosulfan I

R.T.: 6.259 min
Delta R.T.: 0.000 min
Response: 579515455
Conc: 73.10 ng/ml

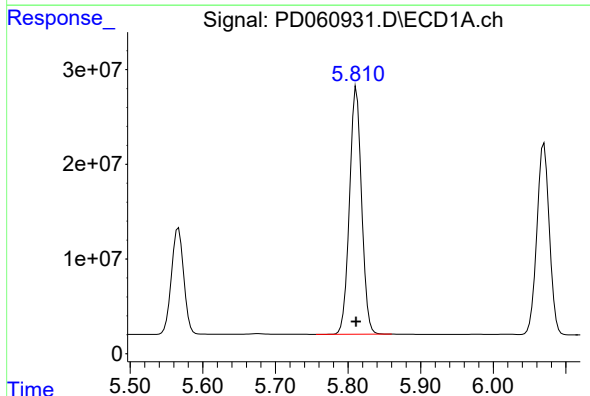


#13 Dieldrin

R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 302840207
Conc: 156.25 ng/ml

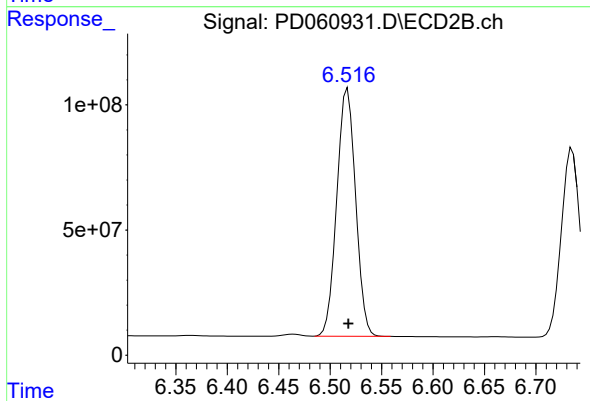

#13 Dieldrin


R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 1261453524
Conc: 148.11 ng/ml

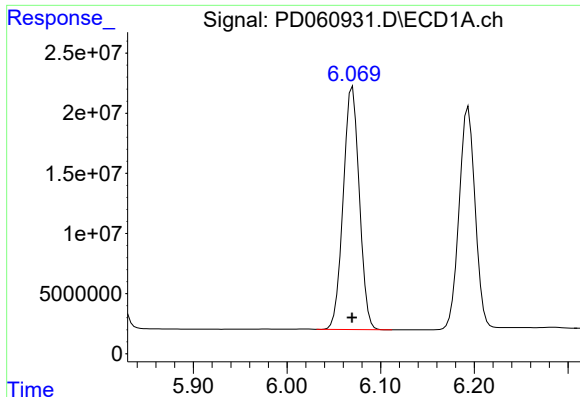

#14 Endrin


R.T.: 6.070 min
Delta R.T.: 0.000 min
Response: 241295792
Conc: 150.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

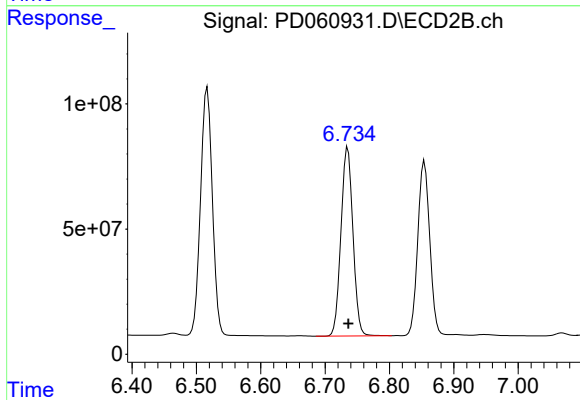


#14 Endrin

R.T.: 6.735 min
Delta R.T.: 0.000 min
Response: 975263314
Conc: 147.91 ng/ml

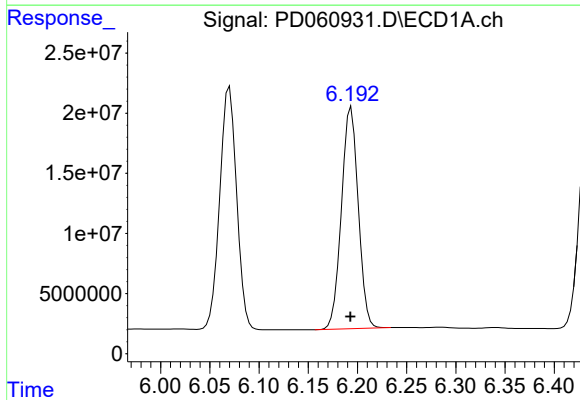


#16 4,4'-DDD

R.T.: 6.194 min
Delta R.T.: 0.000 min
Response: 218932549
Conc: 155.68 ng/ml

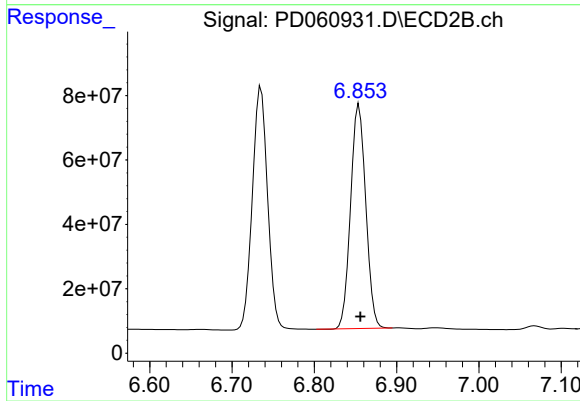

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: -0.001 min
Response: 890528105
Conc: 150.96 ng/ml

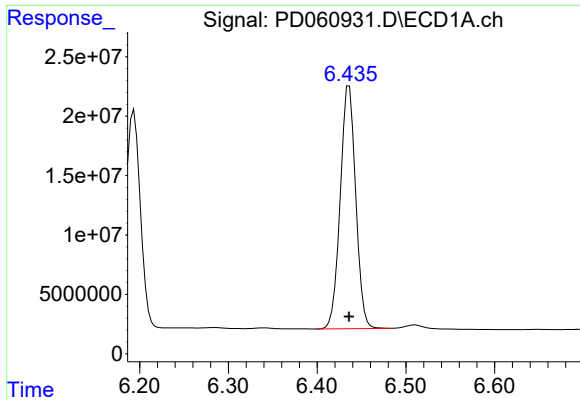

#17 4,4'-DDT


R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 247740979
Conc: 158.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

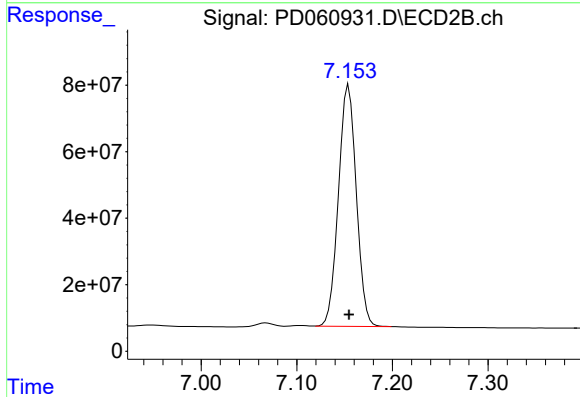


#17 4,4'-DDT

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 943333267
Conc: 151.07 ng/ml

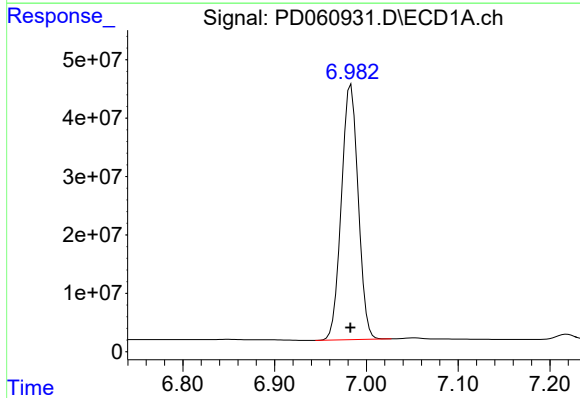


#20 Methoxychlor

R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 555152323
Conc: 710.00 ng/ml

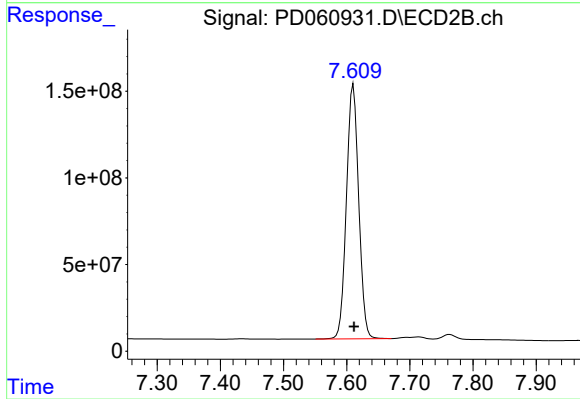

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: -0.001 min
Response: 1981020863
Conc: 673.66 ng/ml

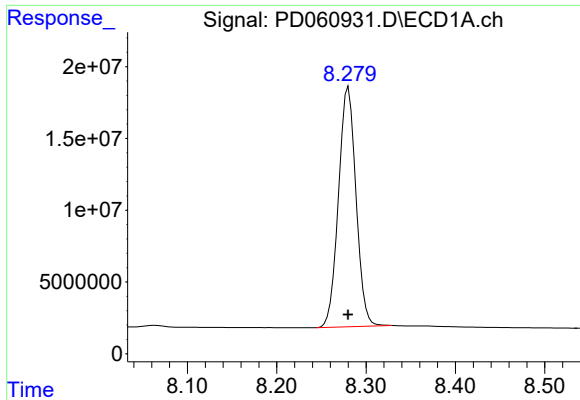

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 227394508
Conc: 137.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

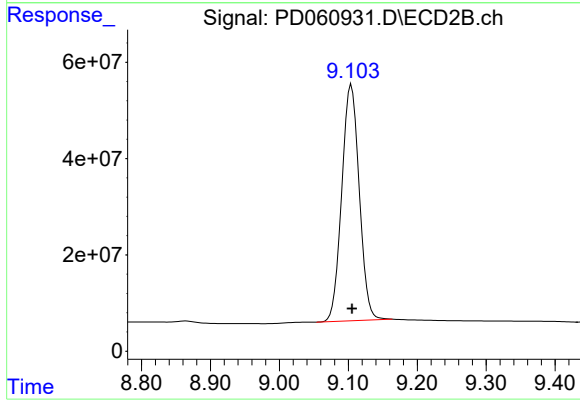

#27 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: -0.001 min
Response: 866368124
Conc: 136.32 ng/ml