

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 12:23
 Operator : DD\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 12:55:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 07 12:53:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.020	91559145	493.0E6	72.970	74.012
27)	SA Decachlor...	8.280	9.105	222.8E6	820.1E6	144.139	136.199
Target Compounds							
5)	MB Aldrin	4.780	5.515	148.3E6	694.6E6	77.897	75.524
6)	B beta-BHC	4.473	4.865	58228989	295.0E6	71.923	74.357
7)	B delta-BHC	4.680	5.083	139.1E6	706.8E6	78.041	75.035
8)	B Heptachlo...	5.224	5.902	135.7E6	608.4E6	76.373	72.624
10)	B trans-Chl...	5.452	6.135	142.6E6	643.4E6	76.281	74.089
11)	B cis-Chlor...	5.512	6.209	138.9E6	611.6E6	75.842	74.502
12)	B 4,4'-DDE	5.675	6.364	270.7E6	1126.4E6	154.846	149.765
15)	B Endosulfa...	6.342	6.943	219.8E6	932.4E6	163.135	147.711
18)	B Endrin al...	6.511	7.067	184.3E6	773.0E6	150.097	148.589
19)	B Endosulfa...	6.726	7.291	193.9E6	902.3E6	160.276	144.086
21)	B Endrin ke...	7.220	7.763	254.7E6	953.2E6	156.630	143.429

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 12:23
Operator : DD\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 12:55:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 07 12:53:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

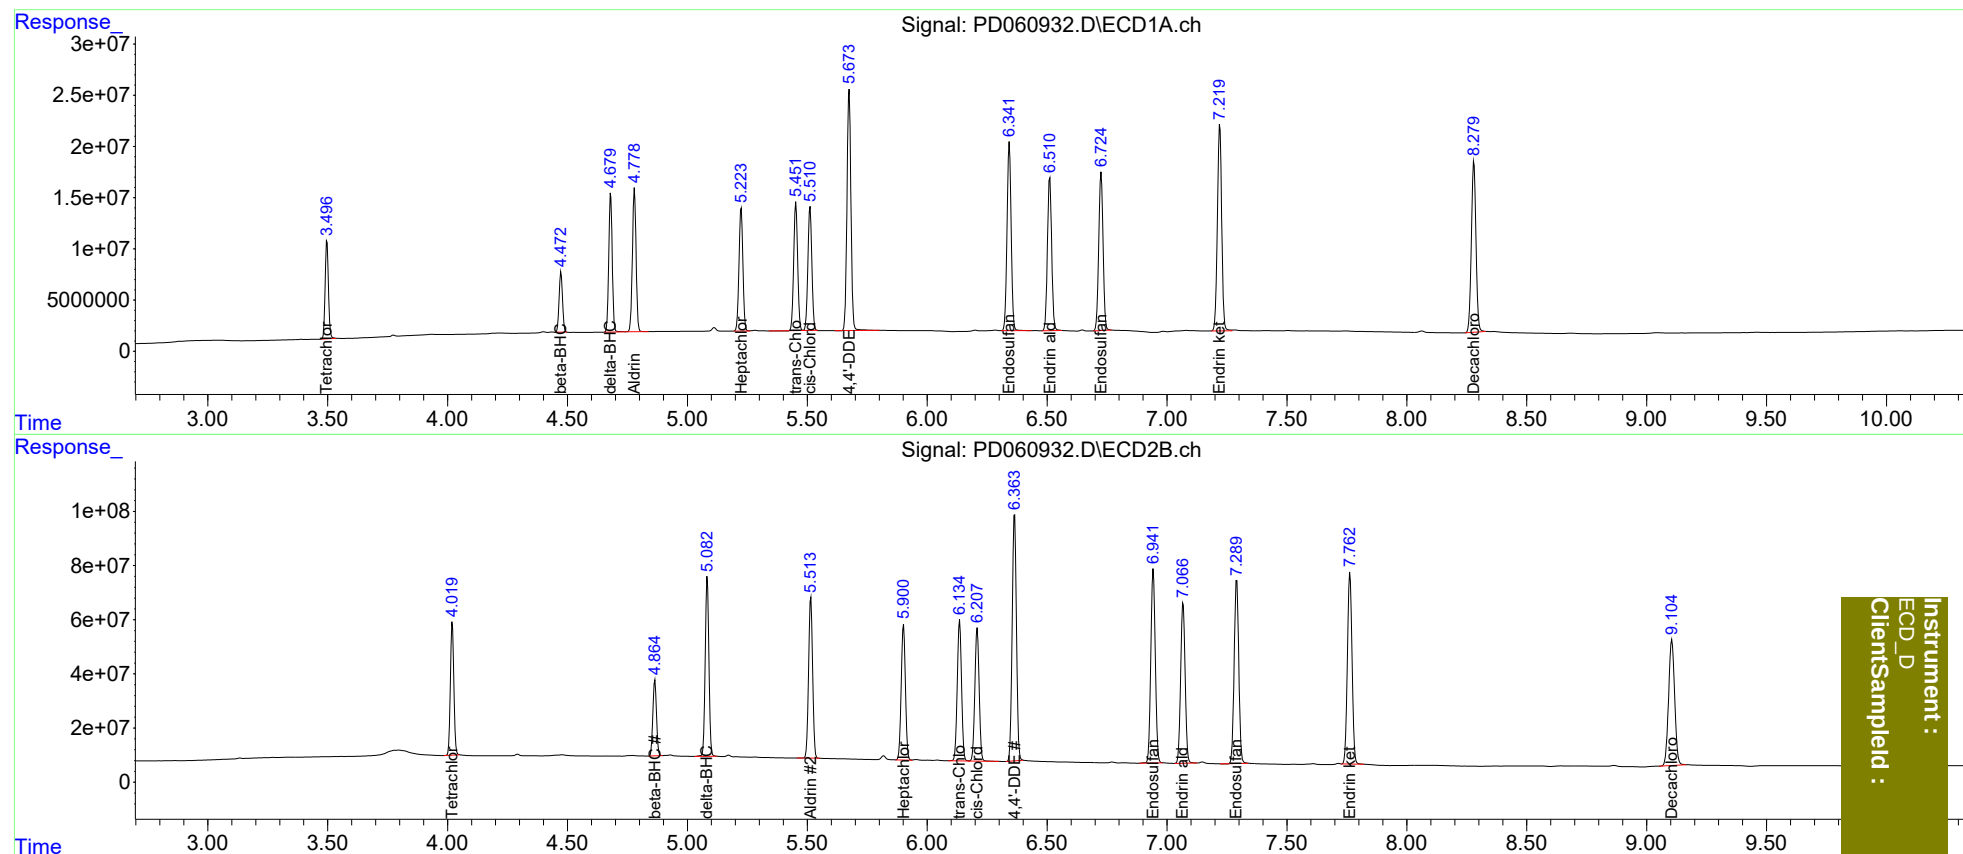


Instrument :
ECD_D
ClientSampled :

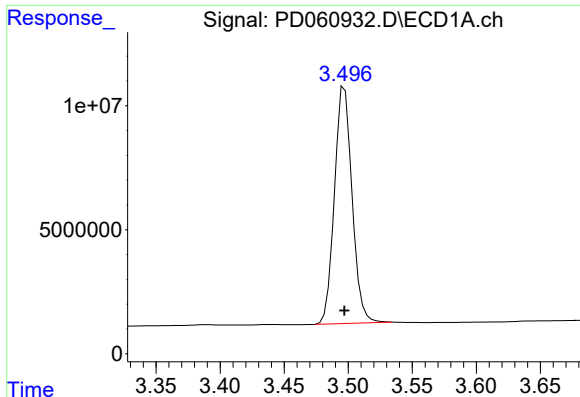

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 91559145
Conc: 72.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

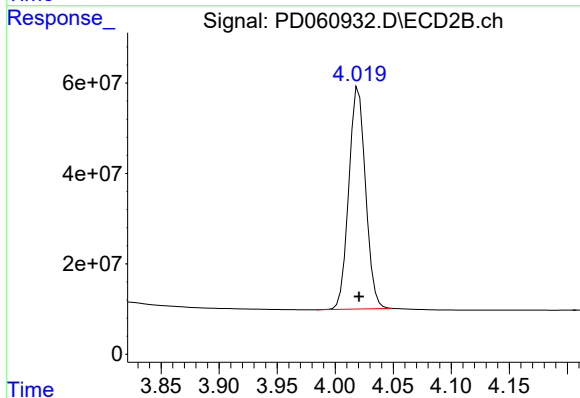


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.000 min
Response: 493002144
Conc: 74.01 ng/ml

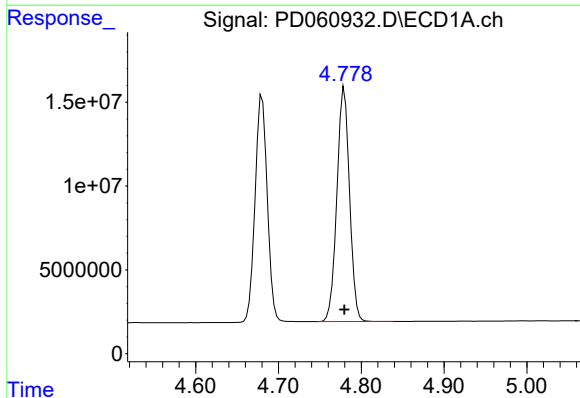


#5 Aldrin

R.T.: 4.780 min
Delta R.T.: 0.000 min
Response: 148314079
Conc: 77.90 ng/ml

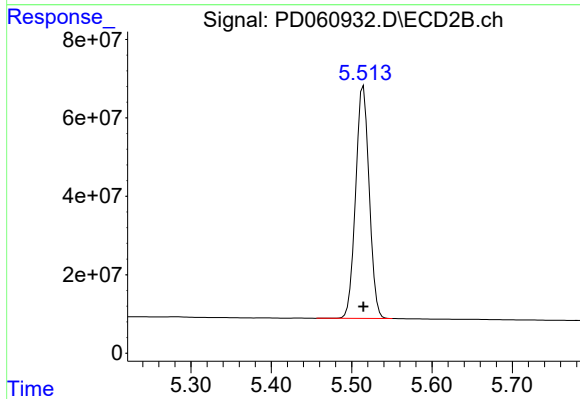

#5 Aldrin


R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 694551754
Conc: 75.52 ng/ml

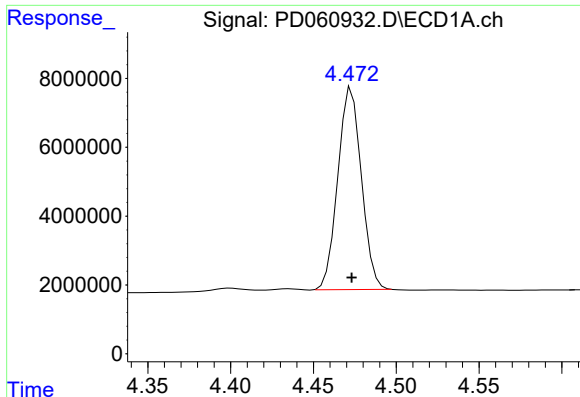

#6 beta-BHC


R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 58228989
Conc: 71.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

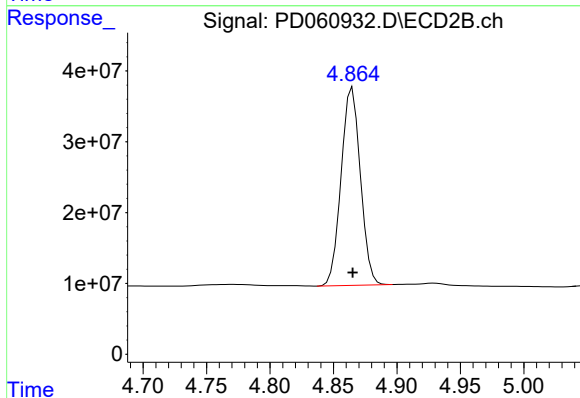


#6 beta-BHC

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 294997709
Conc: 74.36 ng/ml

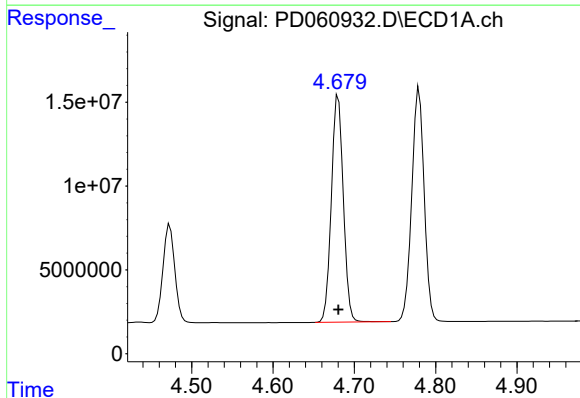


#7 delta-BHC

R.T.: 4.680 min
Delta R.T.: 0.000 min
Response: 139098159
Conc: 78.04 ng/ml

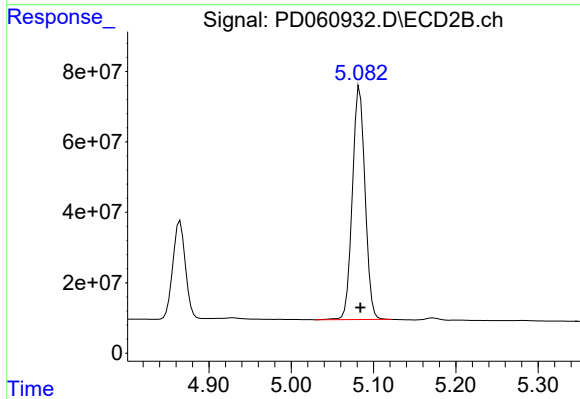

#7 delta-BHC


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 706798900
Conc: 75.04 ng/ml

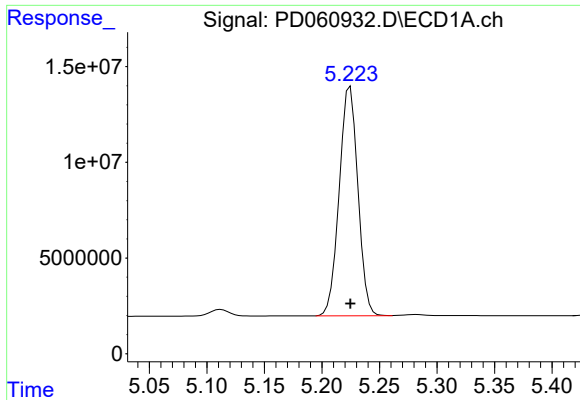

#8 Heptachlor epoxide


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 135672622
Conc: 76.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

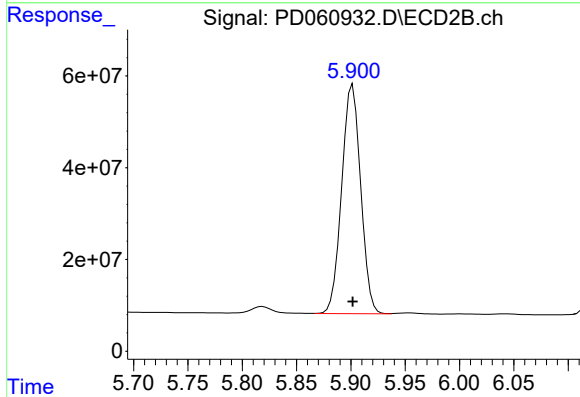


#8 Heptachlor epoxide

R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 608449207
Conc: 72.62 ng/ml

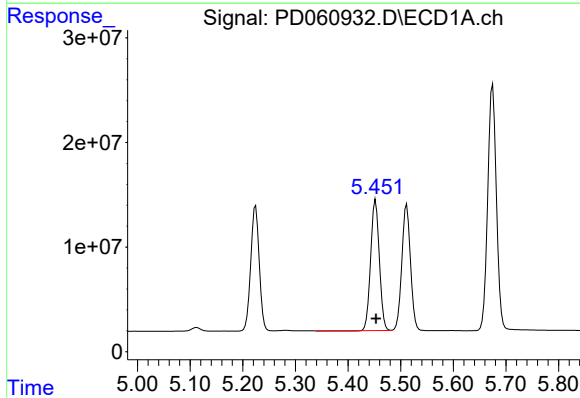


#10 trans-Chlordane

R.T.: 5.452 min
Delta R.T.: 0.000 min
Response: 142558715
Conc: 76.28 ng/ml

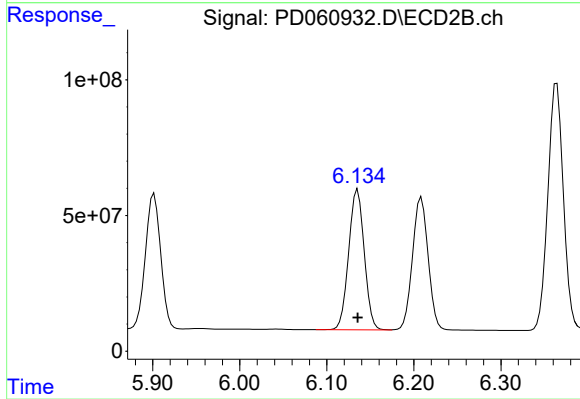

#10 trans-Chlordane


R.T.: 6.135 min
Delta R.T.: 0.000 min
Response: 643443705
Conc: 74.09 ng/ml

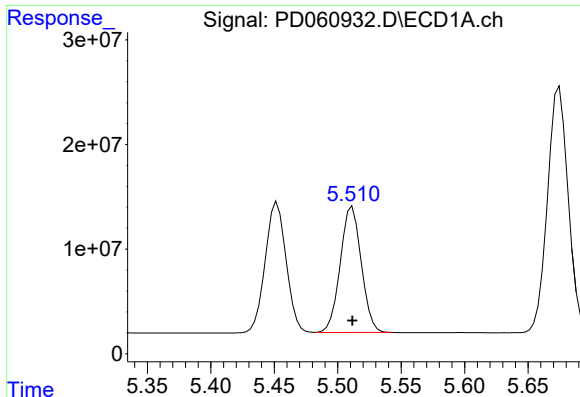

#11 cis-Chlordane


R.T.: 5.512 min
Delta R.T.: 0.000 min
Response: 138867450
Conc: 75.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

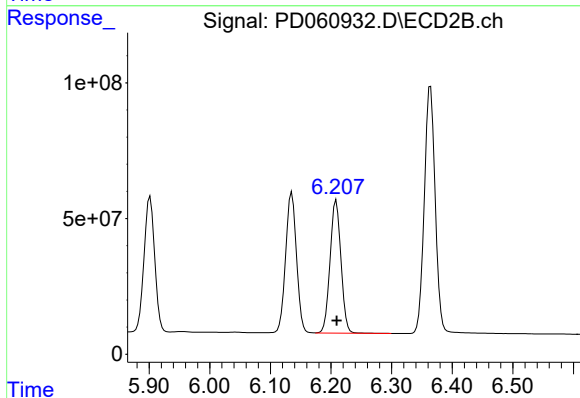


#11 cis-Chlordane

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 611646688
Conc: 74.50 ng/ml

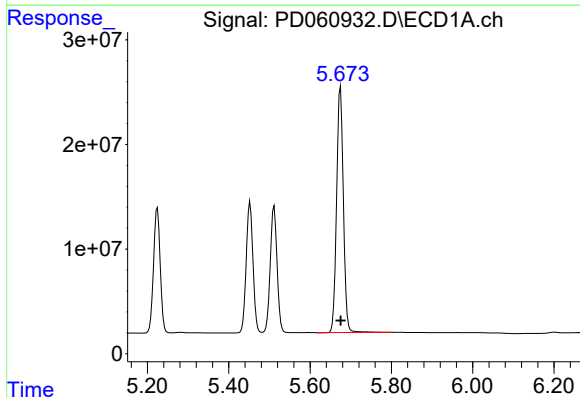


#12 4,4'-DDE

R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 270722185
Conc: 154.85 ng/ml

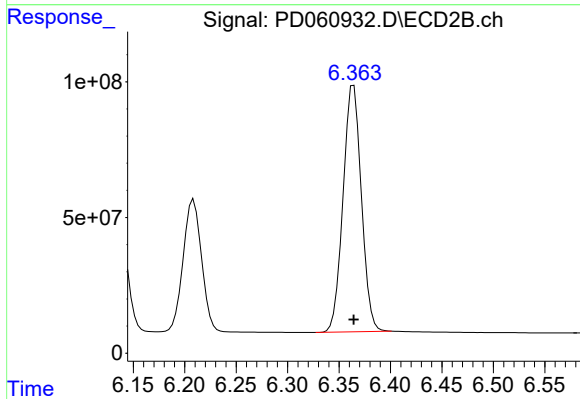

#12 4,4'-DDE


R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 1126363060
Conc: 149.77 ng/ml

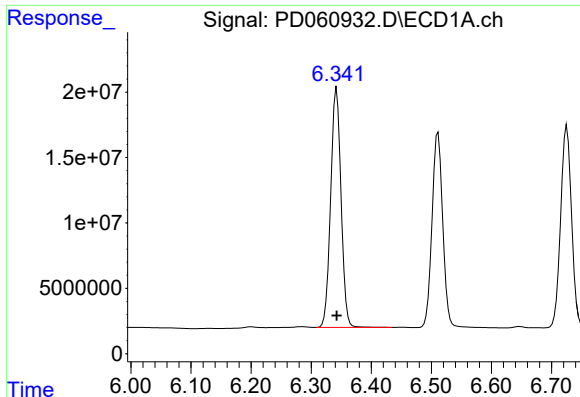

#15 Endosulfan II


R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 219798486
Conc: 163.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

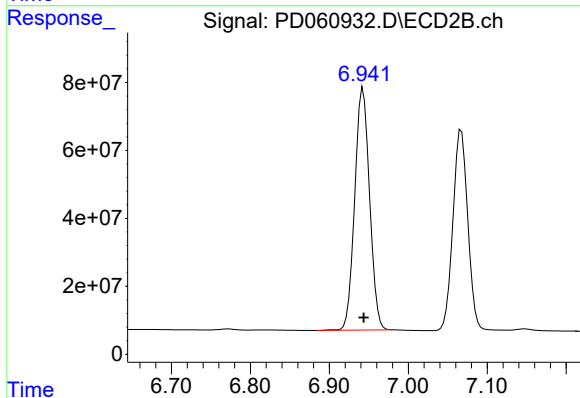


#15 Endosulfan II

R.T.: 6.943 min
Delta R.T.: 0.000 min
Response: 932386850
Conc: 147.71 ng/ml

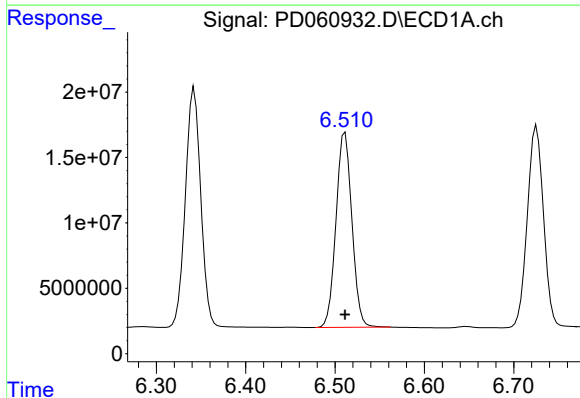


#18 Endrin aldehyde

R.T.: 6.511 min
Delta R.T.: 0.000 min
Response: 184299636
Conc: 150.10 ng/ml

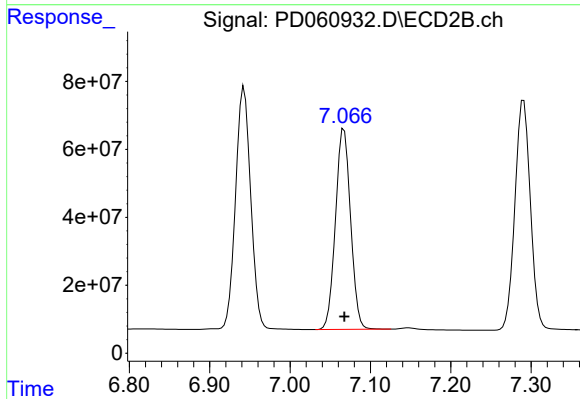

#18 Endrin aldehyde


R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 773035212
Conc: 148.59 ng/ml

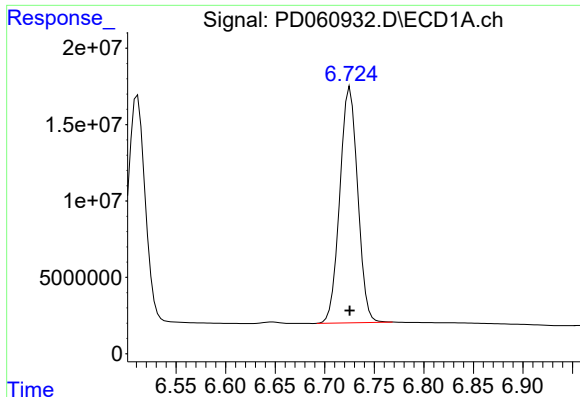

#19 Endosulfan Sulfate


R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 193888454
Conc: 160.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

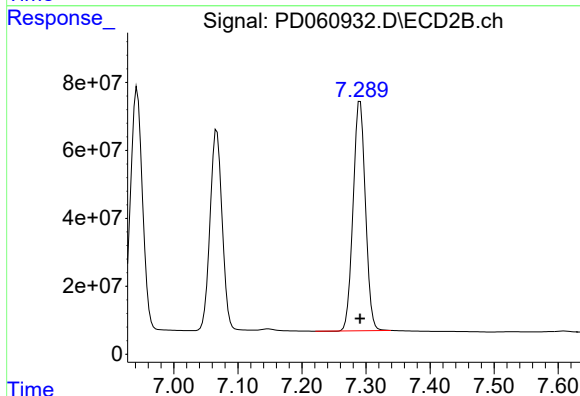


#19 Endosulfan Sulfate

R.T.: 7.291 min
Delta R.T.: 0.000 min
Response: 902272660
Conc: 144.09 ng/ml

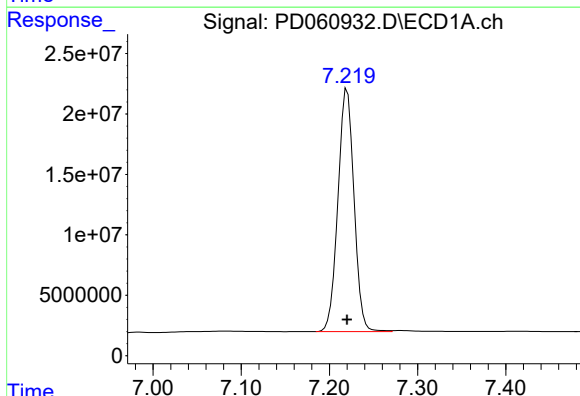


#21 Endrin ketone

R.T.: 7.220 min
Delta R.T.: 0.000 min
Response: 254670519
Conc: 156.63 ng/ml

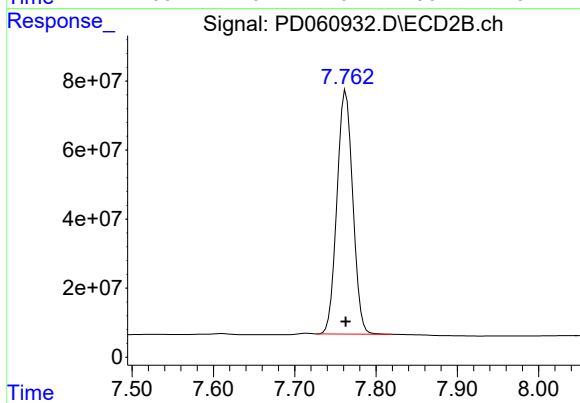

#21 Endrin ketone


R.T.: 7.763 min
Delta R.T.: 0.000 min
Response: 953170255
Conc: 143.43 ng/ml

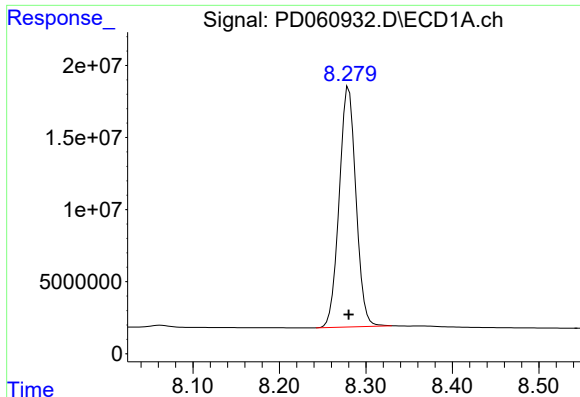

#27 Decachlorobiphenyl

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 222776327
Conc: 144.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

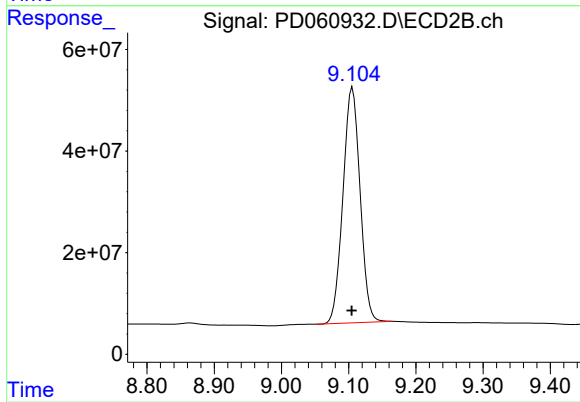

#27 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 820128763
Conc: 136.20 ng/ml