

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 14:04
 Operator : DD\AJ
 Sample : L5214-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 03:37:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 03:28:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.021	24221922	129.3E6	18.248	18.613
27)	SA Decachlor...	8.281	9.105	60532756	233.9E6	37.619	37.927
Target Compounds							
2)	A alpha-BHC	3.938	4.411	2267673	10229657	1.163	0.960
3)	MA gamma-BHC...	4.223	4.697	2047035	10691398	1.095	1.091
4)	MA Heptachlor	4.529	5.209	2038089	9395284	1.006	0.955
5)	MB Aldrin	4.780	5.515	1817215	9216319	0.945	1.000
6)	B beta-BHC	4.472	4.866	882040	3257798	1.084m	0.821
7)	B delta-BHC	4.679	5.084	1578478	9298080	0.877m	0.984
8)	B Heptachlo...	5.224	5.900	1830352	8781853	1.014	1.068m
9)	A Endosulfan I	5.564	6.260	1810136	7025494	1.033m	0.902
10)	B trans-Chl...	5.453	6.136	1851595	9267509	0.979	1.069
11)	B cis-Chlor...	5.511	6.210	1842550	8111502	0.997	0.987
12)	B 4,4'-DDE	5.675	6.365	1822427	7528137	1.049	1.012
13)	MA Dieldrin	5.811	6.517	1903343	8566326	0.987	1.021
14)	MA Endrin	6.067	6.735	1492753	6567450	0.944m	1.011
15)	B Endosulfa...	6.342	6.944	1713568	6583395	1.198m	1.060
16)	A 4,4'-DDD	6.194	6.856	1377393	5995723	0.985	1.028
17)	MA 4,4'-DDT	6.435	7.153	1363662	6161873	0.875	0.998m
18)	B Endrin al...	6.511	7.067	1451221	5979256	1.167	1.137
19)	B Endosulfa...	6.723	7.291	2044590	6837782	1.566m	1.108 #
20)	A Methoxychlor	6.982	7.611	691046	3415376	0.904m	1.199 #
21)	B Endrin ke...	7.219	7.763	1878910	6887711	1.130	1.062

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 14:04
Operator : DD\AJ
Sample : L5214-01
Misc : PEST MDL 1 PPB
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 03:37:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

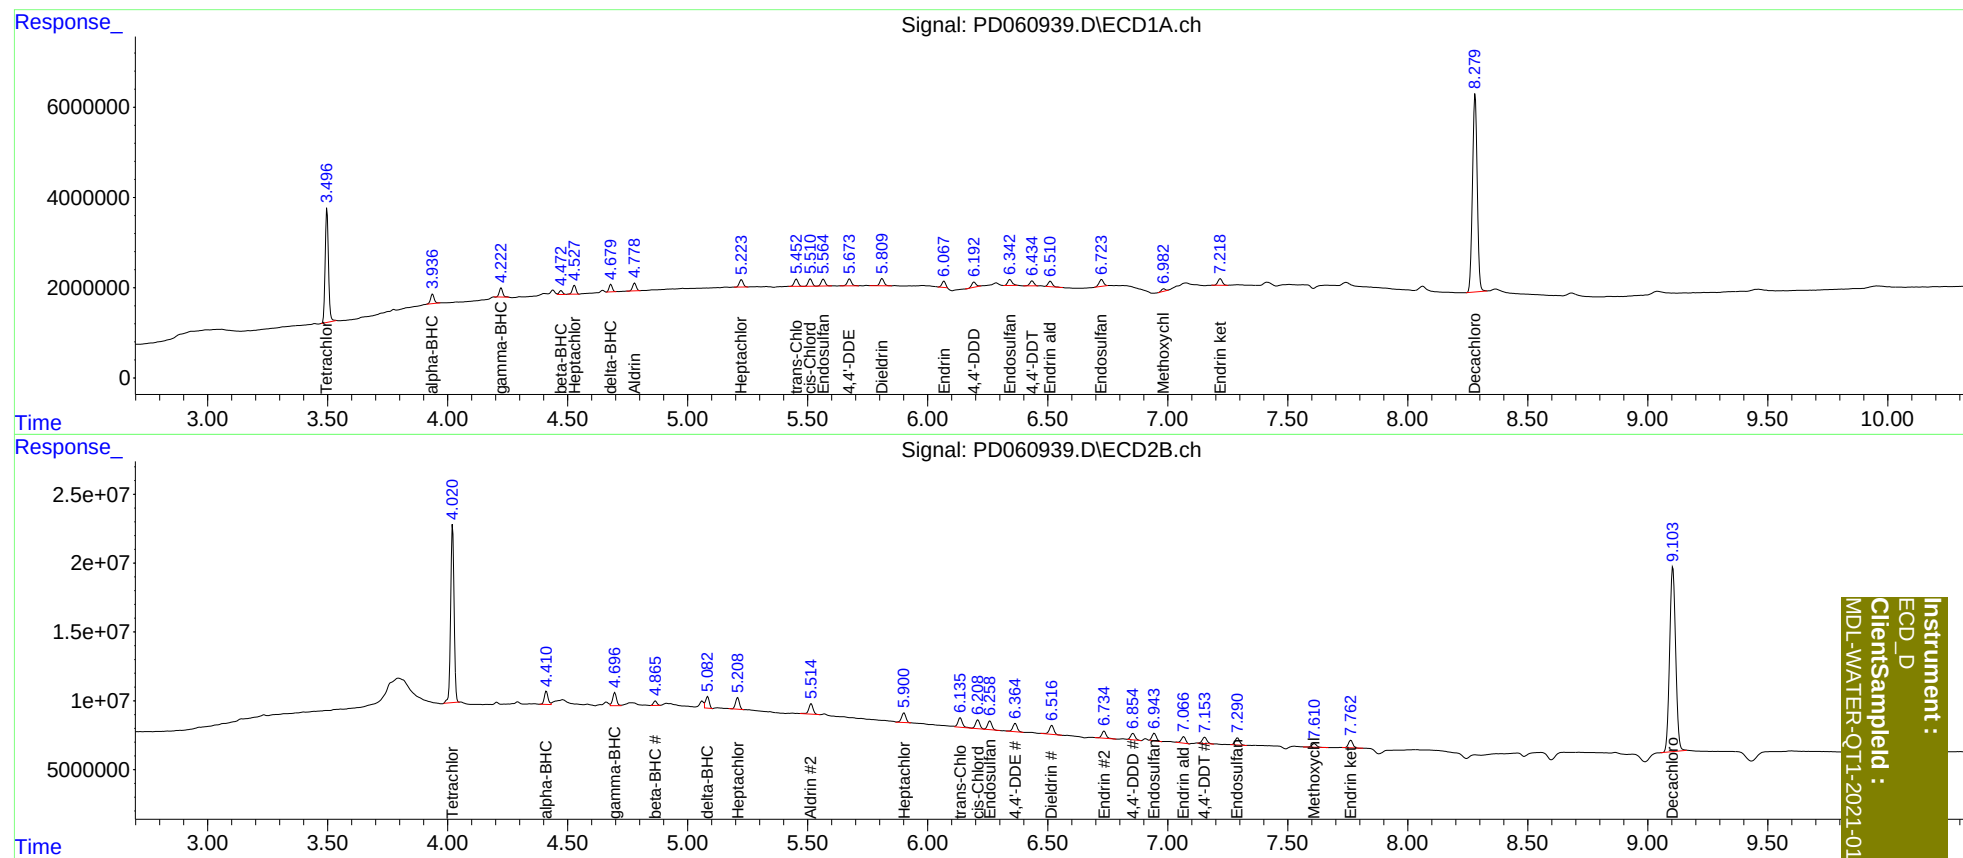

Instrument :
ECD_D
ClientSample :
MDL-WATER-QT1-2021-01