

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
 Data File : PD060916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2021 08:40
 Operator : DD\AJ
 Sample : RESC15
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 03:35:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 03:28:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.020	25465296	137.8E6	19.185	19.840
2)	SA Decachlor...	8.281	9.102	60566725	231.3E6	37.640	37.501
Target Compounds							
2)	A alpha-BHC	3.938	4.411	18892831	106.4E6	9.691	9.985
3)	MA gamma-BHC...	4.224	4.696	18231378	98392607	9.749	10.041
4)	MA Heptachlor	4.529	5.207	19156689	89909579	9.460	9.142
5)	MB Aldrin	4.780	5.514	18992442	92640398	9.878	10.051
6)	B beta-BHC	4.474	4.865	8484932	40693652	10.424	10.253
7)	B delta-BHC	4.681	5.083	17713510	96297789	9.836	10.188
8)	B Heptachlo...	5.225	5.901	17830239	80928858	9.880	9.845
9)	A Endosulfan I	5.566	6.259	15858716	76941012	9.054	9.876
10)	B trans-Chl...	5.453	6.135	18526195	85997931	9.794	9.920
11)	B cis-Chlor...	5.512	6.208	18040776	82088533	9.759	9.985
12)	B 4,4'-DDE	5.676	6.364	34142804	148.3E6	19.657	19.930
13)	MA Dieldrin	5.811	6.516	36930566	163.8E6	19.144	19.517
14)	MA Endrin	6.069	6.734	30255347	123.7E6	19.136	19.050
15)	B Endosulfa...	6.343	6.943	28149916	123.5E6	19.688	19.879
16)	A 4,4'-DDD	6.194	6.854	27000163	112.8E6	19.304	19.332
17)	MA 4,4'-DDT	6.436	7.153	28985614	113.6E6	18.609	18.398
18)	B Endrin al...	6.512	7.066	25069861	103.8E6	20.160	19.750
19)	B Endosulfa...	6.726	7.290	26292656	121.9E6	20.142	19.753
20)	A Methoxychlor	6.983	7.610	69521814	250.5E6	90.960	87.962
21)	B Endrin ke...	7.220	7.762	33069133	131.3E6	19.893	20.238

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 08:40
Operator : DD\AJ
Sample : RESC15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 03:35:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

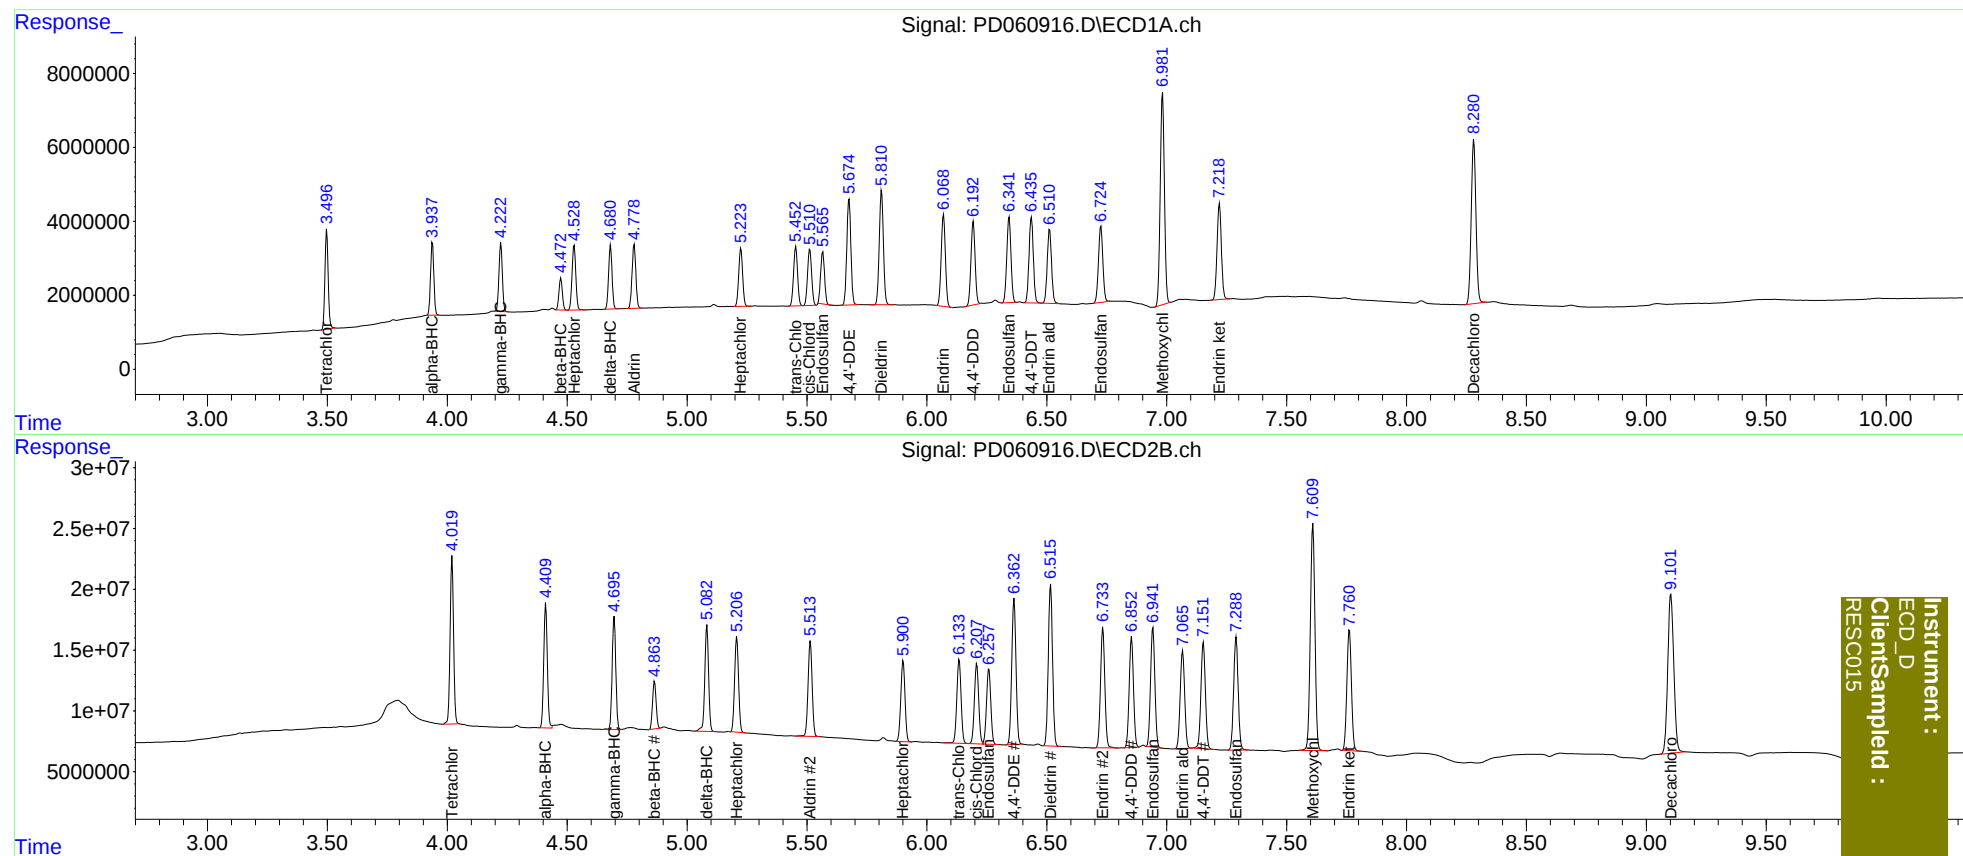

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060916.D
Acq On : 07 Jan 2021 08:40
Operator : DD\AJ
Sample : RESC15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Title : GC Extractables
Last Update : Fri Jan 08 03:28:22 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.498	3.938	100.00%
3.938	4.224	100.00%
4.224	4.474	100.00%
4.474	4.529	100.00%
4.529	4.681	100.00%
4.681	4.780	100.00%
4.780	5.225	100.00%
5.225	5.453	100.00%
5.453	5.512	100.00%
5.512	5.566	100.00%
5.566	5.676	100.00%
5.676	5.811	100.00%
5.811	6.069	100.00%
6.069	6.194	100.00%
6.194	6.343	100.00%
6.343	6.436	100.00%
6.436	6.512	100.00%
6.512	6.726	100.00%
6.726	6.983	100.00%
6.983	7.220	100.00%
7.220	8.281	100.00%

Signal #2


4.020	4.411	100.00%
4.411	4.696	100.00%
4.696	4.865	100.00%
4.865	5.083	100.00%
5.083	5.207	100.00%
5.207	5.514	100.00%
5.514	5.901	100.00%
5.901	6.135	100.00%
6.135	6.208	100.00%
6.208	6.259	97.61%
6.259	6.364	100.00%
6.364	6.516	100.00%
6.516	6.734	100.00%
6.734	6.854	100.00%
6.854	6.943	100.00%
6.943	7.066	100.00%
7.066	7.153	100.00%
7.153	7.290	100.00%
7.290	7.610	100.00%
7.610	7.762	100.00%
7.762	9.103	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010721\
Data File : PD060916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2021 08:40
Operator : DD\AJ
Sample : RESC15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 03:35:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

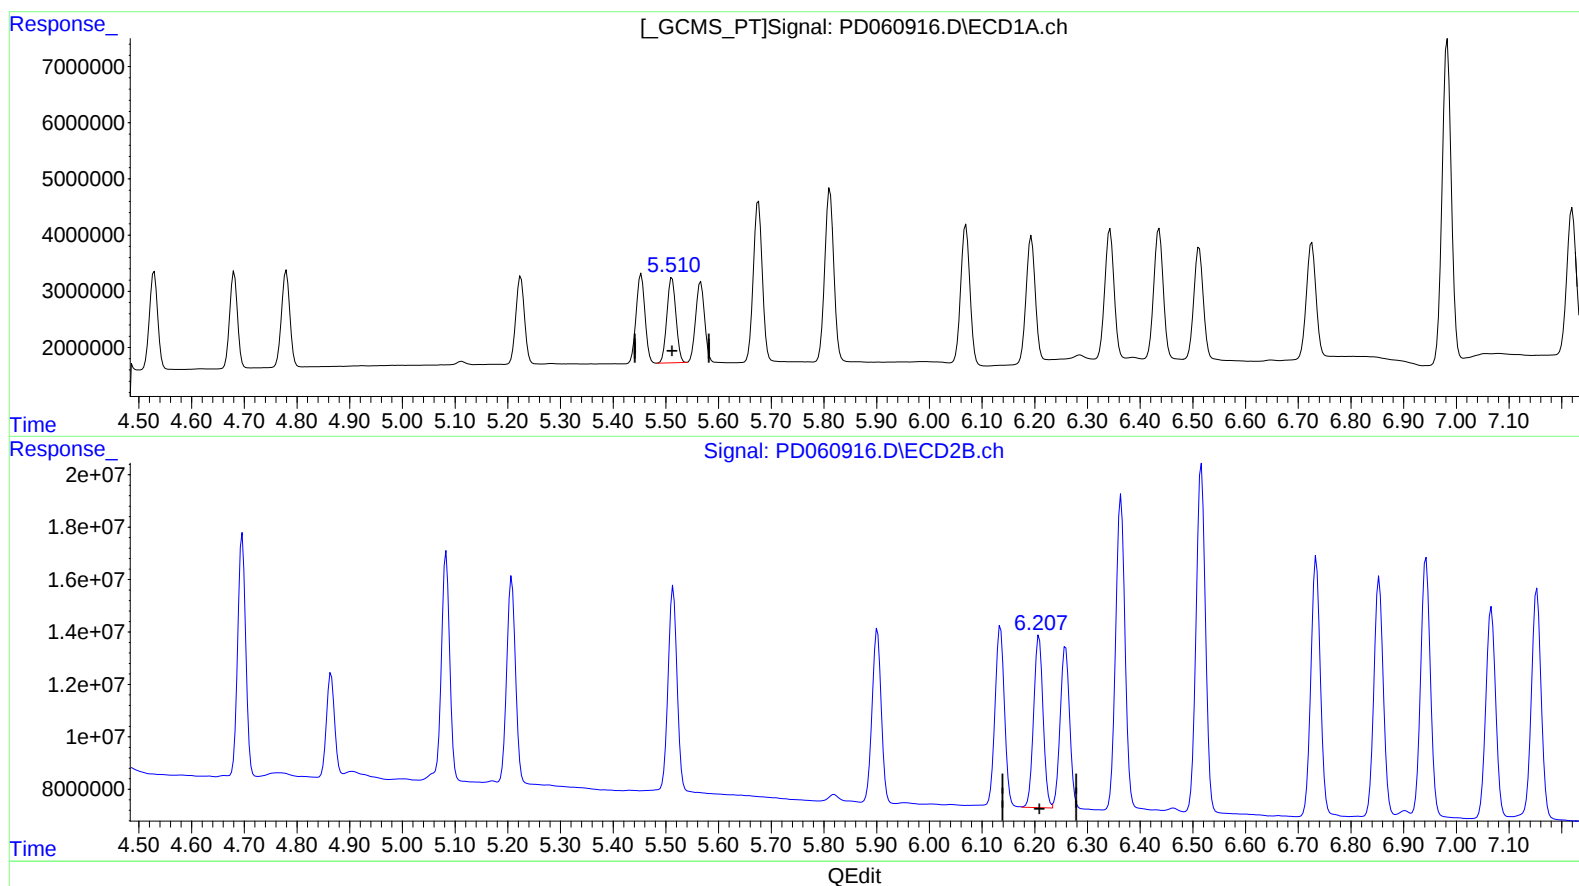

(11) cis-Chlordane (B)

5.512min 9.759 ng/ml

response 18040776

(11) cis-Chlordane #2 (B)

6.208min 9.985 ng/ml

response 82088533