

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010722\
 Data File : PD067644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2022 16:36
 Operator : AR\AJ
 Sample : N1067-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 124035

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/10/2022
 Supervised By : Ankita Jodhani 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 06:15:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.431	3.959	19606423	71041443	10.789	10.767m
28) SA Decachlor...	8.150	9.012	6682864	34598488	7.523	7.280

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010722\
Data File : PD067644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2022 16:36
Operator : AR\AJ
Sample : N1067-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
124035


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/10/2022
Supervised By : Ankita Jodhani 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 06:15:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

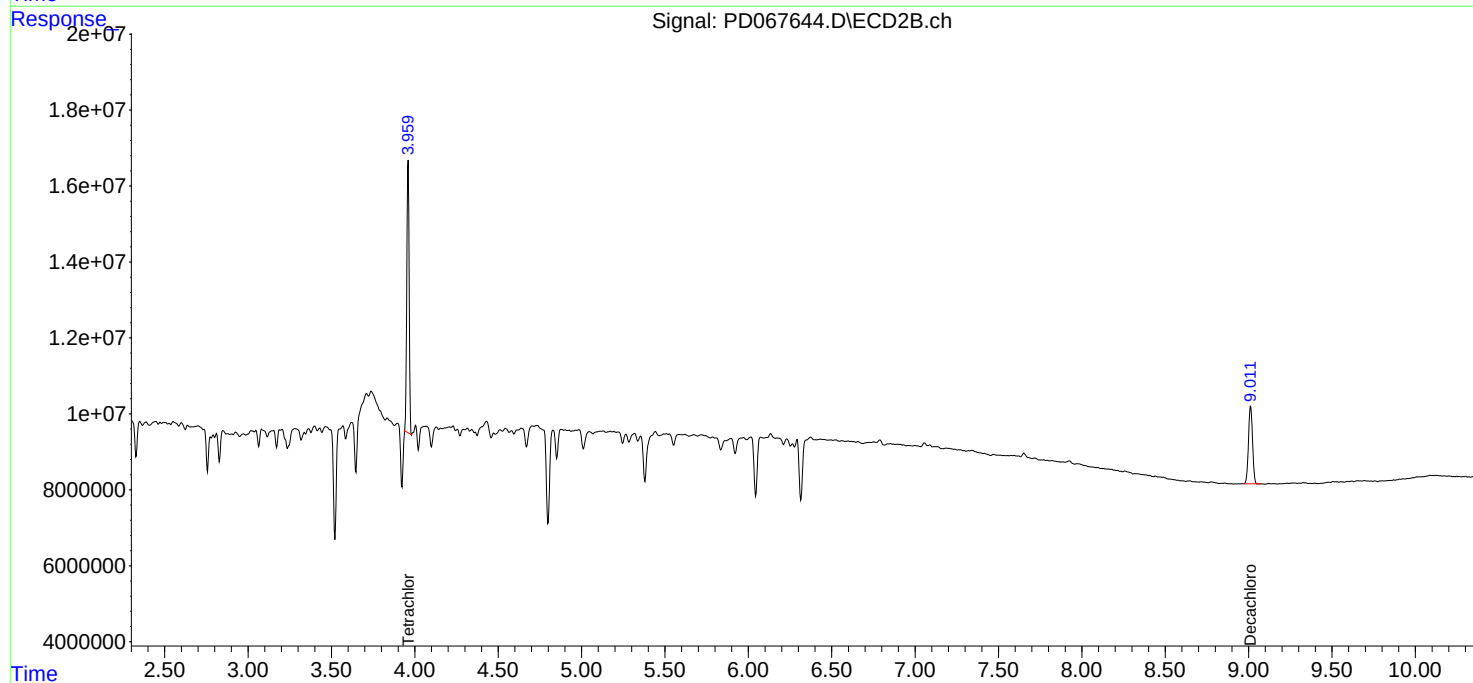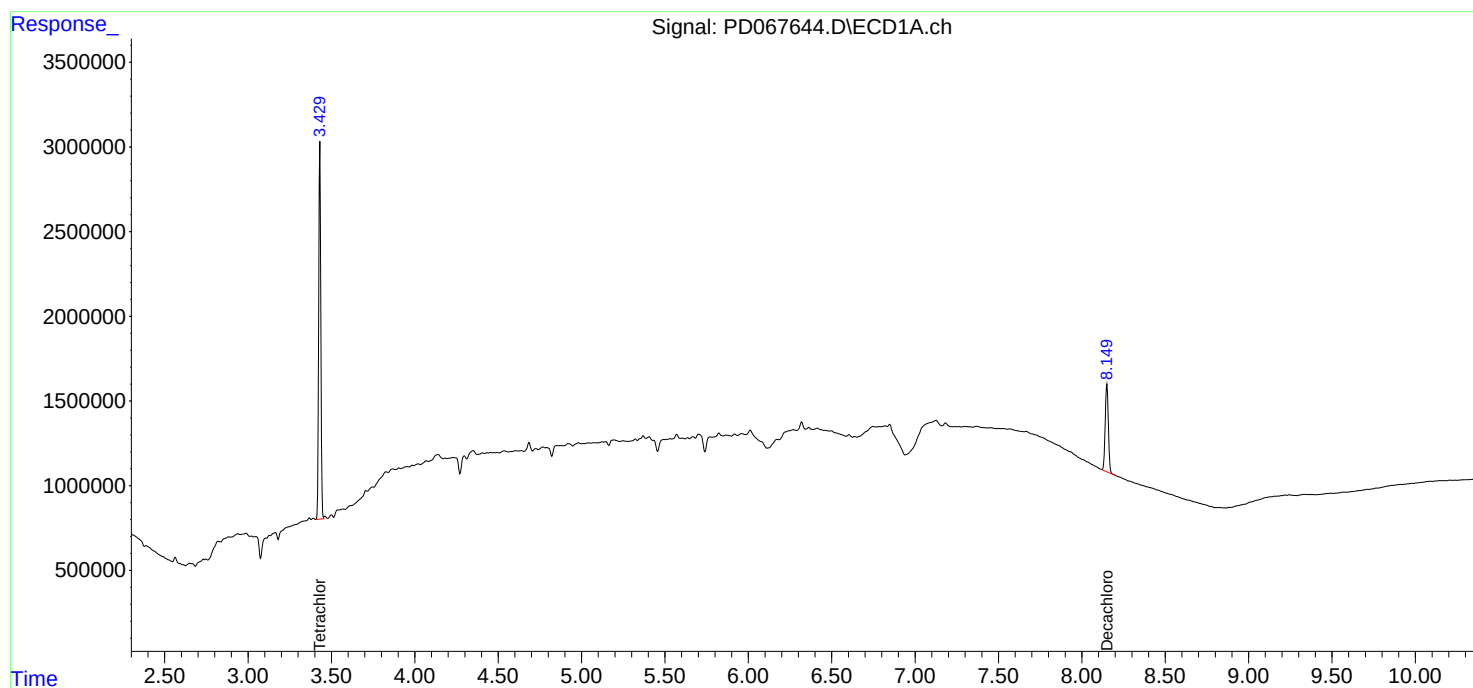

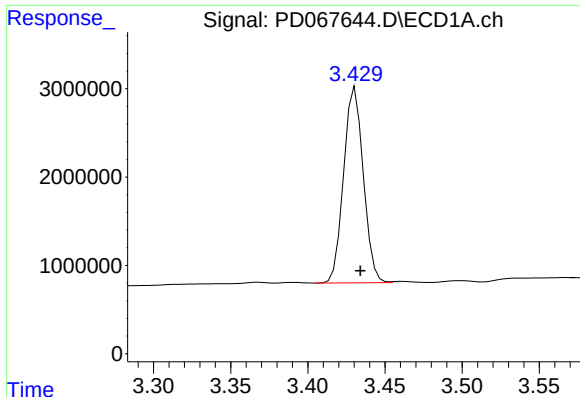


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.003 min
Response: 19606423
Conc: 10.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
124035


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/10/2022
Supervised By :Ankita Jodhani 01/10/2022

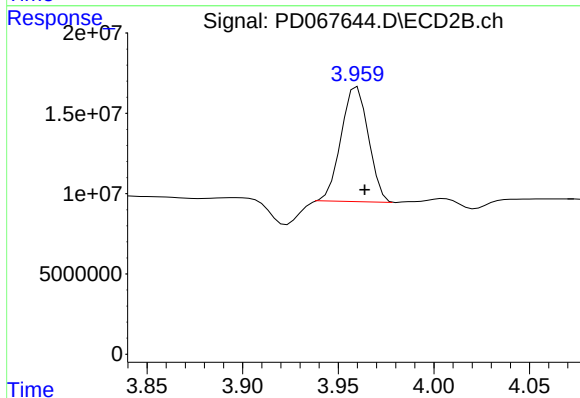


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.005 min
Response: 71041443
Conc: 10.77 ng/ml m

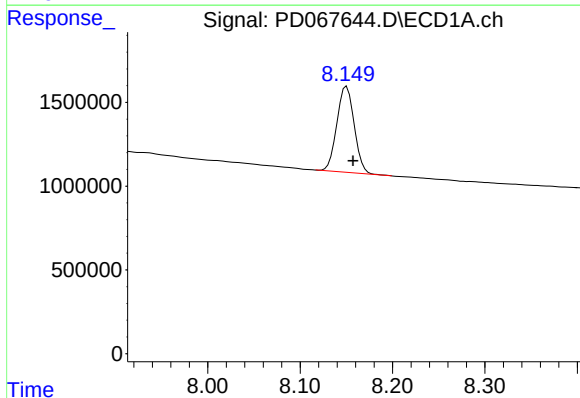

#28 Decachlorobiphenyl

R.T.: 8.150 min
Delta R.T.: -0.007 min
Response: 6682864
Conc: 7.52 ng/ml

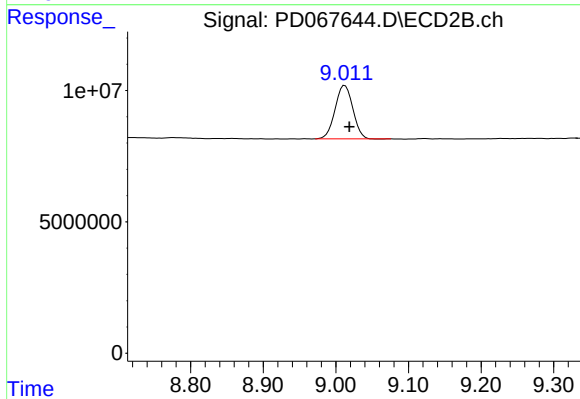

#28 Decachlorobiphenyl

R.T.: 9.012 min
Delta R.T.: -0.006 min
Response: 34598488
Conc: 7.28 ng/ml