

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010920\
 Data File : PD056893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2020 19:10
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 06:04:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010920CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 06:00:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	31618428	58312220	38.797	39.244
27)	SA Decachlor...	7.953	8.992	72406096	111.3E6	76.179	77.188
Target Compounds							
2)	A alpha-BHC	3.711	4.346	47455522	85873238	40.791	41.089
3)	MA gamma-BHC...	3.986	4.628	45201089	81947984	39.485	40.562
4)	MA Heptachlor	4.271	5.134	42556013	82904848	39.595	39.692
9)	A Endosulfan I	5.276	6.176	36421887	68606577	39.654	39.418
13)	MA Dieldrin	5.515	6.431	83781827	153.1E6	81.150	80.844
14)	MA Endrin	5.768	6.648	68926294	123.0E6	79.039	79.758
16)	A 4,4'-DDD	5.902	6.770	62310803	116.1E6	80.793	81.187
17)	MA 4,4'-DDT	6.138	7.068	62342335	118.1E6	85.176	82.848
20)	A Methoxychlor	6.686	7.525	155.1E6	307.0E6	388.475	392.899


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD010920\
Data File : PD056893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2020 19:10
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA401

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 06:04:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010920CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 06:00:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

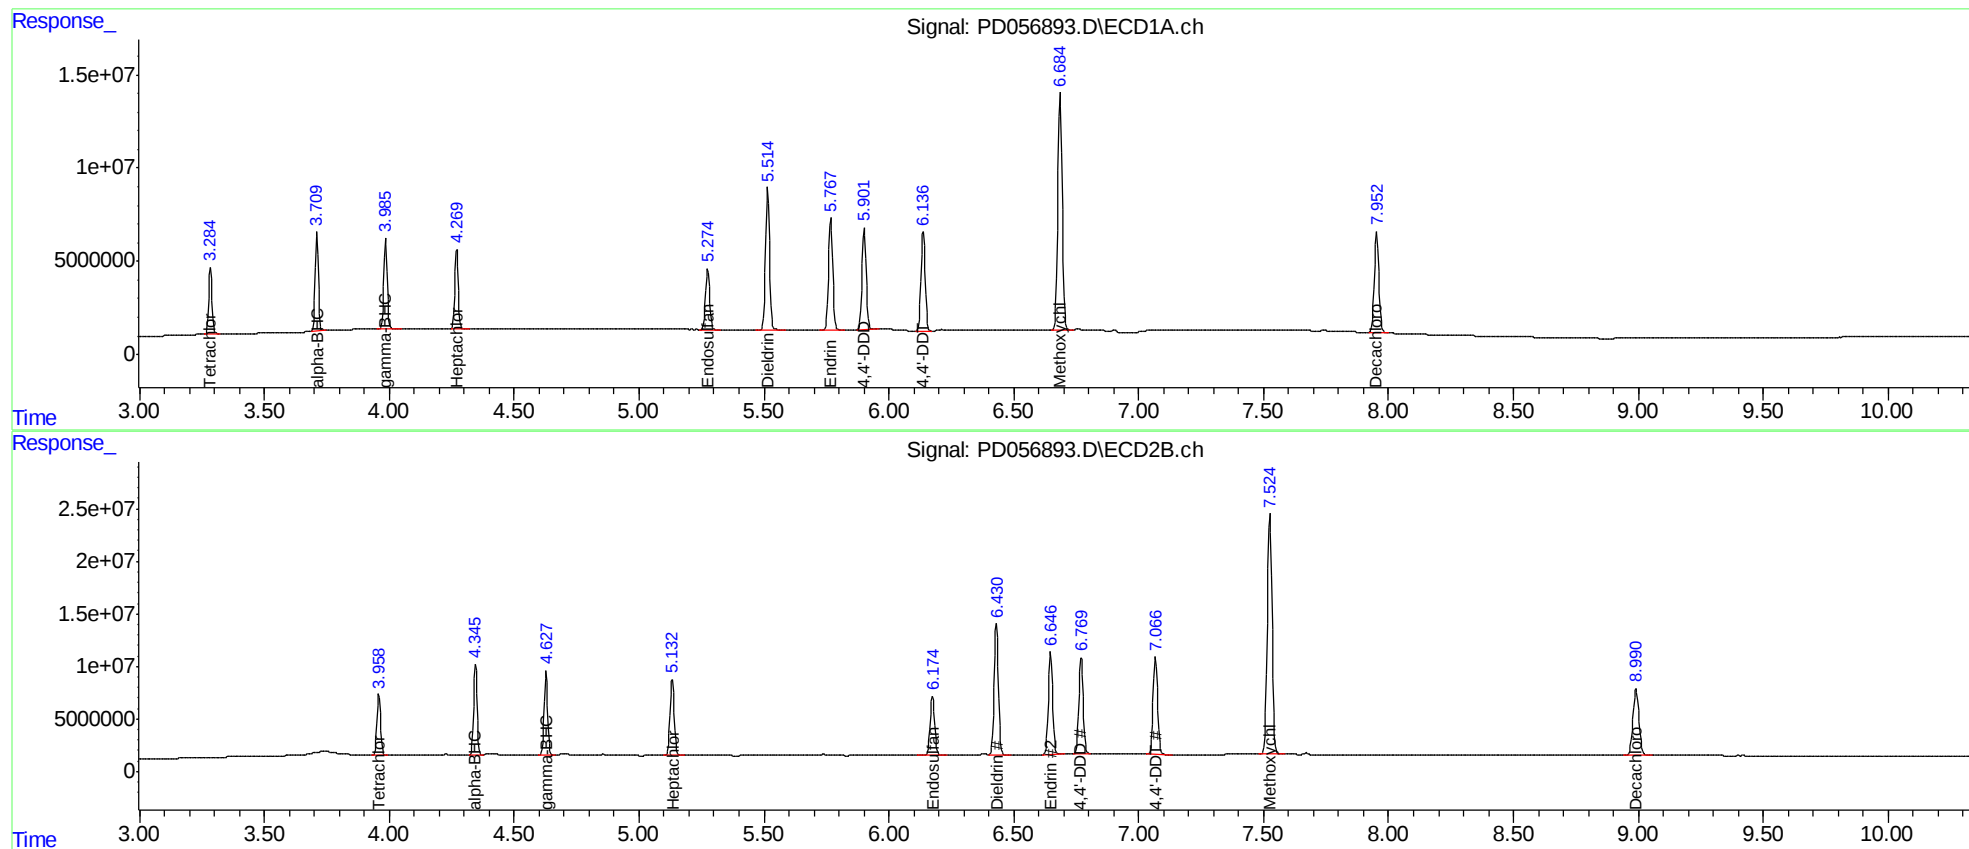


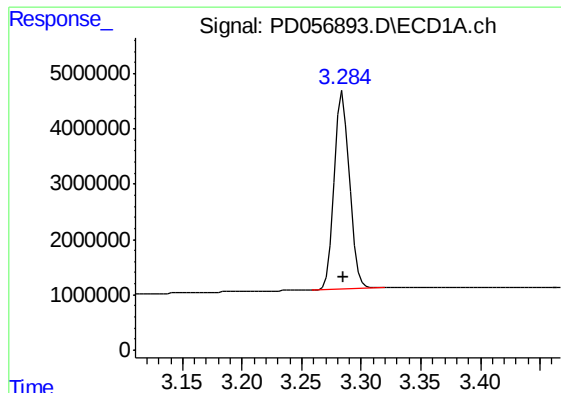

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 31618428
Conc: 38.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

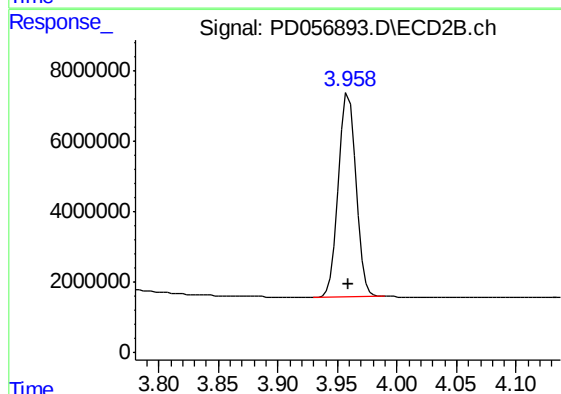


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 58312220
Conc: 39.24 ng/ml

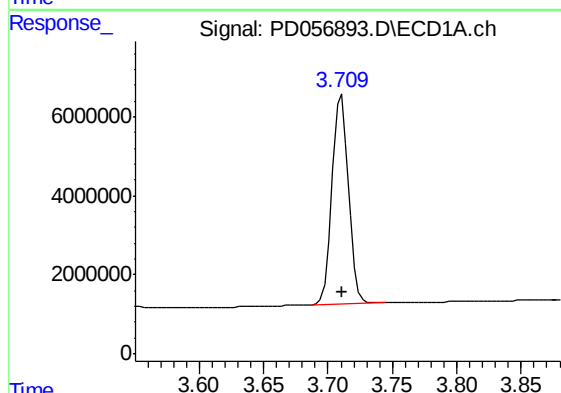


#2 alpha-BHC

R.T.: 3.711 min
Delta R.T.: 0.000 min
Response: 47455522
Conc: 40.79 ng/ml

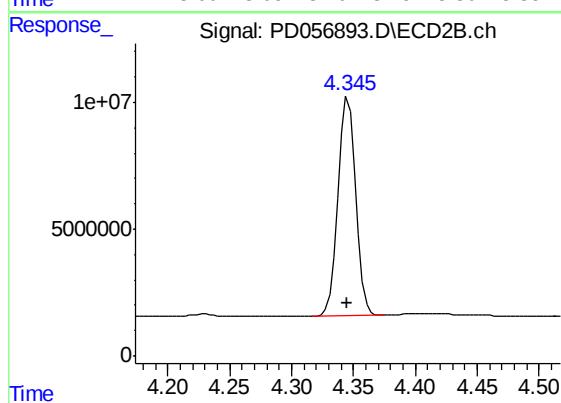

#2 alpha-BHC


R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 85873238
Conc: 41.09 ng/ml

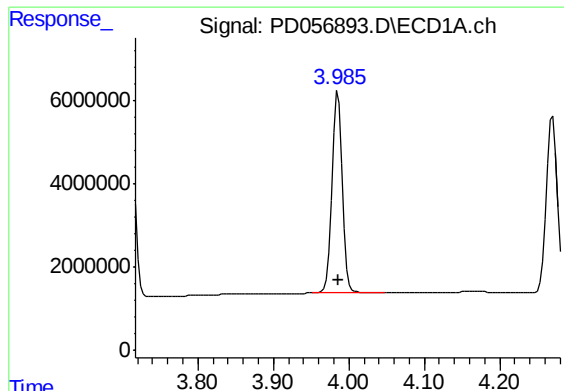

#3 gamma-BHC (Lindane)


R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 45201089
Conc: 39.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

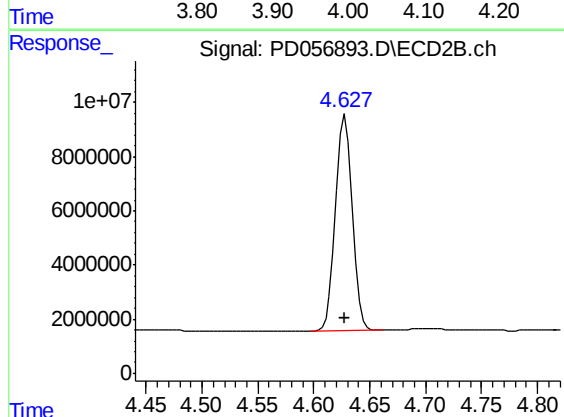


#3 gamma-BHC (Lindane)

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 81947984
Conc: 40.56 ng/ml

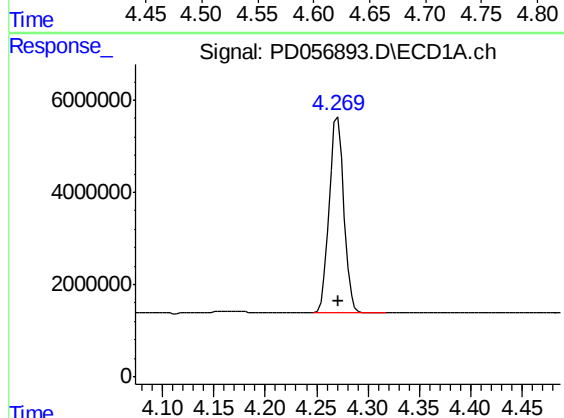


#4 Heptachlor

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 42556013
Conc: 39.59 ng/ml

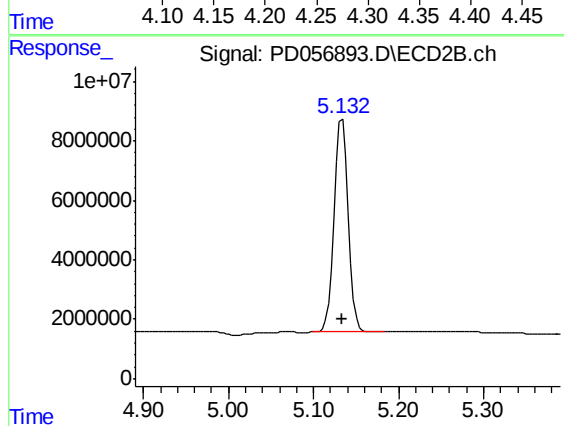

#4 Heptachlor


R.T.: 5.134 min
Delta R.T.: 0.000 min
Response: 82904848
Conc: 39.69 ng/ml

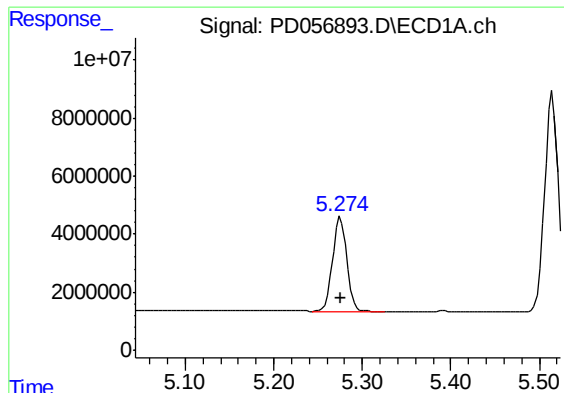

#9 Endosulfan I


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 36421887
Conc: 39.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

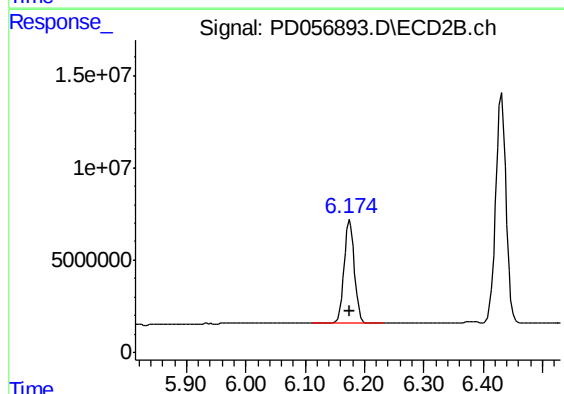


#9 Endosulfan I

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 68606577
Conc: 39.42 ng/ml

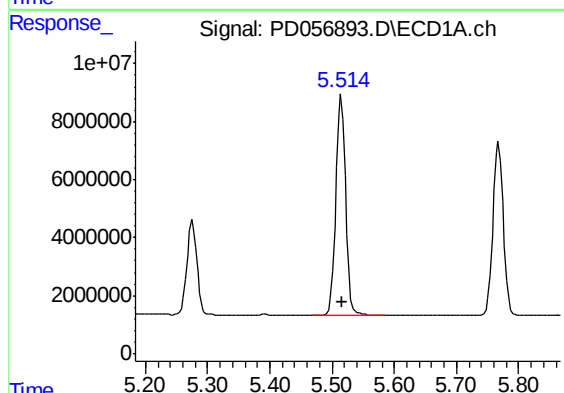


#13 Dieldrin

R.T.: 5.515 min
Delta R.T.: 0.000 min
Response: 83781827
Conc: 81.15 ng/ml

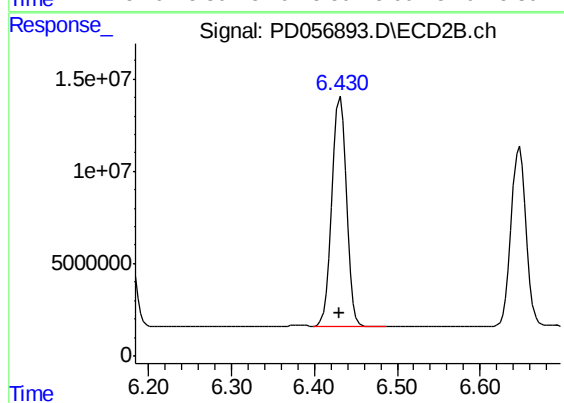

#13 Dieldrin


R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 153131246
Conc: 80.84 ng/ml

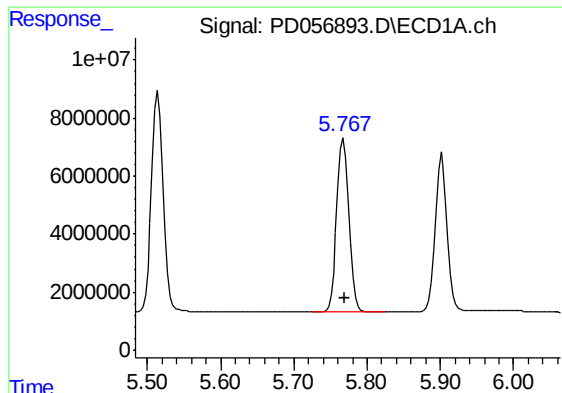

#14 Endrin


R.T.: 5.768 min
Delta R.T.: 0.000 min
Response: 68926294
Conc: 79.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

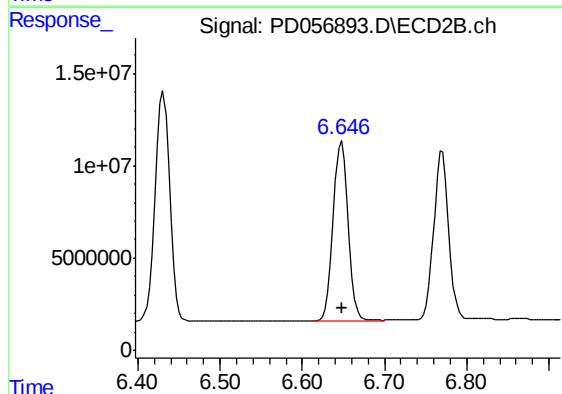


#14 Endrin

R.T.: 6.648 min
Delta R.T.: 0.000 min
Response: 122976898
Conc: 79.76 ng/ml

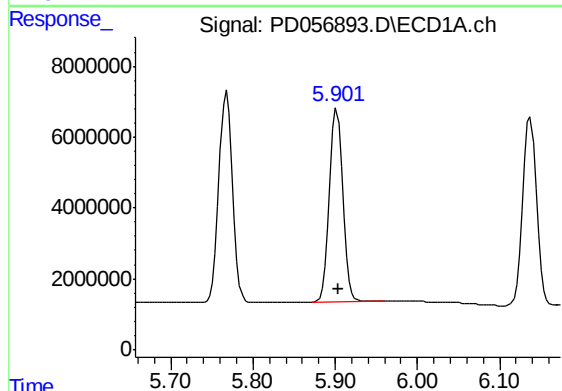


#16 4,4'-DDD

R.T.: 5.902 min
Delta R.T.: -0.001 min
Response: 62310803
Conc: 80.79 ng/ml

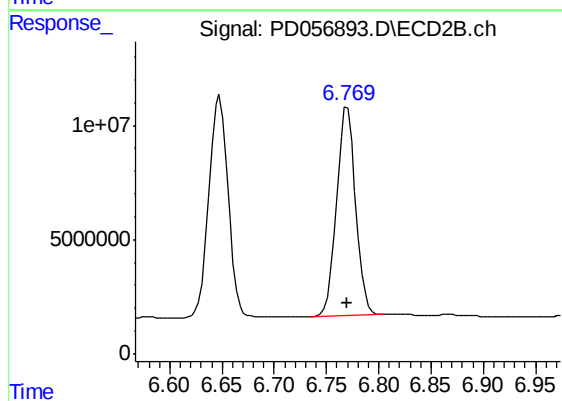

#16 4,4'-DDD


R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 116093690
Conc: 81.19 ng/ml

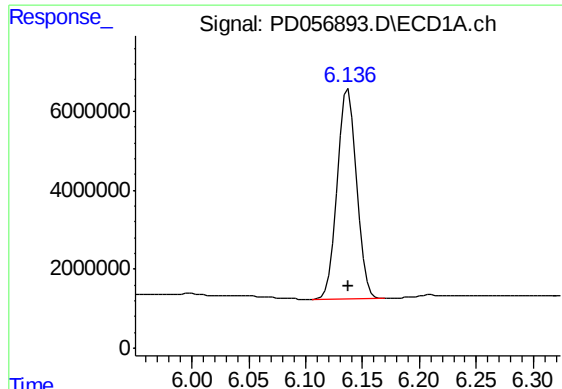

#17 4,4'-DDT


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 62342335
Conc: 85.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

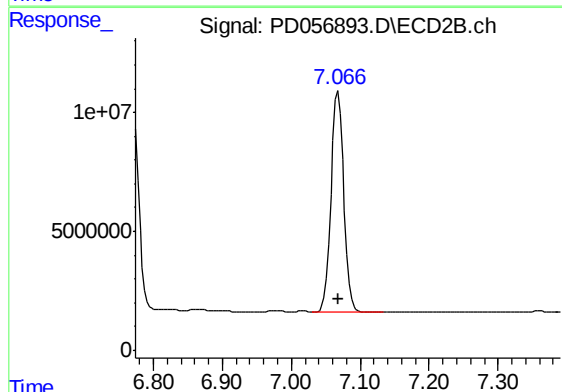


#17 4,4'-DDT

R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 118091125
Conc: 82.85 ng/ml

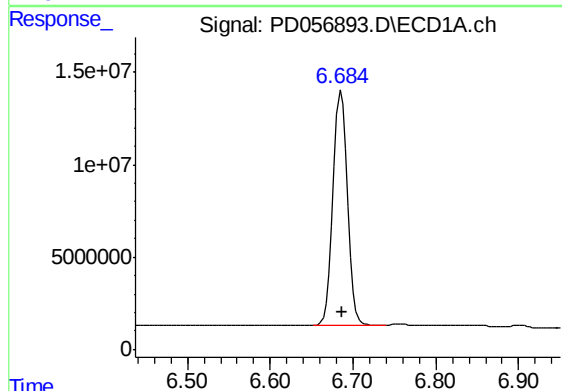


#20 Methoxychlor

R.T.: 6.686 min
Delta R.T.: 0.000 min
Response: 155093776
Conc: 388.48 ng/ml

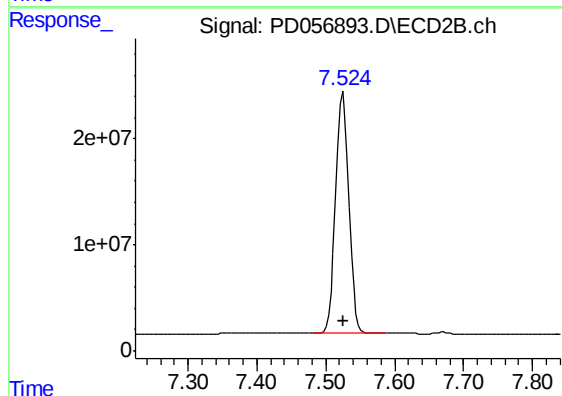

#20 Methoxychlor


R.T.: 7.525 min
Delta R.T.: 0.000 min
Response: 307025945
Conc: 392.90 ng/ml

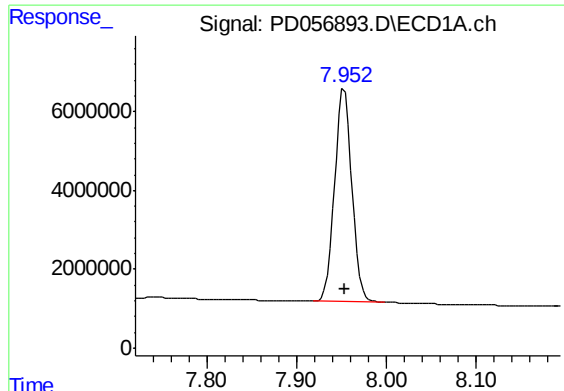

#27 Decachlorobiphenyl

R.T.: 7.953 min
Delta R.T.: 0.000 min
Response: 72406096
Conc: 76.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

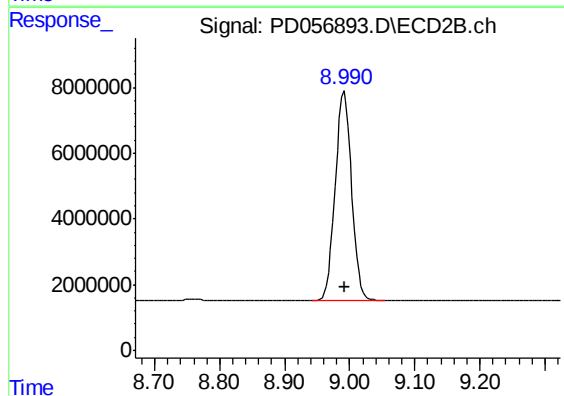

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 111273608
Conc: 77.19 ng/ml