

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011019\
 Data File : PD050931.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jan 2019 12:15
 Operator : AJ\SJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 03:52:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 03:41:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.227	4.048	32873288	669.2E6	22.009	22.485
28) SA	Decachlor...	7.834	9.163	29290722	488.0E6	24.133	24.457
Target Compounds							
9) A	Endosulfan I	5.176	6.296	23106032	386.2E6	10.839	12.274
10) B	gamma-Chl...	5.072	6.171	24792751	414.0E6	10.584	11.919
12) B	4,4'-DDE	5.298	6.400	47701039	759.4E6	22.099	23.034
13) MA	Dieldrin	5.412	6.554	52486575	783.0E6	22.410	23.473
19) B	Endosulfa...	6.305	7.330	40909207	591.5E6	20.885	21.910
20) A	Methoxychlor	6.579	7.651	108.3E6	1249.5E6	113.332	102.638
21) B	Endrin ke...	6.781	7.804	41707266	519.3E6	19.595	20.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011019\
Data File : PD050931.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jan 2019 12:15
Operator : AJ\SJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 03:52:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 03:41:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

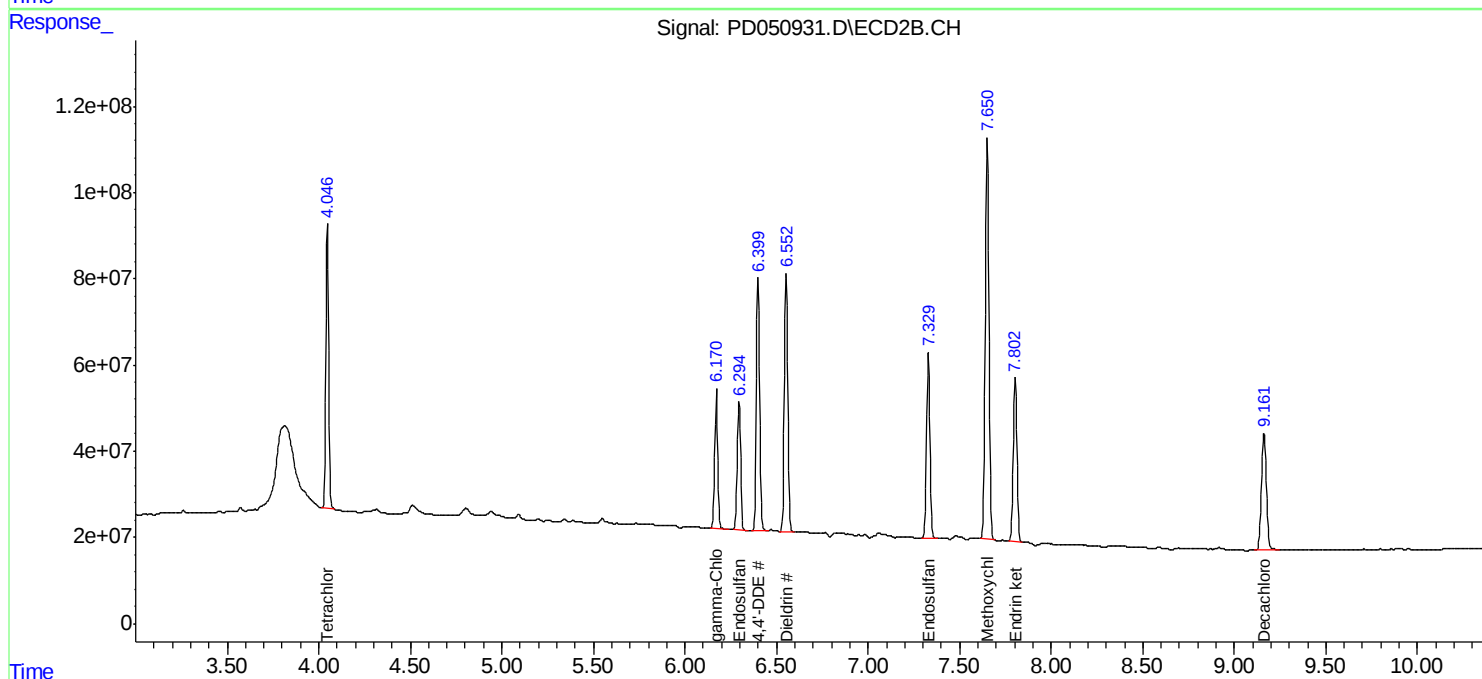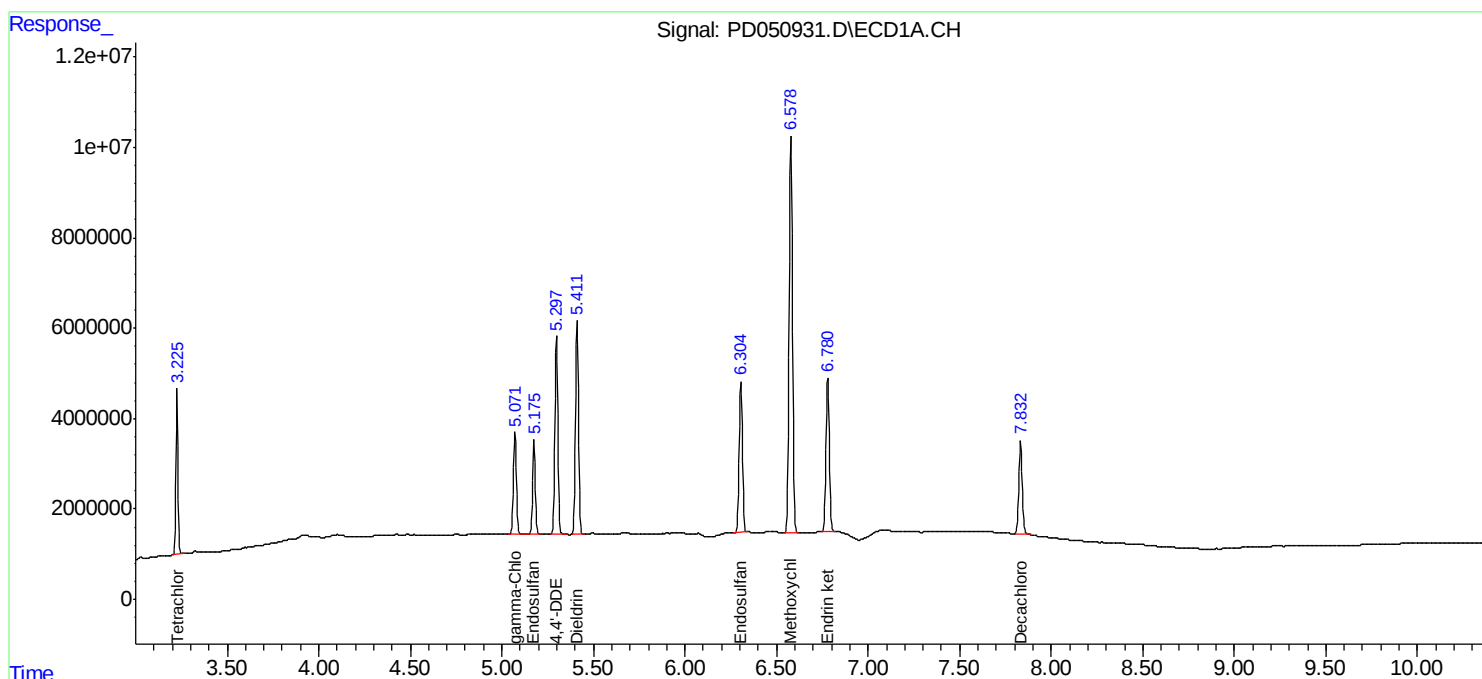


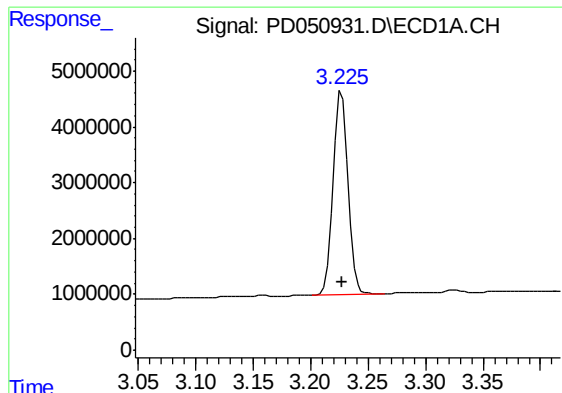

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 32873288
Conc: 22.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

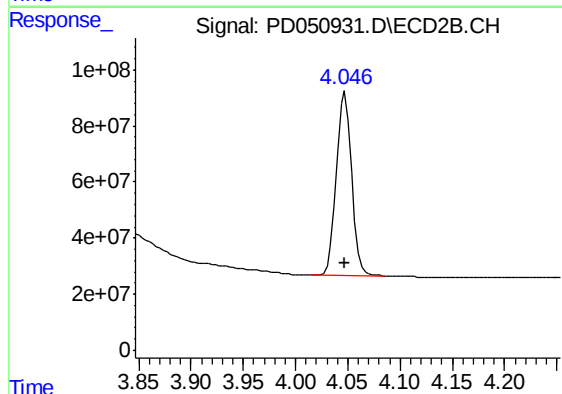


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 669158122
Conc: 22.48 ng/ml

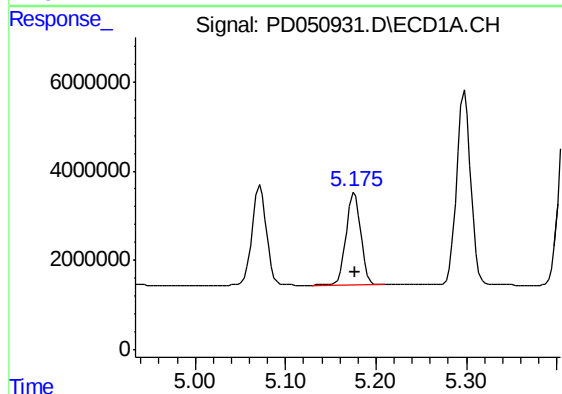


#9 Endosulfan I

R.T.: 5.176 min
Delta R.T.: 0.000 min
Response: 23106032
Conc: 10.84 ng/ml

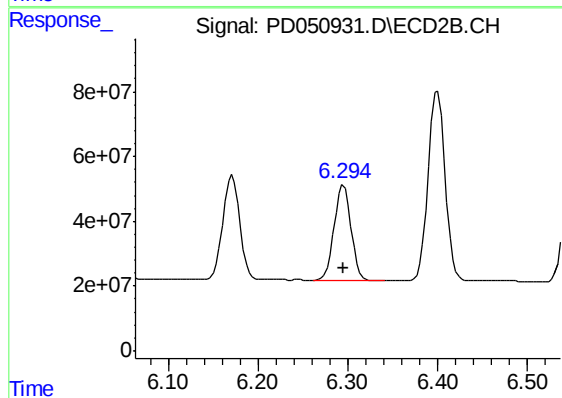

#9 Endosulfan I


R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 386206140
Conc: 12.27 ng/ml

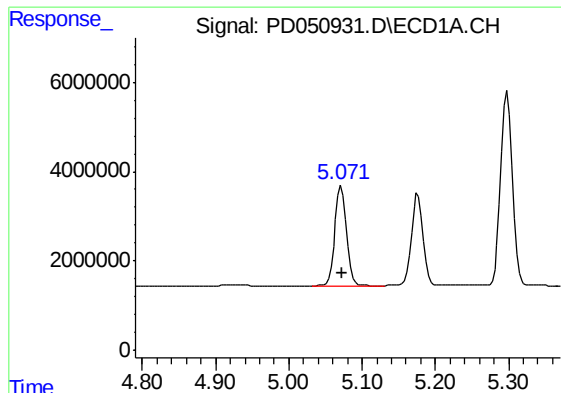

#10 gamma-Chlordane


R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 24792751
Conc: 10.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

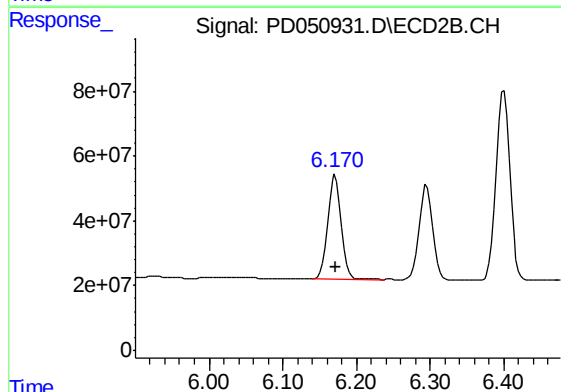


#10 gamma-Chlordane

R.T.: 6.171 min
Delta R.T.: 0.000 min
Response: 413958140
Conc: 11.92 ng/ml

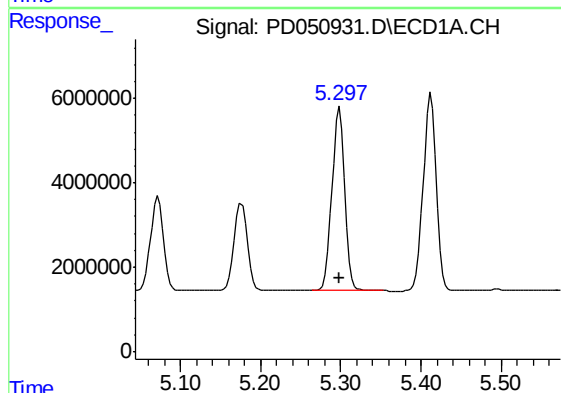


#12 4,4'-DDE

R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 47701039
Conc: 22.10 ng/ml

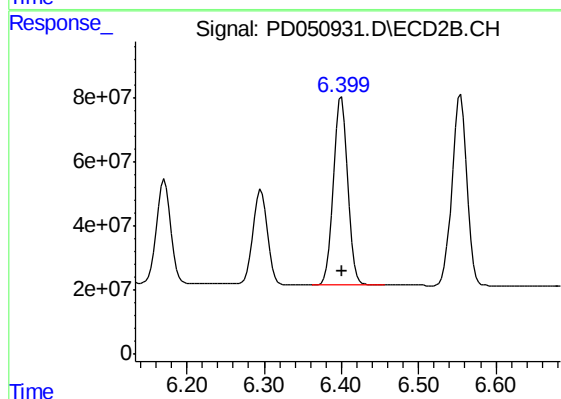

#12 4,4'-DDE


R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 759383050
Conc: 23.03 ng/ml

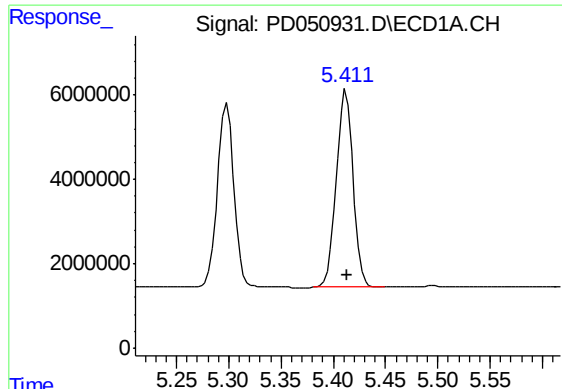

#13 Dielddrin


R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 52486575
Conc: 22.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

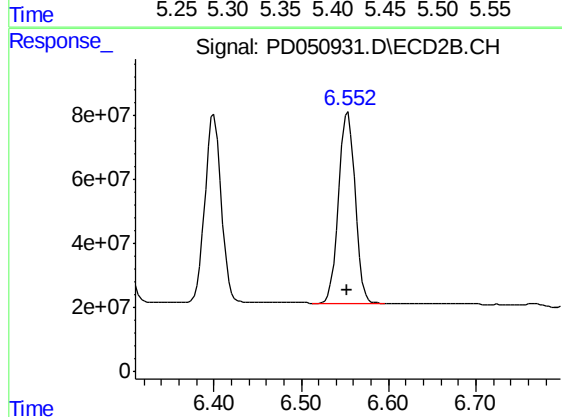


#13 Dielddrin

R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 783001591
Conc: 23.47 ng/ml

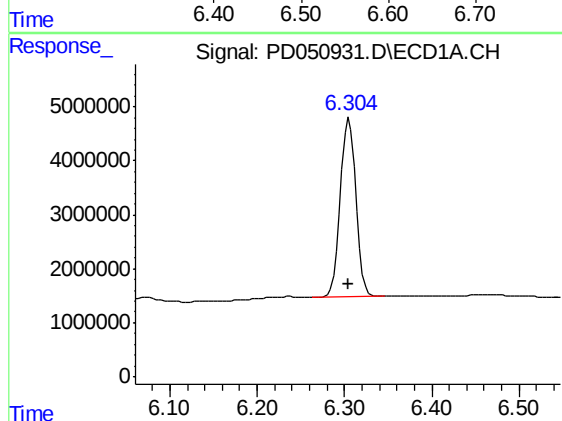


#19 Endosulfan Sulfate

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 40909207
Conc: 20.88 ng/ml

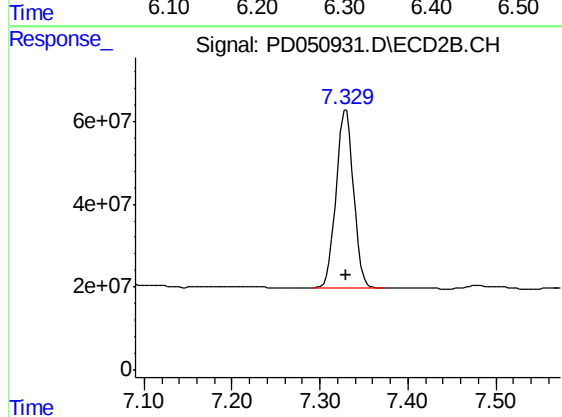

#19 Endosulfan Sulfate


R.T.: 7.330 min
Delta R.T.: 0.000 min
Response: 591453276
Conc: 21.91 ng/ml

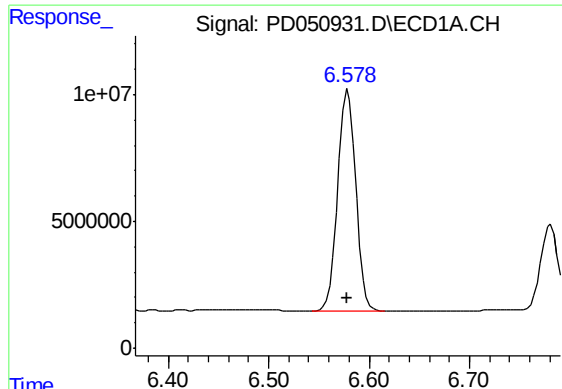

#20 Methoxychlor


R.T.: 6.579 min
Delta R.T.: 0.001 min
Response: 108310772
Conc: 113.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

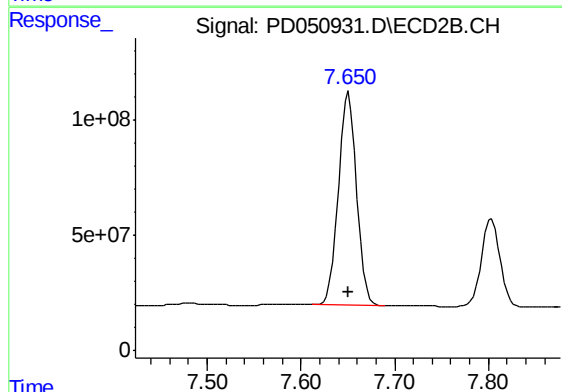


#20 Methoxychlor

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 1249458701
Conc: 102.64 ng/ml

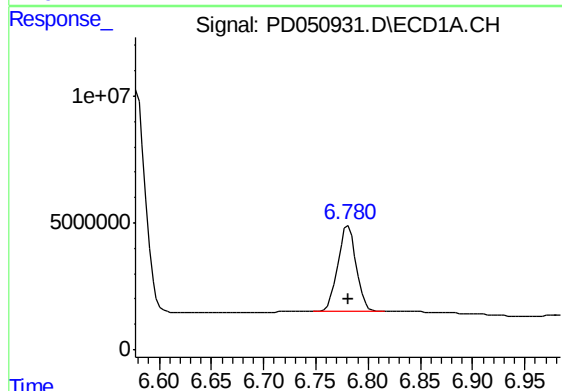


#21 Endrin ketone

R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 41707266
Conc: 19.59 ng/ml

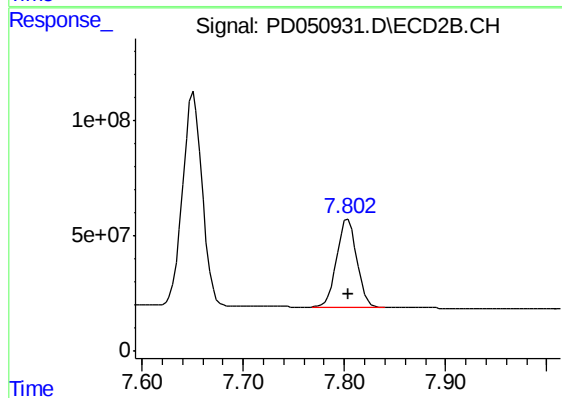

#21 Endrin ketone


R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 519276542
Conc: 20.43 ng/ml

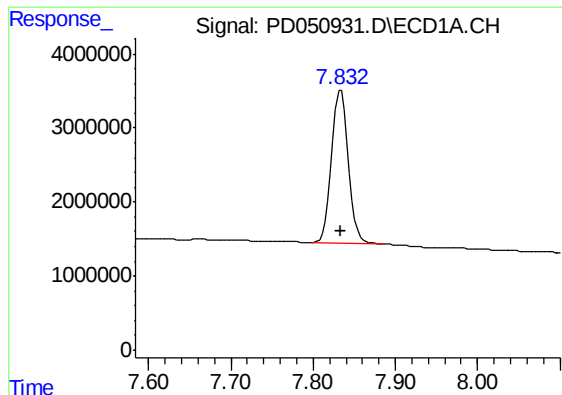

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: 0.000 min
Response: 29290722
Conc: 24.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

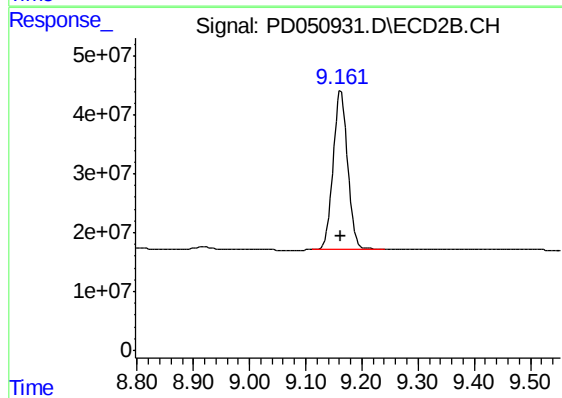

#28 Decachlorobiphenyl

R.T.: 9.163 min
Delta R.T.: 0.000 min
Response: 488027068
Conc: 24.46 ng/ml