

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011020\
 Data File : PD056923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2020 15:52
 Operator : AJ\MA
 Sample : L1067-04MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFAL9MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 23:09:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010920CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 06:39:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.960	17725305	33217107	21.885	22.519
27)	SA Decachlor...	7.954	8.994	33906459	52365492	35.804	35.537
Target Compounds							
3)	MA gamma-BHC...	3.987	4.629	63122595	107.5E6	54.085	53.475
4)	MA Heptachlor	4.273	5.134	59301530	114.5E6	55.234	55.027
5)	MB Aldrin	4.511	5.438	56304525	104.2E6	53.805	54.331
13)	MA Dieldrin	5.518	6.432	117.5E6	213.5E6	114.127	113.270
14)	MA Endrin	5.769	6.649	100.7E6	177.2E6	116.702	115.551
17)	MA 4,4'-DDT	6.139	7.069	87795778	162.6E6	122.822	114.800

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011020\
Data File : PD056923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2020 15:52
Operator : AJ\MA
Sample : L1067-04MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 23:09:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010920CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 06:39:54 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

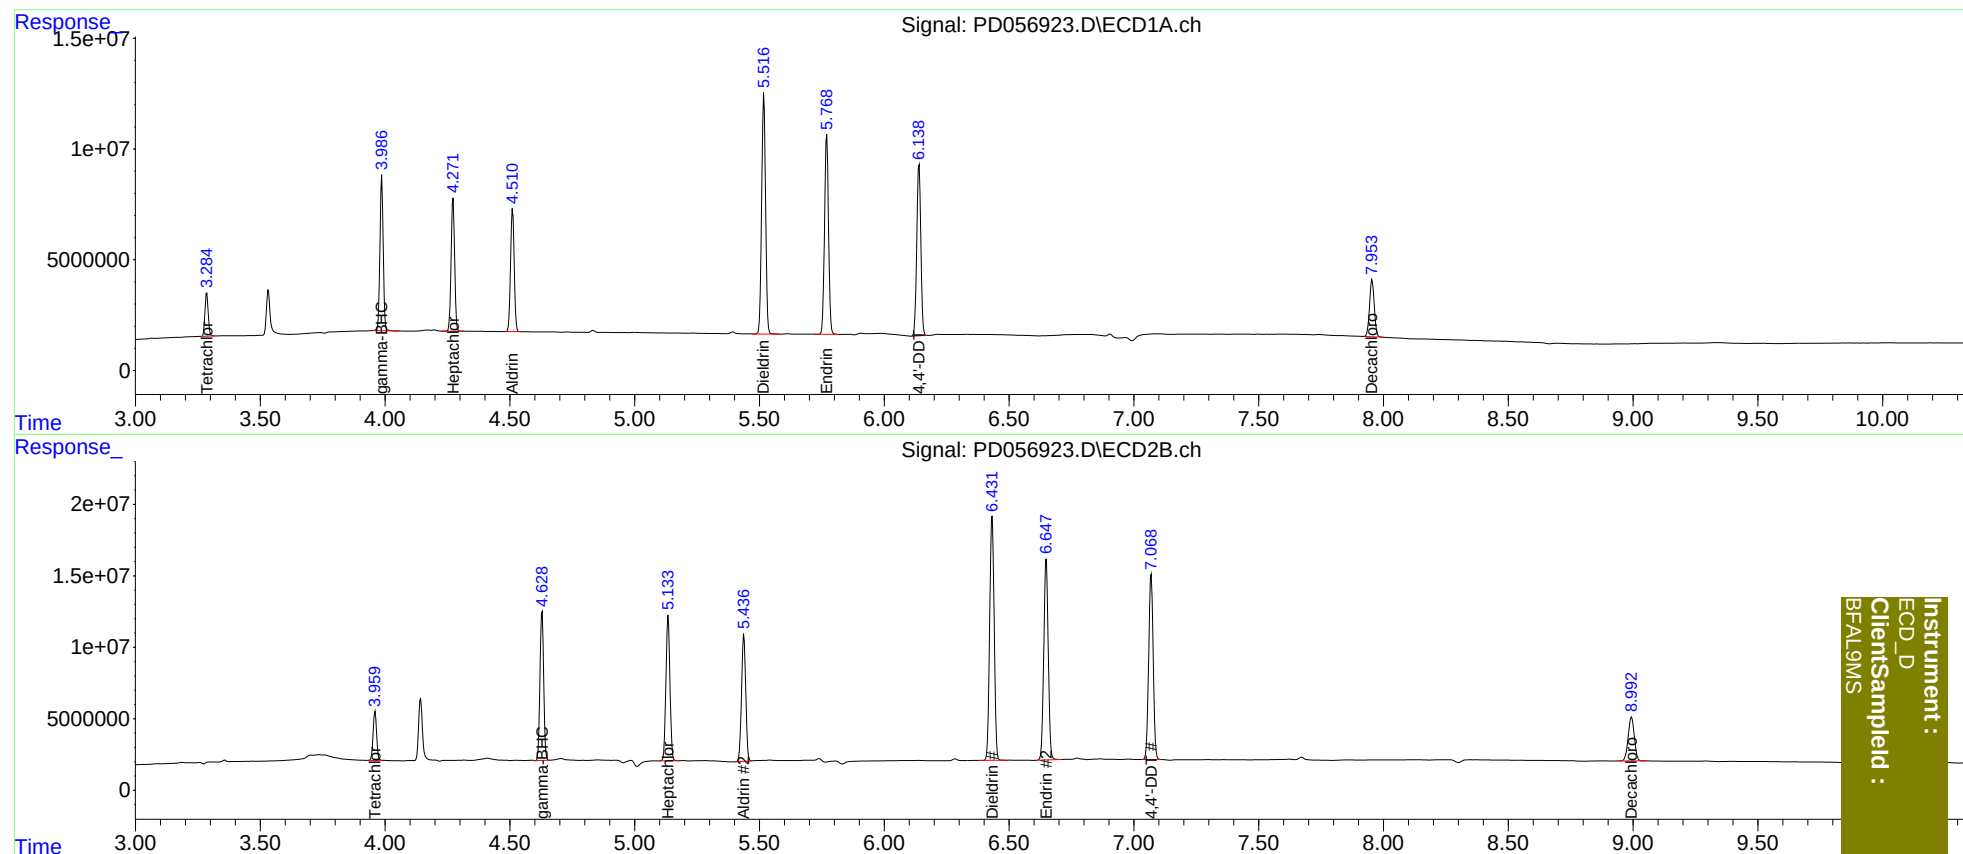

Instrument :
ECD_D
ClientSampled :
BFAL9MS