

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
 Data File : PD067656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 11:47
 Operator : AR\AJ
 Sample : N1035-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 QUARTERLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/11/2022
 Supervised By :Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:57:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.435	3.958	51962341	111.3E6	28.594m	16.863m#
28) SA Decachlor...	8.156	9.010	16936244	104.4E6	19.066m	21.960m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
Data File : PD067656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 11:47
Operator : AR\AJ
Sample : N1035-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
QUARTERLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2022
Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:57:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

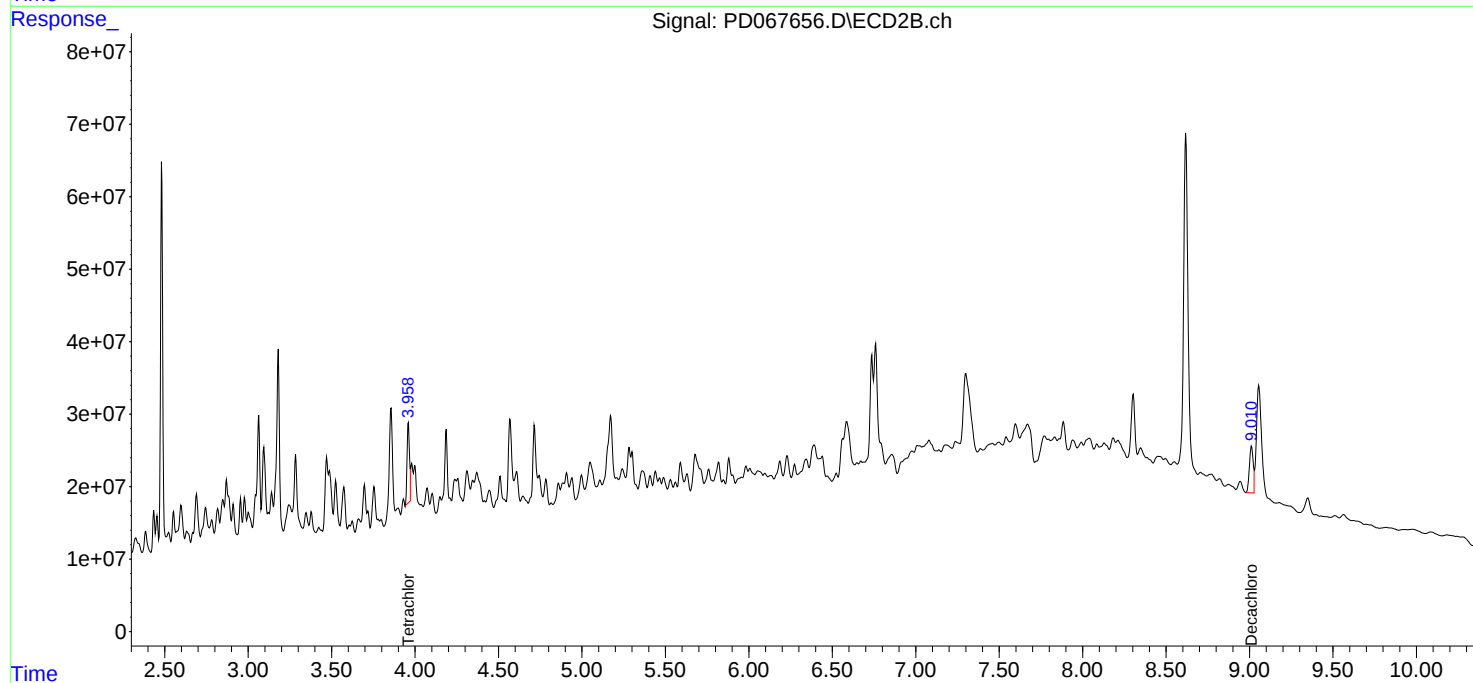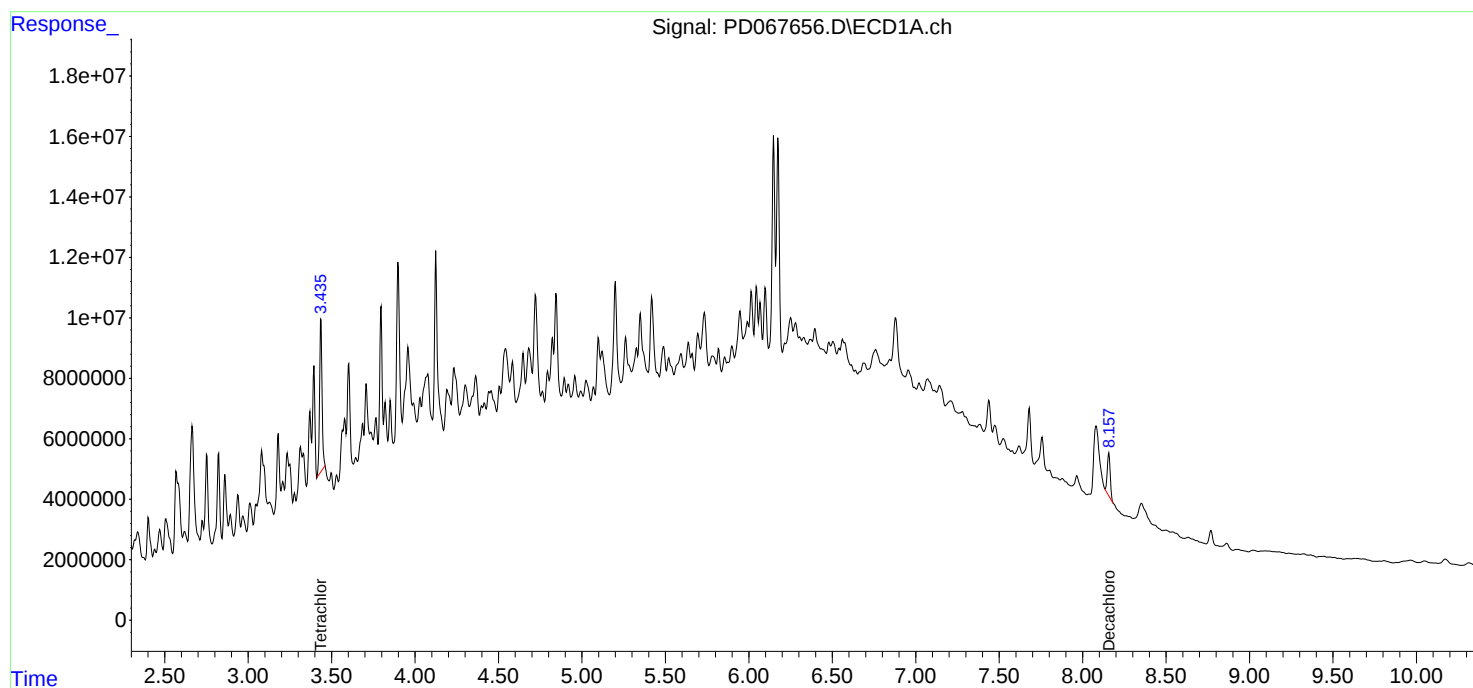

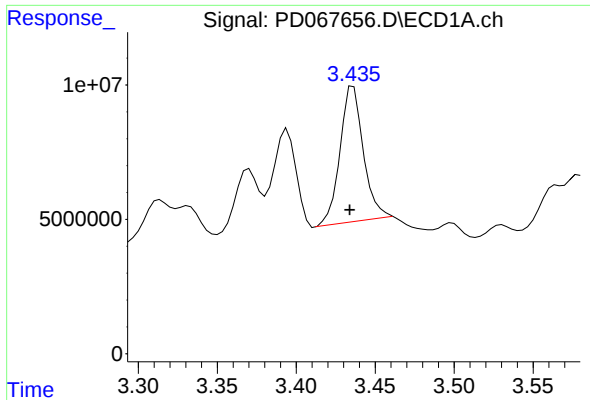


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 51962341
Conc: 28.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
QUARTERLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

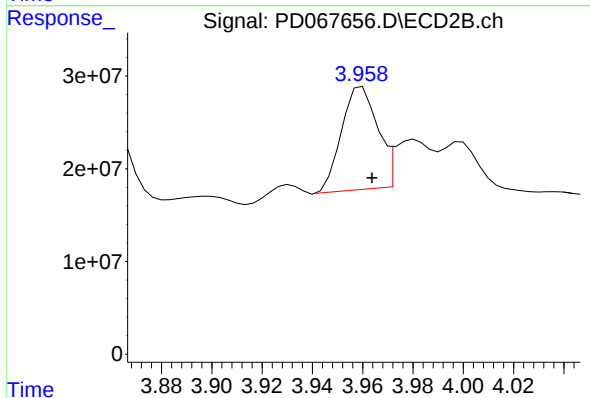


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: -0.005 min
Response: 111267174
Conc: 16.86 ng/ml m

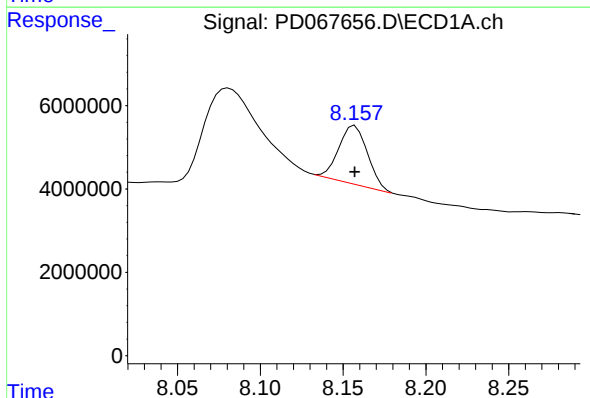

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.000 min
Response: 16936244
Conc: 19.07 ng/ml m

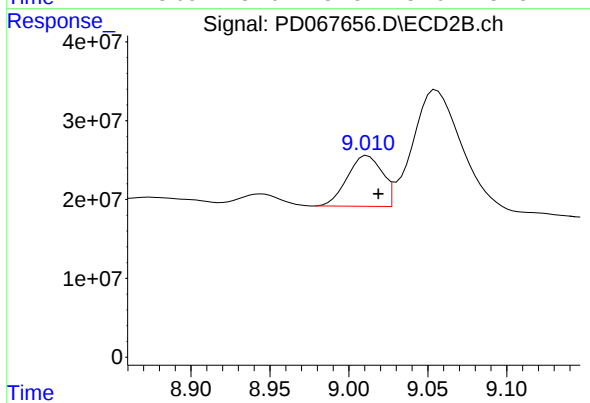

#28 Decachlorobiphenyl

R.T.: 9.010 min
Delta R.T.: -0.008 min
Response: 104366035
Conc: 21.96 ng/ml m