

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
 Data File : PD067658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 12:51
 Operator : AR\AJ
 Sample : N1071-02DL 50X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FM-E1-01-4.5DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/11/2022
 Supervised By :Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:58:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
11) B	alpha-Chl...	5.414	6.137	1214845	11560038	0.502 1.783 #
12) B	4,4'-DDE	5.577	6.296	2321564	7444556	1.049m 1.209m
16) A	4,4'-DDD	6.093	6.792	35009515	99166538	20.378 19.810
17) MA	4,4'-DDT	6.332	7.089	777.5E6	1939.6E6	475.836 362.483

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
Data File : PD067658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 12:51
Operator : AR\AJ
Sample : N1071-02DL 50X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2022
Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:58:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

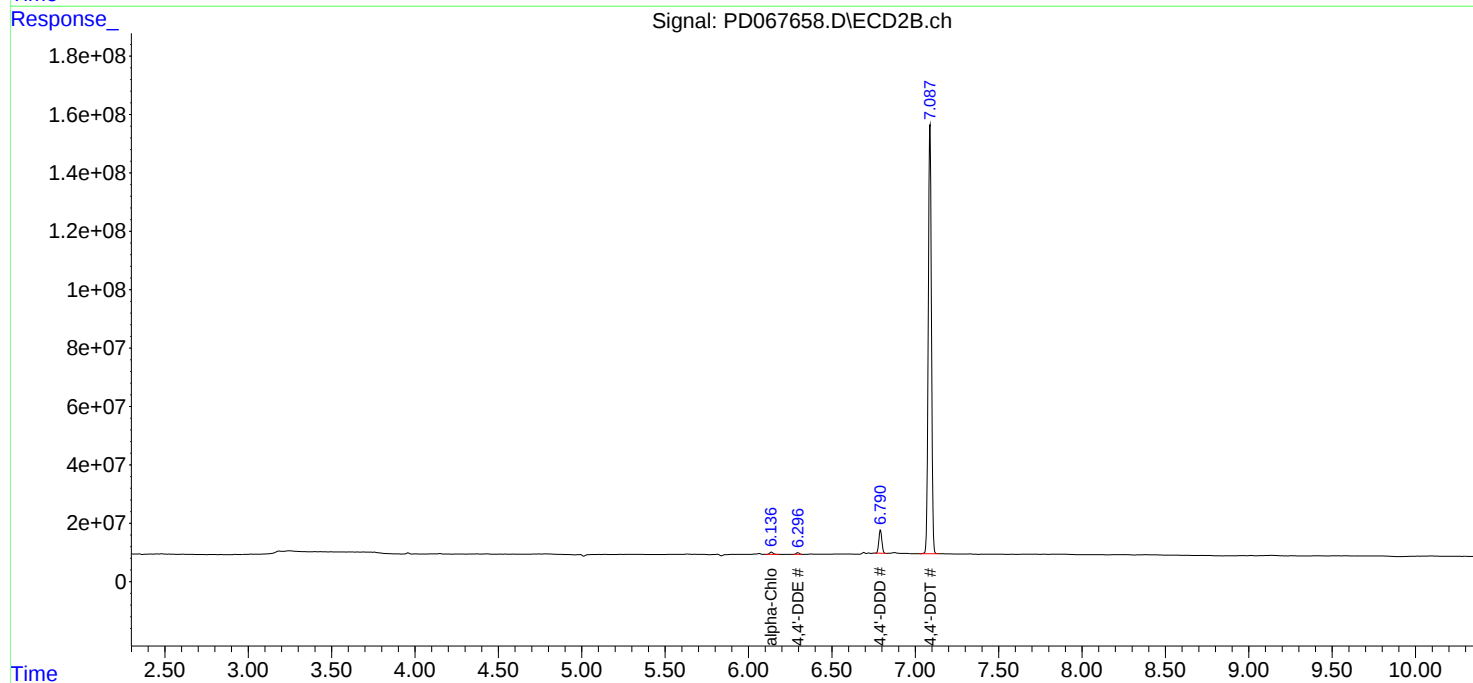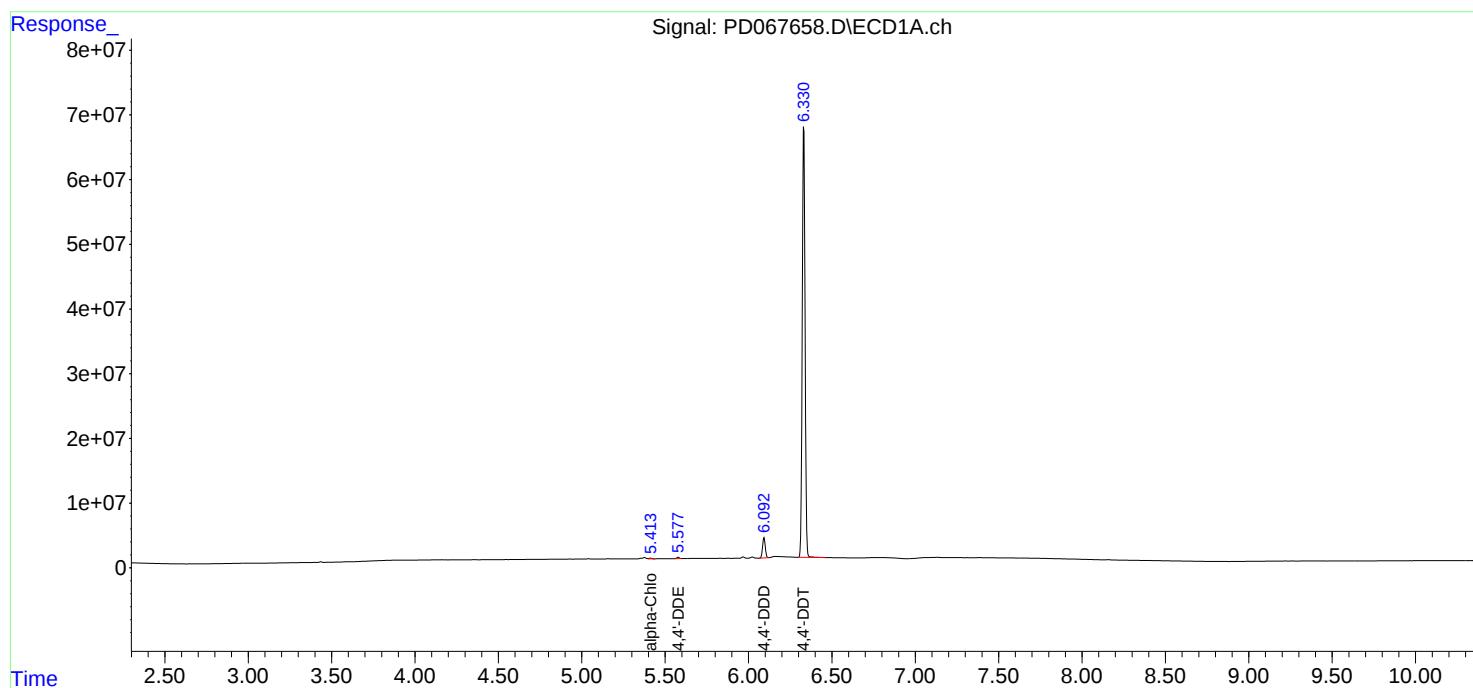

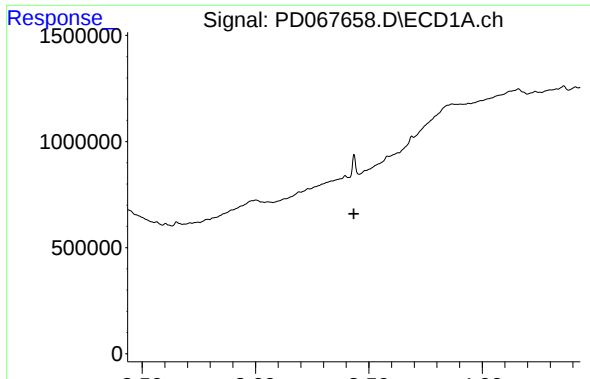


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

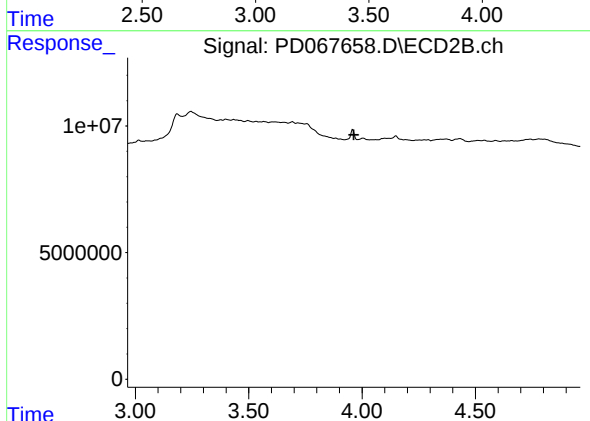


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.964 min
Response: 0
Conc: N.D.

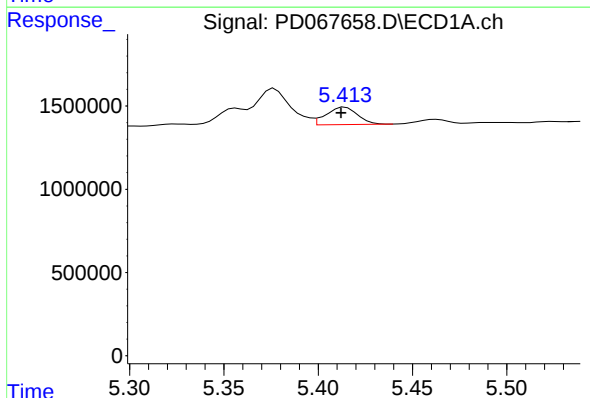


#11 alpha-Chlordane

R.T.: 5.414 min
Delta R.T.: 0.002 min
Response: 1214845
Conc: 0.50 ng/ml

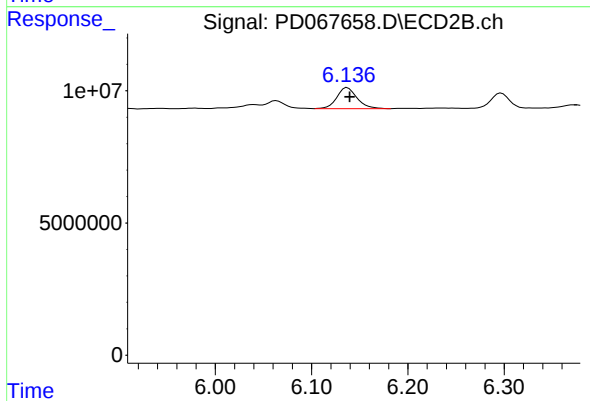

#11 alpha-Chlordane

R.T.: 6.137 min
Delta R.T.: -0.002 min
Response: 11560038
Conc: 1.78 ng/ml

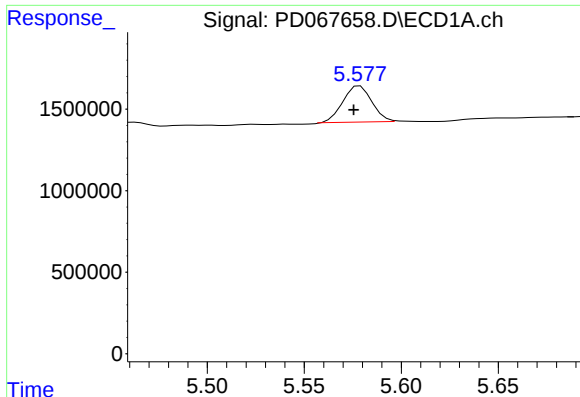


#12 4,4'-DDE

R.T.: 5.577 min
Delta R.T.: 0.002 min
Response: 2321564
Conc: 1.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

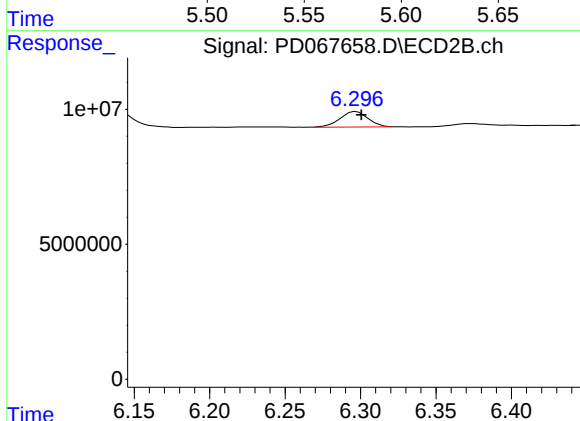


#12 4,4'-DDE

R.T.: 6.296 min
Delta R.T.: -0.005 min
Response: 7444556
Conc: 1.21 ng/ml m

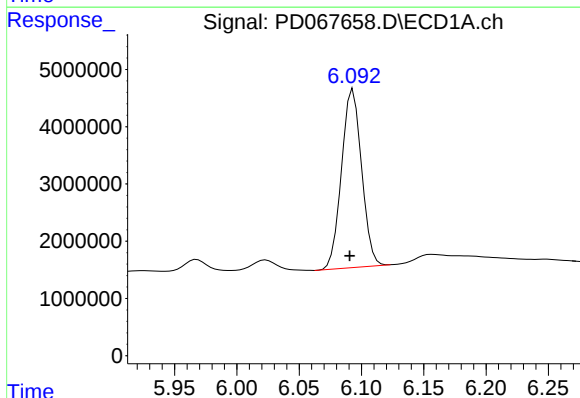


#16 4,4'-DDD

R.T.: 6.093 min
Delta R.T.: 0.003 min
Response: 35009515
Conc: 20.38 ng/ml

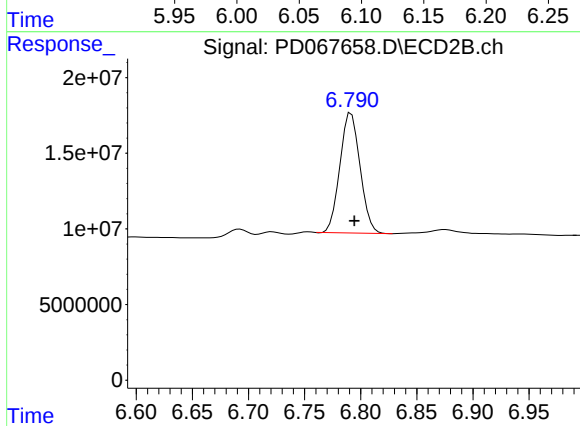

#16 4,4'-DDD

R.T.: 6.792 min
Delta R.T.: -0.003 min
Response: 99166538
Conc: 19.81 ng/ml

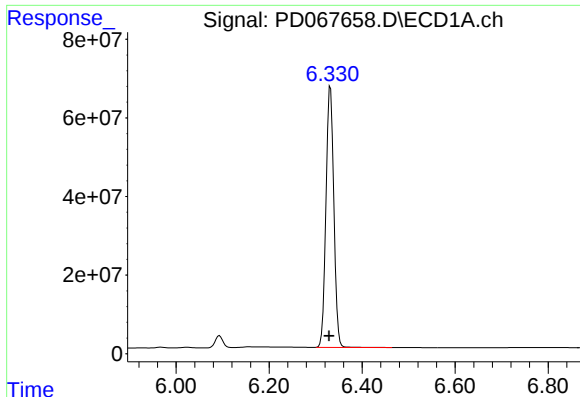


#17 4,4'-DDT

R.T.: 6.332 min
Delta R.T.: 0.003 min
Response: 777522841
Conc: 475.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

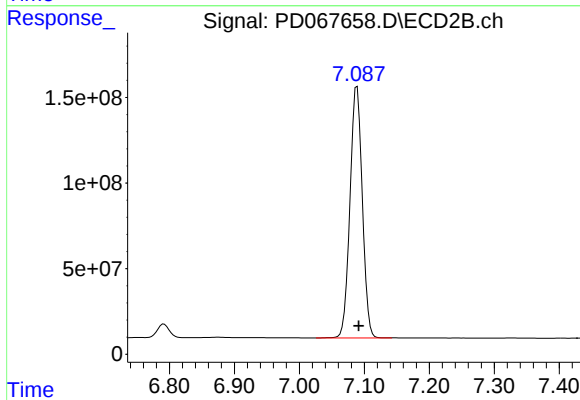


#17 4,4'-DDT

R.T.: 7.089 min
Delta R.T.: -0.003 min
Response: 1939622747
Conc: 362.48 ng/ml

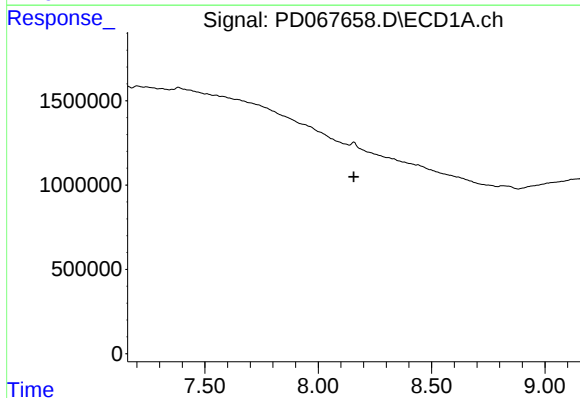

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.

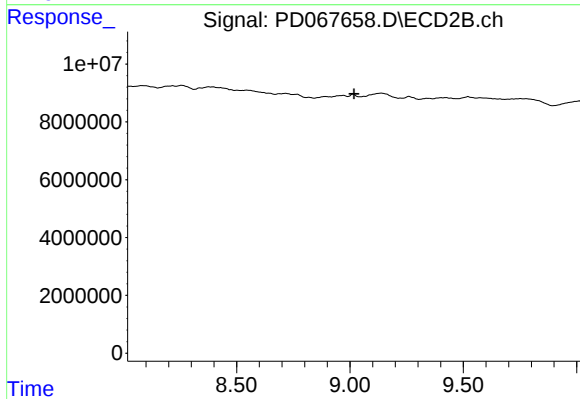

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.019 min
Response: 0
Conc: N.D.