

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
 Data File : PD067659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2022 13:20
 Operator : AR\AJ
 Sample : N1071-02DL2 500X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FM-E1-01-4.5DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/11/2022
 Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:58:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
16) A	4,4'-DDD	6.093	6.791	5763140	16694714	3.355 3.335
17) MA	4,4'-DDT	6.331	7.087	77280106	235.8E6	47.295m 44.064m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011022\
Data File : PD067659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2022 13:20
Operator : AR\AJ
Sample : N1071-02DL2 500X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/11/2022
Supervised By : Ankita Jodhani 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:58:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

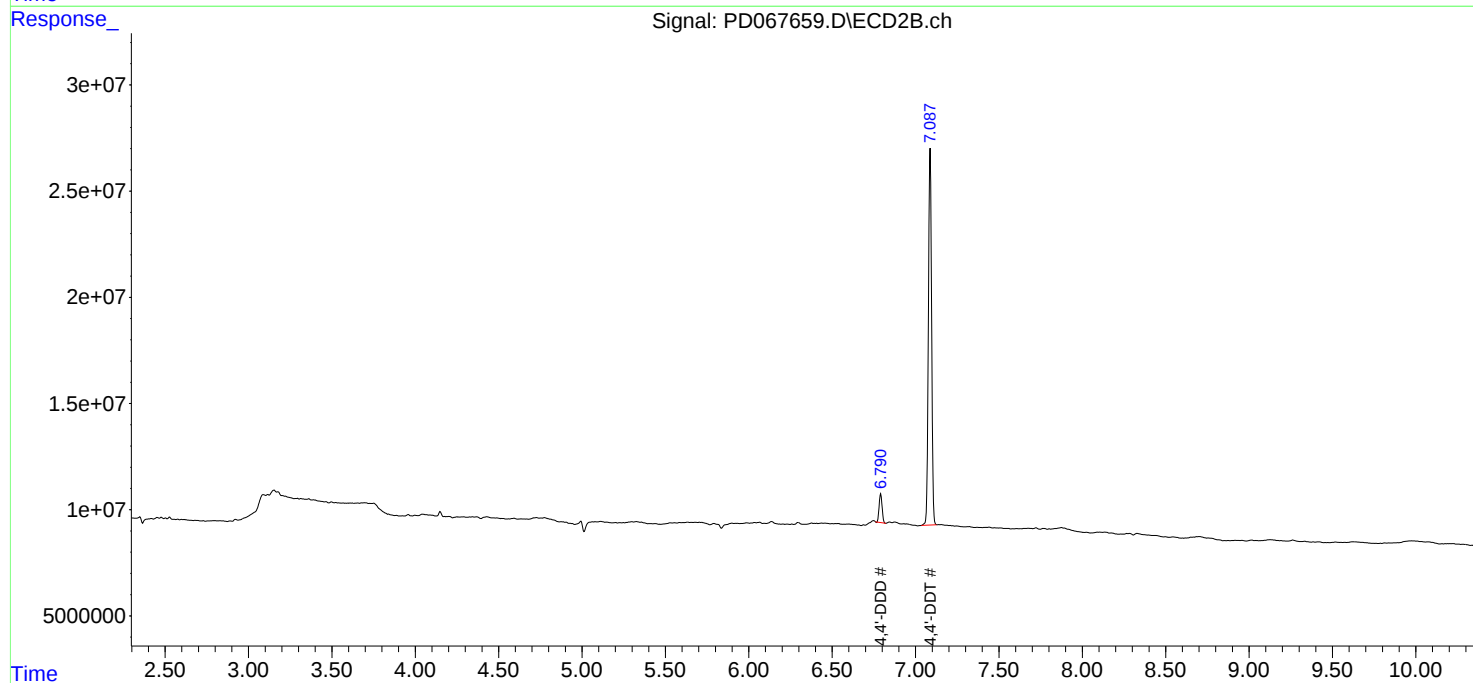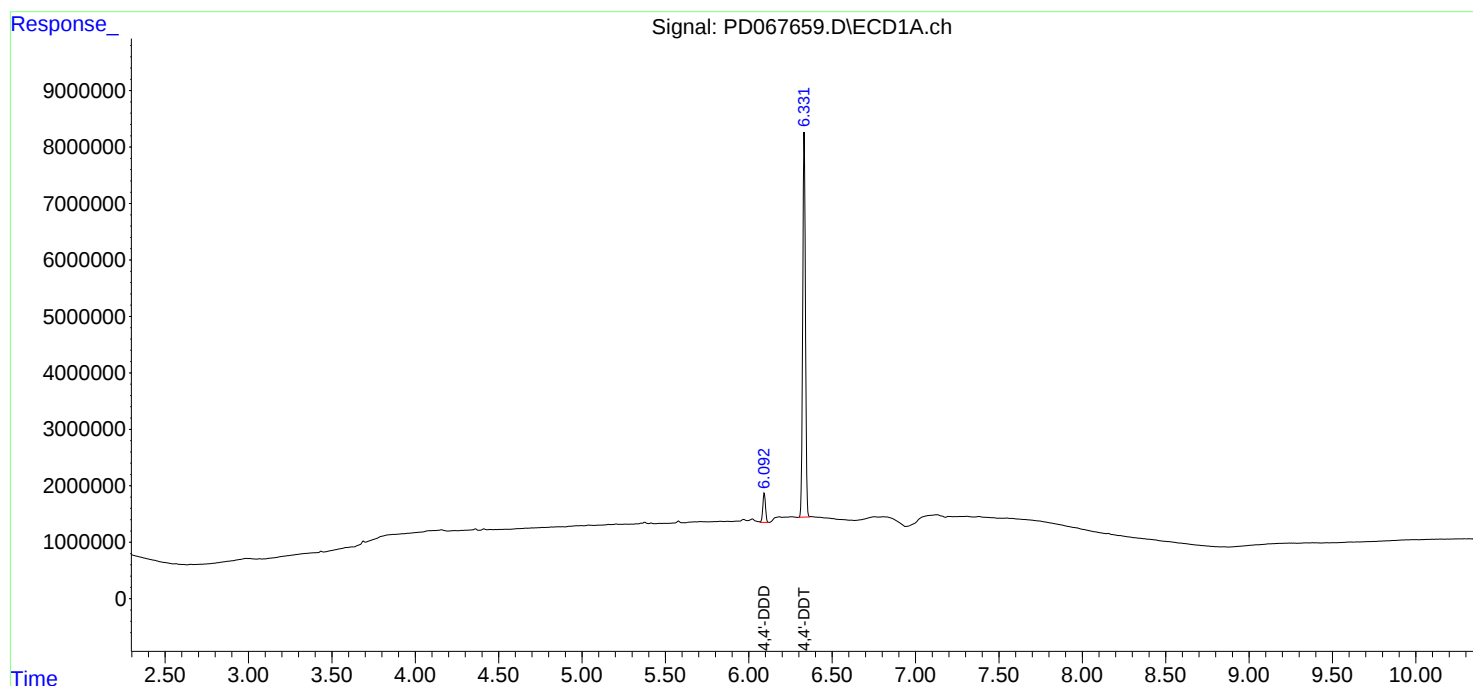

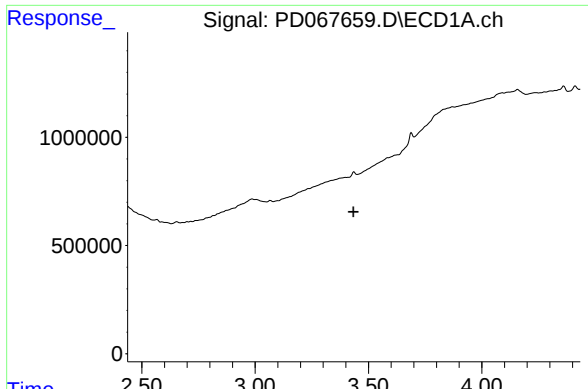


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

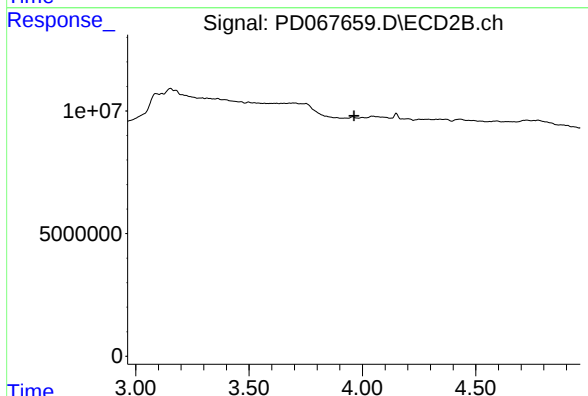


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.964 min
Response: 0
Conc: N.D.

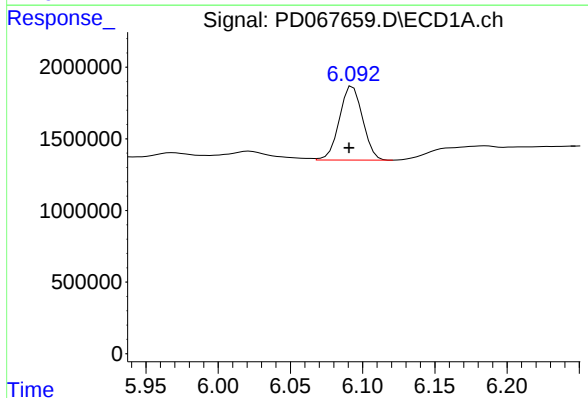


#16 4,4'-DDD

R.T.: 6.093 min
Delta R.T.: 0.003 min
Response: 5763140
Conc: 3.35 ng/ml

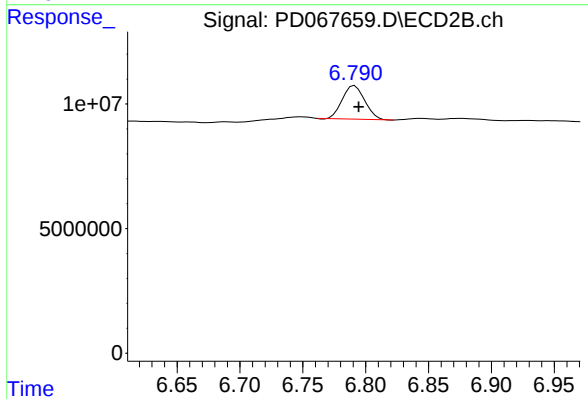

#16 4,4'-DDD

R.T.: 6.791 min
Delta R.T.: -0.003 min
Response: 16694714
Conc: 3.34 ng/ml

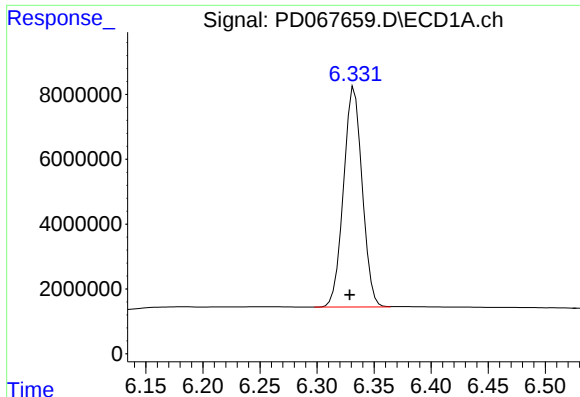


#17 4,4'-DDT

R.T.: 6.331 min
Delta R.T.: 0.002 min
Response: 77280106
Conc: 47.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
FM-E1-01-4.5DL2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/11/2022
Supervised By :Ankita Jodhani 01/13/2022

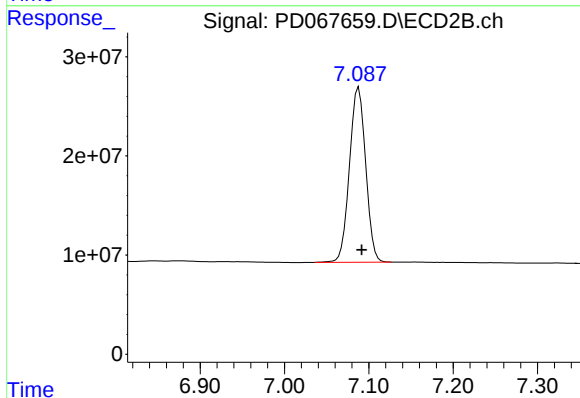


#17 4,4'-DDT

R.T.: 7.087 min
Delta R.T.: -0.005 min
Response: 235781709
Conc: 44.06 ng/ml m

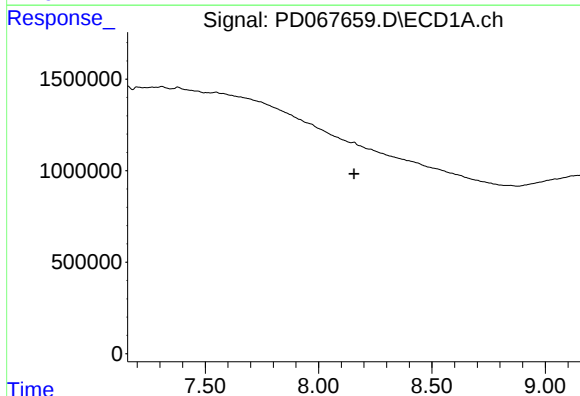

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.

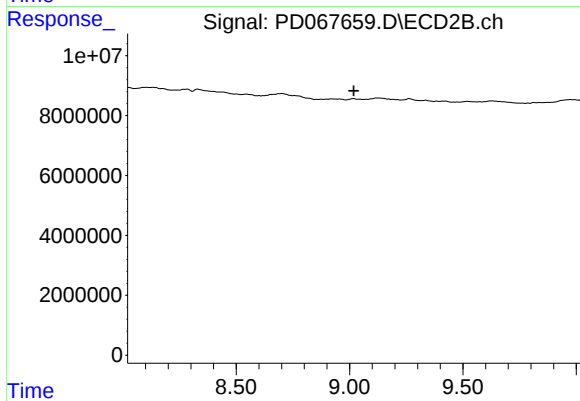

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.019 min
Response: 0
Conc: N.D.