

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
 Data File : PD080729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2024 09:09
 Operator : AR\AJ
 Sample : RESC017
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 14:17:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.797	28220065	49236288	19.831	19.282
2)	SA Decachlor...	9.121	7.942	76297989	102.0E6	38.847	38.137
Target Compounds							
2)	A alpha-BHC	4.023	3.300	23242409	39355441	9.869	9.620
3)	MA gamma-BHC...	4.358	3.629	22674953	37049953	9.904	9.709
4)	MA Heptachlor	4.951	3.971	24150747	36597100	9.989	9.908
5)	MB Aldrin	5.295	4.252	23268506	37067312	10.279	10.133
6)	B beta-BHC	4.552	3.925	10854204	17539548	10.526	9.942
7)	B delta-BHC	4.801	4.156	23828223	38159891	9.989	9.696
8)	B Heptachlo...	5.722	4.754	22121639	34164471	10.157	9.949
9)	A Endosulfan I	6.109	5.124	21223827	32291048	10.000	10.039
10)	B trans-Chl...	5.978	5.004	20743375	32742314	10.056	9.832
11)	B cis-Chlor...	6.058	5.068	21495629	33595363	10.129	9.781
12)	B 4,4'-DDE	6.229	5.257	38595632	60841291	19.632	19.316
13)	MA Dieldrin	6.385	5.389	43193844	68715708	19.352	19.418
14)	MA Endrin	6.615	5.664	35372459	58100753	19.426	19.574
15)	B Endosulfa...	6.834	5.957	40366558	58470769	20.629	19.700
16)	A 4,4'-DDD	6.747	5.811	32253215	52852618	19.316	19.512
17)	MA 4,4'-DDT	7.062	6.063	33399713	51063475	19.694	18.968
18)	B Endrin al...	6.964	6.137	29590762	45713301	20.548	20.413
19)	B Endosulfa...	7.199	6.360	36029603	55139569	20.117	19.704
20)	A Methoxychlor	7.537	6.638	91710349	144.6E6	99.296	102.163
21)	B Endrin ke...	7.686	6.866	40557421	64393995	20.644	20.466

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
Data File : PD080729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 09:09
Operator : AR\AJ
Sample : RESC017
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 14:17:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

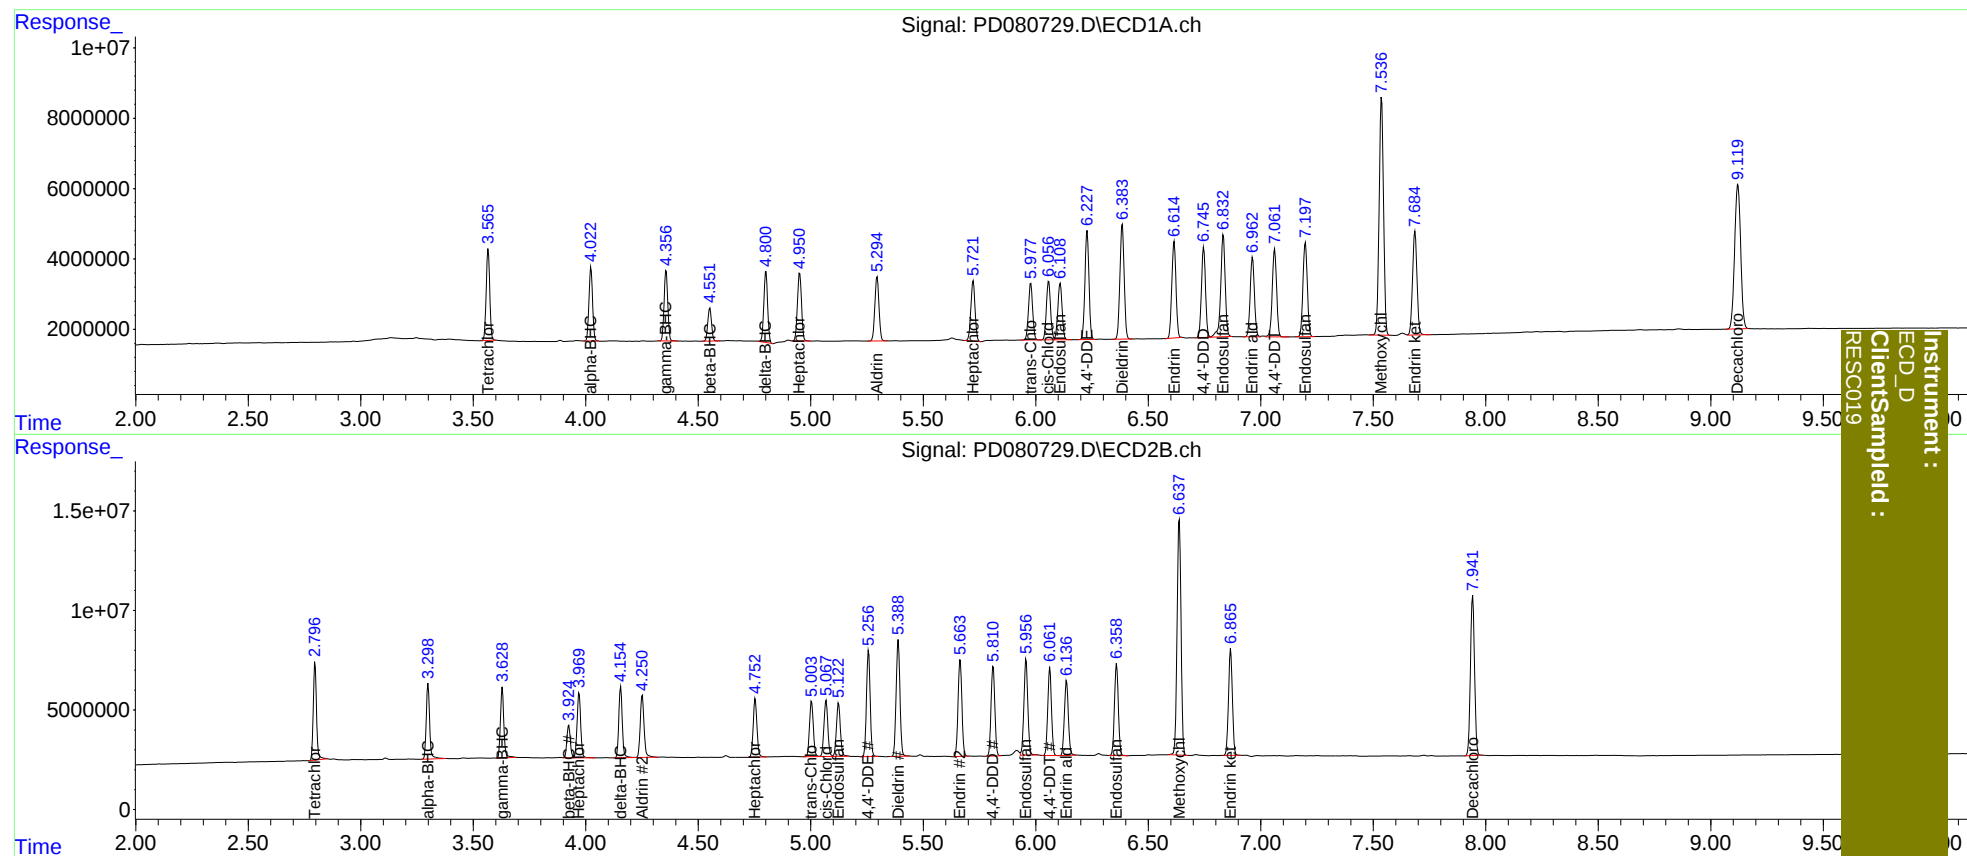

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
Data File : PD080729.D
Acq On : 10 Jan 2024 09:09
Operator : AR\AJ
Sample : RESC017
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Title : GC Extractables
Last Update : Wed Jan 10 14:12:04 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.567	4.023	100.00%
4.023	4.358	100.00%
4.358	4.552	100.00%
4.552	4.801	100.00%
4.801	4.951	100.00%
4.951	5.295	100.00%
5.295	5.722	100.00%
5.722	5.978	100.00%
5.978	6.058	99.70%
6.058	6.109	97.93%
6.109	6.229	100.00%
6.229	6.385	100.00%
6.385	6.615	100.00%
6.615	6.747	100.00%
6.747	6.834	100.00%
6.834	6.964	100.00%
6.964	7.062	100.00%
7.062	7.199	100.00%
7.199	7.537	100.00%
7.537	7.686	100.00%
7.686	9.121	100.00%

Signal #2


2.797	3.300	100.00%
3.300	3.629	100.00%
3.629	3.925	100.00%
3.925	3.971	96.00%
3.971	4.156	100.00%
4.156	4.252	100.00%
4.252	4.754	100.00%
4.754	5.004	100.00%
5.004	5.068	100.00%
5.068	5.124	99.40%
5.124	5.257	100.00%
5.257	5.389	100.00%
5.389	5.664	100.00%
5.664	5.811	100.00%
5.811	5.957	100.00%
5.957	6.063	100.00%
6.063	6.137	100.00%
6.137	6.360	100.00%
6.360	6.638	100.00%
6.638	6.866	100.00%
6.866	7.942	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
Data File : PD080729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 09:09
Operator : AR\AJ
Sample : RESC017
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 14:17:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

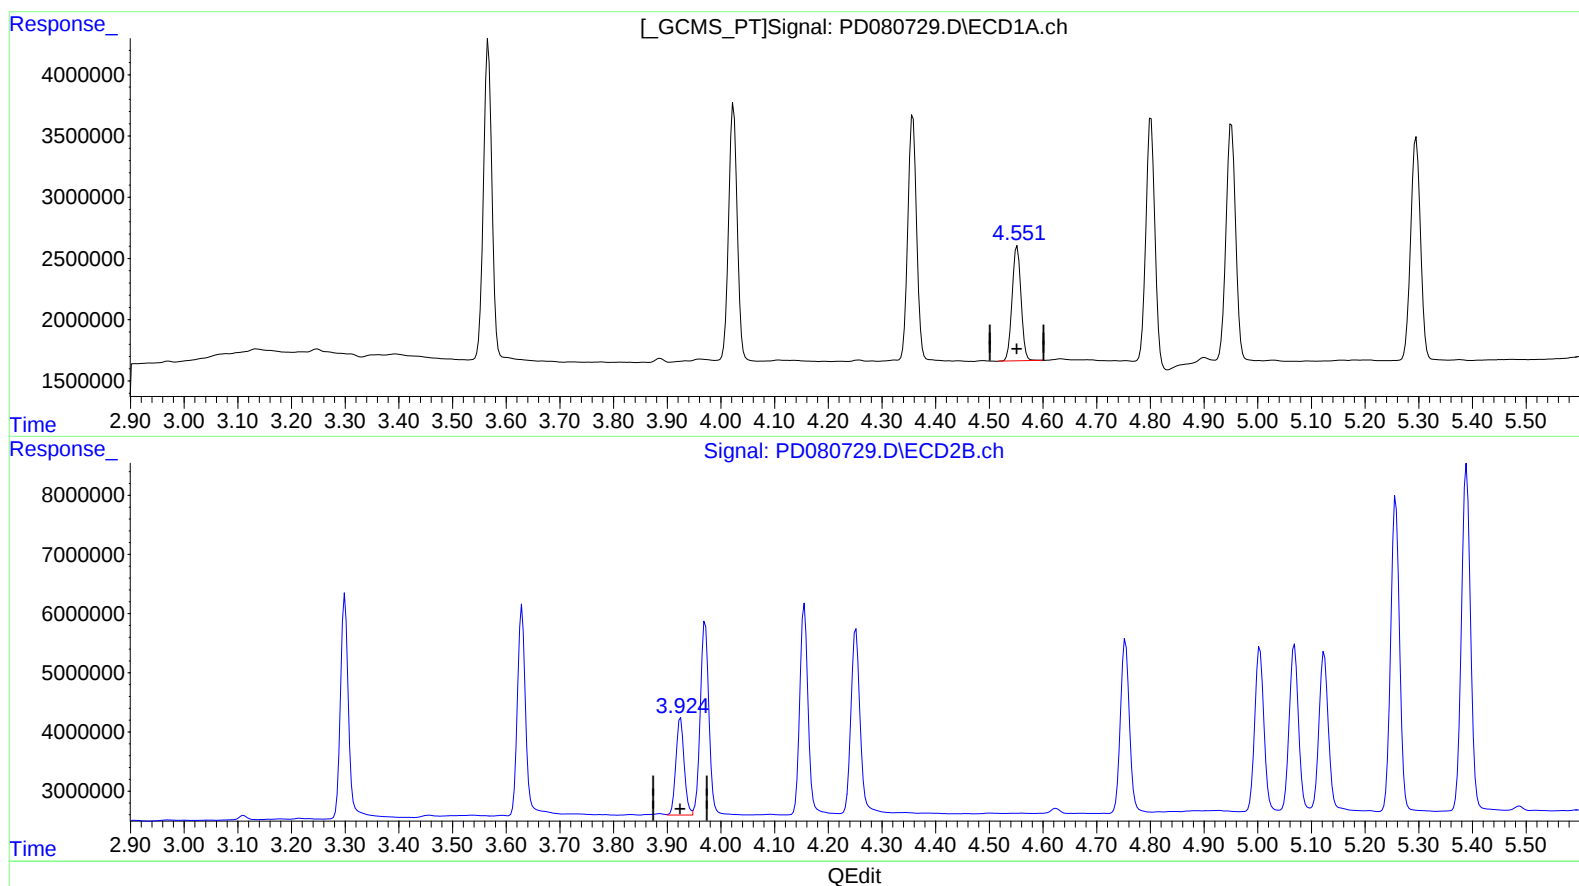

(6) beta-BHC (B)

4.552min 10.526 ng/ml

response 10854204

(6) beta-BHC #2 (B)

3.925min 9.942 ng/ml


response 17539548

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
Data File : PD080729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 09:09
Operator : AR\AJ
Sample : RESC017
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 14:17:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

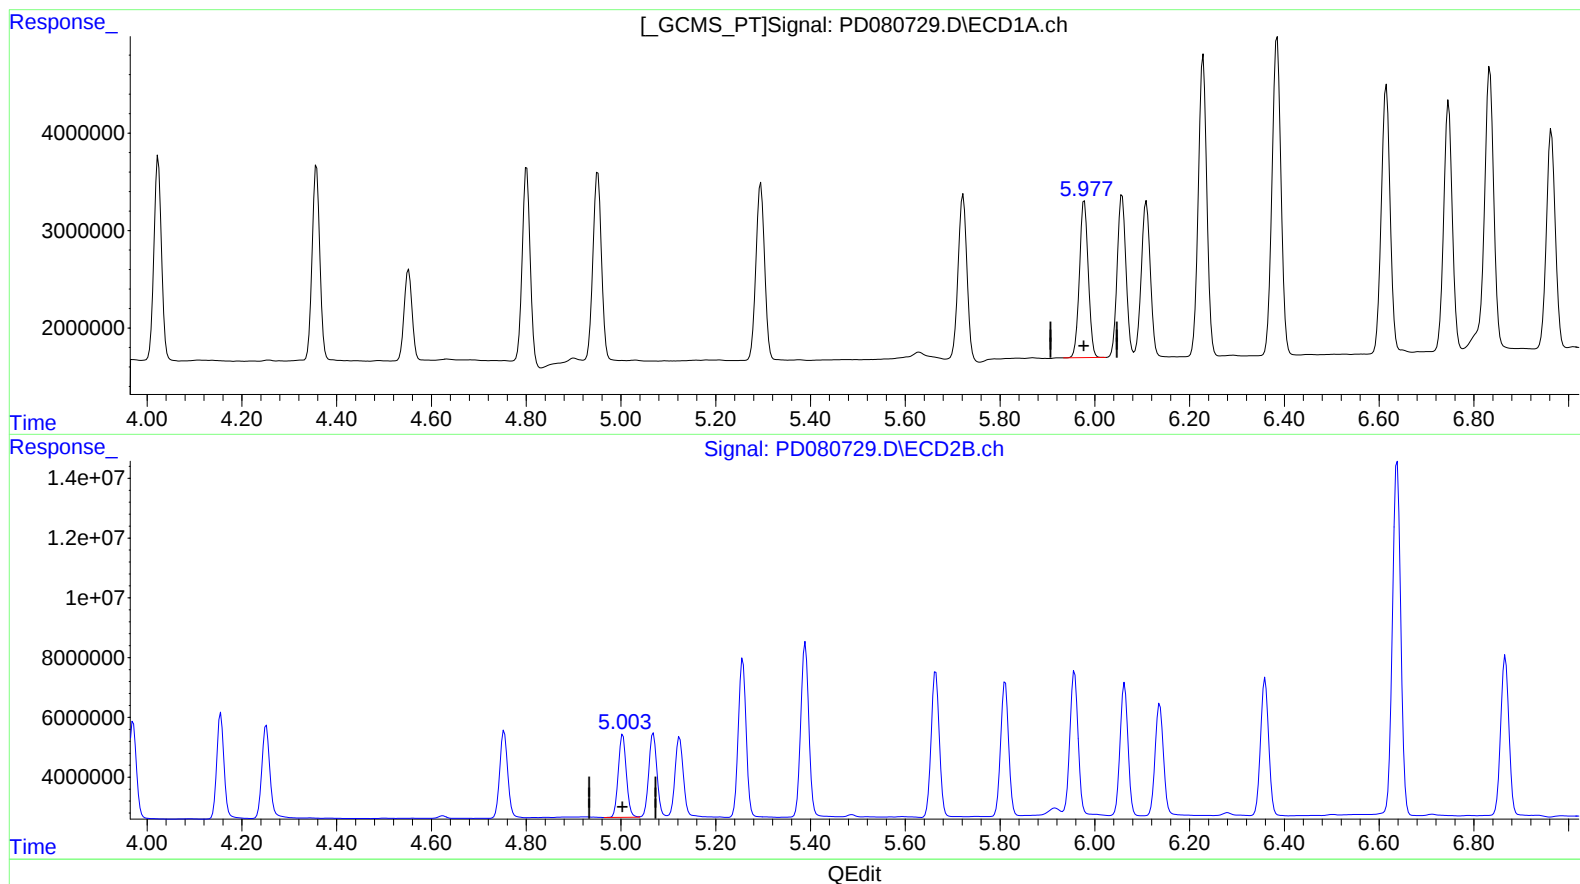

(10) trans-Chlordane (B)

5.978min 10.056 ng/ml

response 20743375

(10) trans-Chlordane #2 (B)

5.004min 9.832 ng/ml


response 32742314

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011024\
Data File : PD080729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 09:09
Operator : AR\AJ
Sample : RESC017
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 14:17:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

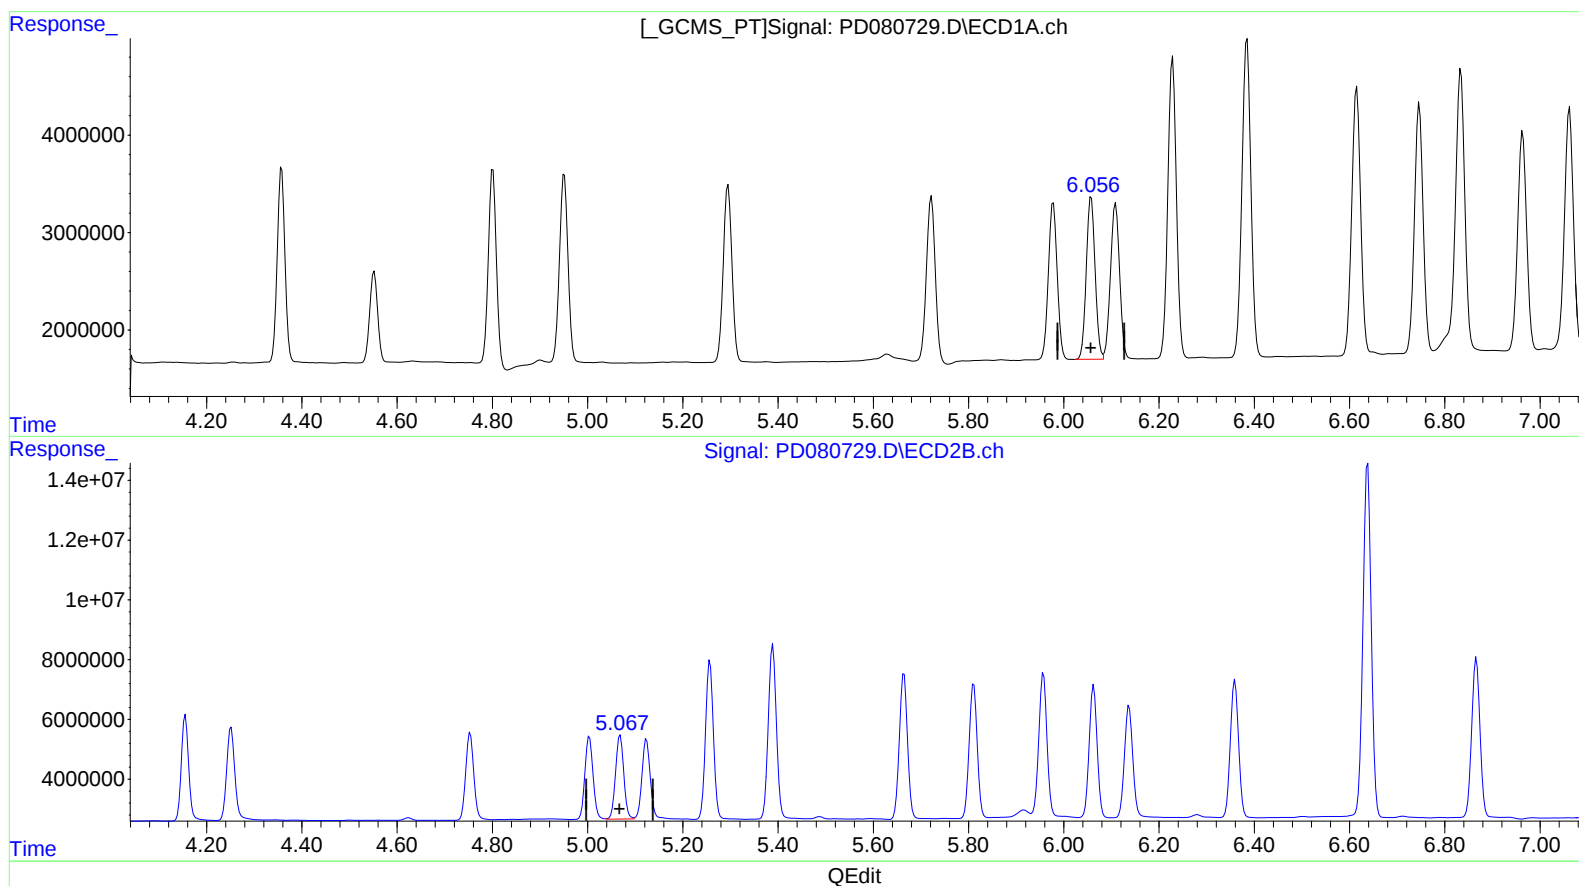

(11) cis-Chlordane (B)

6.058min 10.129 ng/ml

response 21495629

(11) cis-Chlordane #2 (B)

5.068min 9.781 ng/ml

response 33595363