

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
 Data File : PD050965.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2019 4:24
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 08:02:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 03:41:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	0.000	4.444	0	16118667	N.D.	0.354 #
3) MA	gamma-BHC...	0.000	4.736	0	57858265	N.D.	1.392 #
6) B	beta-BHC	0.000	4.902	0	60237930	N.D.	3.329 #
8) B	Heptachlo...	0.000	5.932	0	161.8E6	N.D.	4.640 #
9) A	Endosulfan I	0.000	6.316	0	2383334	N.D.	0.076 #
19) B	Endosulfa...	6.243f	0.000	916093	0	0.468	N.D. #
20) A	Methoxychlor	0.000	7.584f	0	18482253	N.D.	1.518 #
21) B	Endrin ke...	6.755	0.000	288037	0	0.135	N.D. #
24)	Chlordane-2	0.000	5.457	0	4774663	N.D.	3.559 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
Data File : PD050965.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2019 4:24
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 08:02:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 03:41:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

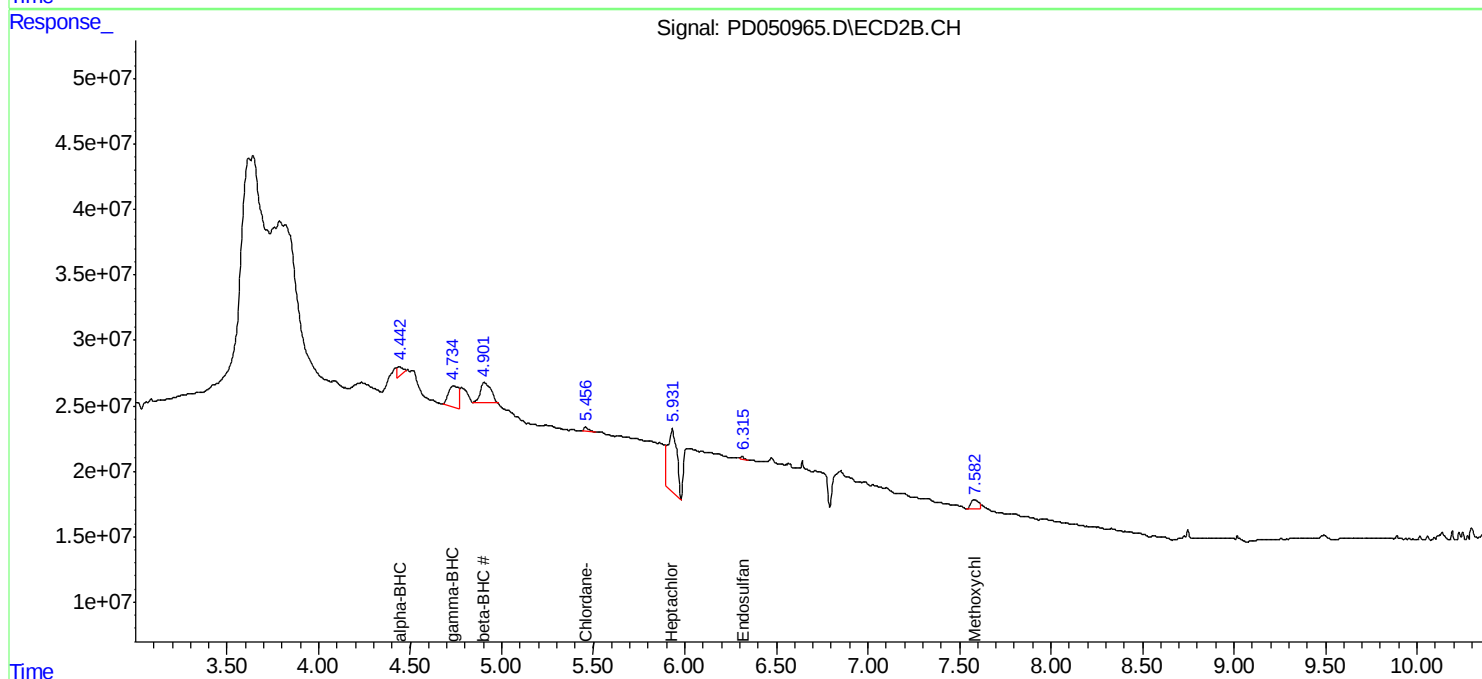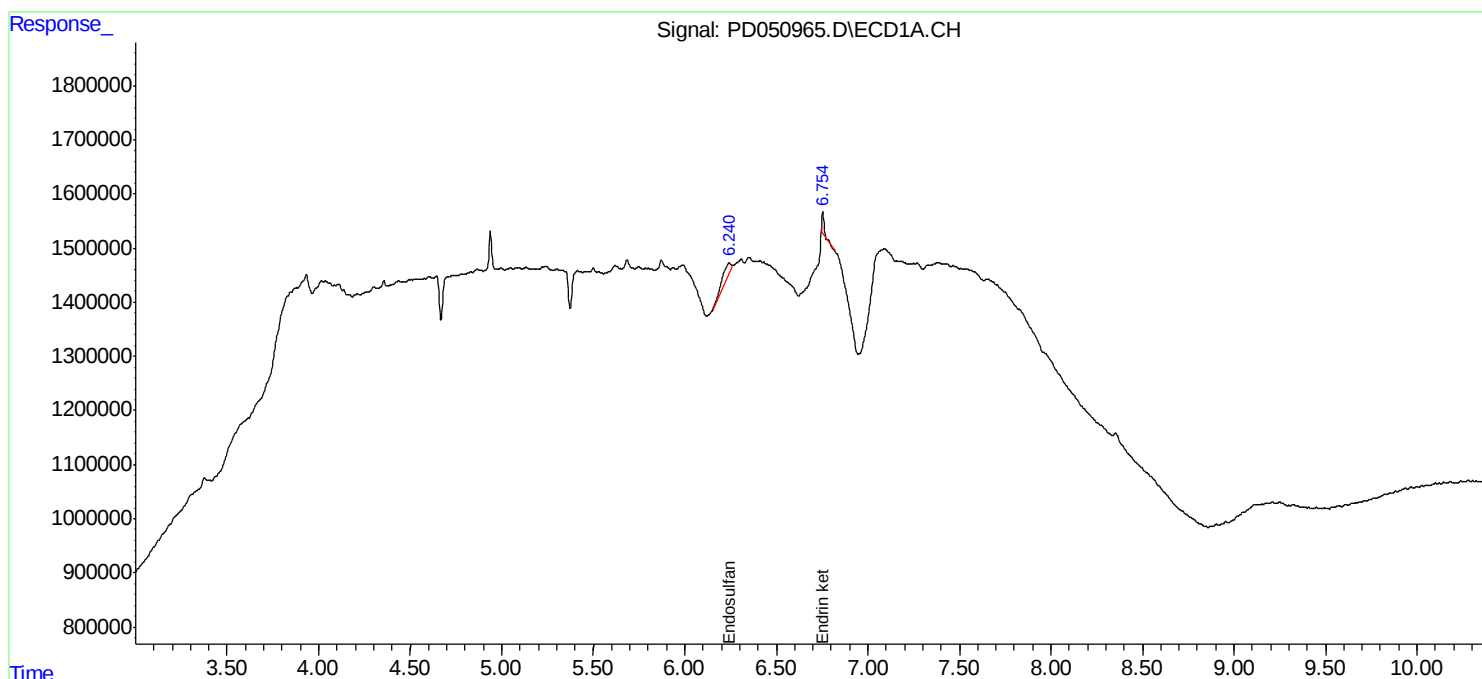


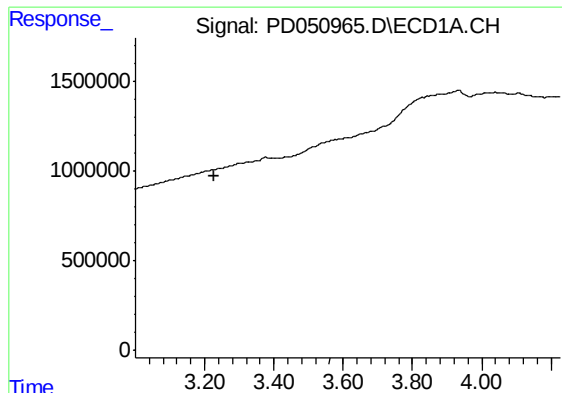

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

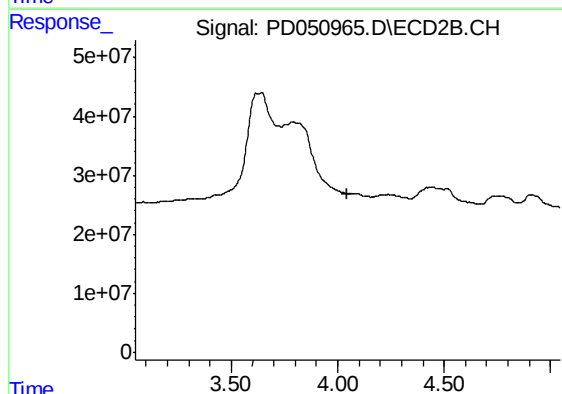


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

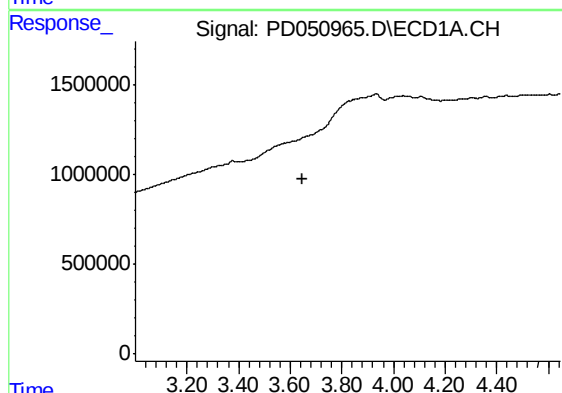


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.648 min
Response: 0
Conc: N.D.

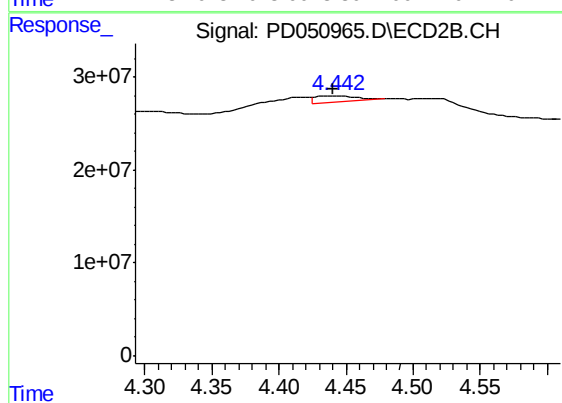

#2 alpha-BHC


R.T.: 4.444 min
Delta R.T.: 0.003 min
Response: 16118667
Conc: 0.35 ng/ml

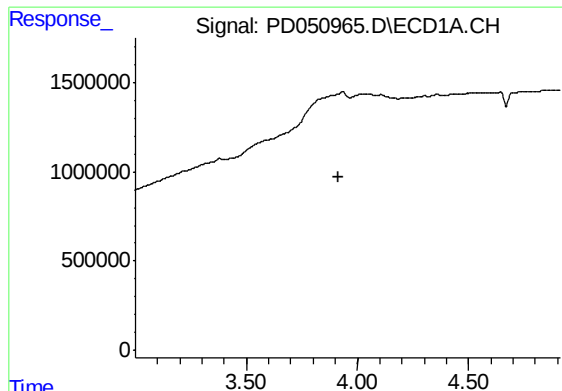

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

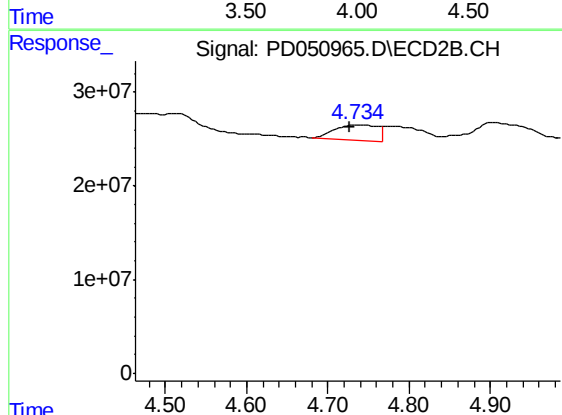


#3 gamma-BHC (Lindane)

R.T.: 4.736 min
Delta R.T.: 0.008 min
Response: 57858265
Conc: 1.39 ng/ml

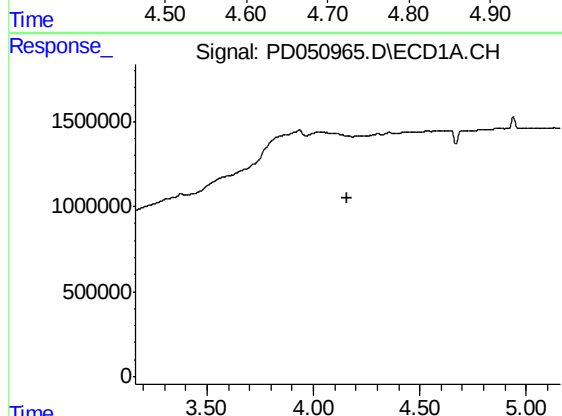


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.161 min
Response: 0
Conc: N.D.

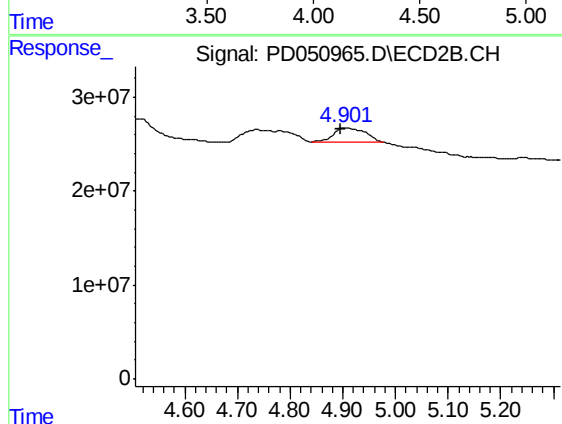

#6 beta-BHC


R.T.: 4.902 min
Delta R.T.: 0.005 min
Response: 60237930
Conc: 3.33 ng/ml

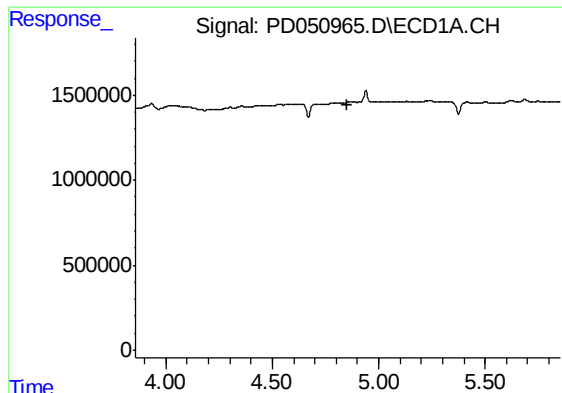

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.855 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

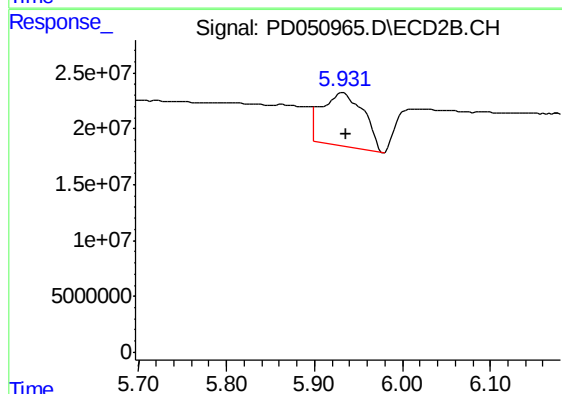


#8 Heptachlor epoxide

R.T.: 5.932 min
Delta R.T.: -0.004 min
Response: 161780966
Conc: 4.64 ng/ml

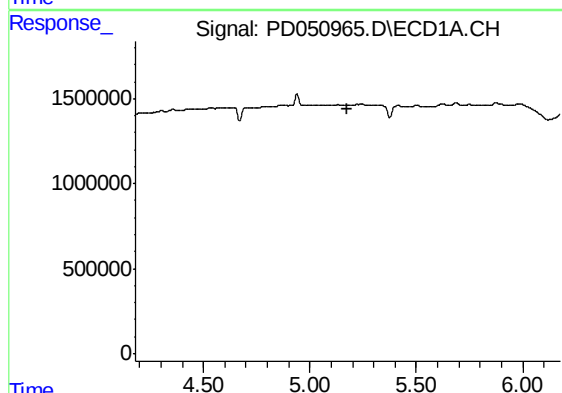


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

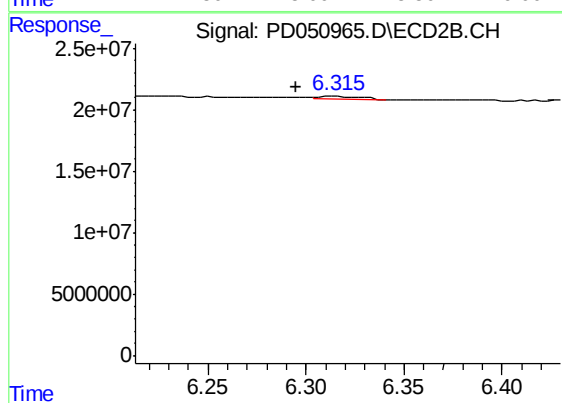

#9 Endosulfan I


R.T.: 6.316 min
Delta R.T.: 0.021 min
Response: 2383334
Conc: 0.08 ng/ml

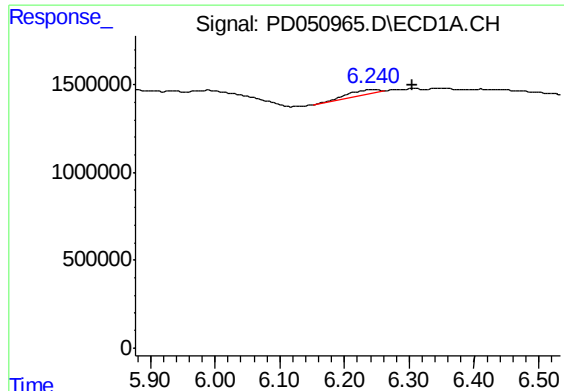

#19 Endosulfan Sulfate


R.T.: 6.243 min
Delta R.T.: -0.063 min
Response: 916093
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

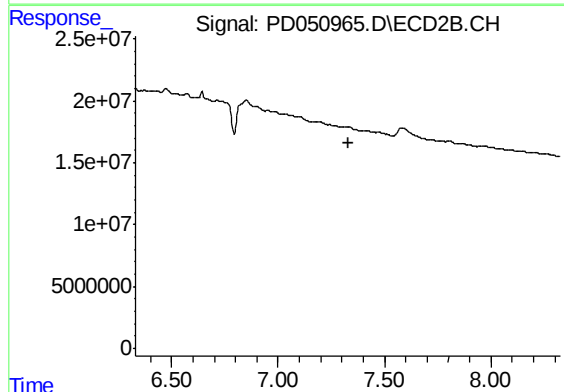


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

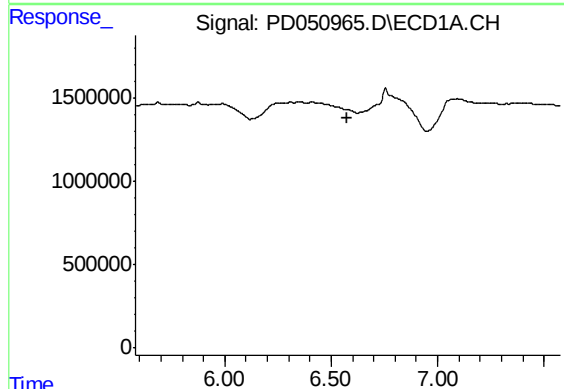


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.578 min
Response: 0
Conc: N.D.

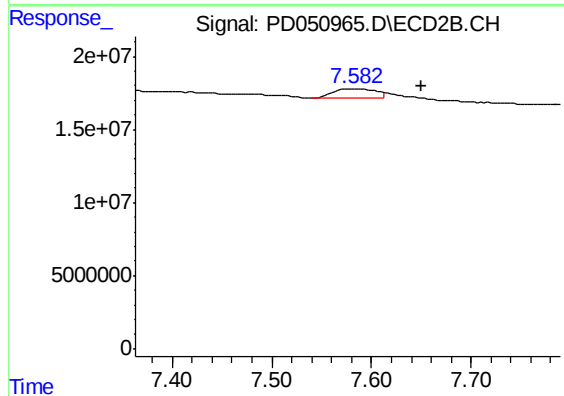

#20 Methoxychlor


R.T.: 7.584 min
Delta R.T.: -0.067 min
Response: 18482253
Conc: 1.52 ng/ml

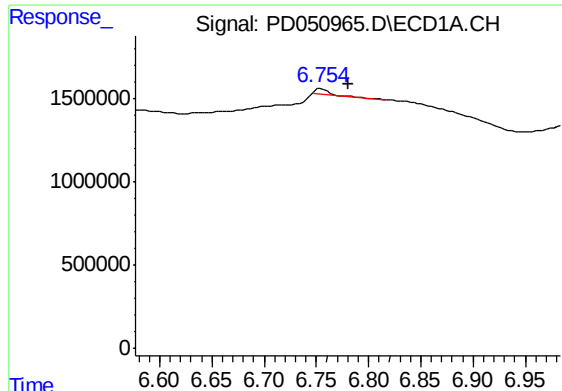

#21 Endrin ketone


R.T.: 6.755 min
Delta R.T.: -0.026 min
Response: 288037
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

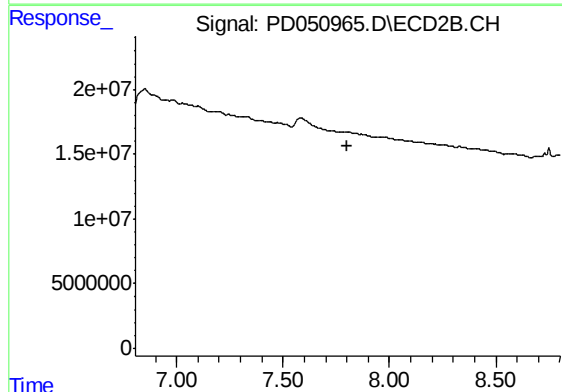


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.804 min
Response: 0
Conc: N.D.

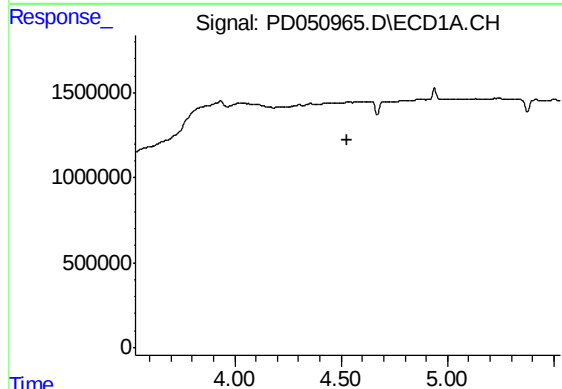


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.531 min
Response: 0
Conc: N.D.

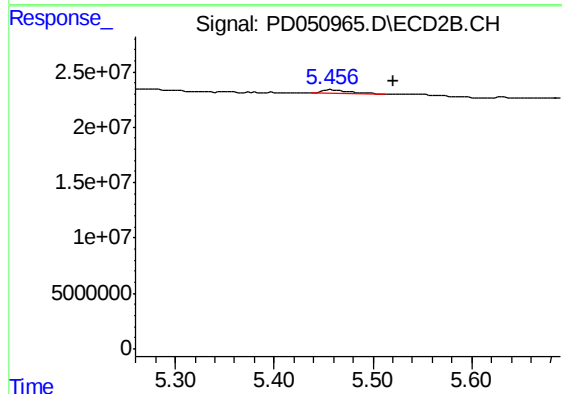

#24 Chlordane-2


R.T.: 5.457 min
Delta R.T.: -0.064 min
Response: 4774663
Conc: 3.56 ng/ml

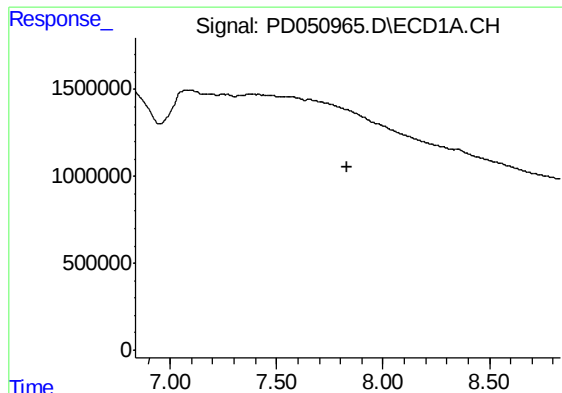

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.834 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

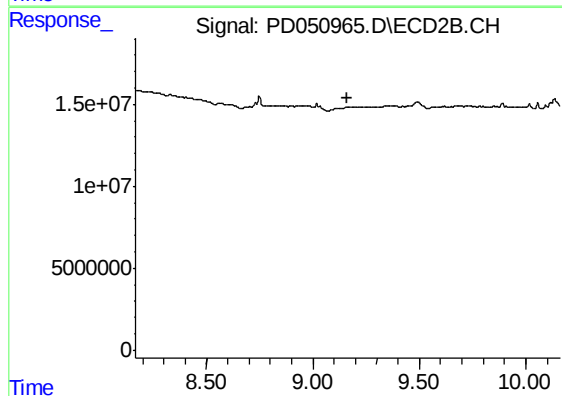

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.164 min
Response: 0
Conc: N.D.