

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
 Data File : PD050966.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2019 4:38
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 08:03:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 03:41:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.047	31637378	637.0E6	21.181	21.406
28)	SA Decachlor...	7.834	9.164	24600813	377.8E6	20.269	18.934
Target Compounds							
3)	MA gamma-BHC...	3.929	0.000	1400370	0	0.594	N.D. #
6)	B beta-BHC	4.103f	4.941f	244046	21281740	0.258	1.176 #
8)	B Heptachlo...	0.000	5.929	0	215.3E6	N.D.	6.174 #
10)	B gamma-Chl...	0.000	6.121f	0	7487077	N.D.	0.216 #
14)	MA Endrin	0.000	6.824f	0	293666	N.D.	0.010 #
16)	A 4,4'-DDD	0.000	6.824f	0	293666	N.D.	0.011 #
19)	B Endosulfa...	6.241f	0.000	849747	0	0.434	N.D. #
20)	A Methoxychlor	0.000	7.582f	0	25242812	N.D.	2.074 #
23)	Chlordane-1	4.081	0.000	297192	0	4.354	N.D. #
24)	Chlordane-2	0.000	5.455	0	6201514	N.D.	4.622 #
25)	Chlordane-3	0.000	6.121	0	7487077	N.D.	1.725 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
Data File : PD050966.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2019 4:38
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 08:03:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 03:41:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

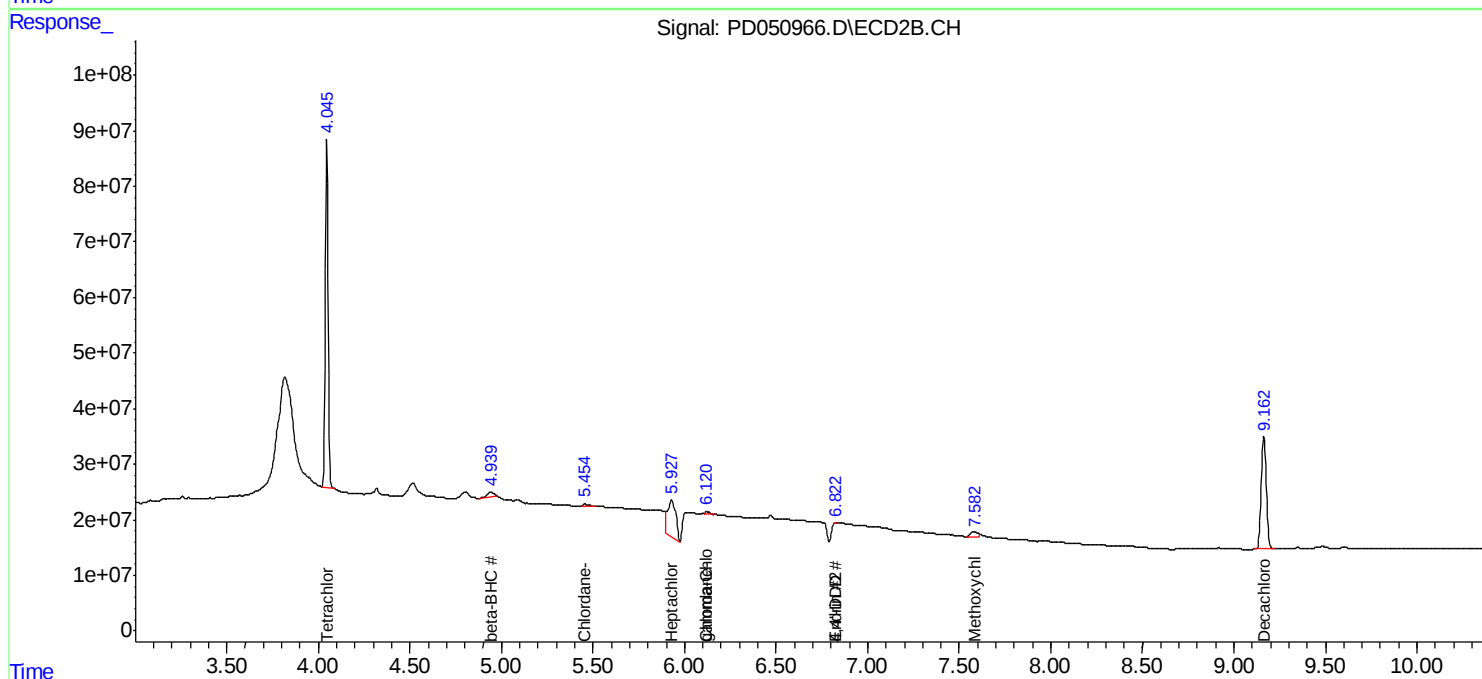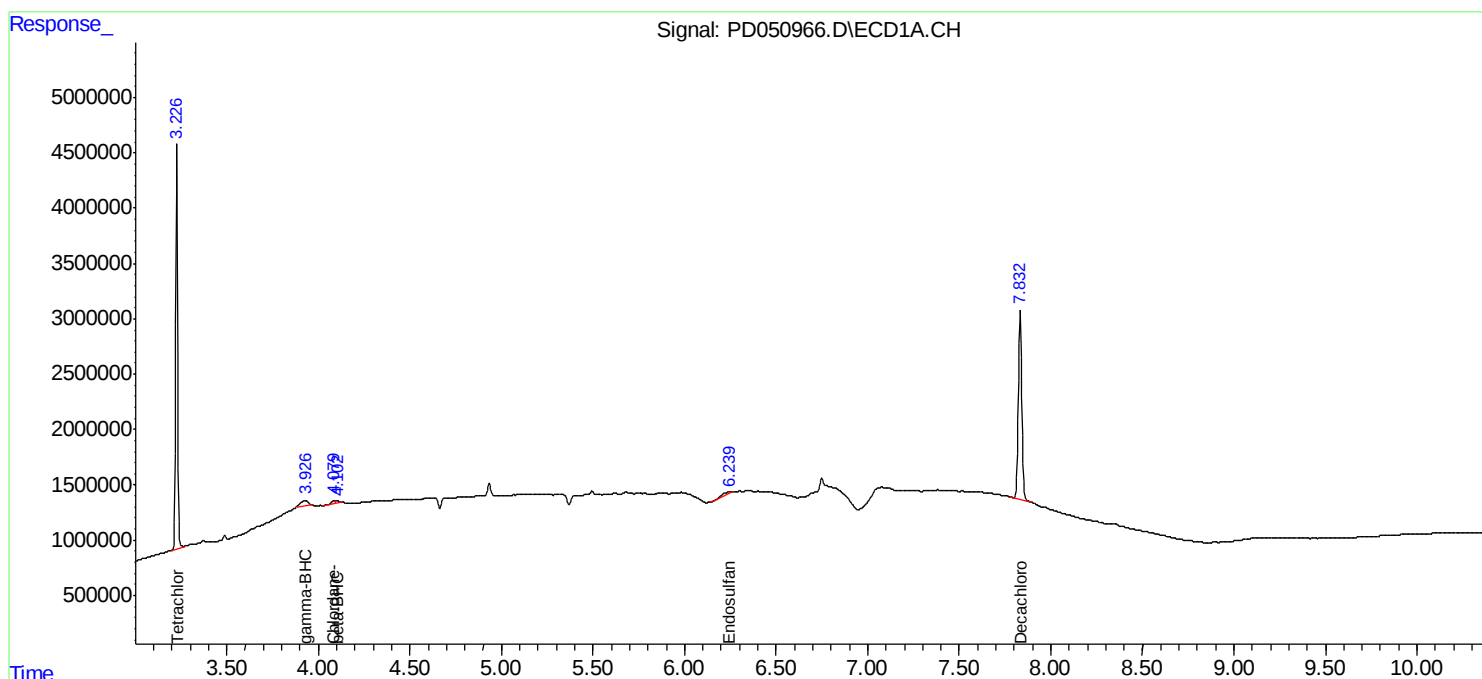


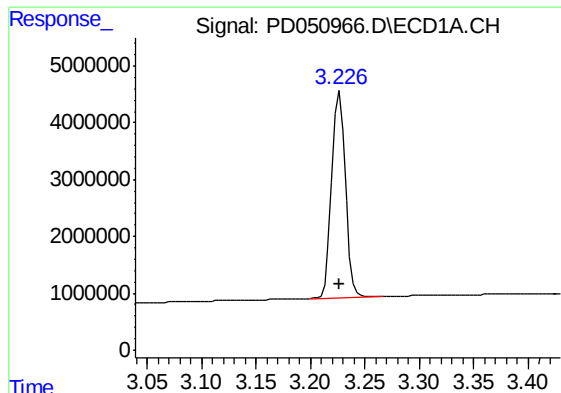

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 31637378
Conc: 21.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

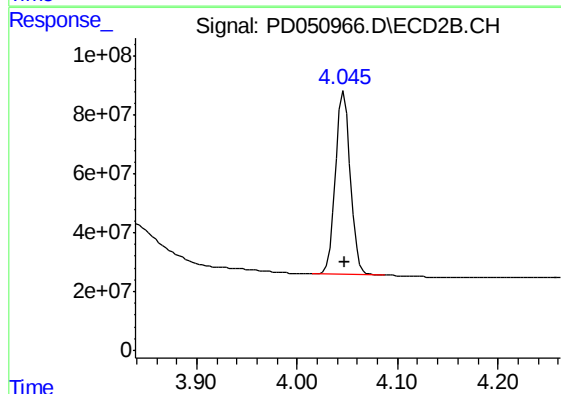


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 637040967
Conc: 21.41 ng/ml

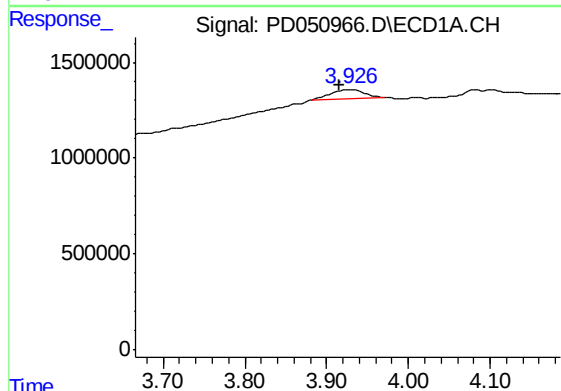


#3 gamma-BHC (Lindane)

R.T.: 3.929 min
Delta R.T.: 0.012 min
Response: 1400370
Conc: 0.59 ng/ml

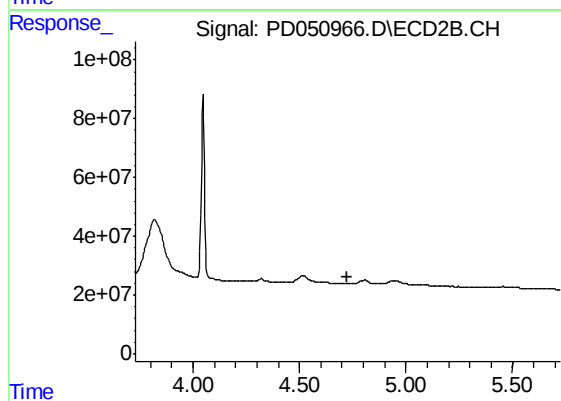

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

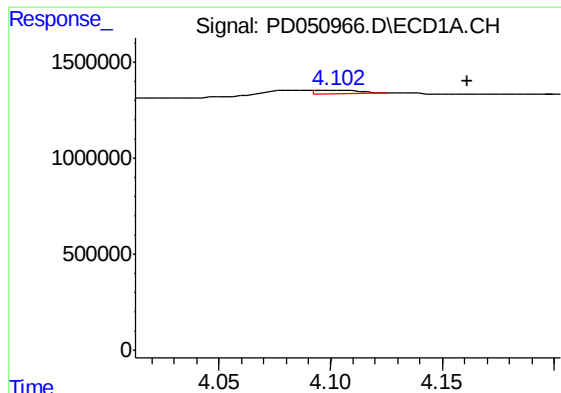

#6 beta-BHC


R.T.: 4.103 min
Delta R.T.: -0.058 min
Response: 244046
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

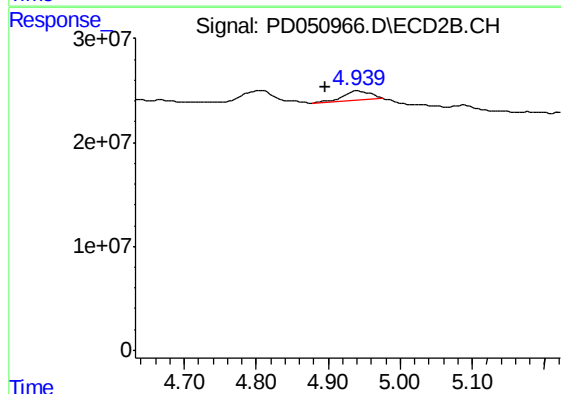


#6 beta-BHC

R.T.: 4.941 min
Delta R.T.: 0.044 min
Response: 21281740
Conc: 1.18 ng/ml

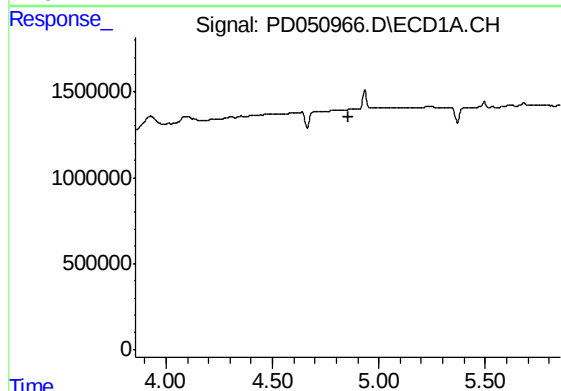


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.855 min
Response: 0
Conc: N.D.

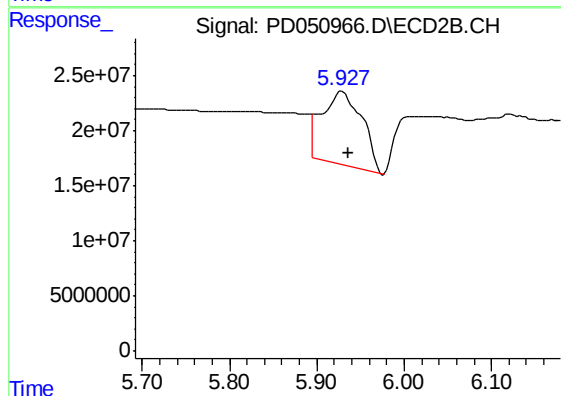

#8 Heptachlor epoxide


R.T.: 5.929 min
Delta R.T.: -0.008 min
Response: 215281978
Conc: 6.17 ng/ml

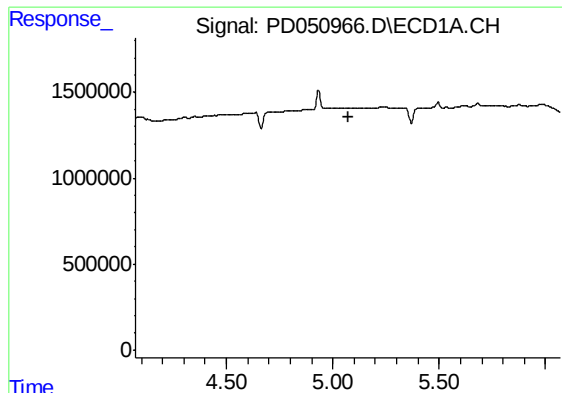

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

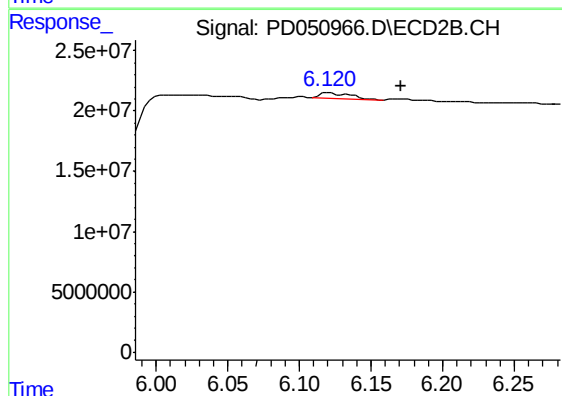


#10 gamma-Chlordane

R.T.: 6.121 min
Delta R.T.: -0.050 min
Response: 7487077
Conc: 0.22 ng/ml

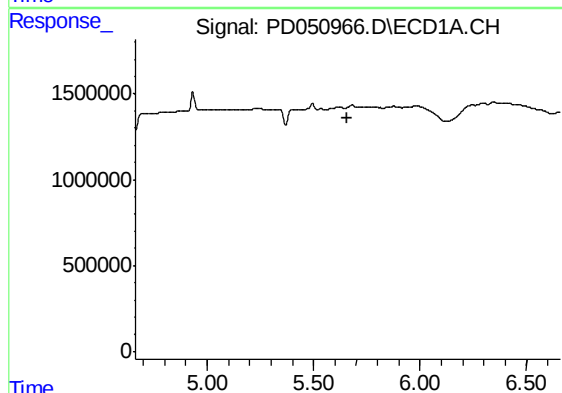


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

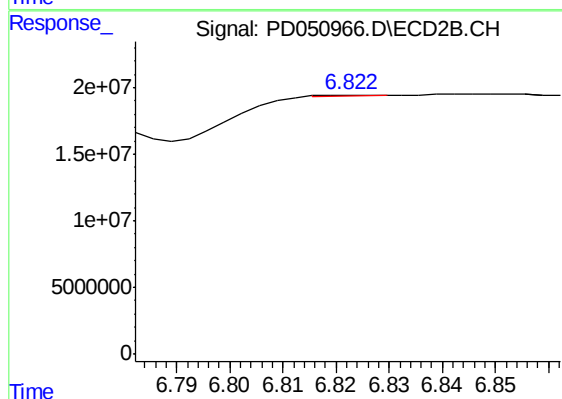

#14 Endrin


R.T.: 6.824 min
Delta R.T.: 0.051 min
Response: 293666
Conc: 0.01 ng/ml

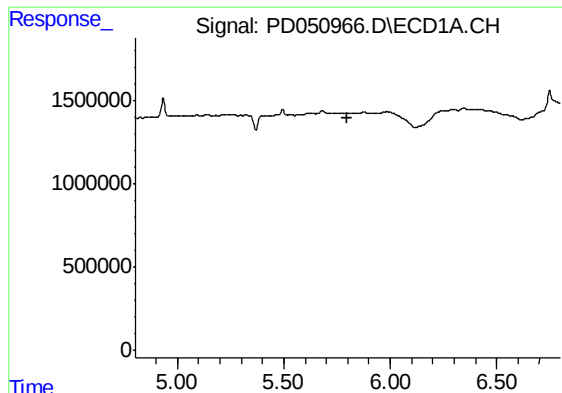

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

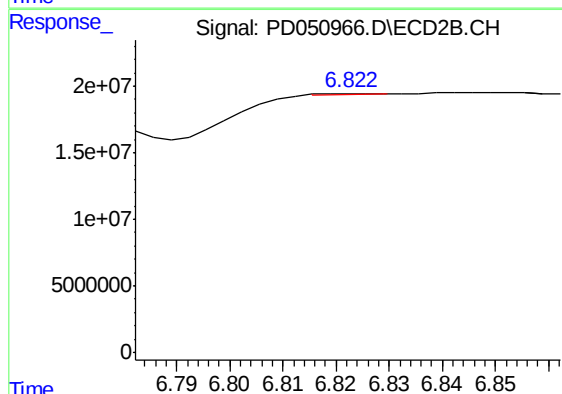


#16 4,4'-DDD

R.T.: 6.824 min
Delta R.T.: -0.068 min
Response: 293666
Conc: 0.01 ng/ml

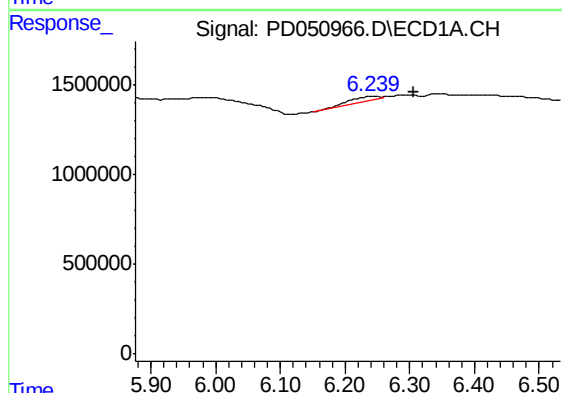


#19 Endosulfan Sulfate

R.T.: 6.241 min
Delta R.T.: -0.064 min
Response: 849747
Conc: 0.43 ng/ml

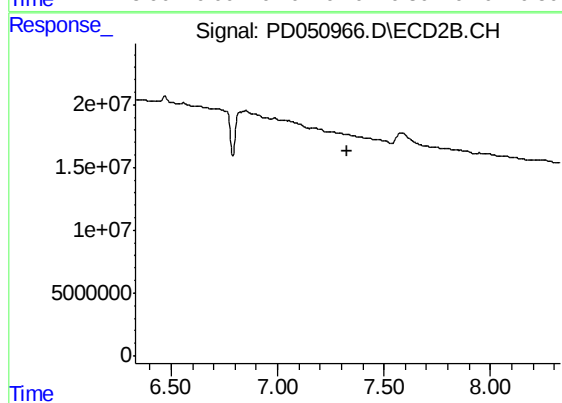

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

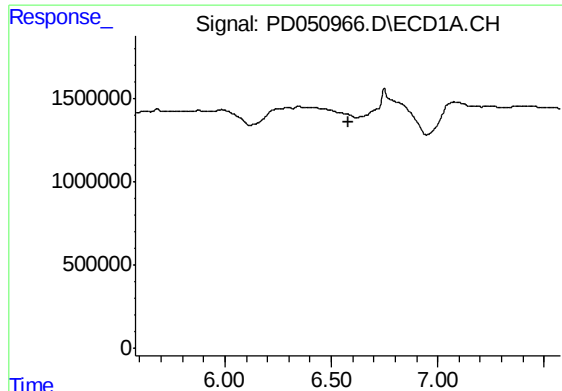

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.578 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

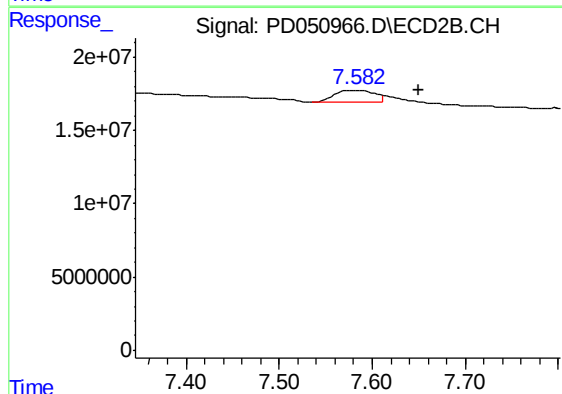


#20 Methoxychlor

R.T.: 7.582 min
Delta R.T.: -0.069 min
Response: 25242812
Conc: 2.07 ng/ml

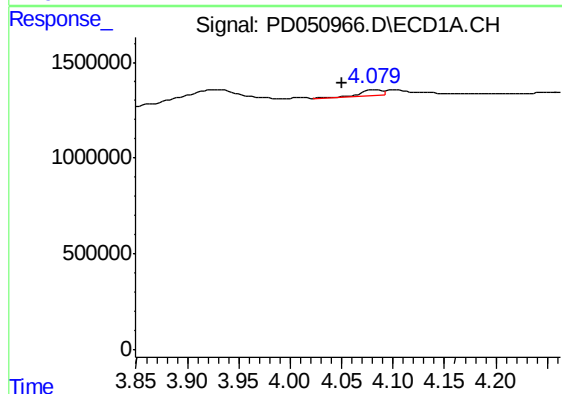


#23 Chlordane-1

R.T.: 4.081 min
Delta R.T.: 0.031 min
Response: 297192
Conc: 4.35 ng/ml

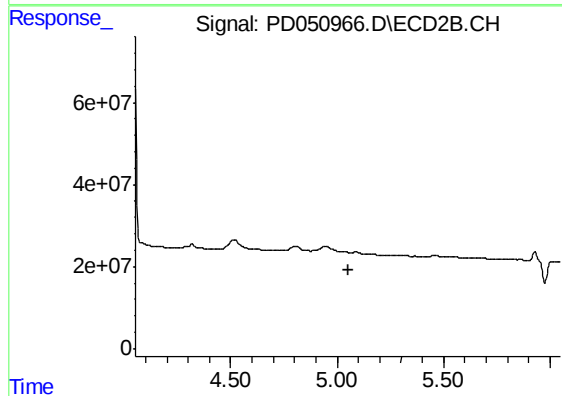

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.051 min
Response: 0
Conc: N.D.

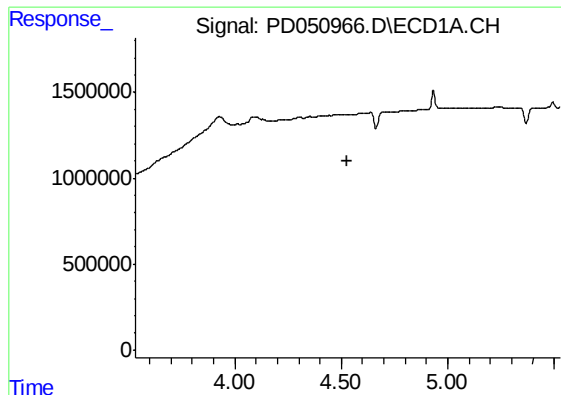

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.531 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

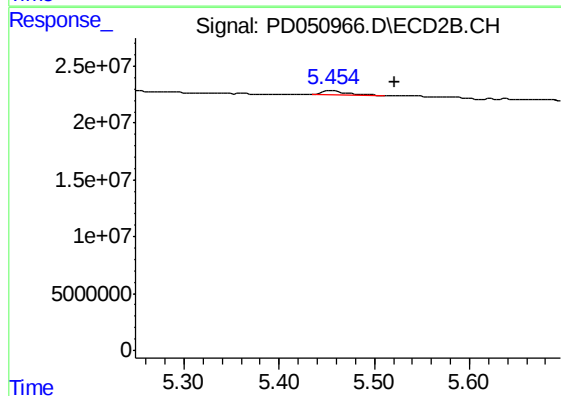


#24 Chlordane-2

R.T.: 5.455 min
Delta R.T.: -0.065 min
Response: 6201514
Conc: 4.62 ng/ml

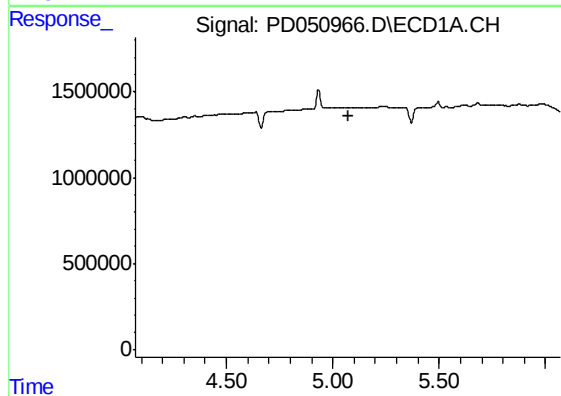


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.073 min
Response: 0
Conc: N.D.

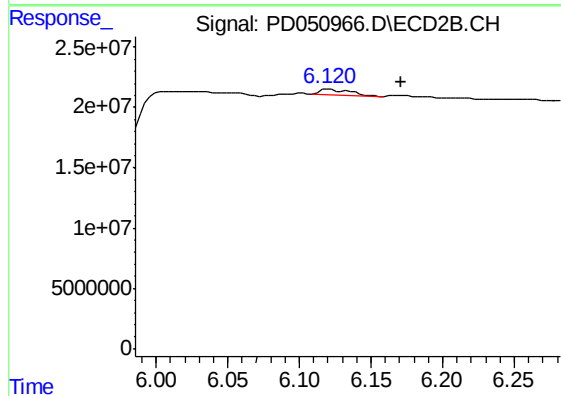

#25 Chlordane-3


R.T.: 6.121 min
Delta R.T.: -0.050 min
Response: 7487077
Conc: 1.73 ng/ml

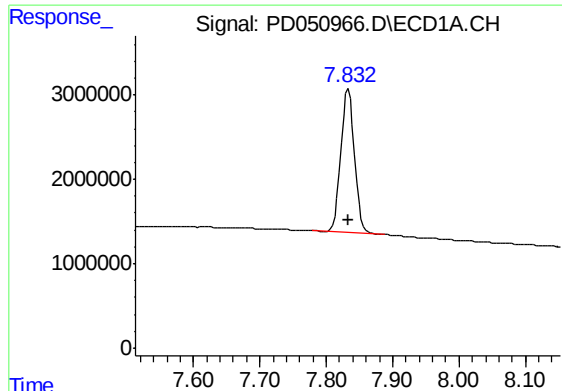

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: 0.000 min
Response: 24600813
Conc: 20.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

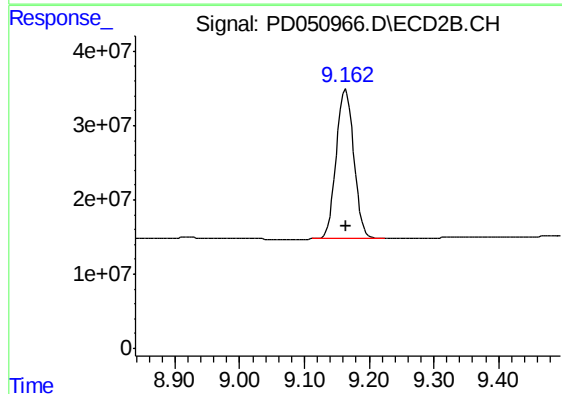

#28 Decachlorobiphenyl

R.T.: 9.164 min
Delta R.T.: 0.000 min
Response: 377827011
Conc: 18.93 ng/ml