

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
 Data File : PD050989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2019 10:43
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:24:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 03:41:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.227	4.047	32415035	632.0E6	21.702	21.236
28)	SA Decachlor...	7.832	9.160	25007043	374.7E6	20.603	18.777
Target Compounds							
3)	MA gamma-BHC...	3.929	0.000	1223435	0	0.519	N.D. #
6)	B beta-BHC	4.104f	4.943f	119726	16569721	0.126	0.916 #
7)	B delta-BHC	0.000	5.143	0	3015764	N.D.	0.078 #
8)	B Heptachlo...	4.786f	5.928	840253	248.6E6	0.374	7.129 #
12)	B 4,4'-DDE	0.000	6.416	0	960680	N.D.	0.029 #
13)	MA Dieldrin	5.436	0.000	1002465	0	0.428	N.D. #
14)	MA Endrin	5.679	0.000	163813	0	0.075	N.D. #
19)	B Endosulfa...	6.242f	0.000	940691	0	0.480	N.D. #
24)	Chlordane-2	0.000	5.454	0	8718698	N.D.	6.498 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011119\
Data File : PD050989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2019 10:43
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:24:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 03:41:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

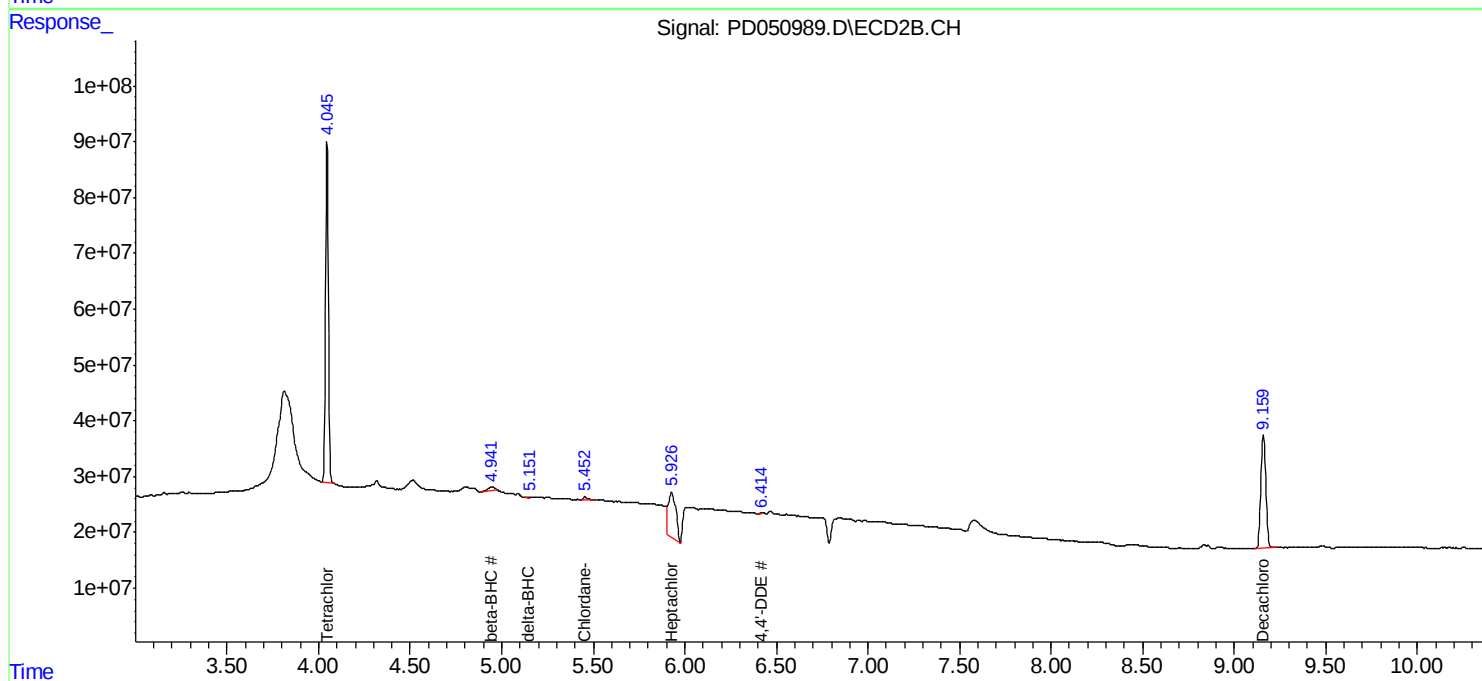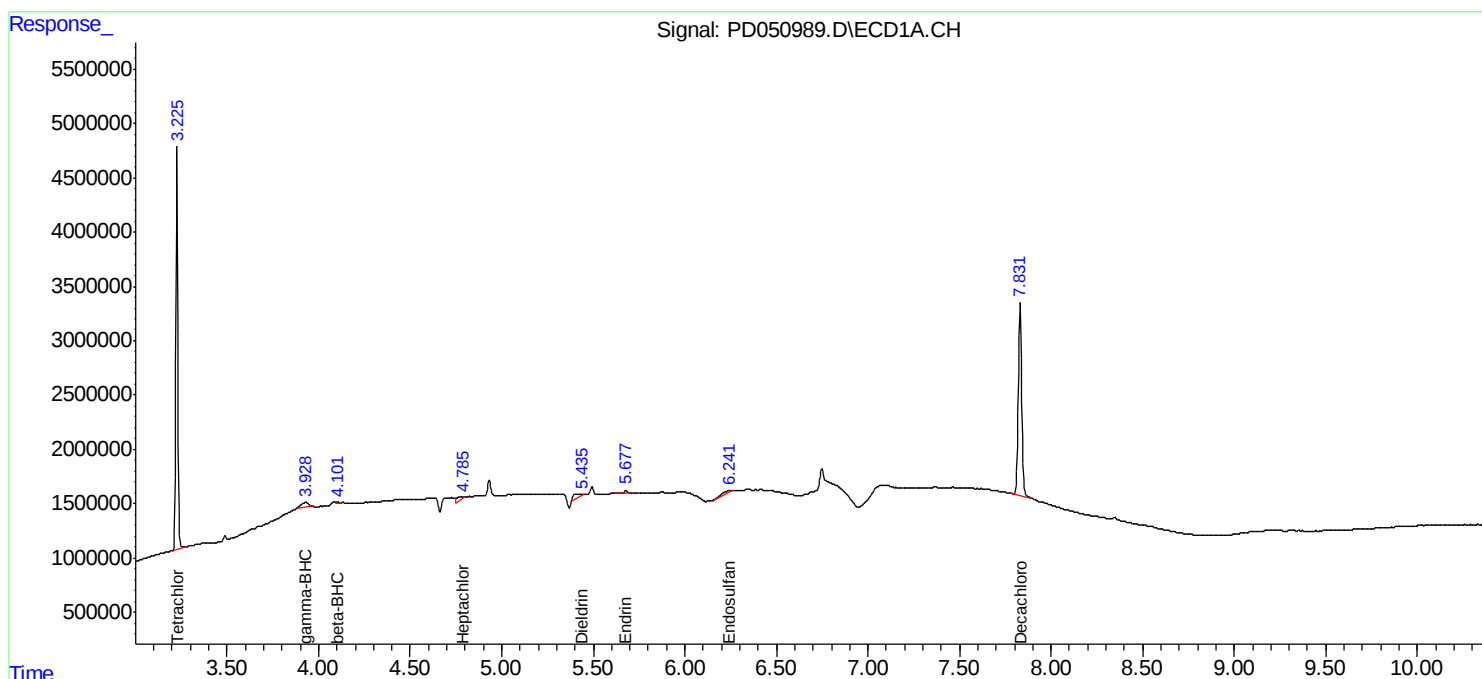


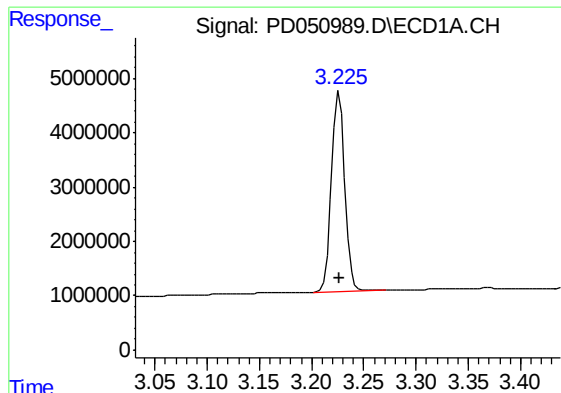

#1 Tetrachloro-m-xylene


R.T.: 3.227 min
Delta R.T.: 0.000 min
Response: 32415035
Conc: 21.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

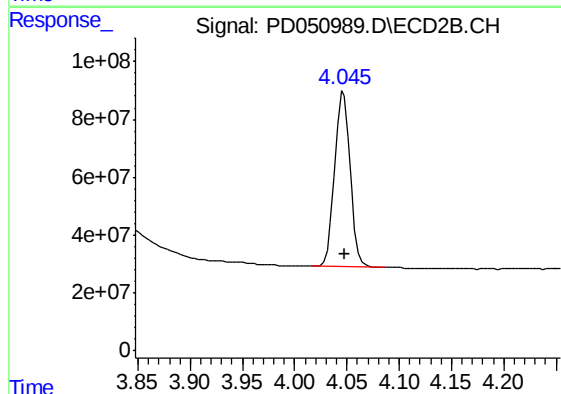


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 631976786
Conc: 21.24 ng/ml

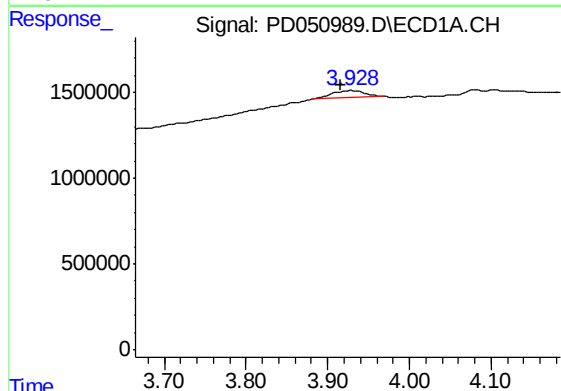


#3 gamma-BHC (Lindane)

R.T.: 3.929 min
Delta R.T.: 0.012 min
Response: 1223435
Conc: 0.52 ng/ml

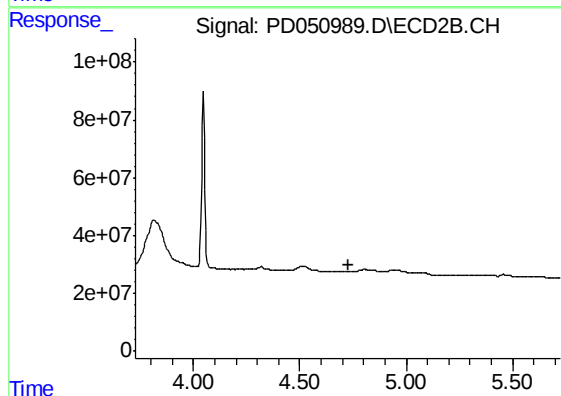

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.727 min
Response: 0
Conc: N.D.

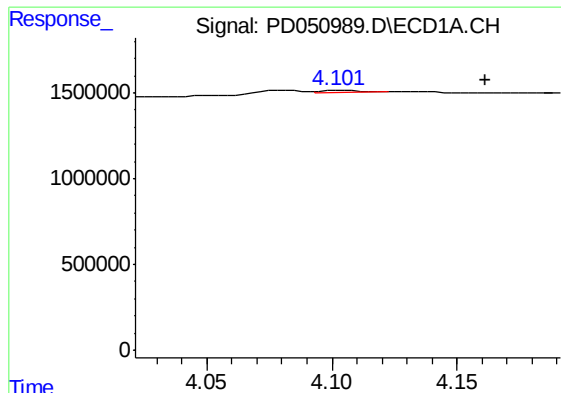

#6 beta-BHC


R.T.: 4.104 min
Delta R.T.: -0.057 min
Response: 119726
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

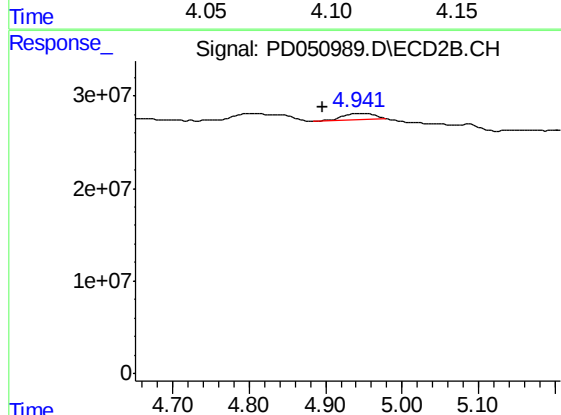


#6 beta-BHC

R.T.: 4.943 min
Delta R.T.: 0.046 min
Response: 16569721
Conc: 0.92 ng/ml

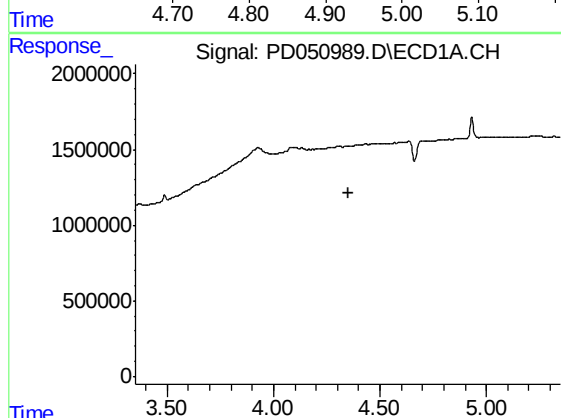


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.351 min
Response: 0
Conc: N.D.

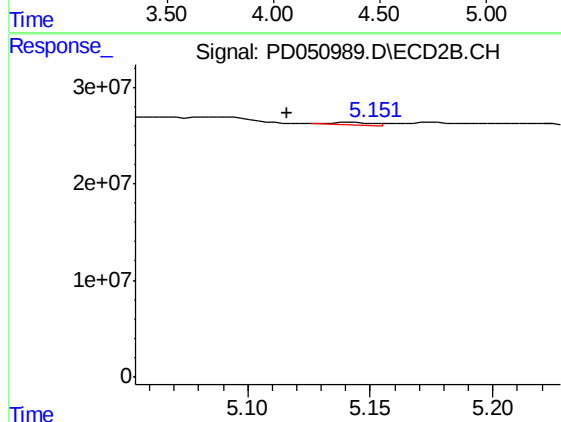

#7 delta-BHC


R.T.: 5.143 min
Delta R.T.: 0.027 min
Response: 3015764
Conc: 0.08 ng/ml

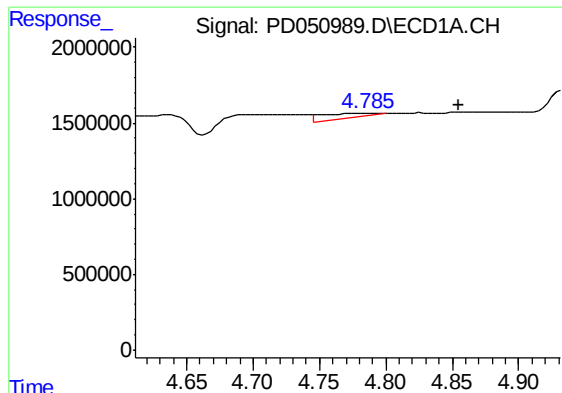

#8 Heptachlor epoxide


R.T.: 4.786 min
Delta R.T.: -0.069 min
Response: 840253
Conc: 0.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

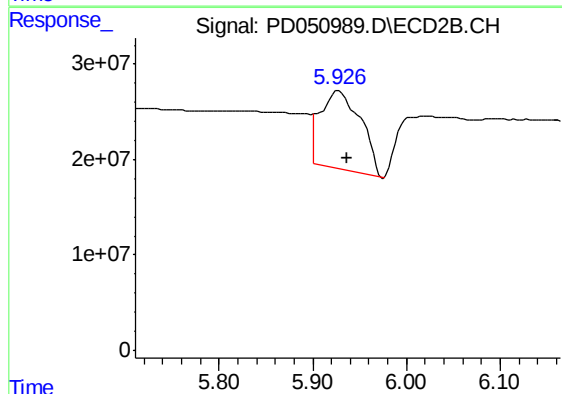


#8 Heptachlor epoxide

R.T.: 5.928 min
Delta R.T.: -0.009 min
Response: 248588938
Conc: 7.13 ng/ml

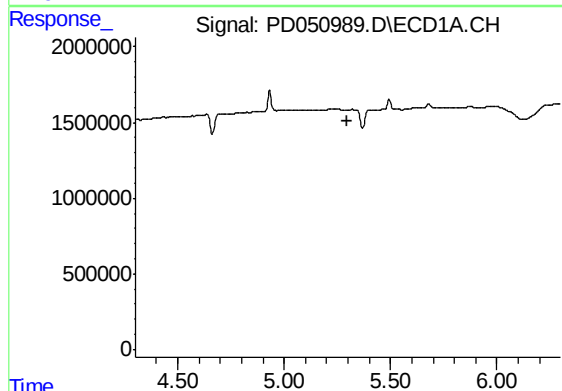


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.299 min
Response: 0
Conc: N.D.

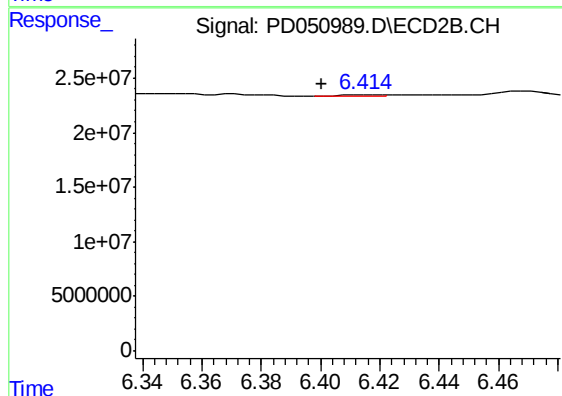

#12 4,4'-DDE


R.T.: 6.416 min
Delta R.T.: 0.016 min
Response: 960680
Conc: 0.03 ng/ml

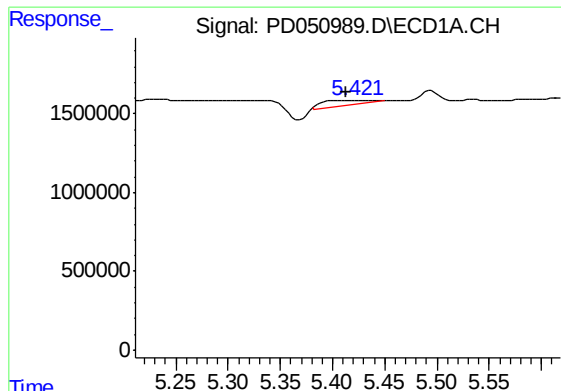

#13 Dieldrin


R.T.: 5.436 min
Delta R.T.: 0.023 min
Response: 1002465
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

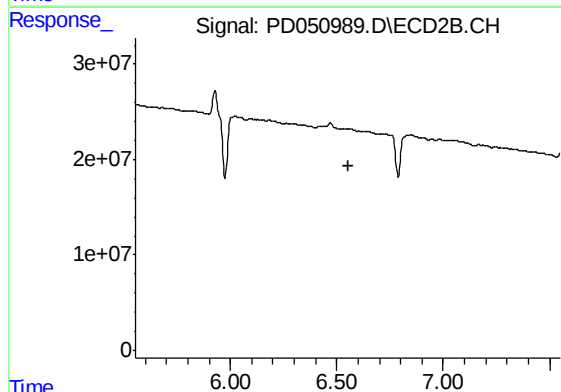


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.553 min
Response: 0
Conc: N.D.

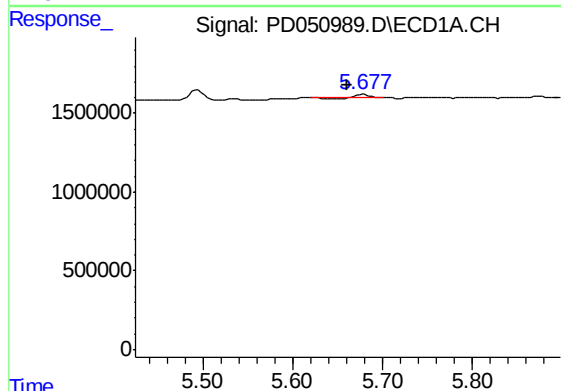


#14 Endrin

R.T.: 5.679 min
Delta R.T.: 0.018 min
Response: 163813
Conc: 0.07 ng/ml

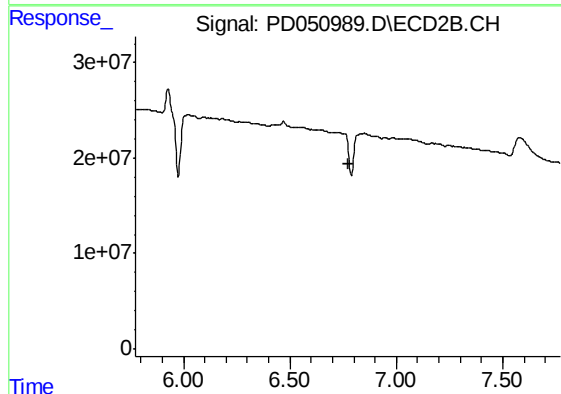

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

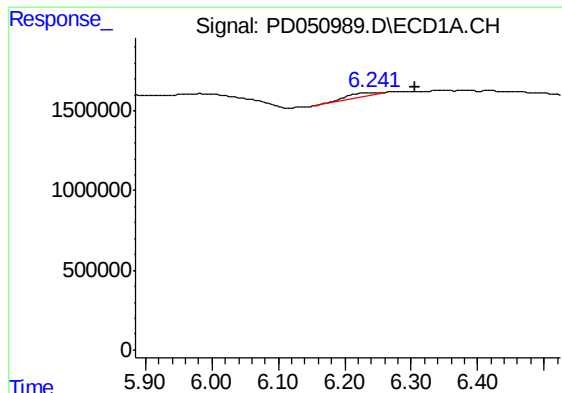

#19 Endosulfan Sulfate


R.T.: 6.242 min
Delta R.T.: -0.063 min
Response: 940691
Conc: 0.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

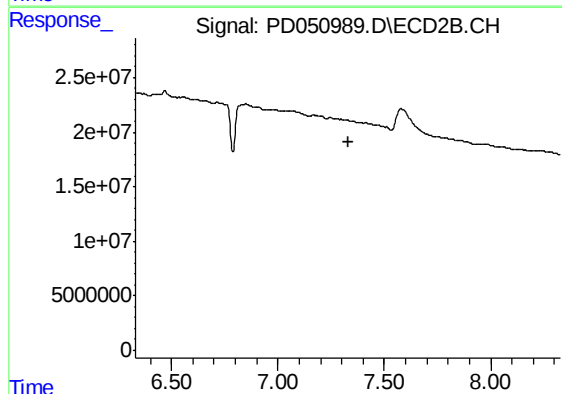


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.330 min
Response: 0
Conc: N.D.

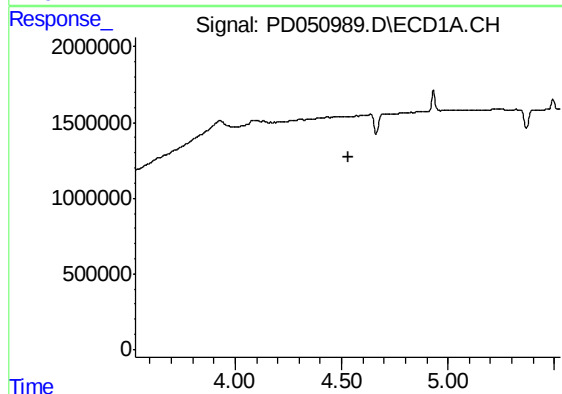


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.531 min
Response: 0
Conc: N.D.

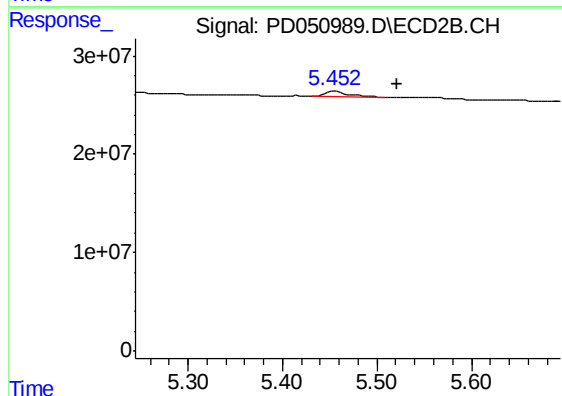

#24 Chlordane-2


R.T.: 5.454 min
Delta R.T.: -0.067 min
Response: 8718698
Conc: 6.50 ng/ml

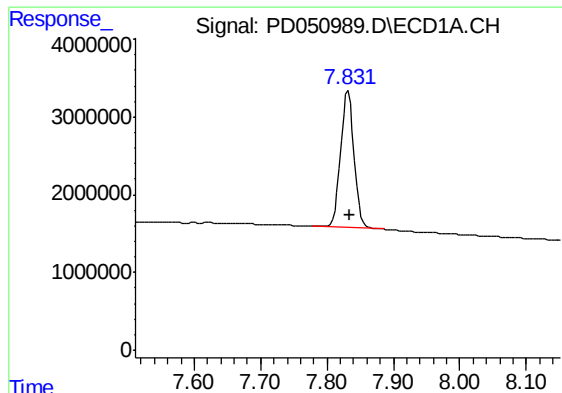

#28 Decachlorobiphenyl

R.T.: 7.832 min
Delta R.T.: -0.002 min
Response: 25007043
Conc: 20.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

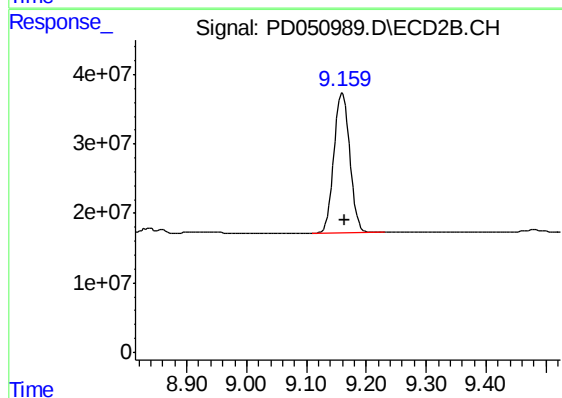

#28 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: -0.004 min
Response: 374691059
Conc: 18.78 ng/ml