

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
 Data File : PD080759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2024 17:14
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2090

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 04:27:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 11 04:26:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.797	14984636	25404618	10.540	10.304
27)	SA Decachlor...	9.118	7.940	41469759	56949757	20.658	20.854
Target Compounds							
2)	A alpha-BHC	4.023	3.299	23783880	40089096	10.165	9.944
3)	MA gamma-BHC...	4.357	3.629	23236371	37725988	10.400	10.010
4)	MA Heptachlor	4.950	3.970	24588204	37111665	10.422	10.171
9)	A Endosulfan I	6.108	5.123	21170274	33001607	10.282	10.310
13)	MA Dieldrin	6.383	5.387	43135064	70986520	19.999	19.971
14)	MA Endrin	6.614	5.662	34756340	58975290	19.782	19.758
16)	A 4,4'-DDD	6.745	5.809	32219706	54859709	19.811	20.005
17)	MA 4,4'-DDT	7.061	6.061	32545736	53157749	19.438	19.465
20)	A Methoxychlor	7.535	6.636	90379657	149.1E6	97.857	102.723


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
Data File : PD080759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 17:14
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 04:27:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 11 04:26:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

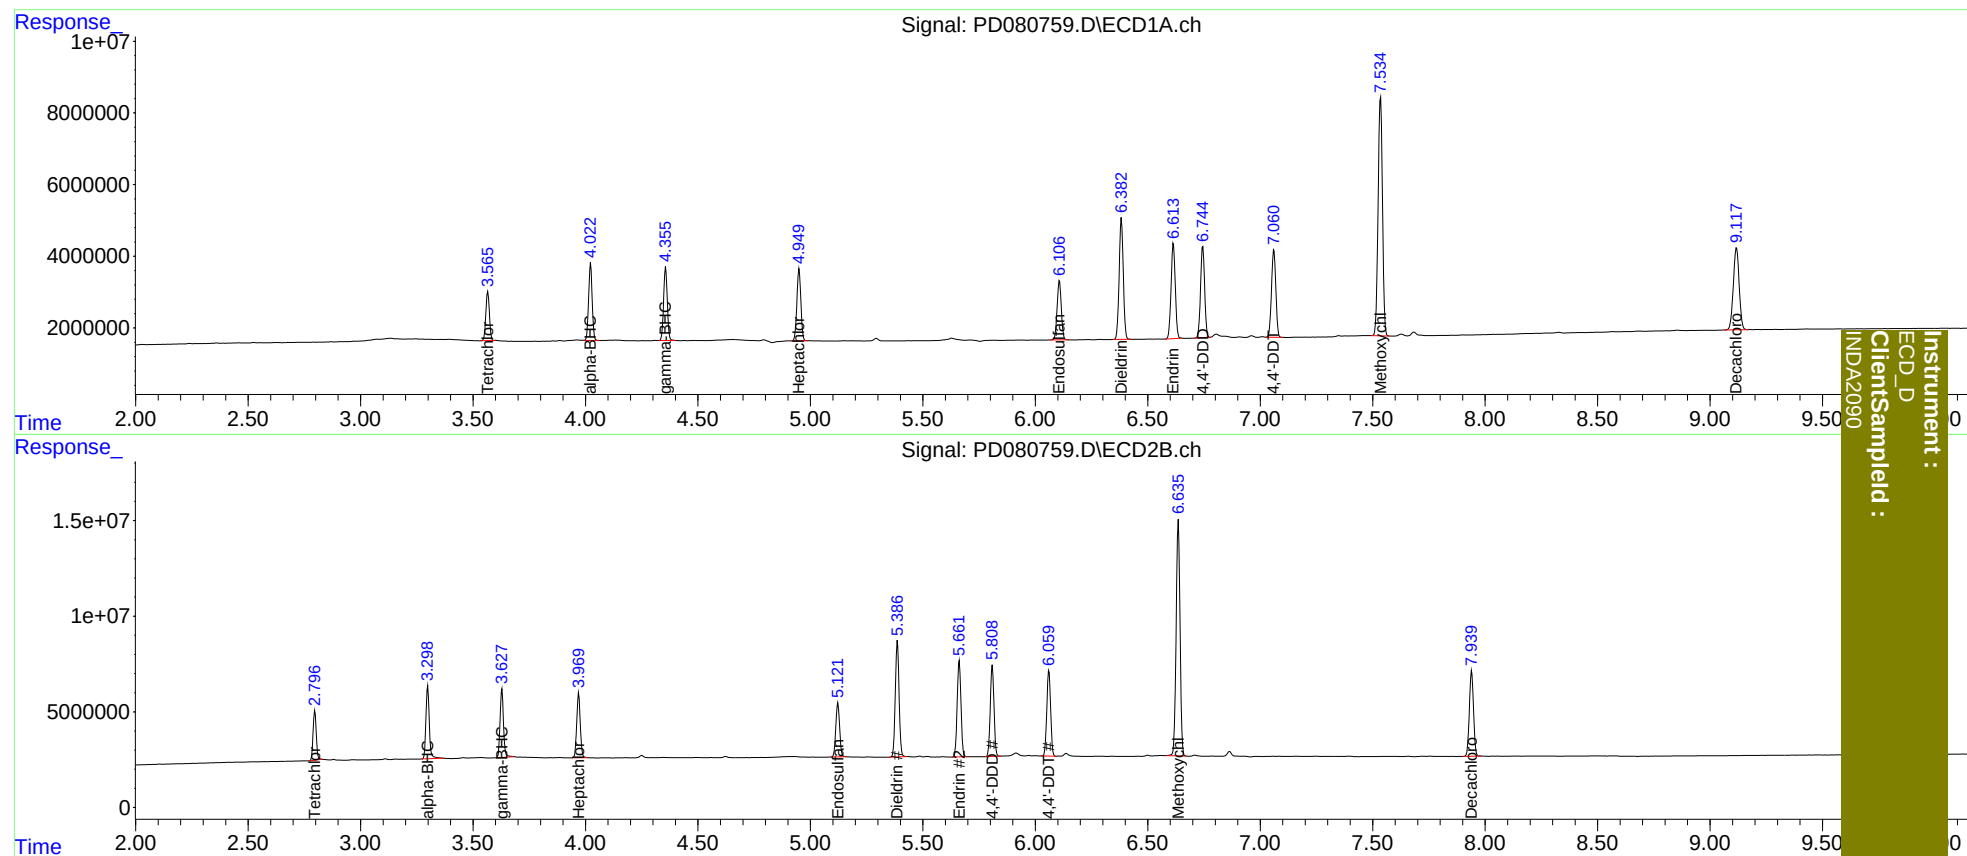


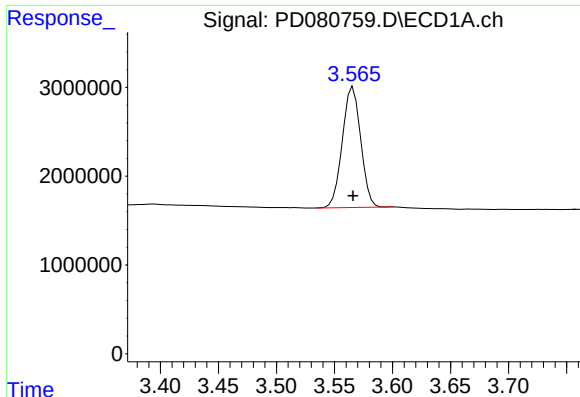

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 14984636
Conc: 10.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

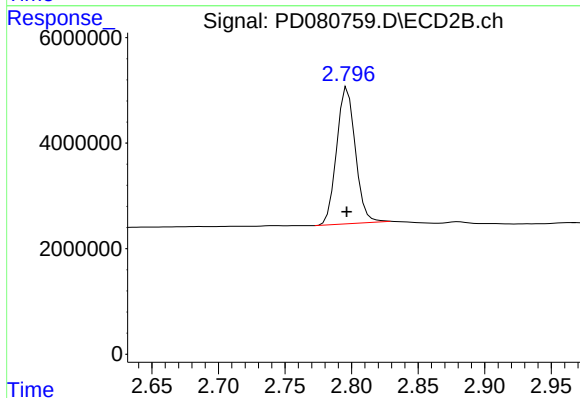


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: 0.000 min
Response: 25404618
Conc: 10.30 ng/ml

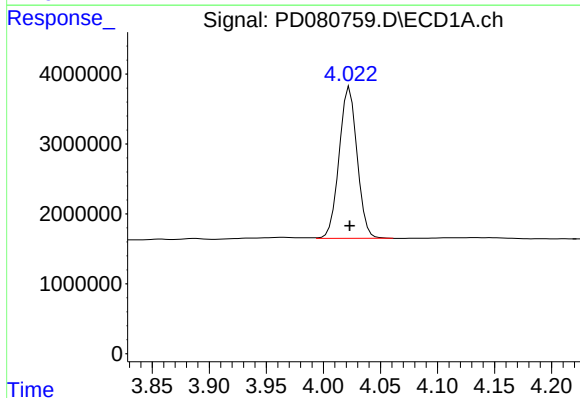


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 23783880
Conc: 10.16 ng/ml

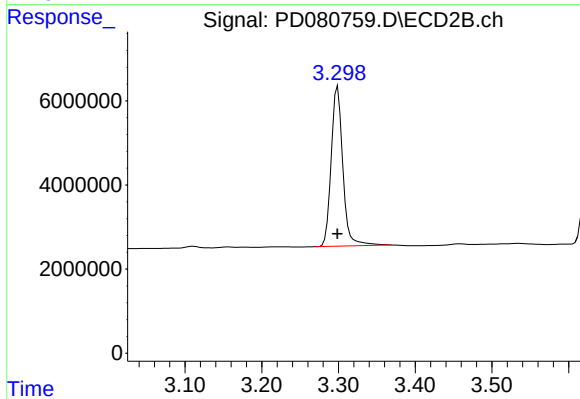

#2 alpha-BHC


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 40089096
Conc: 9.94 ng/ml

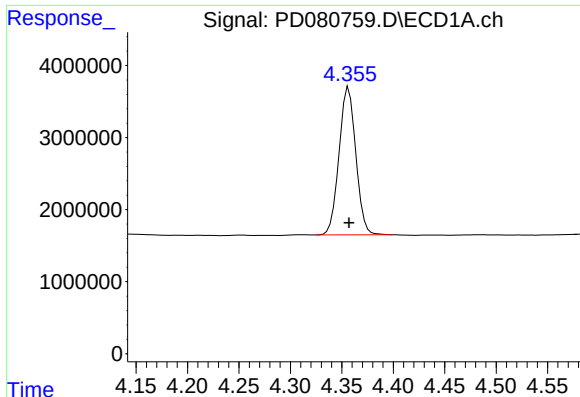

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 23236371
Conc: 10.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

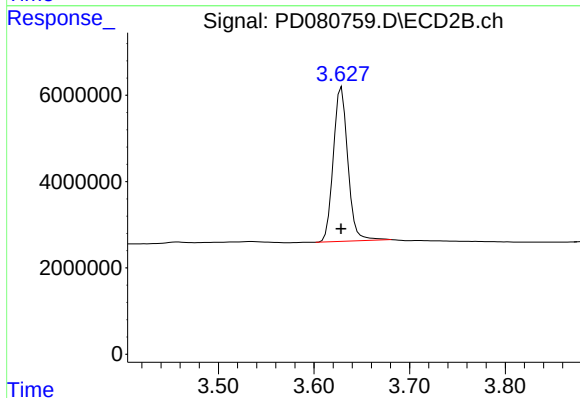


#3 gamma-BHC (Lindane)

R.T.: 3.629 min
Delta R.T.: 0.000 min
Response: 37725988
Conc: 10.01 ng/ml

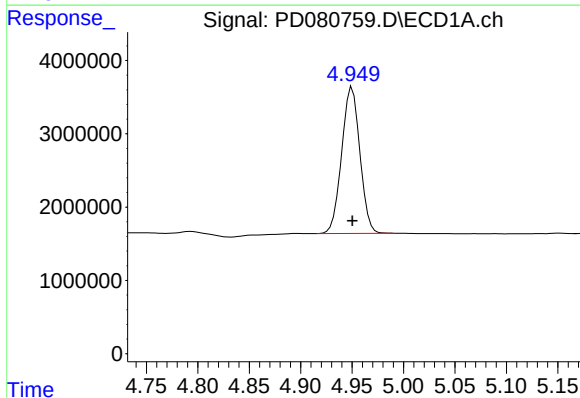


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 24588204
Conc: 10.42 ng/ml

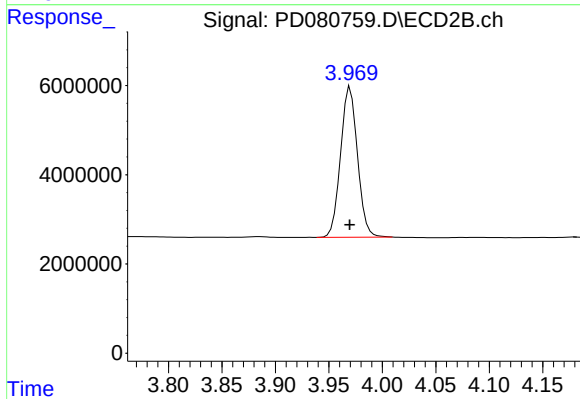

#4 Heptachlor


R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 37111665
Conc: 10.17 ng/ml

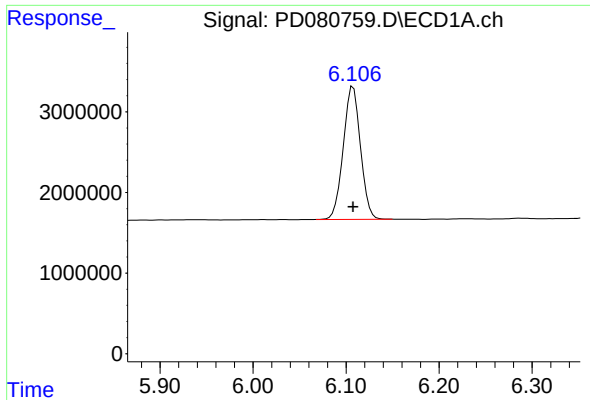

#9 Endosulfan I


R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 21170274
Conc: 10.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

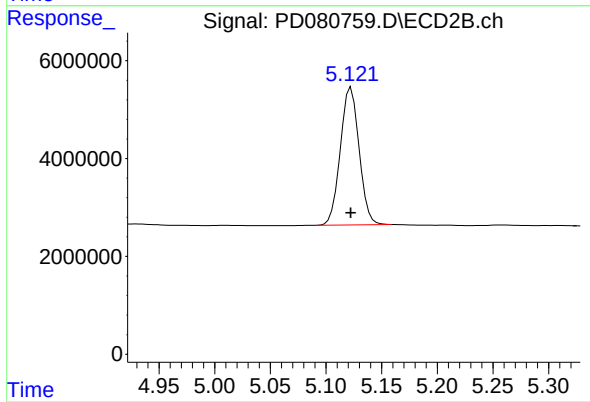


#9 Endosulfan I

R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 33001607
Conc: 10.31 ng/ml

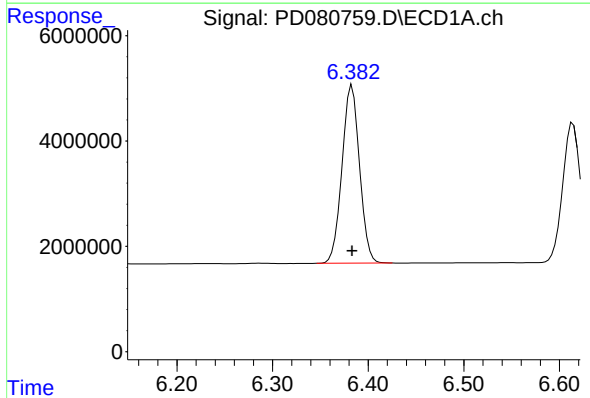


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 43135064
Conc: 20.00 ng/ml

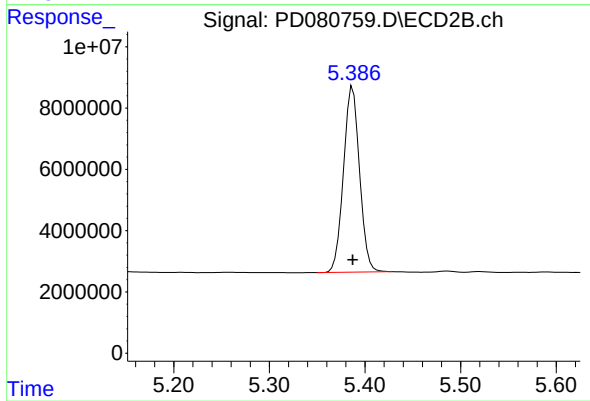

#13 Dieldrin


R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 70986520
Conc: 19.97 ng/ml

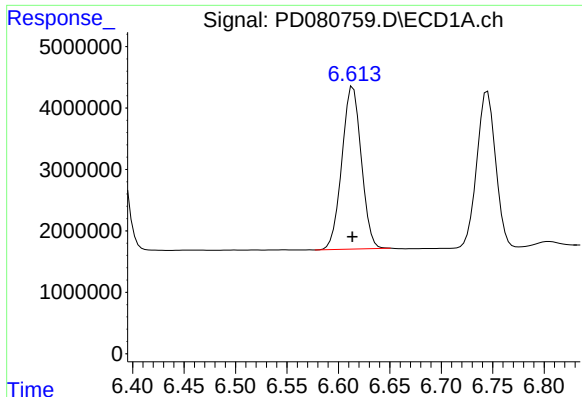

#14 Endrin


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 34756340
Conc: 19.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

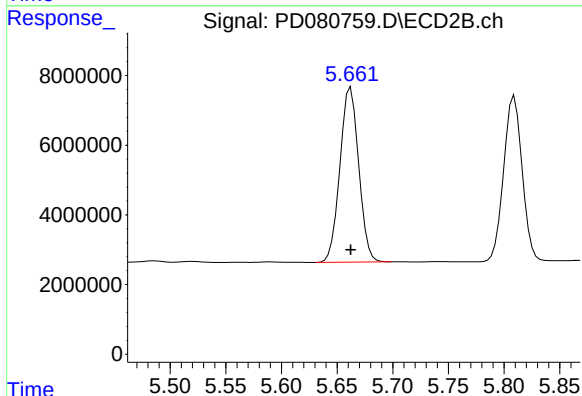


#14 Endrin

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 58975290
Conc: 19.76 ng/ml

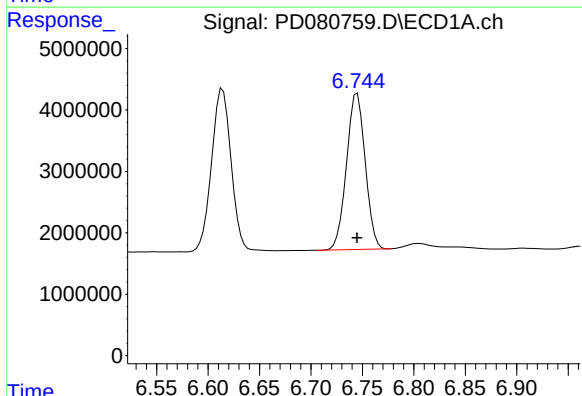


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 32219706
Conc: 19.81 ng/ml

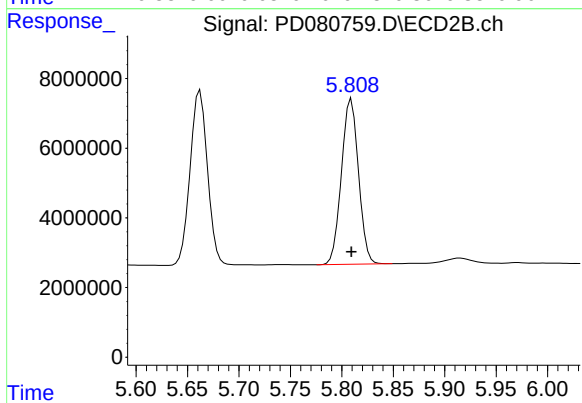

#16 4,4'-DDD


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 54859709
Conc: 20.01 ng/ml

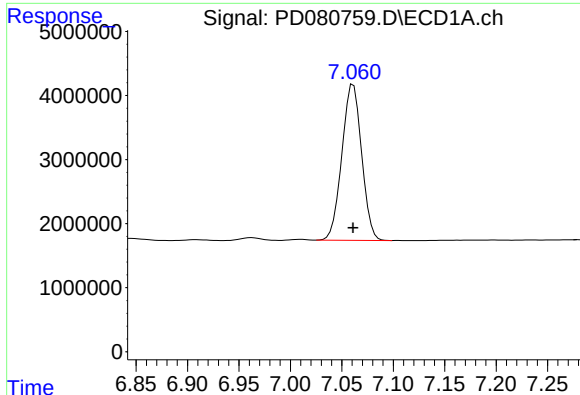

#17 4,4'-DDT


R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 32545736
Conc: 19.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

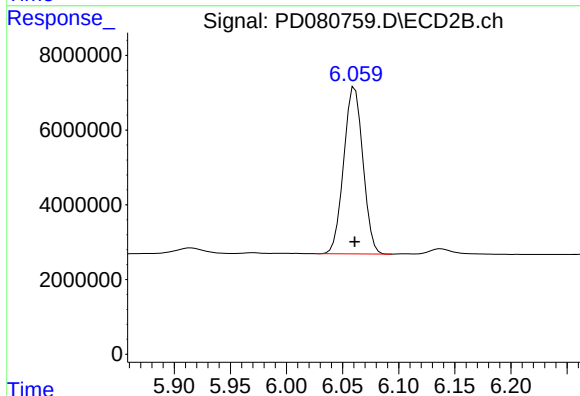


#17 4,4'-DDT

R.T.: 6.061 min
Delta R.T.: 0.000 min
Response: 53157749
Conc: 19.46 ng/ml

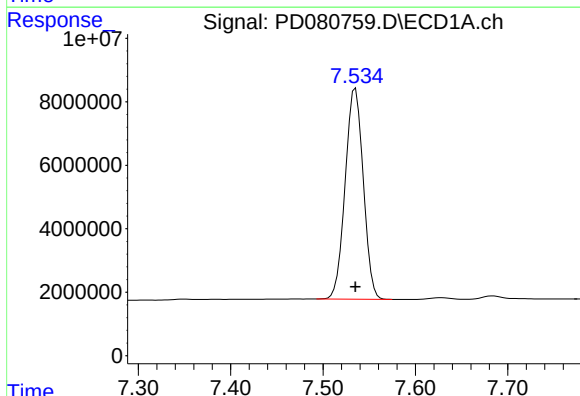


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 90379657
Conc: 97.86 ng/ml

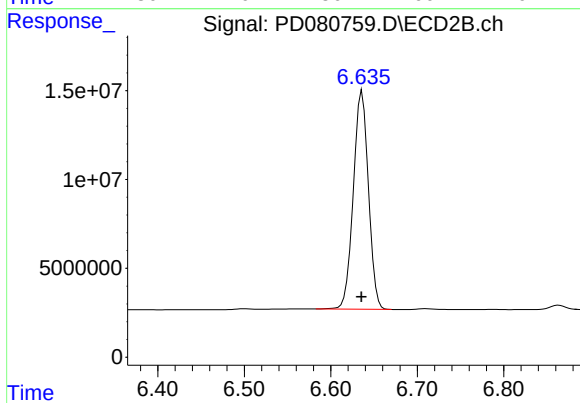

#20 Methoxychlor


R.T.: 6.636 min
Delta R.T.: 0.000 min
Response: 149058486
Conc: 102.72 ng/ml

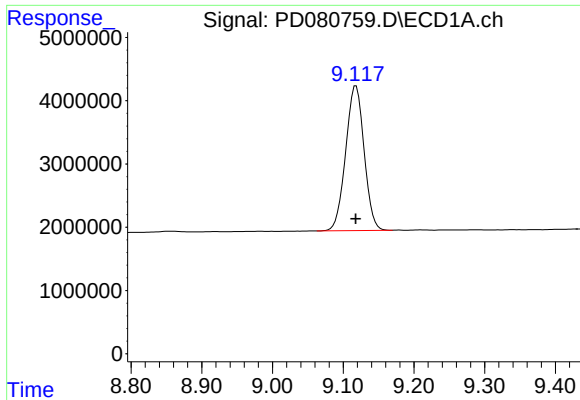

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 41469759
Conc: 20.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2090

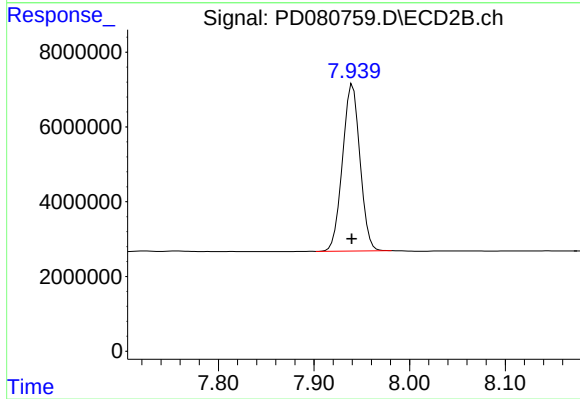

#27 Decachlorobiphenyl

R.T.: 7.940 min
Delta R.T.: 0.000 min
Response: 56949757
Conc: 20.85 ng/ml