

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
 Data File : PD080763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2024 18:08
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4094

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 04:28:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 11 04:26:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	56393509	97384590	39.668	39.500
27)	SA Decachlor...	9.117	7.939	151.3E6	207.8E6	75.371	76.107
Target Compounds							
2)	A alpha-BHC	4.023	3.298	97897030	165.7E6	41.838	41.108
3)	MA gamma-BHC...	4.357	3.628	92263961	153.2E6	41.296	40.640
4)	MA Heptachlor	4.950	3.969	94499127	145.9E6	40.056	39.983
9)	A Endosulfan I	6.107	5.122	80646970	126.6E6	39.168	39.566
13)	MA Dieldrin	6.383	5.387	175.0E6	286.5E6	81.129	80.617
14)	MA Endrin	6.613	5.662	139.1E6	234.5E6	79.148	78.560
16)	A 4,4'-DDD	6.745	5.809	130.9E6	220.0E6	80.454	80.219
17)	MA 4,4'-DDT	7.060	6.060	137.9E6	222.7E6	82.343	81.553
20)	A Methoxychlor	7.535	6.635	361.6E6	546.5E6	391.518	376.590


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
Data File : PD080763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 18:08
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 04:28:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 11 04:26:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

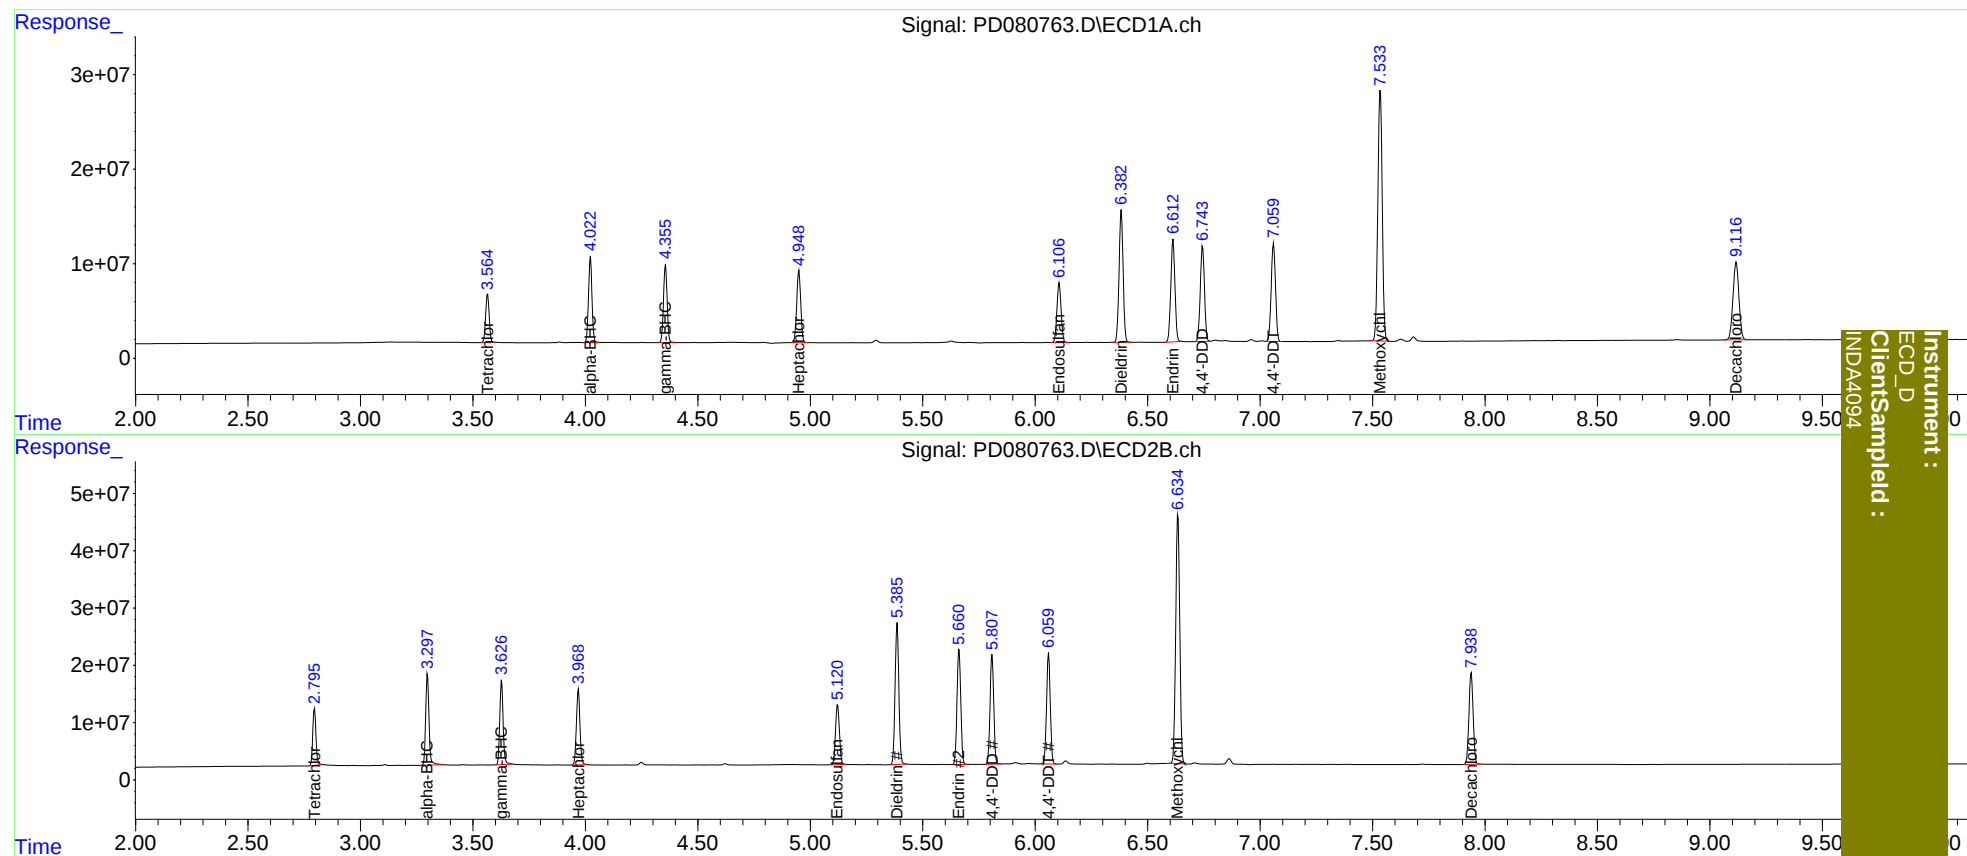


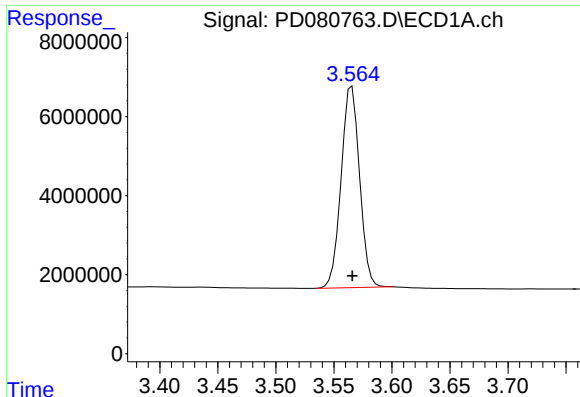

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 56393509
Conc: 39.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

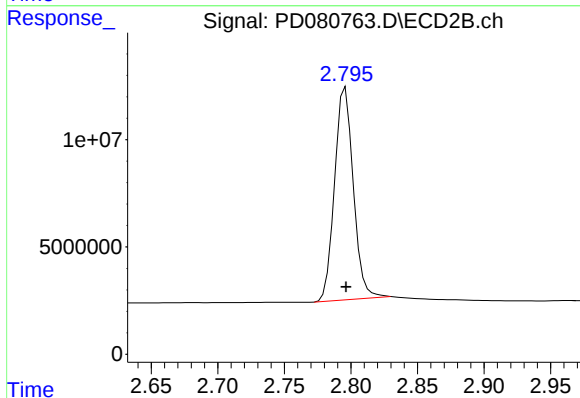


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 97384590
Conc: 39.50 ng/ml

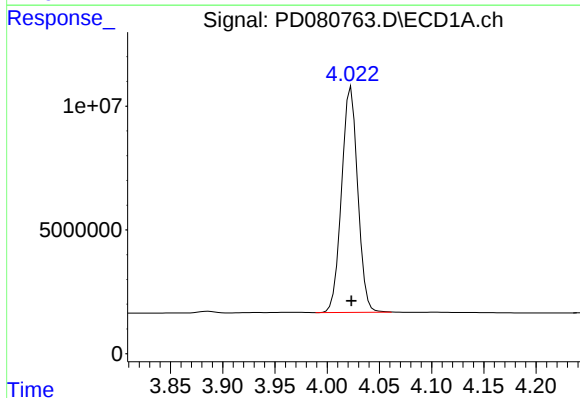


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 97897030
Conc: 41.84 ng/ml

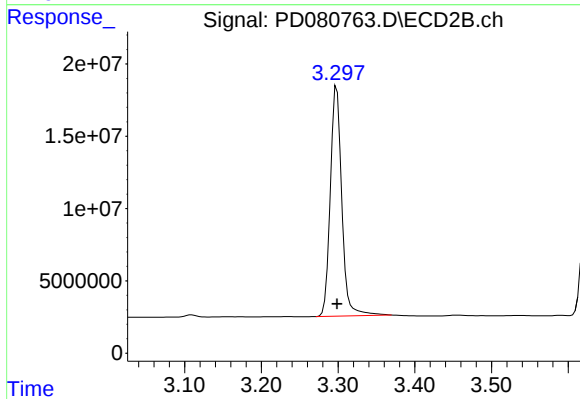

#2 alpha-BHC


R.T.: 3.298 min
Delta R.T.: 0.000 min
Response: 165734741
Conc: 41.11 ng/ml

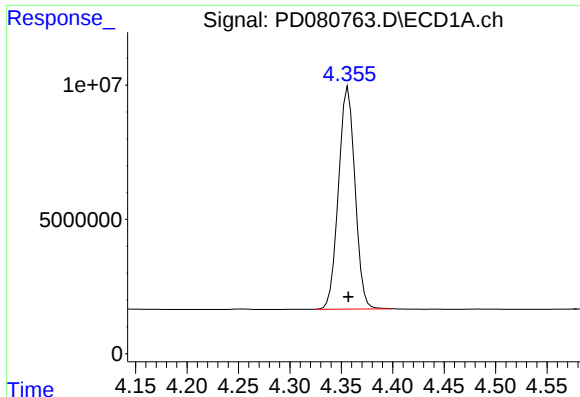

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 92263961
Conc: 41.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

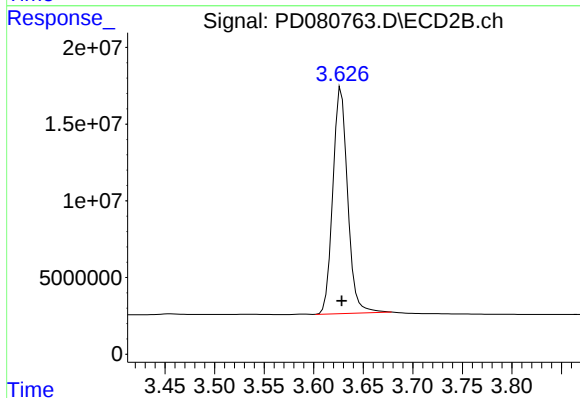


#3 gamma-BHC (Lindane)

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 153159351
Conc: 40.64 ng/ml

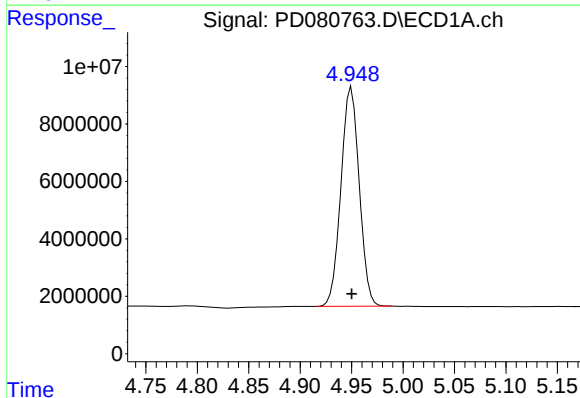


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 94499127
Conc: 40.06 ng/ml

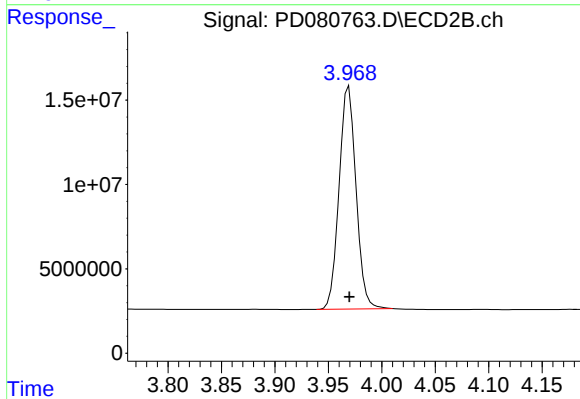

#4 Heptachlor


R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 145892603
Conc: 39.98 ng/ml

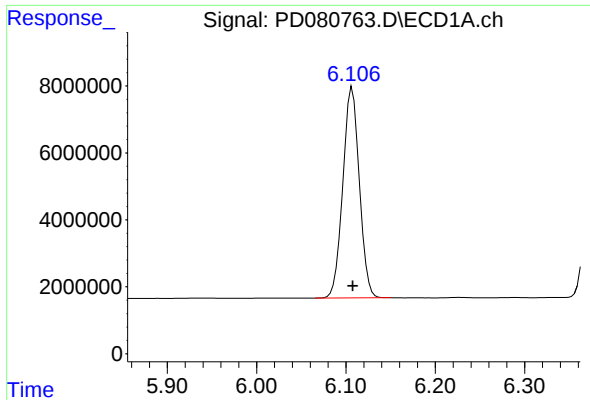

#9 Endosulfan I


R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 80646970
Conc: 39.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

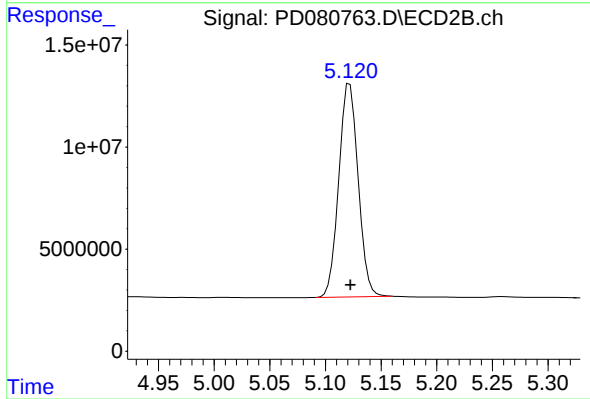


#9 Endosulfan I

R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 126643433
Conc: 39.57 ng/ml

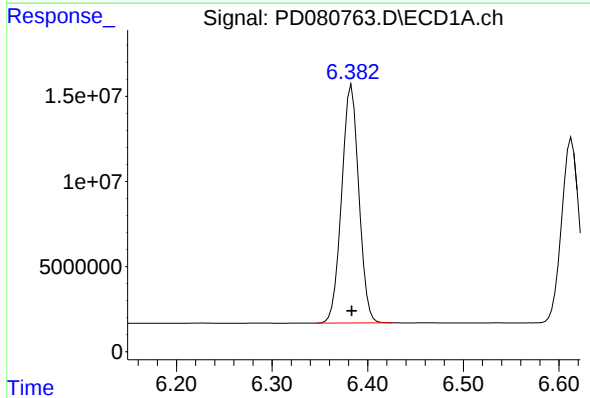


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 174983465
Conc: 81.13 ng/ml

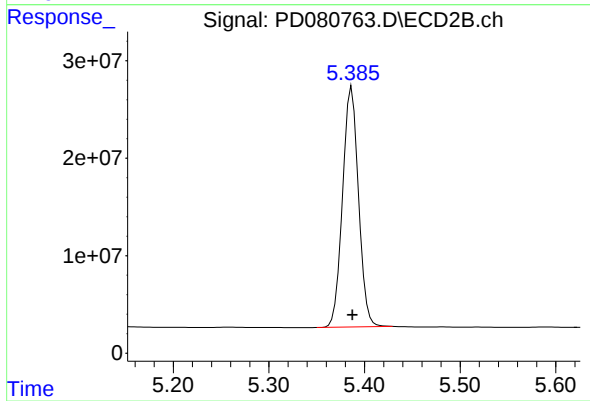

#13 Dieldrin


R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 286545214
Conc: 80.62 ng/ml

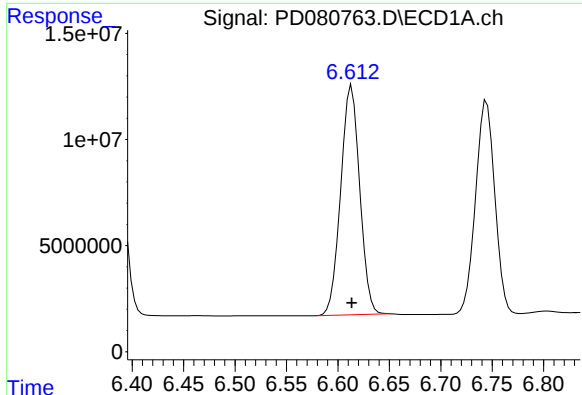

#14 Endrin


R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 139060217
Conc: 79.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

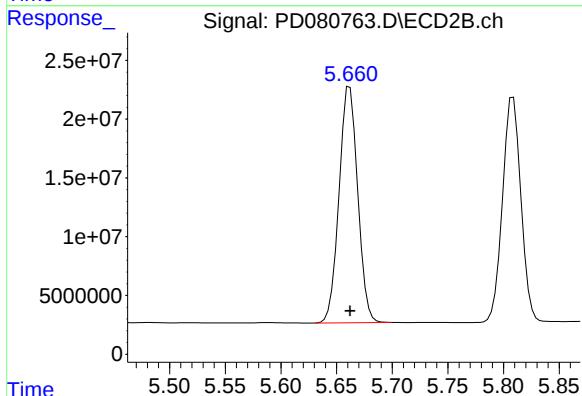


#14 Endrin

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 234489654
Conc: 78.56 ng/ml

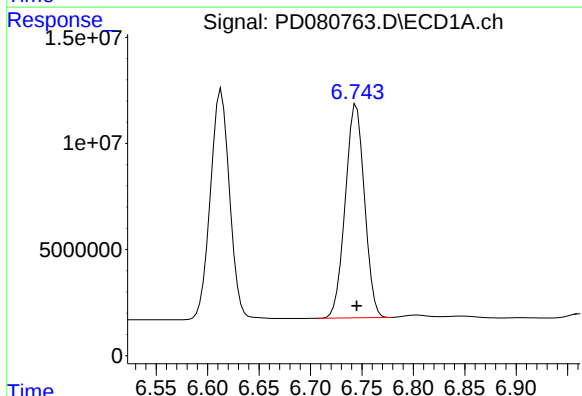


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 130850633
Conc: 80.45 ng/ml

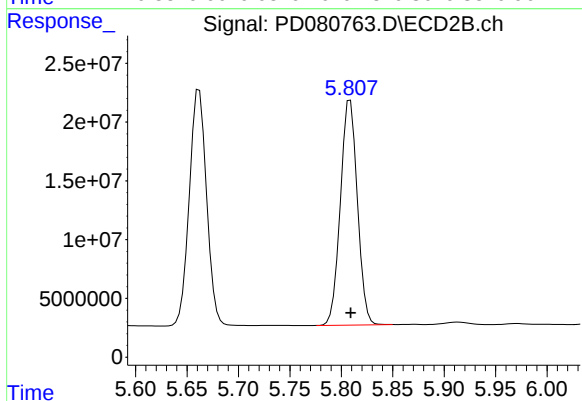

#16 4,4'-DDD


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 219984646
Conc: 80.22 ng/ml

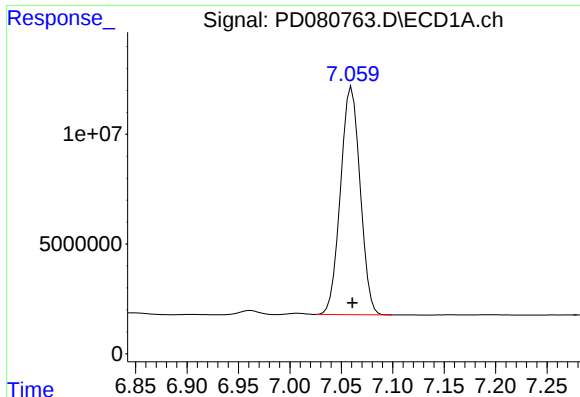

#17 4,4'-DDT


R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 137870851
Conc: 82.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

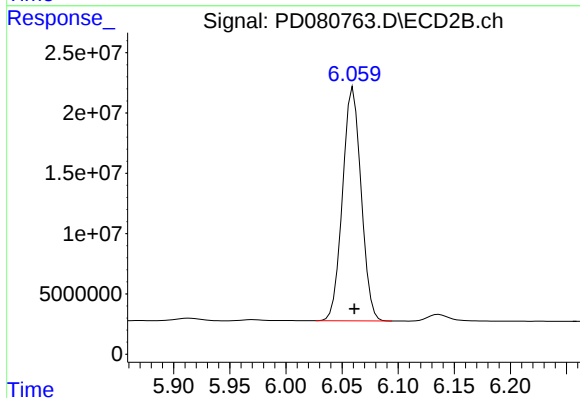


#17 4,4'-DDT

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 222717809
Conc: 81.55 ng/ml

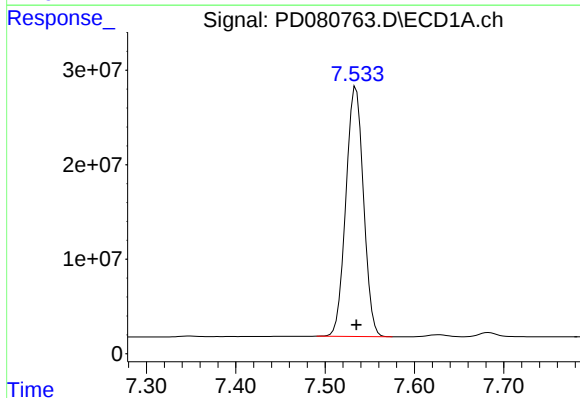


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 361602560
Conc: 391.52 ng/ml

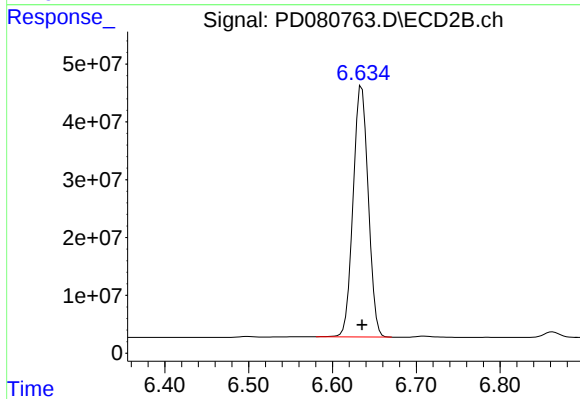

#20 Methoxychlor


R.T.: 6.635 min
Delta R.T.: 0.000 min
Response: 546460839
Conc: 376.59 ng/ml

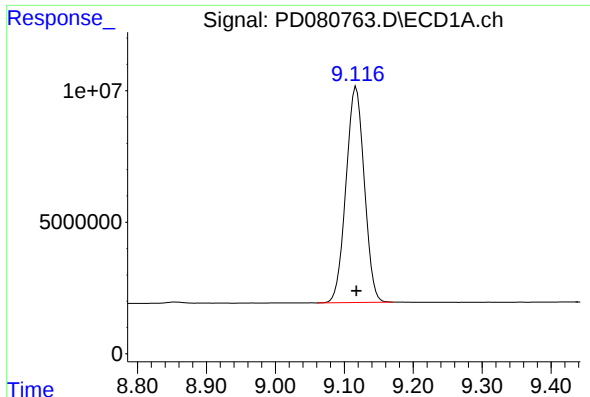

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 151301235
Conc: 75.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4094

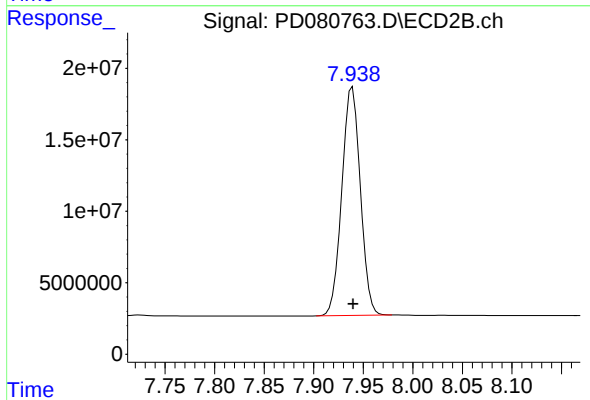

#27 Decachlorobiphenyl

R.T.: 7.939 min
Delta R.T.: 0.000 min
Response: 207843157
Conc: 76.11 ng/ml