

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
 Data File : PD080765.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jan 2024 18:34
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5096

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 04:28:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 11 04:26:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	110.1E6	191.9E6	77.421	77.851
27)	SA Decachlor...	9.118	7.938	293.3E6	410.6E6	146.126	150.358
Target Compounds							
2)	A alpha-BHC	4.023	3.299	203.4E6	338.5E6	86.934	83.955
3)	MA gamma-BHC...	4.357	3.628	191.5E6	311.6E6	85.725	82.678
4)	MA Heptachlor	4.949	3.970	193.4E6	293.6E6	81.973	80.458
9)	A Endosulfan I	6.107	5.122	161.3E6	253.6E6	78.315	79.229
13)	MA Dieldrin	6.382	5.387	359.8E6	577.4E6	166.794	162.439
14)	MA Endrin	6.613	5.662	288.1E6	476.3E6	163.961	159.570
16)	A 4,4'-DDD	6.745	5.809	269.2E6	443.7E6	165.525	161.804
17)	MA 4,4'-DDT	7.060	6.060	287.0E6	457.4E6	171.384	167.482
20)	A Methoxychlor	7.535	6.635	721.0E6	1029.9E6	780.611	709.725


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011124\
Data File : PD080765.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jan 2024 18:34
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 04:28:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 11 04:26:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

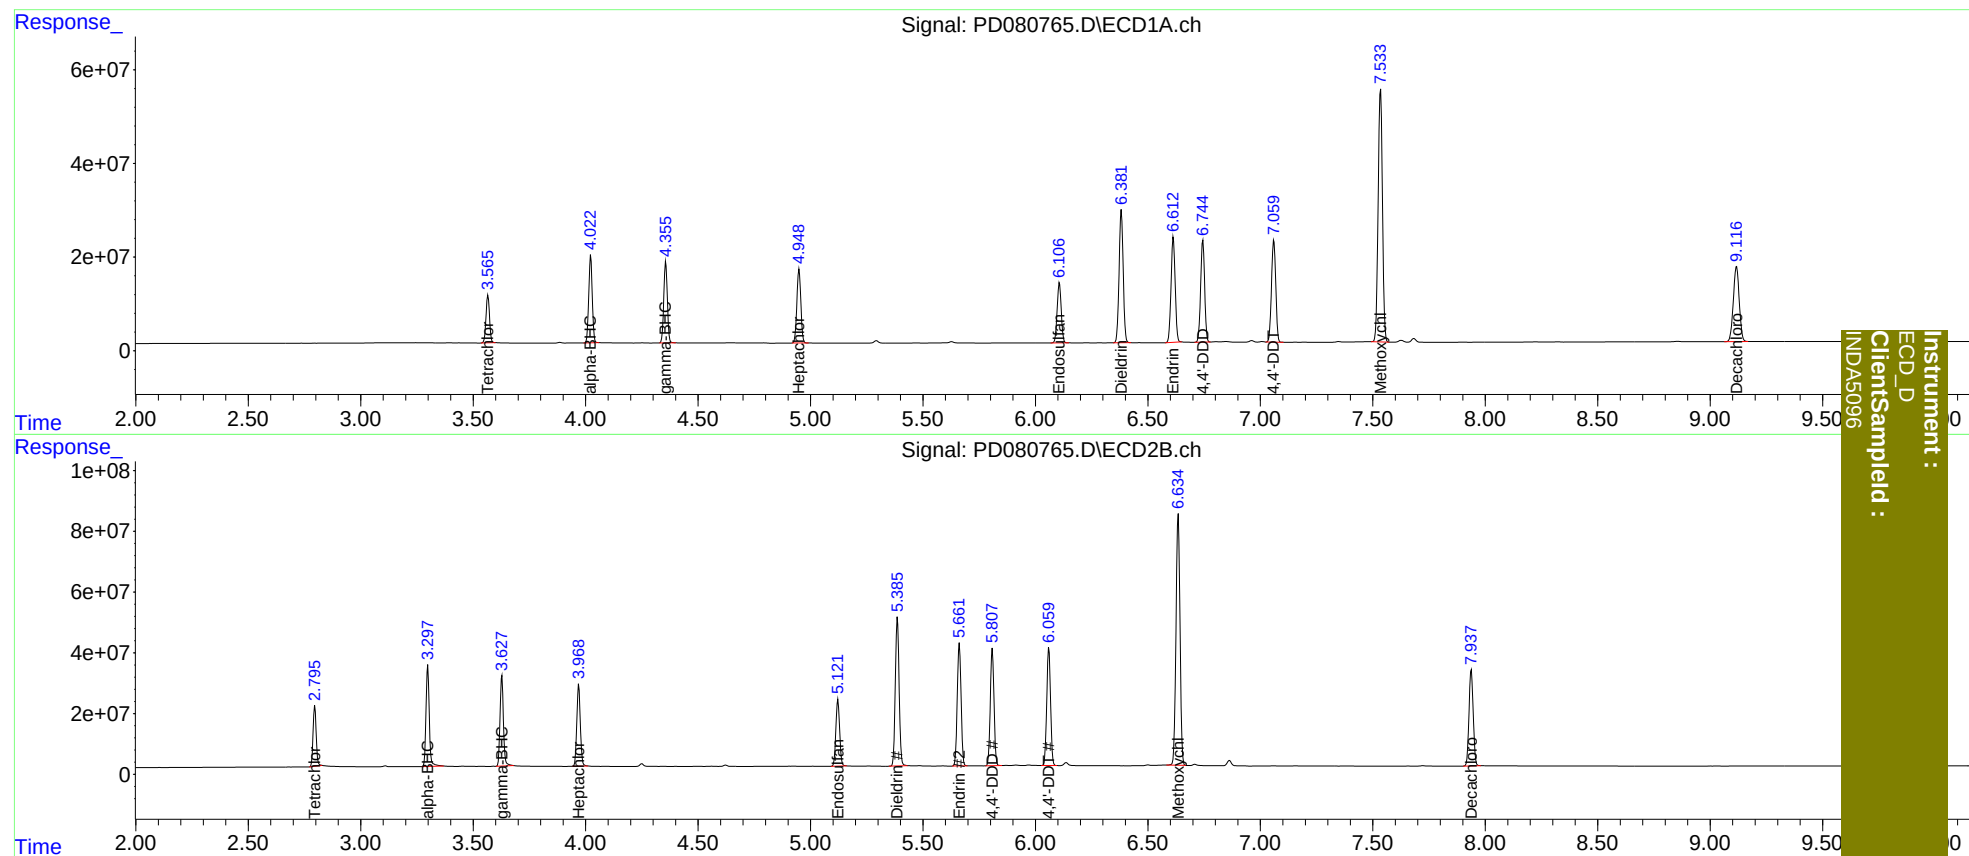


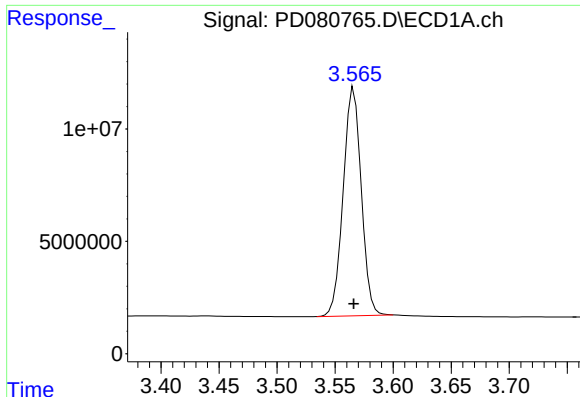

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 110064665
Conc: 77.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

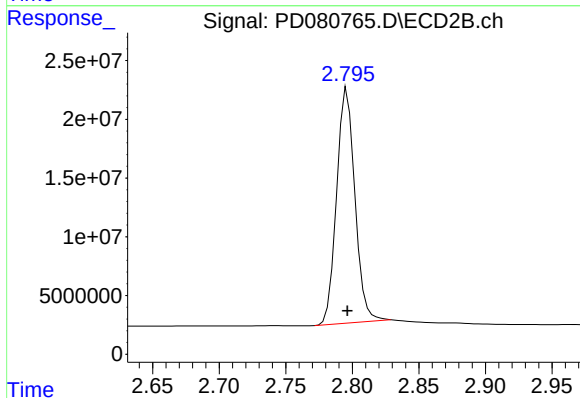


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 191937334
Conc: 77.85 ng/ml

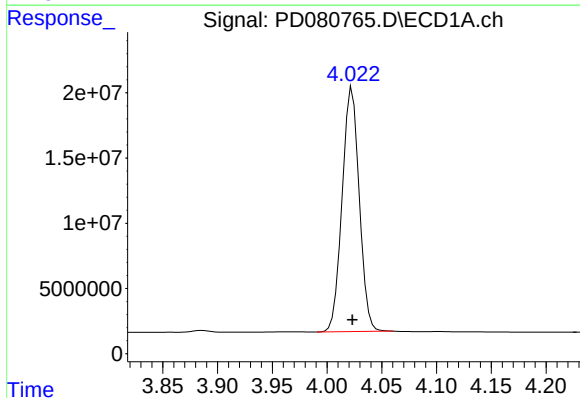


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 203414659
Conc: 86.93 ng/ml

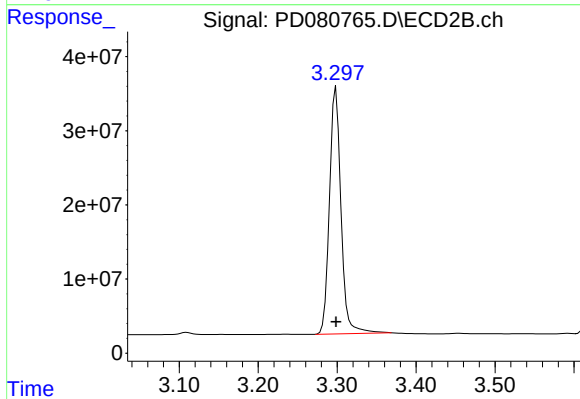

#2 alpha-BHC


R.T.: 3.299 min
Delta R.T.: 0.000 min
Response: 338476623
Conc: 83.95 ng/ml

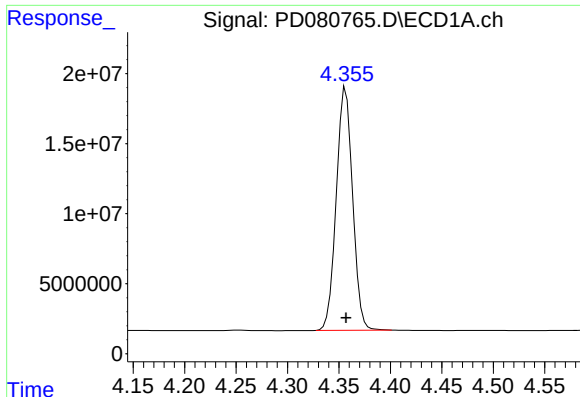

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 191527289
Conc: 85.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

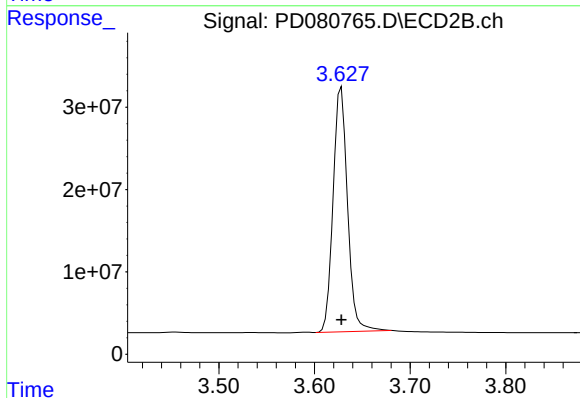


#3 gamma-BHC (Lindane)

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 311585082
Conc: 82.68 ng/ml

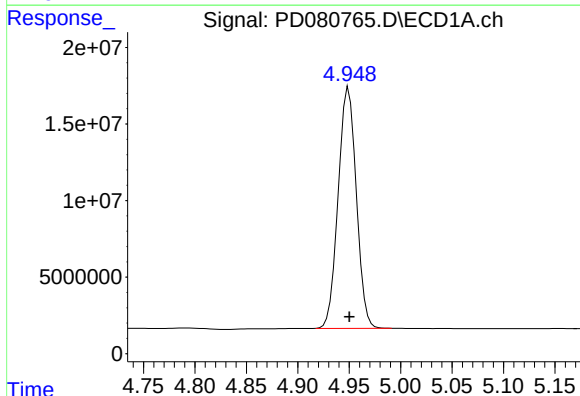


#4 Heptachlor

R.T.: 4.949 min
Delta R.T.: 0.000 min
Response: 193389402
Conc: 81.97 ng/ml

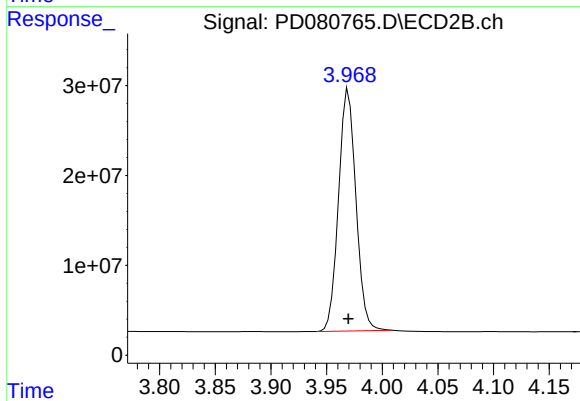

#4 Heptachlor


R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 293582073
Conc: 80.46 ng/ml

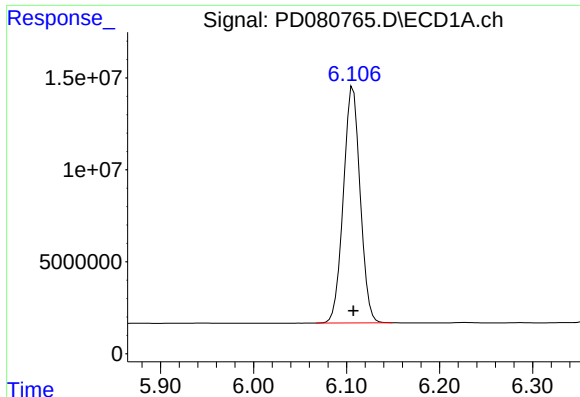

#9 Endosulfan I


R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 161251736
Conc: 78.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

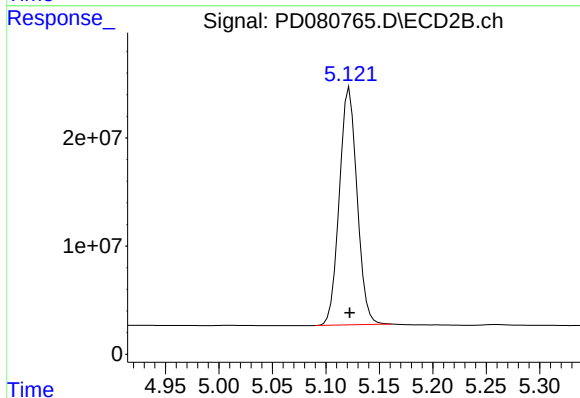


#9 Endosulfan I

R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 253596100
Conc: 79.23 ng/ml

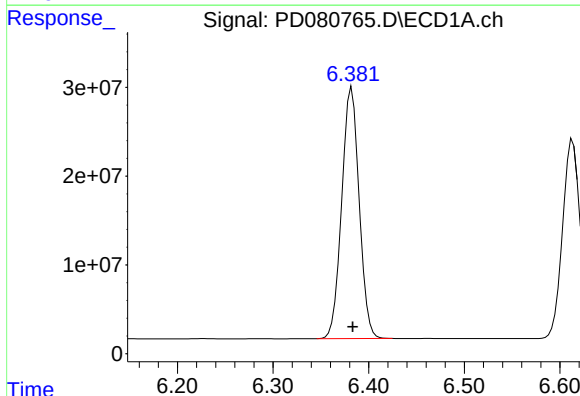


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 359751169
Conc: 166.79 ng/ml

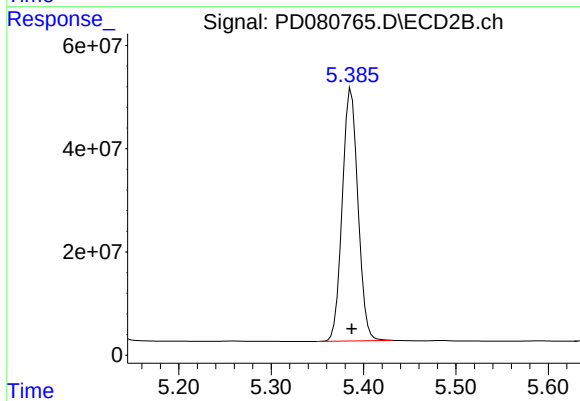

#13 Dieldrin


R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 577376359
Conc: 162.44 ng/ml

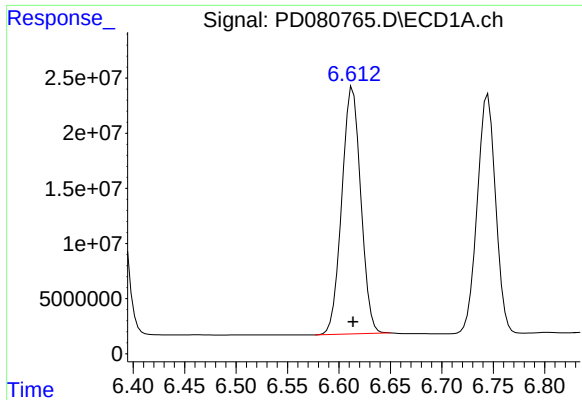

#14 Endrin


R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 288072337
Conc: 163.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

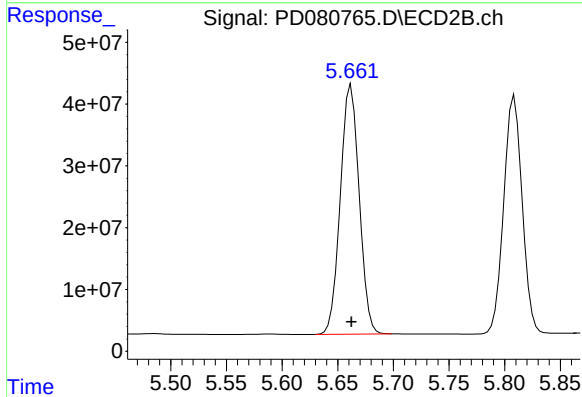


#14 Endrin

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 476292135
Conc: 159.57 ng/ml

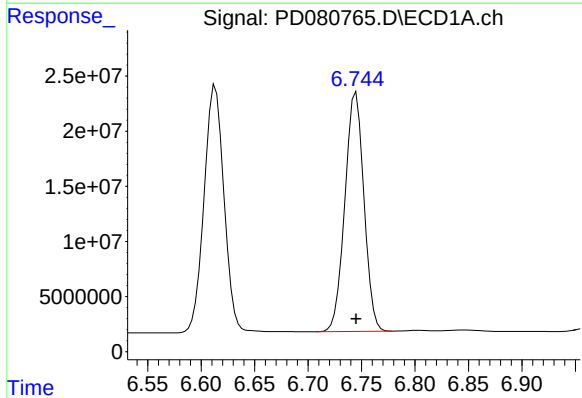


#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 269209219
Conc: 165.53 ng/ml

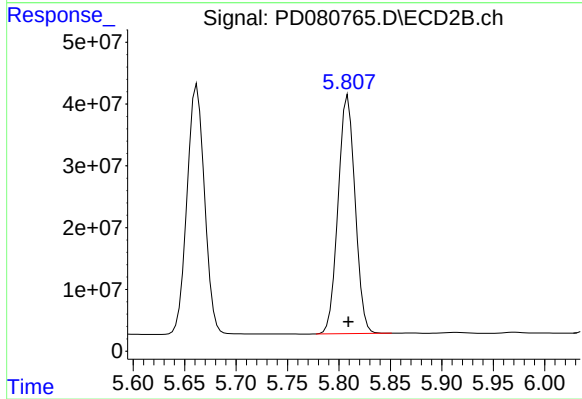

#16 4,4'-DDD


R.T.: 5.809 min
Delta R.T.: 0.000 min
Response: 443713425
Conc: 161.80 ng/ml

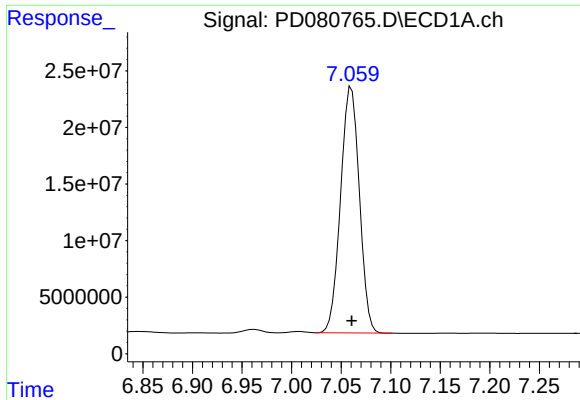

#17 4,4'-DDT


R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 286957186
Conc: 171.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

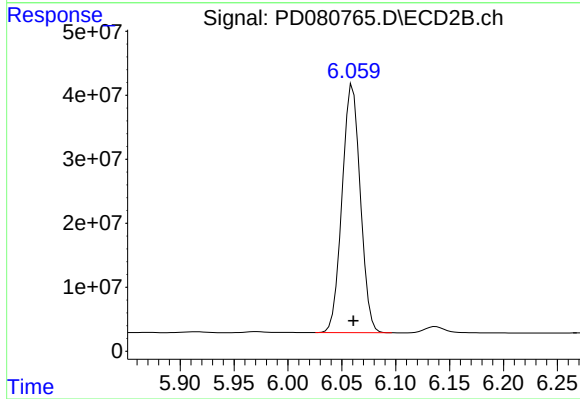


#17 4,4'-DDT

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 457383266
Conc: 167.48 ng/ml

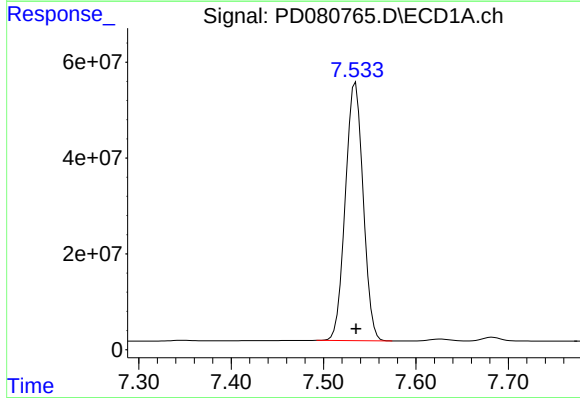


#20 Methoxychlor

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 720965576
Conc: 780.61 ng/ml

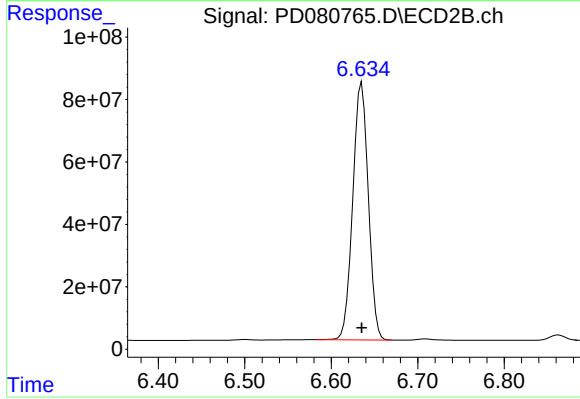

#20 Methoxychlor


R.T.: 6.635 min
Delta R.T.: 0.000 min
Response: 1029863319
Conc: 709.72 ng/ml

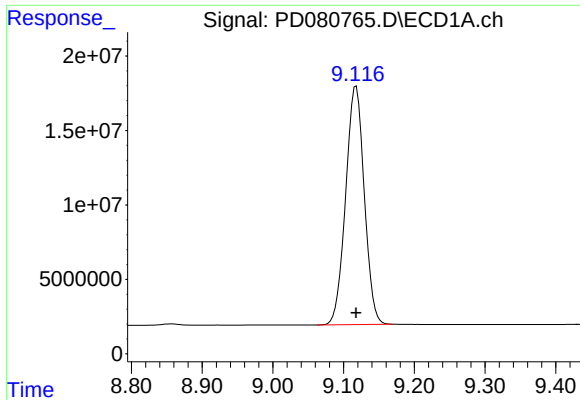

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.000 min
Response: 293335462
Conc: 146.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5096

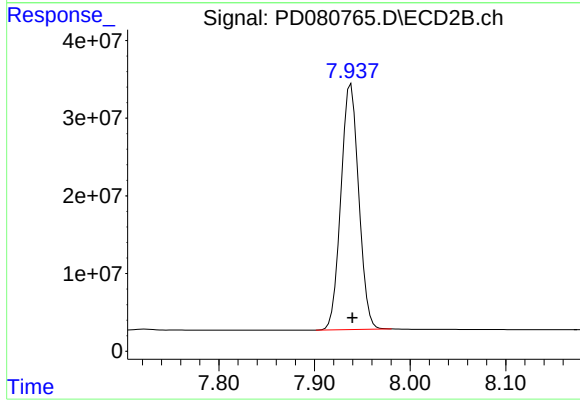

#27 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.001 min
Response: 410619033
Conc: 150.36 ng/ml