

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011221\
 Data File : PD060990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2021 12:22
 Operator : DD\AJ
 Sample : M1053-03MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFN59MSD

Manual Integrations
 APPROVED

Ankita
 1/13/2021 8:53:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 00:43:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 03:28:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	10928475	49851954	8.233	7.179
2)	SA Decachlor...	8.280	9.104	36995279	122.1E6	22.991	19.799m
Target Compounds							
3)	MA gamma-BHC...	4.224	4.697	72049909	329.8E6	38.529	33.660
4)	MA Heptachlor	4.529	5.208	74742321	339.0E6	36.911	34.471
5)	MB Aldrin	4.780	5.515	68660728	322.8E6	35.711	35.020
8)	B Heptachlo...	5.224	5.894	717242	6221050	0.397	0.757 #
9)	A Endosulfan I	5.570	6.261	3394876	3824484	1.938m	0.491m#
10)	B trans-Chl...	5.453	6.121	3156855	119.5E6	1.669	13.790 #
11)	B cis-Chlor...	5.511	6.210	4316998	33130695	2.335	4.030 #
13)	MA Dieldrin	5.809	6.515	156.8E6	586.9E6	81.297m	69.946m
14)	MA Endrin	6.069	6.736	113.9E6	417.9E6	72.022	64.351
15)	B Endosulfa...	6.345	6.929	4225048	5705765	2.955	0.919m#
16)	A 4,4'-DDD	6.187	6.854	8397526	26350132	6.004m	4.518
17)	MA 4,4'-DDT	6.436	7.154	111.3E6	430.6E6	71.484	69.731
20)	A Methoxychlor	6.967	7.598	5825448	8520249	7.622	2.992 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011221\
Data File : PD060990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2021 12:22
Operator : DD\AJ
Sample : M1053-03MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 00:43:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

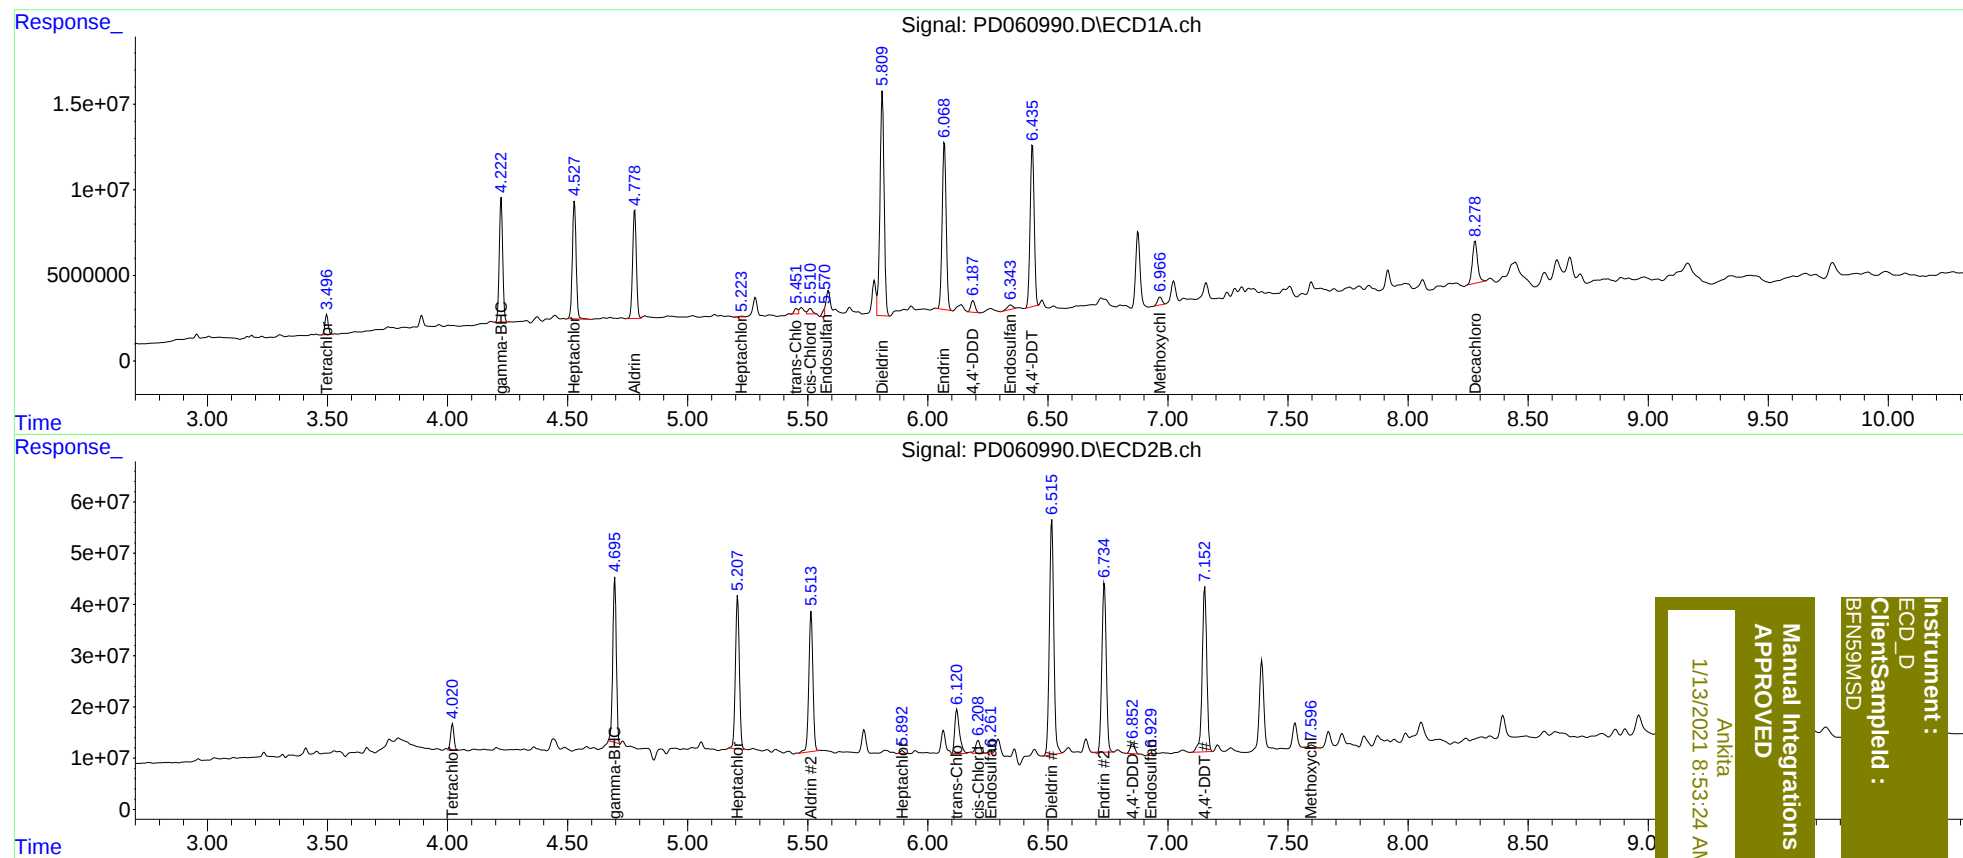

1/13/2021 8:53:24 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
BFNS6MSD