

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011223\
 Data File : PD073589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 19:57
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 01:06:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 13 00:59:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	23650597	10099657	10.213	10.255
27)	SA Decachlor...	9.100	7.934	57645913	17349796	21.847	21.795
Target Compounds							
22)	Toxaphene-1	6.262	5.013	23743399	5270533	1017.716	1077.674
23)	Toxaphene-2	6.465	5.698	30044696	5164565	998.733	1038.814
24)	Toxaphene-3	6.665	5.980	21957713	5975231	999.257	1040.904
25)	Toxaphene-4	7.176	6.615	63862423	18424721	965.679	1001.095
26)	Toxaphene-5	7.598	6.740	49005673	21443183	939.902	981.662

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011223\
Data File : PD073589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 19:57
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 01:06:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 13 00:59:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

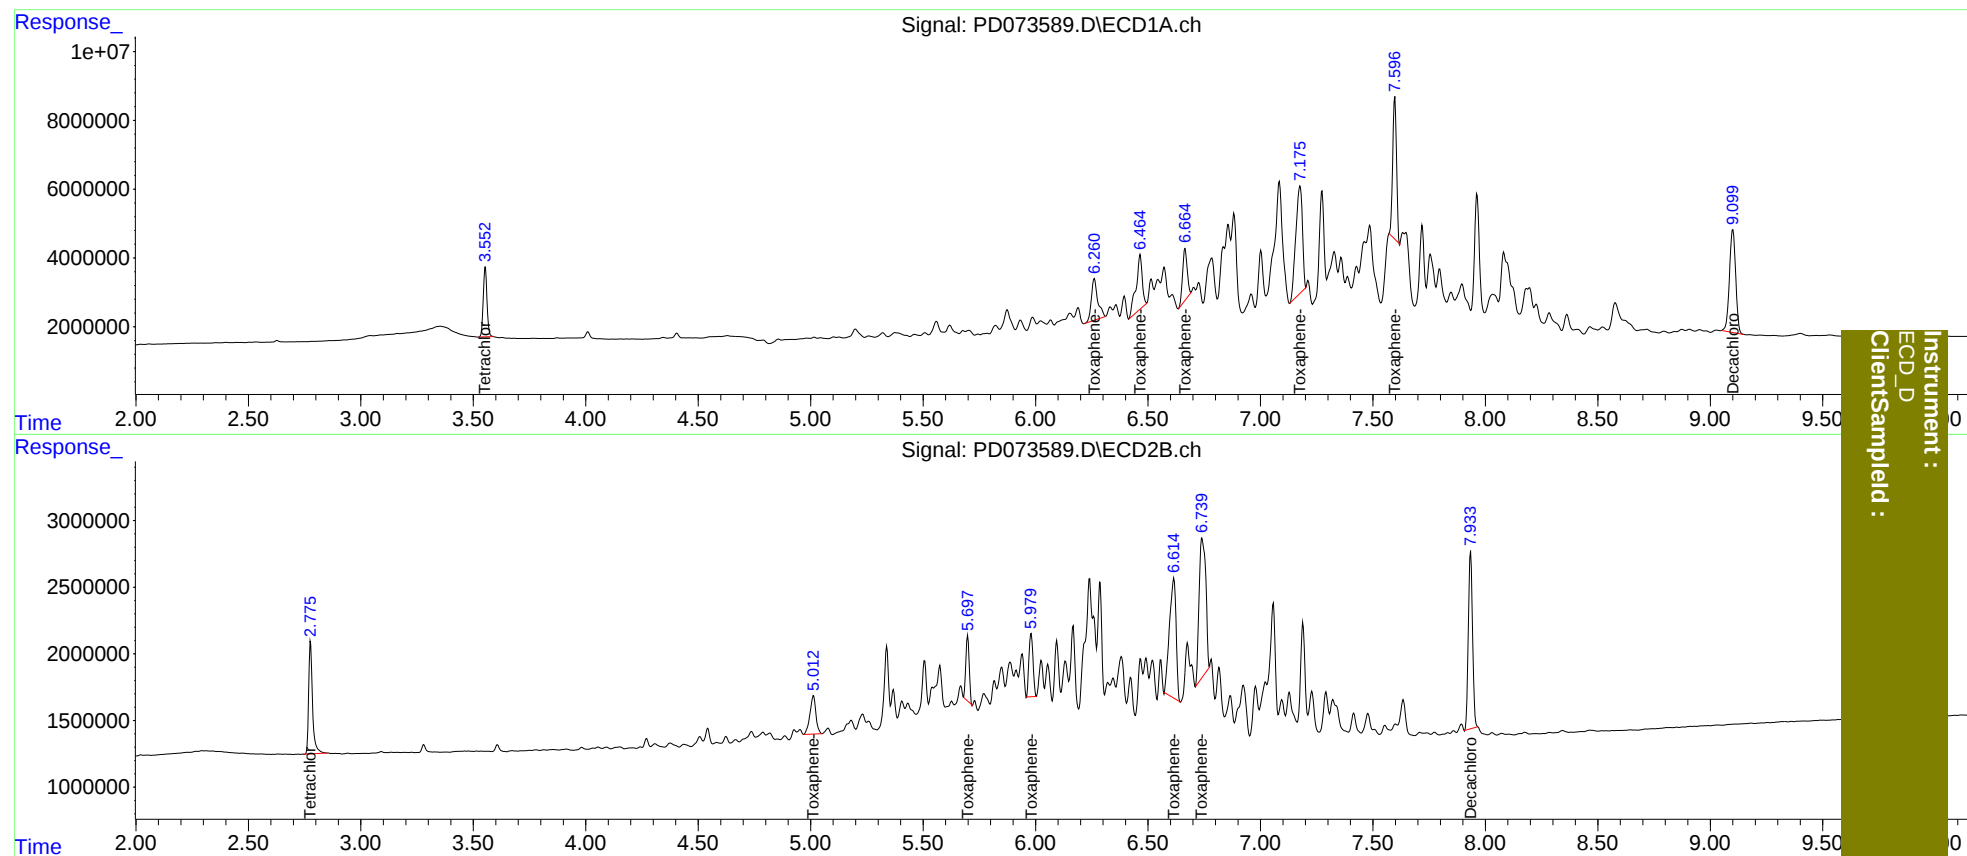

Instrument :
ECD_D
ClientSampled :
0