

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011421\
 Data File : PD061007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 15:44
 Operator : DD\AJ
 Sample : M1127-02MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC8MS

Manual Integrations
 APPROVED

Ankita
 1/29/2021 11:22:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 00:21:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 03:28:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.498	4.021	12122718	64648763	9.133	9.310
2) SA Decachlor...	8.282	9.107	13024422	79162043	8.094	12.836 #
Target Compounds						
3) MA gamma-BHC...	4.224	4.696	51178801	326.2E6	27.368	33.287m
4) MA Heptachlor	4.528	5.209	65315823	310.4E6	32.256m	31.561
5) MB Aldrin	4.780	5.516	54948138	292.4E6	28.579	31.723
13) MA Dieldrin	5.812	6.519	105.3E6	488.7E6	54.581	58.247
14) MA Endrin	6.071	6.737	87995574	372.1E6	55.656	57.305
17) MA 4,4'-DDT	6.437	7.155	82643222	339.5E6	53.058	54.976

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011421\
Data File : PD061007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 15:44
Operator : DD\AJ
Sample : M1127-02MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 00:21:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

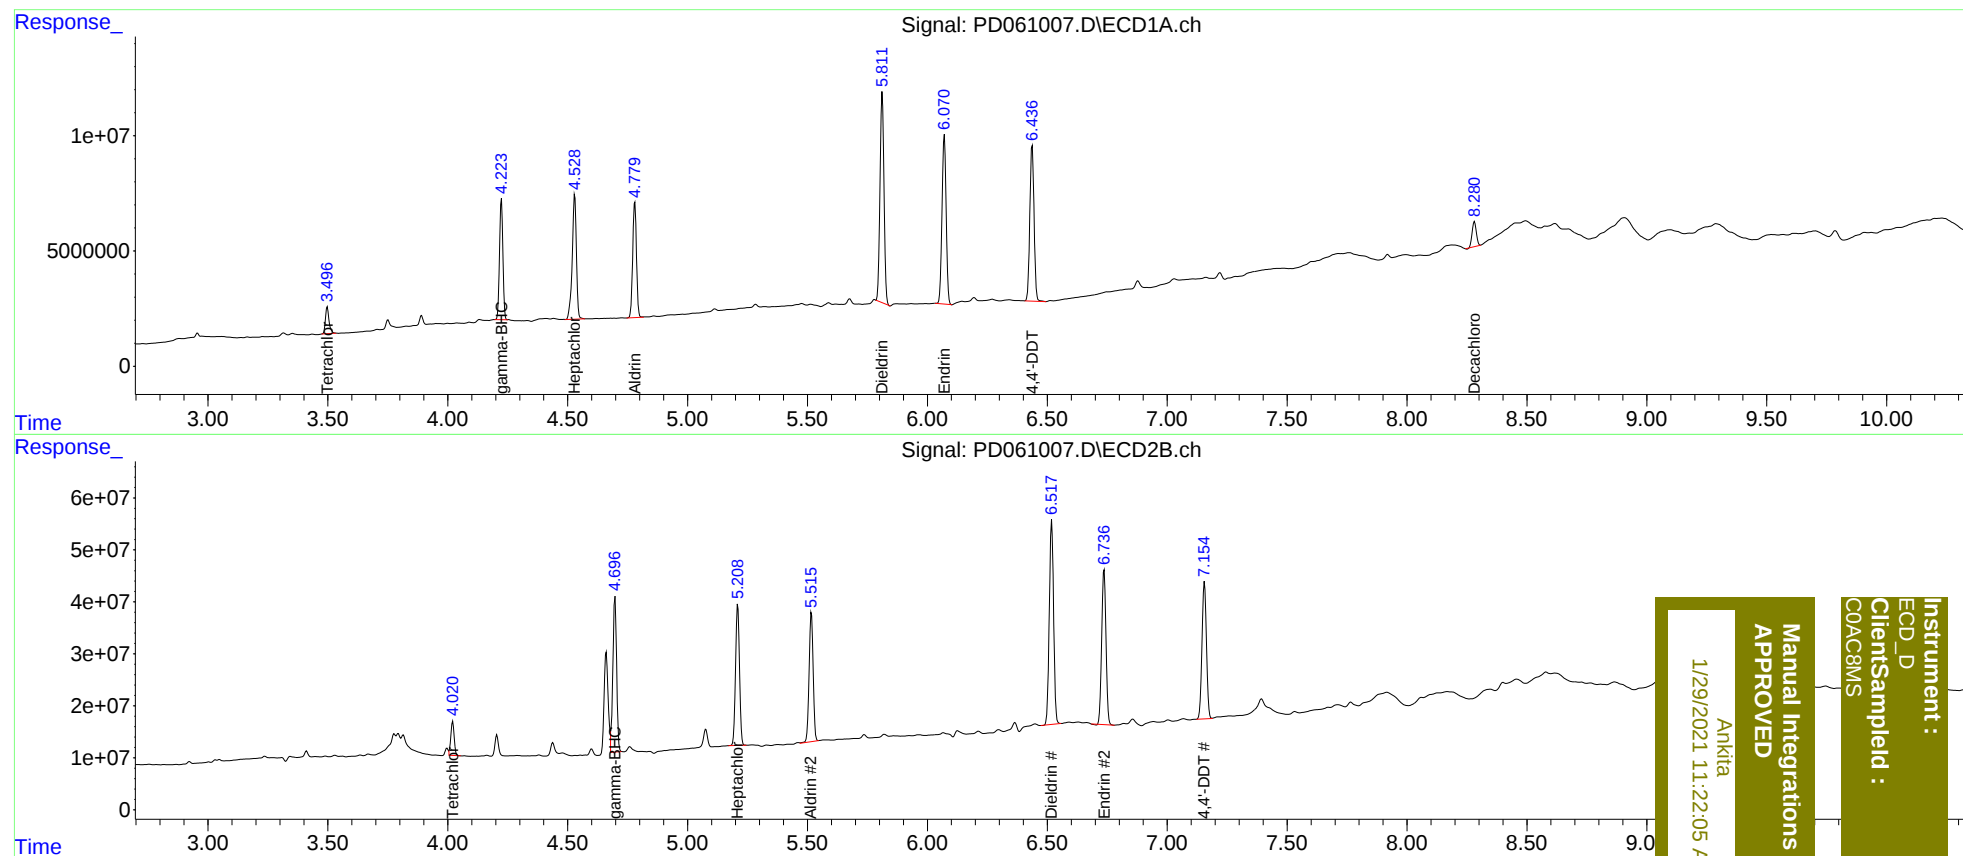

1/29/2021 11:22:05 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
COAC8MS