

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011624\
 Data File : PD080795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2024 18:04
 Operator : AR\AJ
 Sample : P1142-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AX9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/18/2024
 Supervised By :Ankita Jodhani 01/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 04:35:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.797	21317528	38725842	14.981	15.166
27)	SA Decachlor...	9.114	7.938	28010233	36383736	14.261	13.607
Target Compounds							
18)	B Endrin al...	6.943	6.131	42307363	62706041	29.378m	28.001

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011624\
Data File : PD080795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2024 18:04
Operator : AR\AJ
Sample : P1142-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 04:35:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

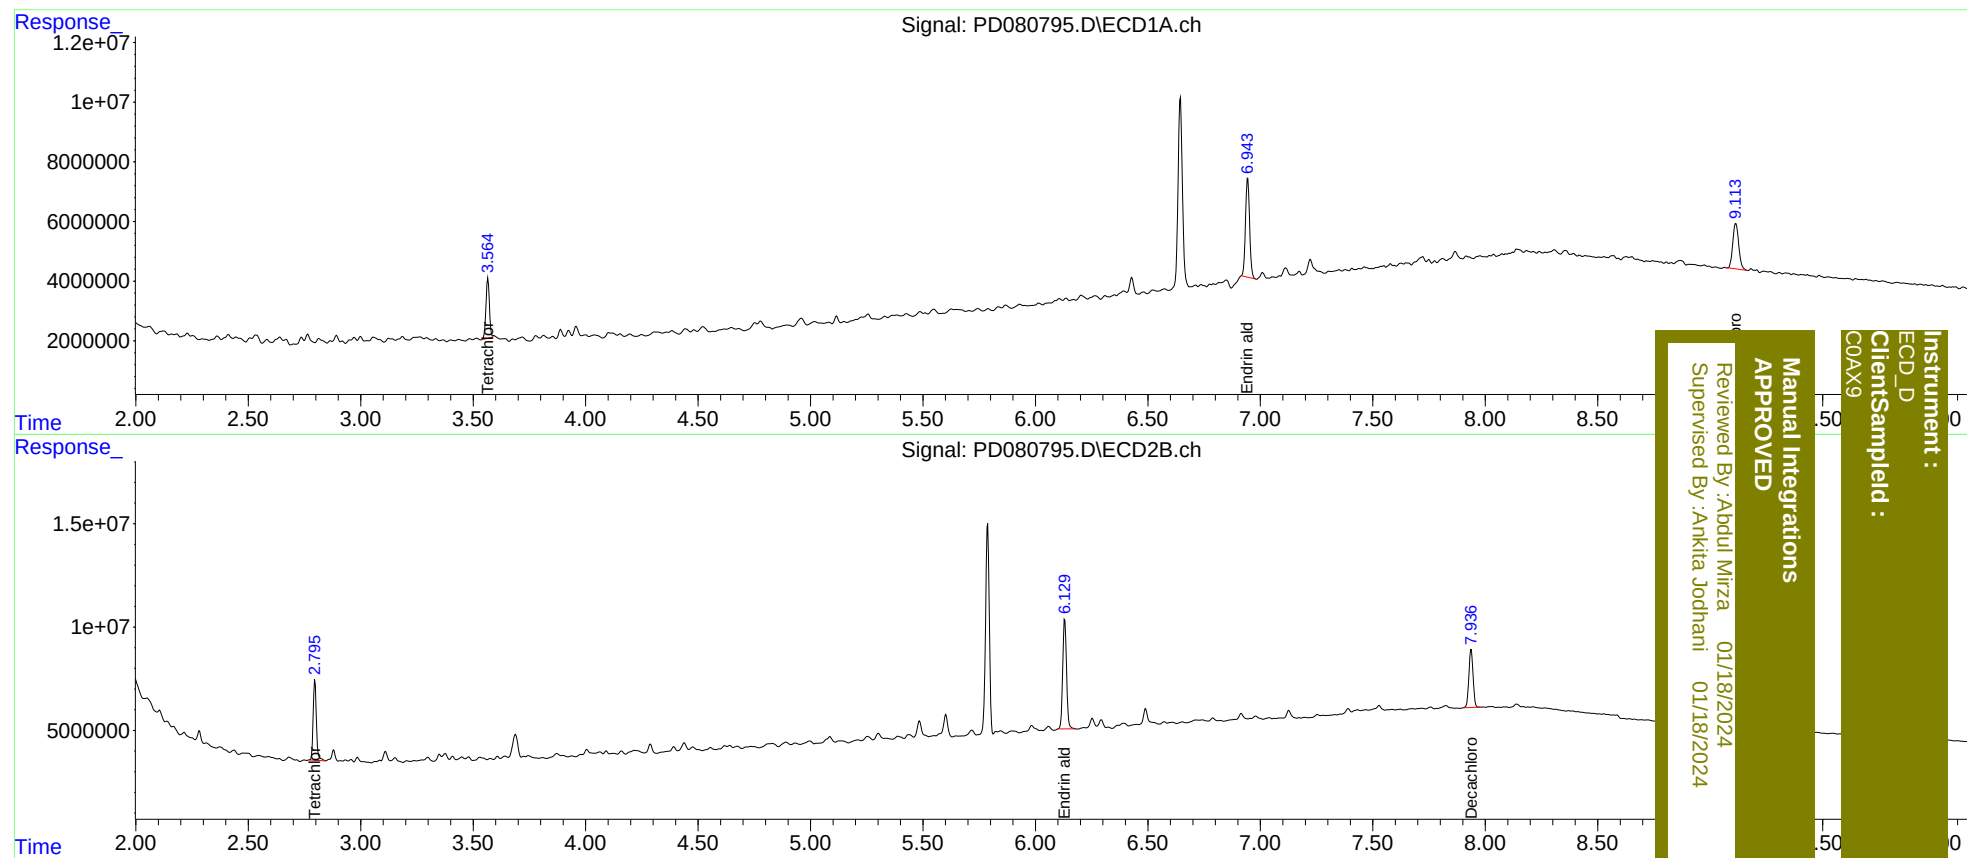

Reviewed By: Aboul Mirza 01/18/2024
Supervised By: Ankita Jodhani 01/18/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAX9