

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011625\
 Data File : PD087404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 12:10
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3051

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 12:50:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 12:50:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	40589617	246.7E6	20.000	20.000
27)	SA Decachlor...	9.088	8.085	129.5E6	570.1E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.005	3.396	81508285	393.5E6	20.000	20.000
3)	MA gamma-BHC...	4.337	3.733	78910353	364.2E6	20.000	20.000
4)	MA Heptachlor	4.937	4.089	80354026	371.0E6	20.000	20.000
9)	A Endosulfan I	6.082	5.255	68628529	316.4E6	20.000	20.000
13)	MA Dieldrin	6.356	5.521	150.2E6	664.9E6	40.000	40.000
14)	MA Endrin	6.583	5.797	127.1E6	592.6E6	40.000	40.000
16)	A 4,4'-DDD	6.713	5.938	108.1E6	533.1E6	40.000	40.000
17)	MA 4,4'-DDT	7.030	6.193	113.8E6	552.1E6	40.000	40.000
20)	A Methoxychlor	7.502	6.764	313.2E6	1235.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011625\
Data File : PD087404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 12:10
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 12:50:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 12:50:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

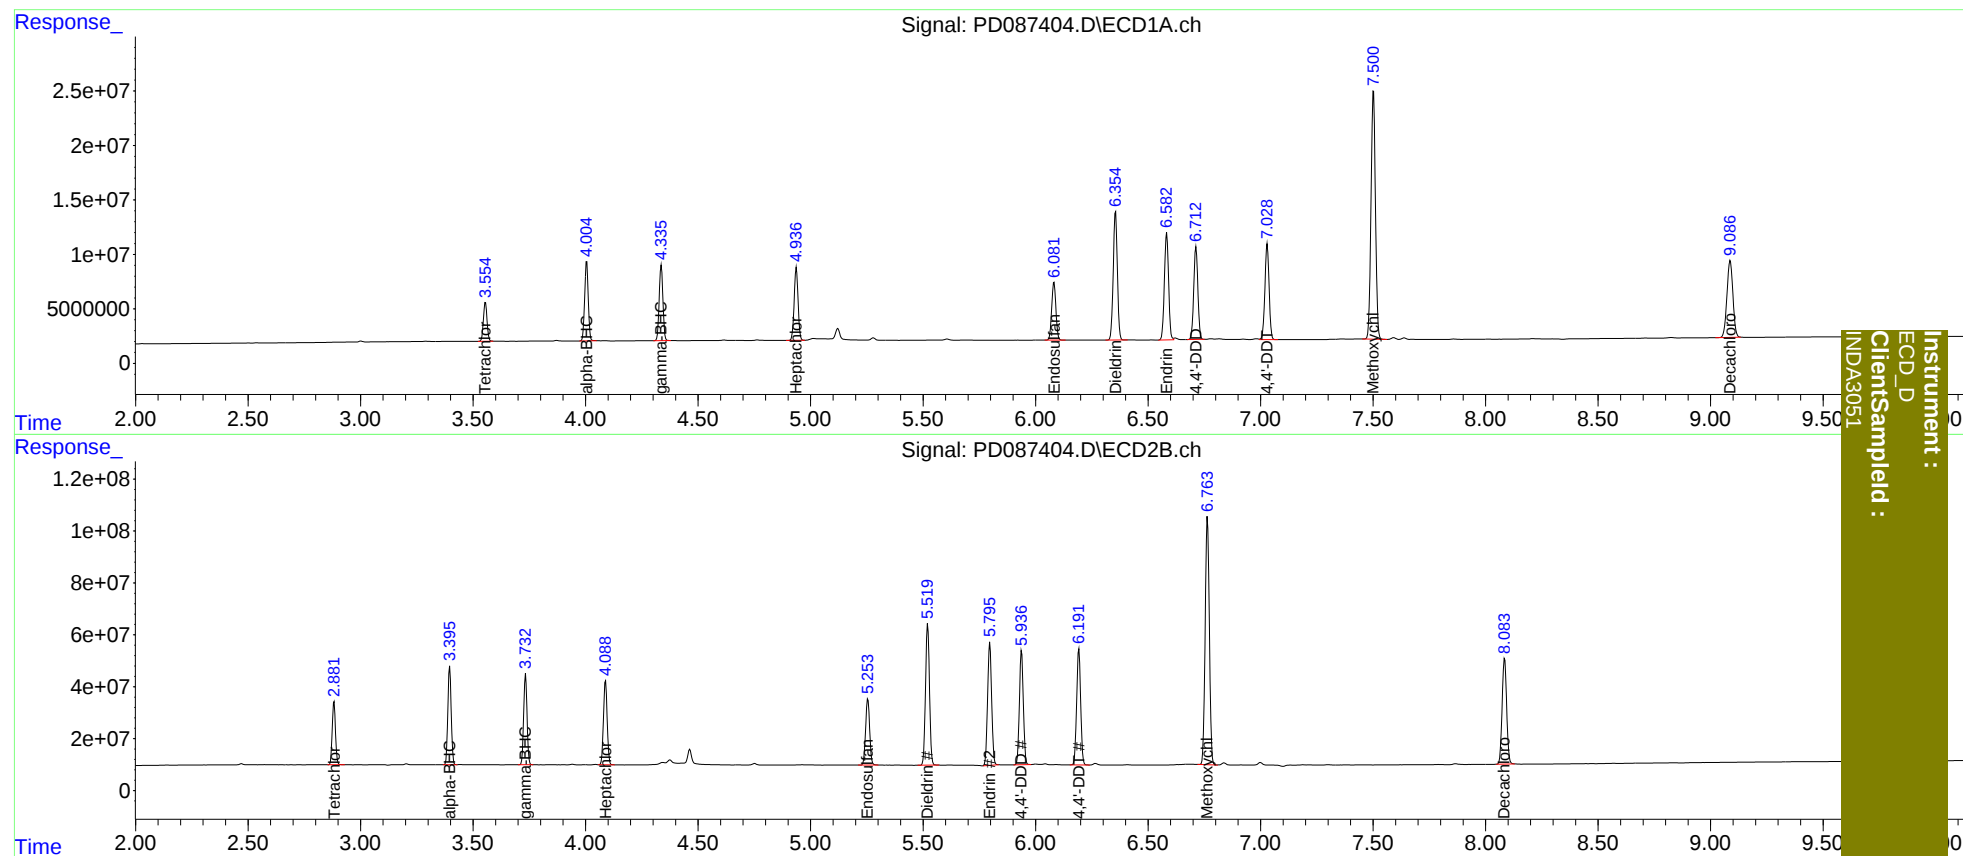


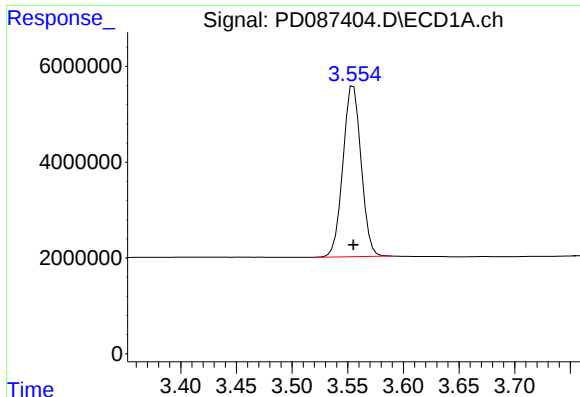

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 40589617
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

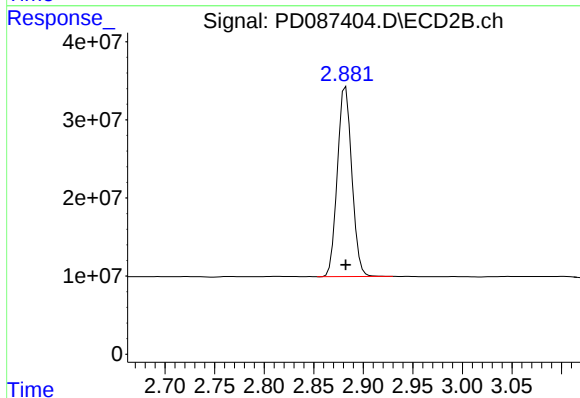


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 246704477
Conc: 20.00 ng/ml

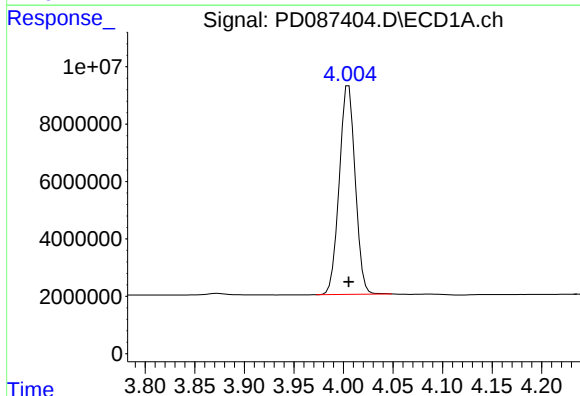


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 81508285
Conc: 20.00 ng/ml

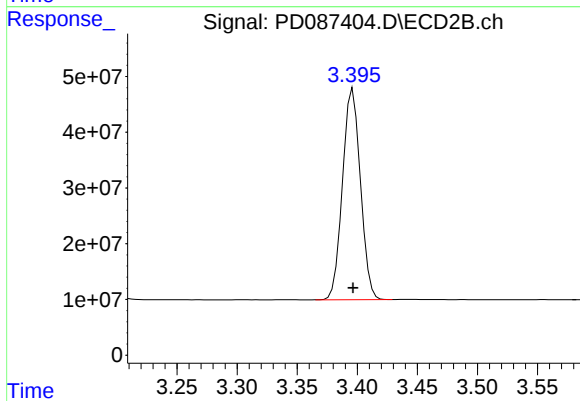

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 393511242
Conc: 20.00 ng/ml

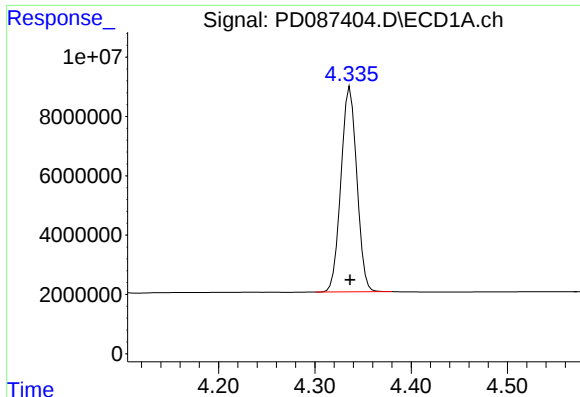

#3 gamma-BHC (Lindane)


R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 78910353
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

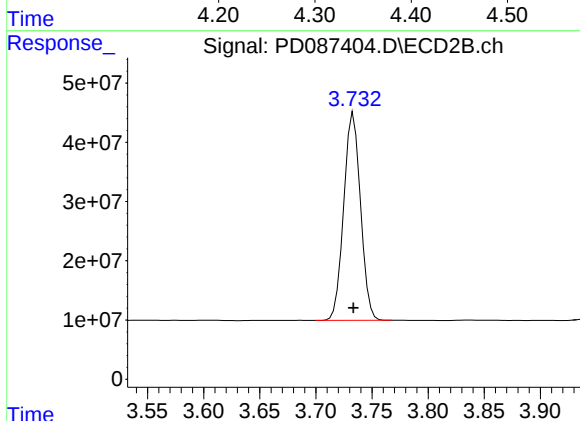


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 364165225
Conc: 20.00 ng/ml

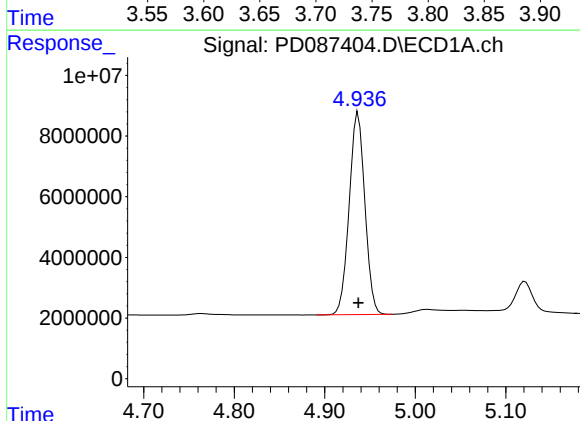


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 80354026
Conc: 20.00 ng/ml

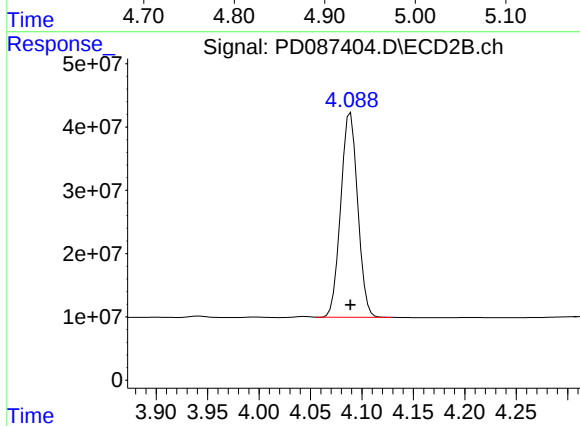

#4 Heptachlor


R.T.: 4.089 min
Delta R.T.: 0.000 min
Response: 370968343
Conc: 20.00 ng/ml

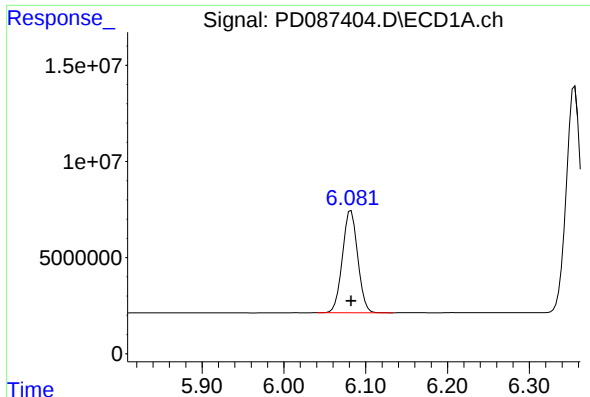

#9 Endosulfan I


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 68628529
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

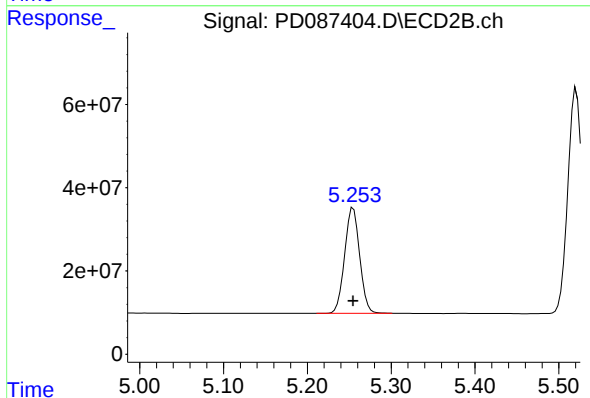


#9 Endosulfan I

R.T.: 5.255 min
Delta R.T.: 0.000 min
Response: 316428704
Conc: 20.00 ng/ml

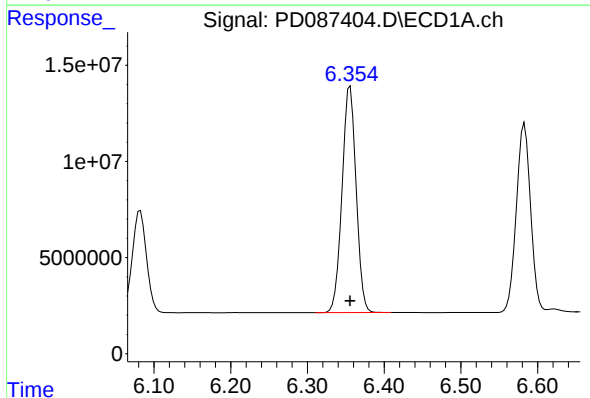


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 150216158
Conc: 40.00 ng/ml

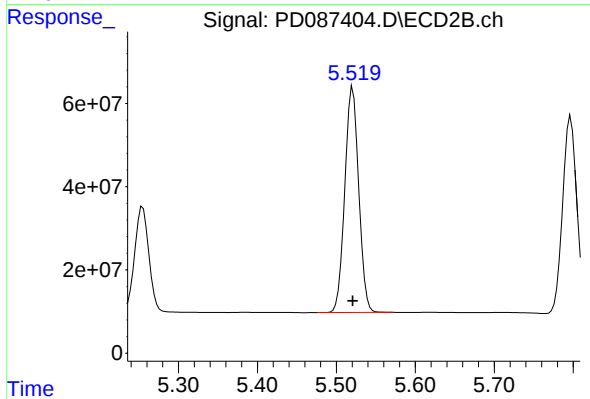

#13 Dieldrin


R.T.: 5.521 min
Delta R.T.: 0.000 min
Response: 664934154
Conc: 40.00 ng/ml

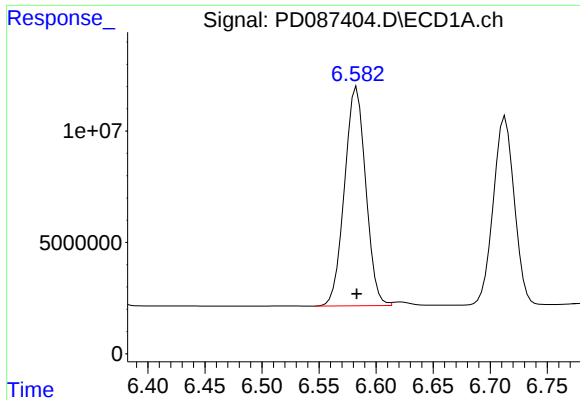

#14 Endrin


R.T.: 6.583 min
Delta R.T.: 0.000 min
Response: 127063844
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

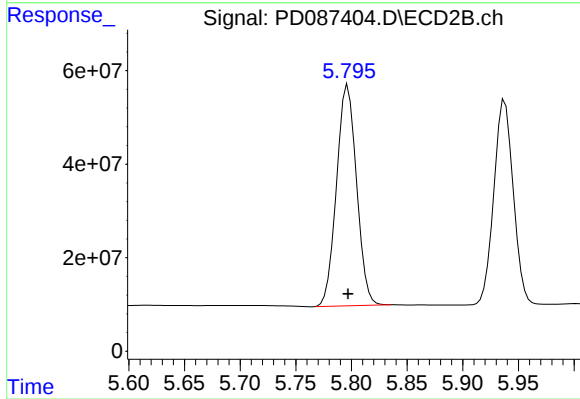


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 592588545
Conc: 40.00 ng/ml

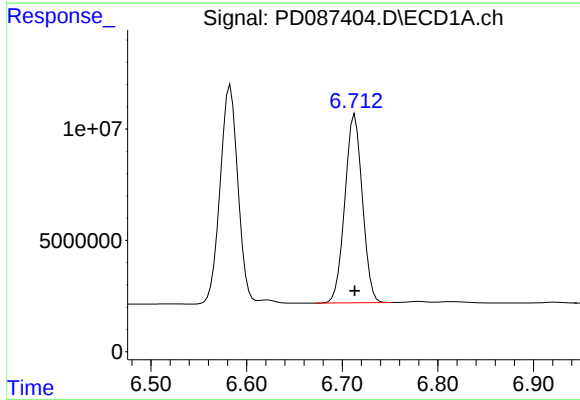


#16 4,4'-DDD

R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 108084611
Conc: 40.00 ng/ml

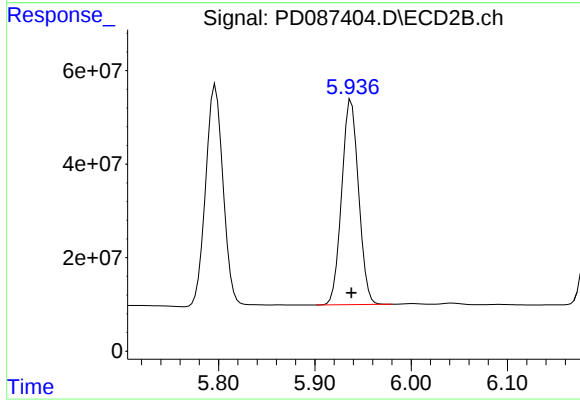

#16 4,4'-DDD


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 533128203
Conc: 40.00 ng/ml

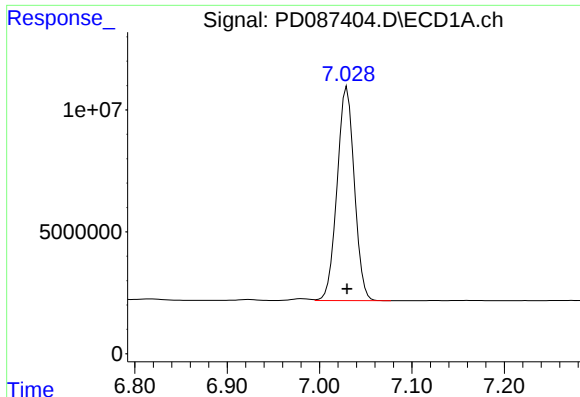

#17 4,4'-DDT


R.T.: 7.030 min
Delta R.T.: 0.000 min
Response: 113763236
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

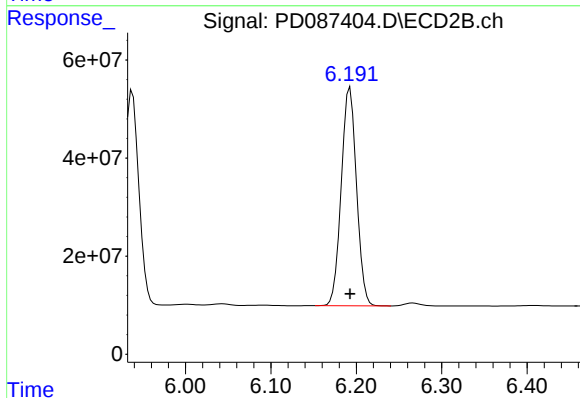


#17 4,4'-DDT

R.T.: 6.193 min
Delta R.T.: 0.000 min
Response: 552133581
Conc: 40.00 ng/ml

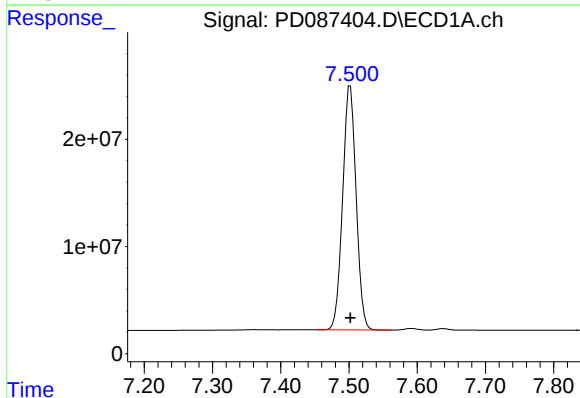


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 313212085
Conc: 200.00 ng/ml

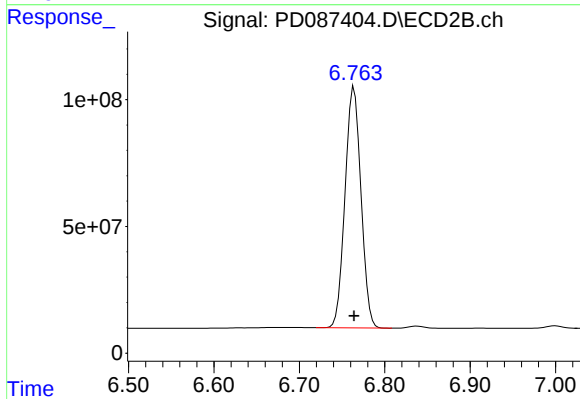

#20 Methoxychlor


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 1235220058
Conc: 200.00 ng/ml

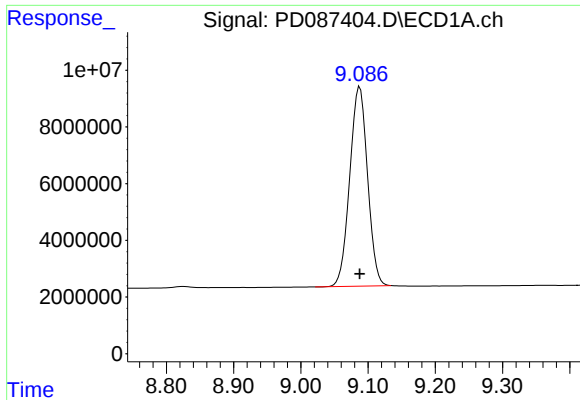

#27 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 129526917
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3051

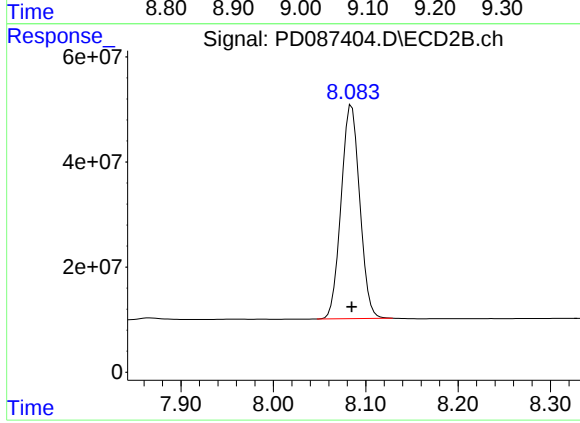

#27 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 570080392
Conc: 40.00 ng/ml