

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011719\
 Data File : PD051061.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2019 17:47
 Operator : AJ\SJ
 Sample : K1147-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Sohil
 1/18/2019 8:41:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 21:17:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 10 03:41:46 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.045	29656167	586.1E6	19.855	19.695
28)	SA Decachlor...	7.825	9.156	27200939	440.9E6	22.411m	22.097

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011719\
Data File : PD051061.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2019 17:47
Operator : AJ\SJ
Sample : K1147-06
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Sohil
1/18/2019 8:41:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 21:17:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011019.M
Quant Title : GC Extractables
QLast Update : Thu Jan 10 03:41:46 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

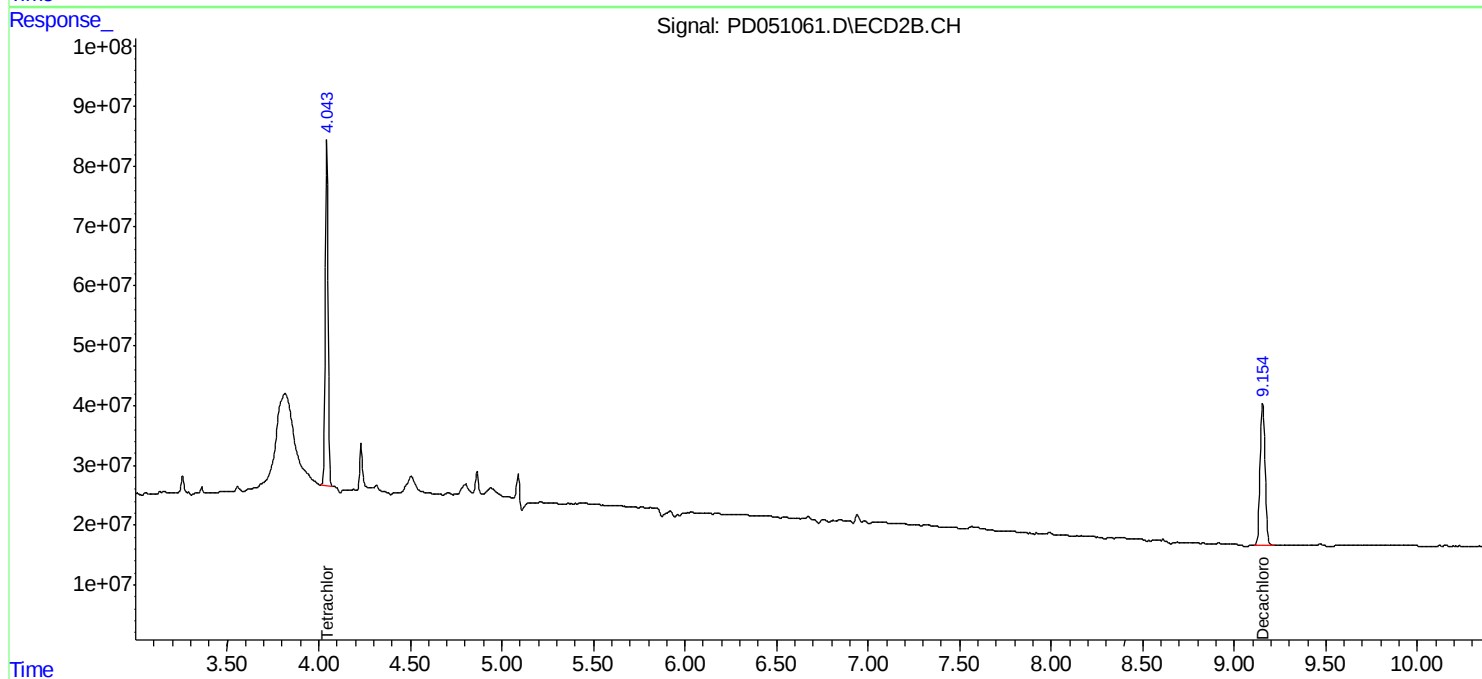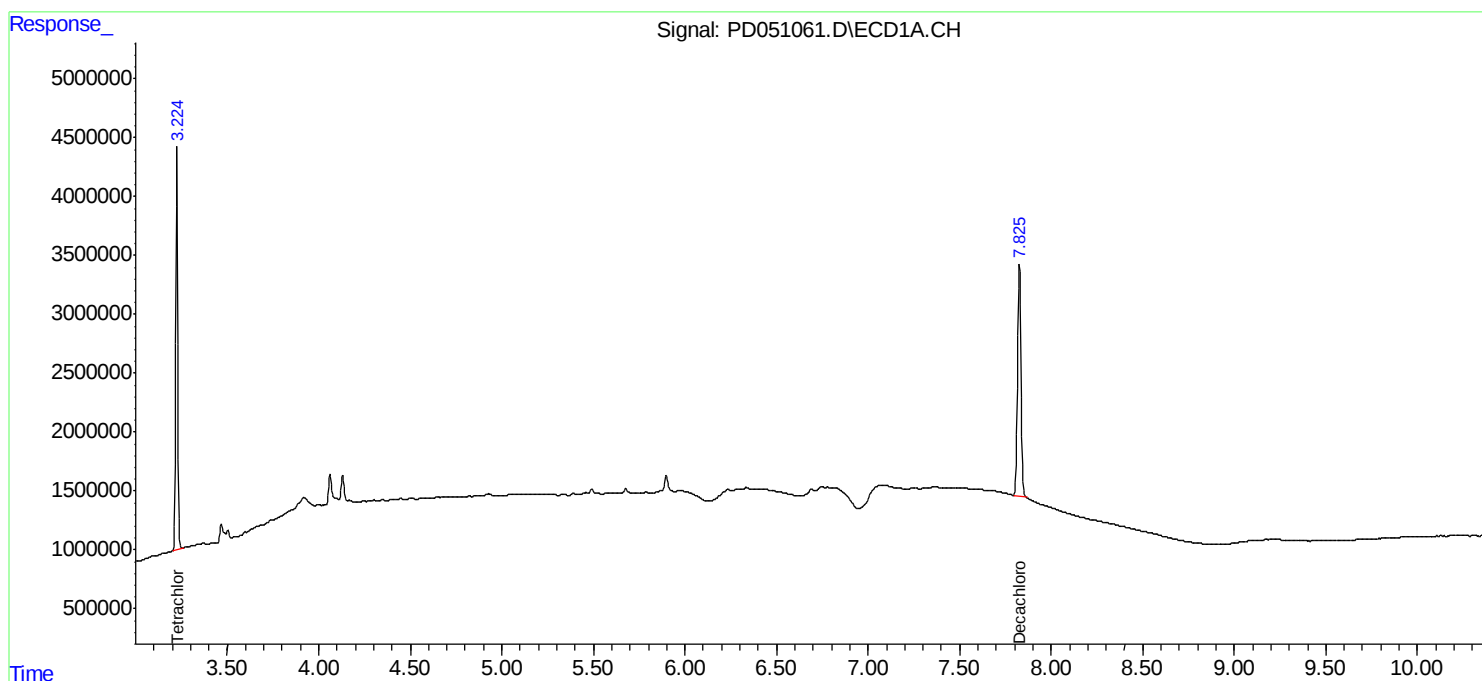

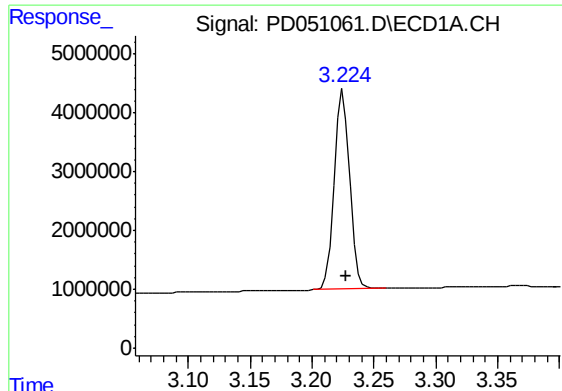


#1 Tetrachloro-m-xylene

R.T.: 3.225 min
Delta R.T.: -0.002 min
Response: 29656167
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Sohil
1/18/2019 8:41:36 AM

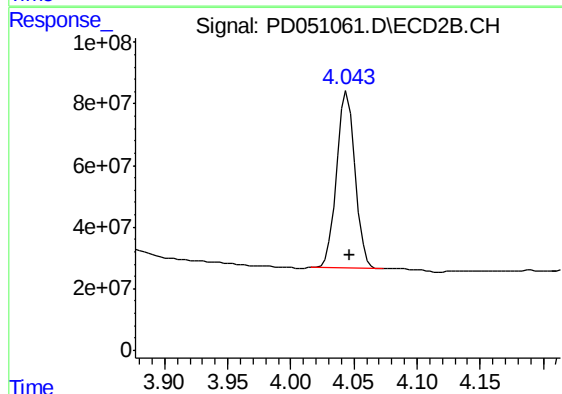


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.002 min
Response: 586114925
Conc: 19.69 ng/ml

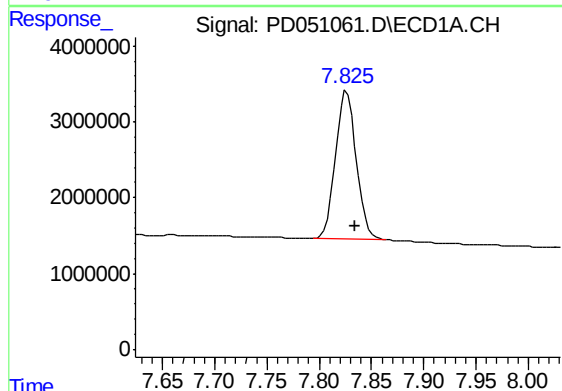

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.009 min
Response: 27200939
Conc: 22.41 ng/ml m

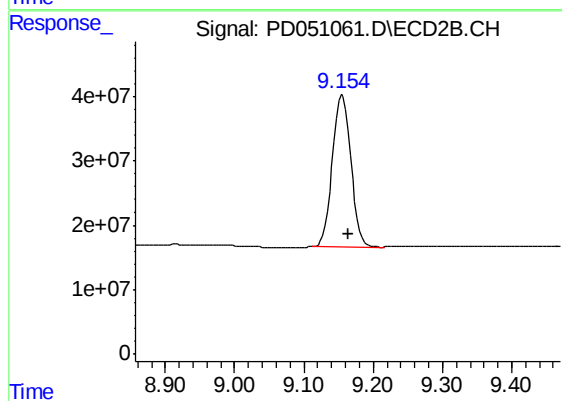

#28 Decachlorobiphenyl

R.T.: 9.156 min
Delta R.T.: -0.008 min
Response: 440925449
Conc: 22.10 ng/ml