

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
 Data File : PD087423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 17:00
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2065

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 01:34:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 17 01:33:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.556	2.883	21608850	134.9E6	10.425	10.721
27) SA Decachlor...	9.087	8.085	70793525	316.0E6	21.355	21.684
Target Compounds						
2) A alpha-BHC	4.005	3.396	40119171	209.4E6	9.662	10.395
3) MA gamma-BHC...	4.337	3.733	39520550	195.3E6	9.795	10.496
4) MA Heptachlor	4.937	4.089	41215082	202.7E6	9.983	10.648
9) A Endosulfan I	6.083	5.254	35658388	171.6E6	10.163	10.586
13) MA Dieldrin	6.356	5.521	75727010	360.7E6	19.706	21.197
14) MA Endrin	6.583	5.797	63686675	324.7E6	19.736	21.375
16) A 4,4'-DDD	6.714	5.938	54592147	289.7E6	19.757	21.143
17) MA 4,4'-DDT	7.030	6.193	56972639	292.7E6	19.643	20.753
20) A Methoxychlor	7.503	6.765	162.6E6	701.0E6	102.034	110.146

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 17:00
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 01:34:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 17 01:33:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

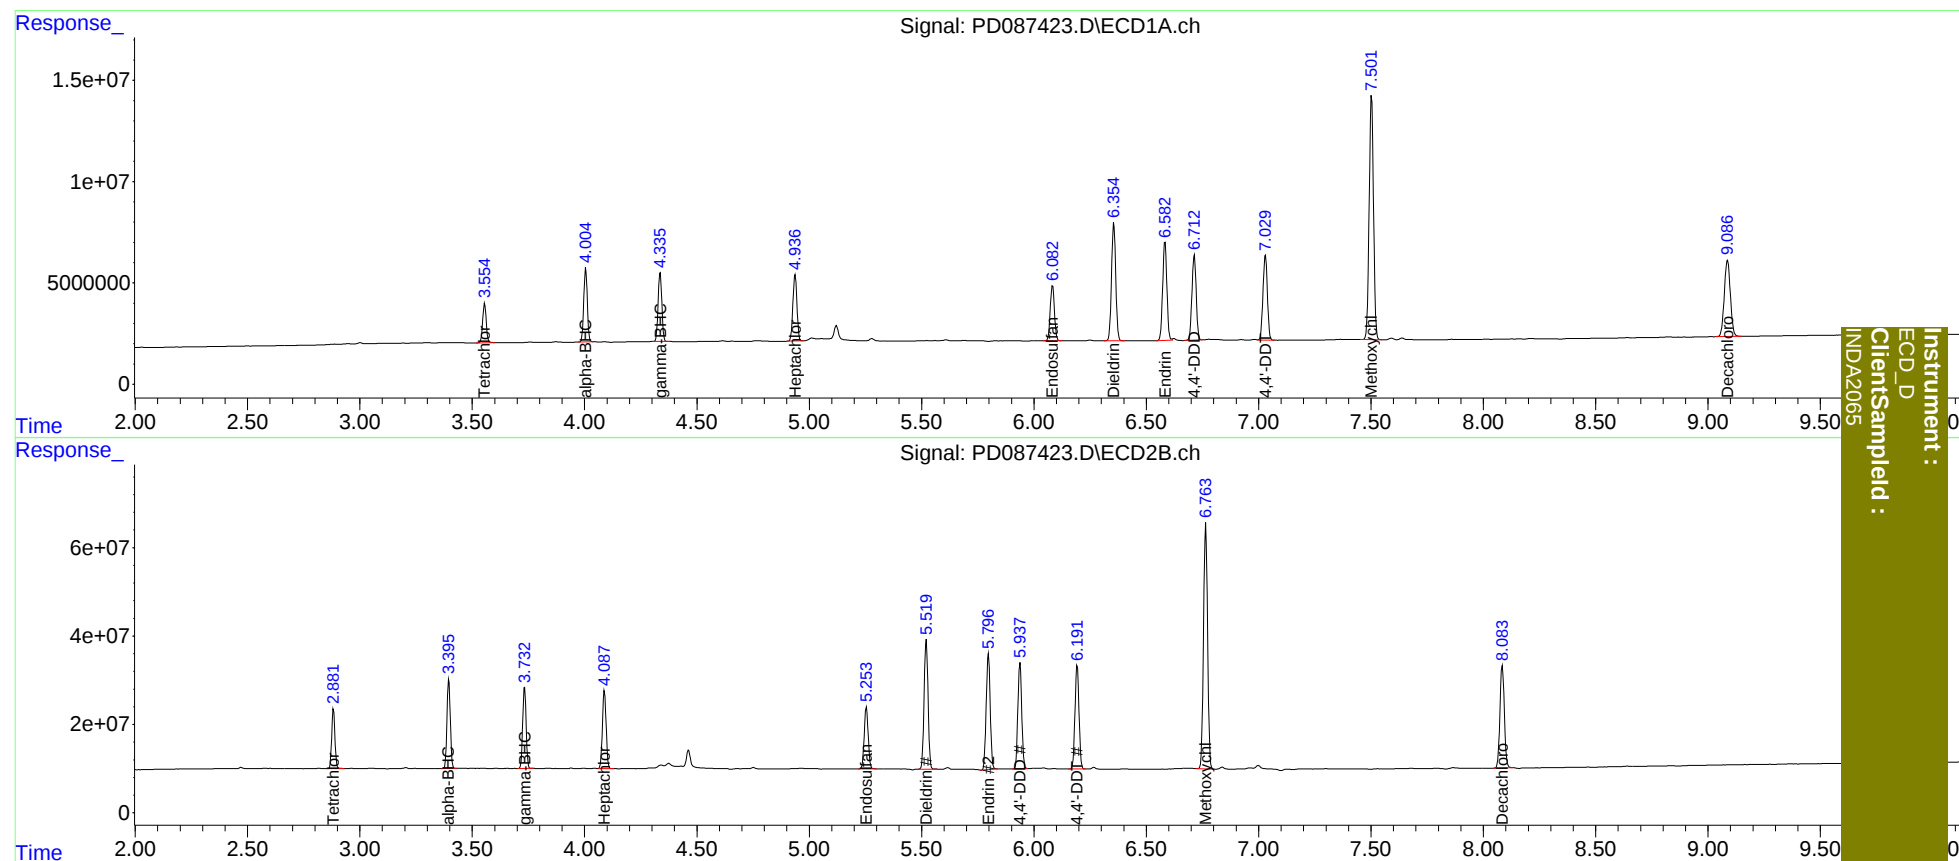

Instrument :
ECD_D
ClientSampled :
INDA2065