

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
 Data File : PD087429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 18:24
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5071

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 01:35:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 17 01:33:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	159.9E6	905.7E6	77.153	71.949
2)	SA Decachlor...	9.086	8.084	491.9E6	2095.1E6	148.394	143.761
Target Compounds							
2)	A alpha-BHC	4.005	3.396	382.3E6	1535.3E6	92.083	76.232
3)	MA gamma-BHC...	4.336	3.733	360.7E6	1404.1E6	89.395	75.446
4)	MA Heptachlor	4.937	4.088	357.5E6	1392.4E6	86.581	73.148
9)	A Endosulfan I	6.082	5.253	289.1E6	1166.2E6	82.393	71.953
13)	MA Dieldrin	6.356	5.520	665.7E6	2488.8E6	173.243	146.242
14)	MA Endrin	6.582	5.796	561.0E6	2187.6E6	173.840	144.018
16)	A 4,4'-DDD	6.713	5.937	481.2E6	1988.5E6	174.134	145.120
17)	MA 4,4'-DDT	7.029	6.192	506.6E6	2111.8E6	174.645	149.742
20)	A Methoxychlor	7.502	6.764	1259.6E6	4041.9E6	790.628	635.120

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 18:24
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 01:35:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 17 01:33:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

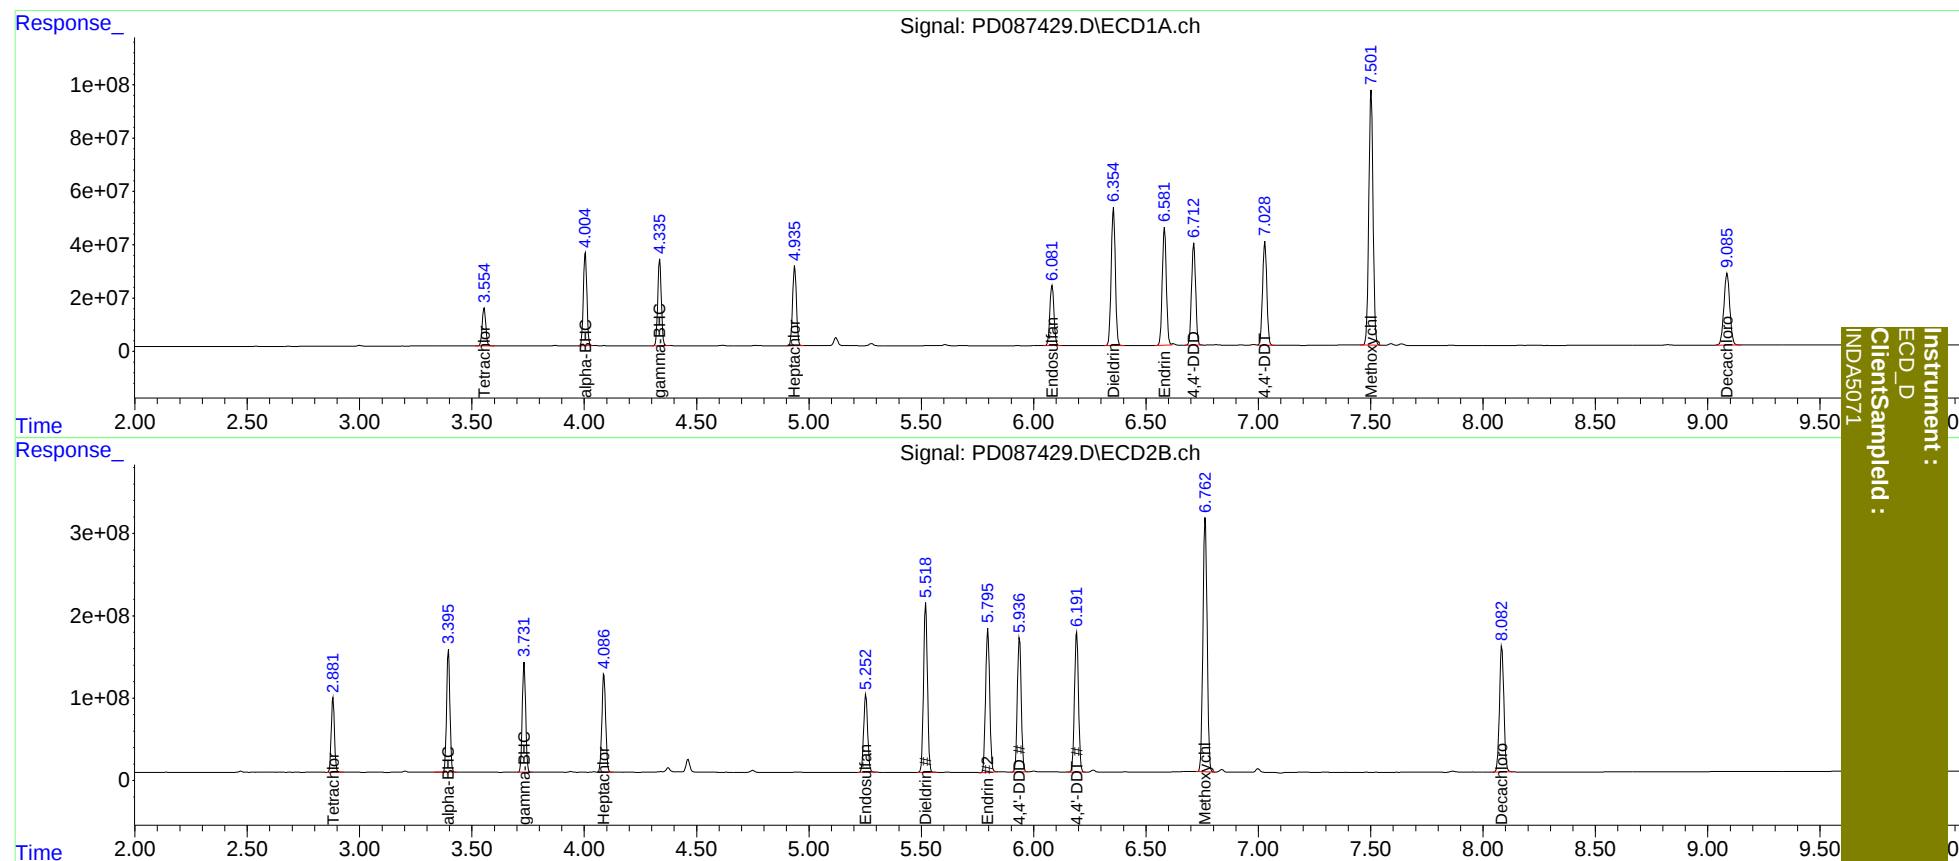

Instrument :
ECD_D
ClientSampled :
INDA5071