


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 14:39
Operator : AR\AJ
Sample : RESC057
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 04:20:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 17 04:06:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

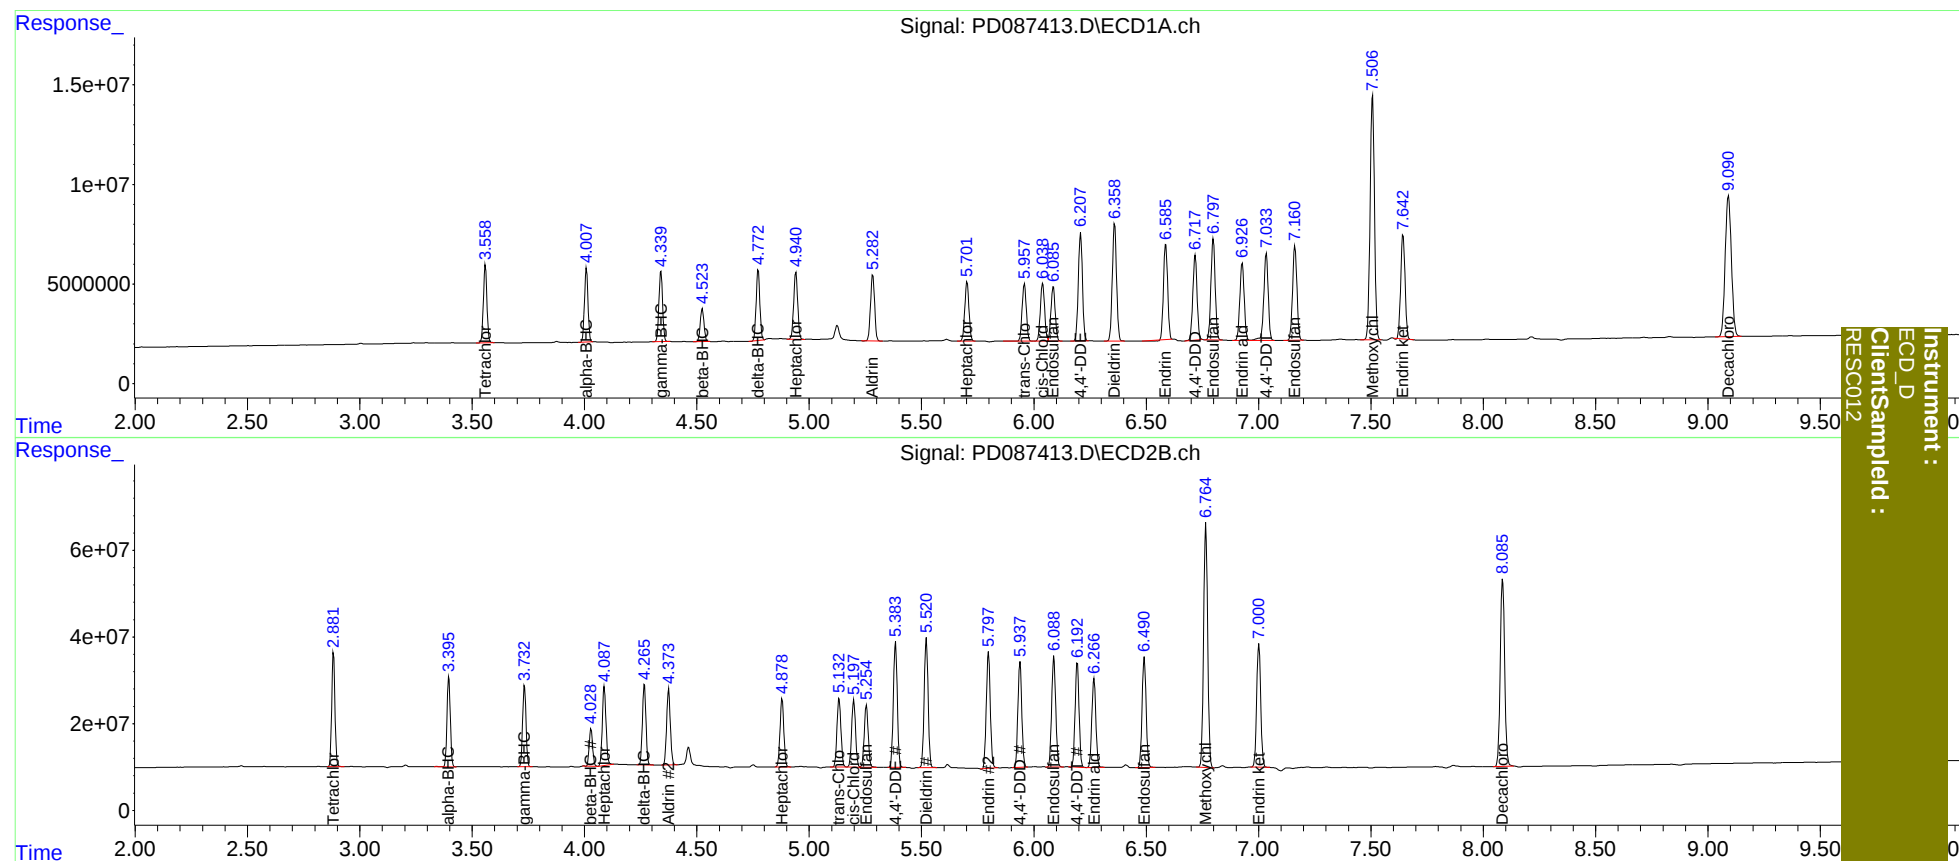

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
 Data File : PD087413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 14:39
 Operator : AR\AJ
 Sample : RESC057
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC012

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 04:20:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 17 04:06:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.883	42782354	263.4E6	20.499	21.233
27)	SA Decachlor...	9.091	8.086	136.4E6	594.2E6	40.654	41.199
Target Compounds							
2)	A alpha-BHC	4.009	3.396	40550271	214.8E6	9.257	10.750
3)	MA gamma-BHC...	4.340	3.733	40340390	198.9E6	9.560	10.774
4)	MA Heptachlor	4.941	4.088	41607604	210.3E6	9.730	11.242
5)	MB Aldrin	5.283	4.375	41623978	201.7E6	9.964	11.235
6)	B beta-BHC	4.525	4.029	19096284	91468742	10.484	10.847
7)	B delta-BHC	4.773	4.267	40519537	200.0E6	9.331	10.559
8)	B Heptachlo...	5.703	4.879	38408621	185.0E6	9.991	10.935
9)	A Endosulfan I	6.087	5.255	36205252	174.5E6	10.130	11.040
10)	B trans-Chl...	5.958	5.133	37305096	194.1E6	9.790	10.851
11)	B cis-Chlor...	6.040	5.198	38498583	187.7E6	10.034	10.871
12)	B 4,4'-DDE	6.208	5.384	69517290	354.8E6	19.020	21.693
13)	MA Dieldrin	6.360	5.521	76778789	365.6E6	19.432	21.934
14)	MA Endrin	6.587	5.798	61909127	328.9E6	18.748	22.109
15)	B Endosulfa...	6.799	6.089	66936046	322.5E6	20.454	21.929
16)	A 4,4'-DDD	6.718	5.939	55382025	293.8E6	19.415	21.969
17)	MA 4,4'-DDT	7.035	6.193	59844019	296.0E6	20.020	21.475
18)	B Endrin al...	6.928	6.268	52817564	256.7E6	20.818	22.610
19)	B Endosulfa...	7.162	6.492	63732876	319.6E6	20.202	22.147
20)	A Methoxychlor	7.507	6.765	166.1E6	708.1E6	104.403	118.119
21)	B Endrin ke...	7.643	7.001	69832970	358.0E6	19.921	22.787

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087413.D
Acq On : 16 Jan 2025 14:39
Operator : AR\AJ
Sample : RESC057
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Title : GC Extractables
Last Update : Fri Jan 17 04:06:07 2025
Integrator: ChemStation

RT#1	RT#2	Resolution
3.559	4.009	100.00%
4.009	4.340	100.00%
4.340	4.525	100.00%
4.525	4.773	100.00%
4.773	4.941	100.00%
4.941	5.283	100.00%
5.283	5.703	100.00%
5.703	5.958	100.00%
5.958	6.040	100.00%
6.040	6.087	94.27%
6.087	6.208	100.00%
6.208	6.360	100.00%
6.360	6.587	100.00%
6.587	6.718	100.00%
6.718	6.799	100.00%
6.799	6.928	100.00%
6.928	7.035	100.00%
7.035	7.162	100.00%
7.162	7.507	100.00%
7.507	7.643	100.00%
7.643	9.091	100.00%

Signal #2


2.883	3.396	100.00%
3.396	3.733	100.00%
3.733	4.029	100.00%
4.029	4.088	100.00%
4.088	4.267	100.00%
4.267	4.375	100.00%
4.375	4.879	100.00%
4.879	5.133	100.00%
5.133	5.198	100.00%
5.198	5.255	100.00%
5.255	5.384	100.00%
5.384	5.521	100.00%
5.521	5.798	100.00%
5.798	5.939	100.00%
5.939	6.089	100.00%
6.089	6.193	100.00%
6.193	6.268	100.00%
6.268	6.492	100.00%
6.492	6.765	100.00%
6.765	7.001	100.00%
7.001	8.086	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 14:39
Operator : AR\AJ
Sample : RESC057
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 04:20:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 17 04:06:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

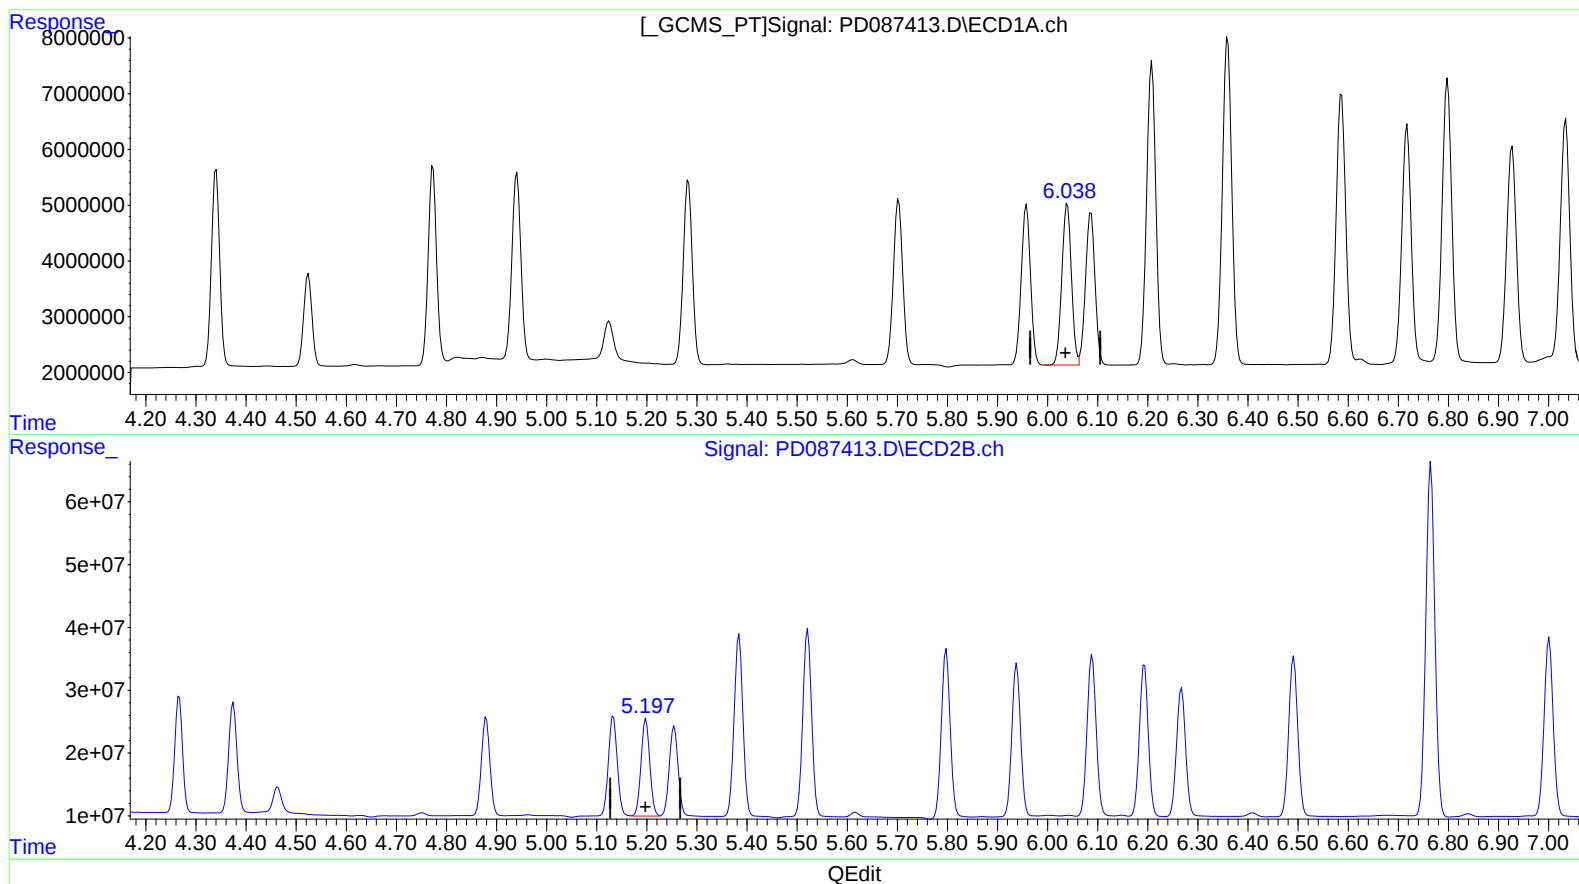

(11) cis-Chlordane (B)

6.040min 10.034 ng/ml

response 38498583

(11) cis-Chlordane #2 (B)

5.198min 10.871 ng/ml

response 187686929