

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
 Data File : PD087431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 18:53
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6073

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 03:58:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 17 03:57:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.555	2.882	332.7E6	1775.6E6	159.409	143.140
27) SA Decachlor...	9.085	8.085	963.7E6	4050.7E6	287.147	280.858
Target Compounds						
2) A alpha-BHC	4.005	3.396	811.7E6	2992.8E6	185.292	149.797
3) MA gamma-BHC...	4.337	3.733	757.9E6	2724.7E6	179.610	147.558
4) MA Heptachlor	4.937	4.088	740.1E6	2632.5E6	173.070	140.755
9) A Endosulfan I	6.083	5.254	586.6E6	2189.3E6	164.117	138.527
13) MA Dieldrin	6.356	5.521	1360.5E6	4656.8E6	344.312	279.357
14) MA Endrin	6.583	5.797	1127.5E6	4059.0E6	341.430	272.867
16) A 4,4'-DDD	6.714	5.938	989.1E6	3710.5E6	346.736	277.461
17) MA 4,4'-DDT	7.030	6.193	1044.6E6	3990.9E6	349.468	289.549
20) A Methoxychlor	7.502	6.765	2467.4E6	6927.0E6	1550.560	1155.562 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011725\
Data File : PD087431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 18:53
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 03:58:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011725CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 17 03:57:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

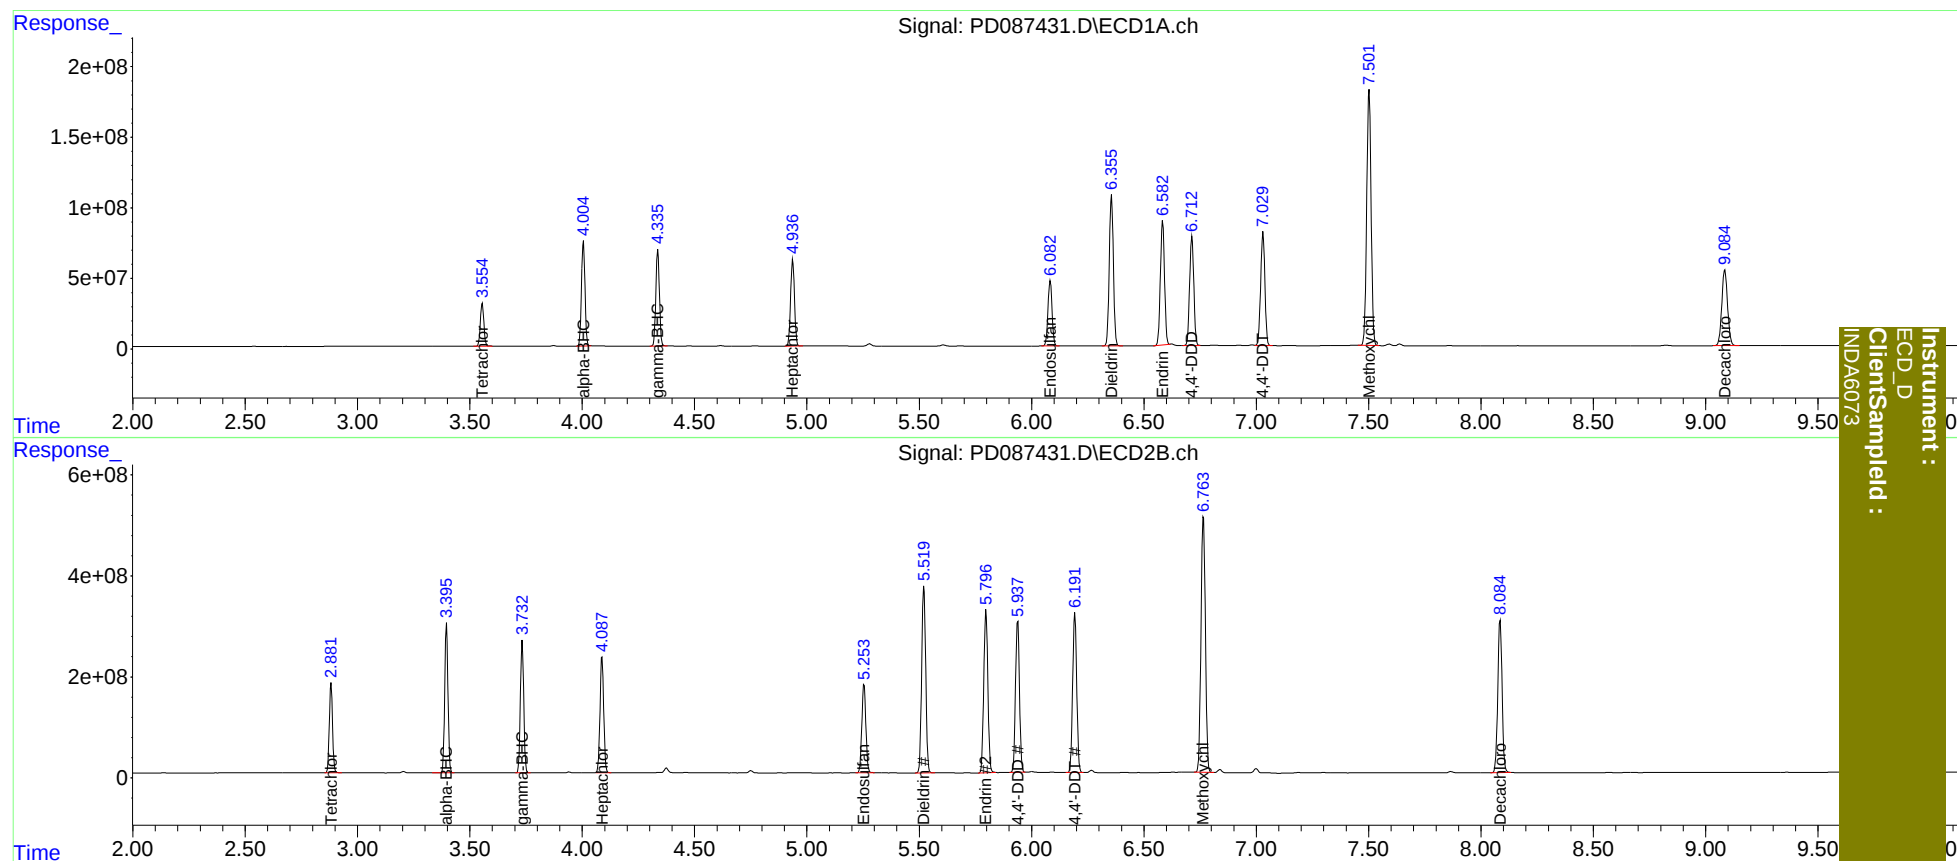

Instrument :
ECD_D
ClientSampled :
INDA6073