

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 07:40
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 06:19:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	3.989	0.000	1922393	0	1.441	N.D.	#
8) B	Heptachlo...	0.000	5.816	0	3051881	N.D.	1.406	#
10) B	gamma-Chl...	0.000	6.054	0	4107279	N.D.	1.845	#
14) MA	Endrin	0.000	6.652	0	2610966	N.D.	1.517	#
18) B	Endrin al...	6.213	0.000	869883	0	1.029	N.D.	#
25)	Chlordane-3	0.000	6.054	0	4107279	N.D.	14.557	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 07:40
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 06:19:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

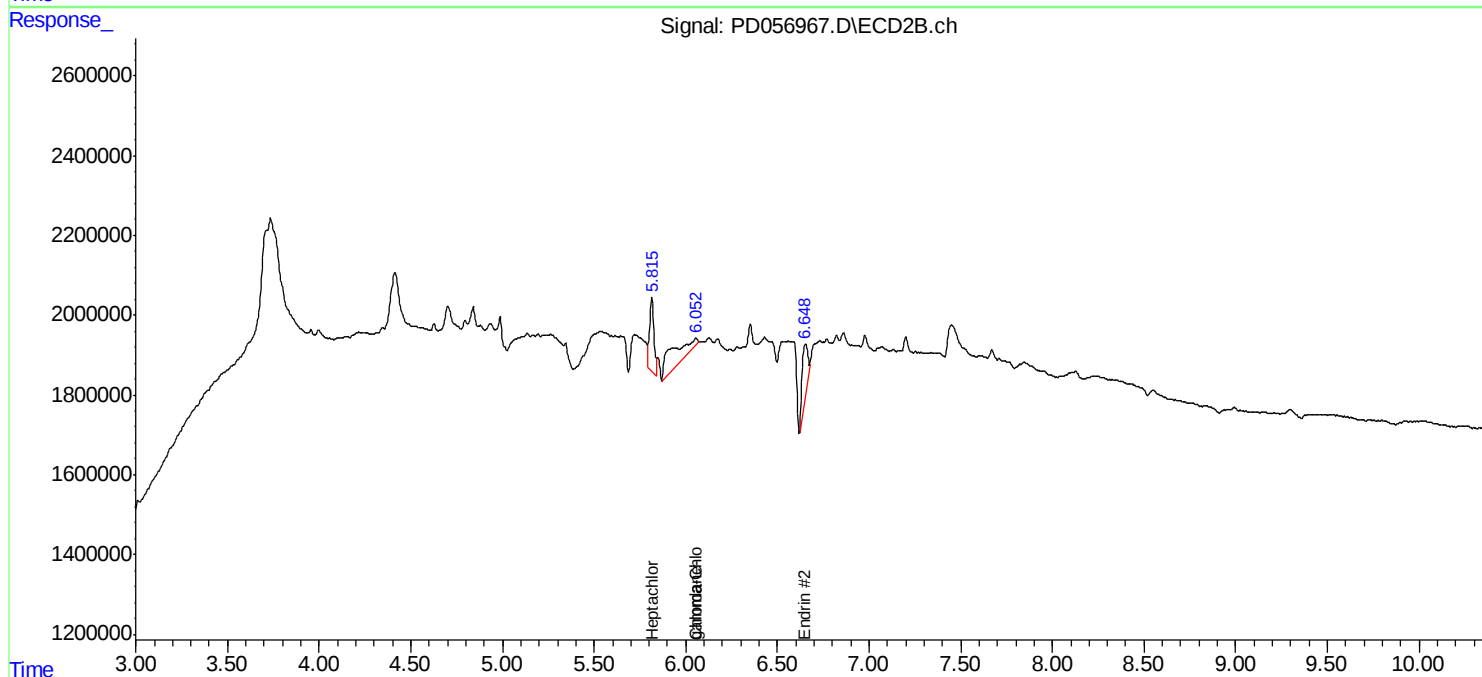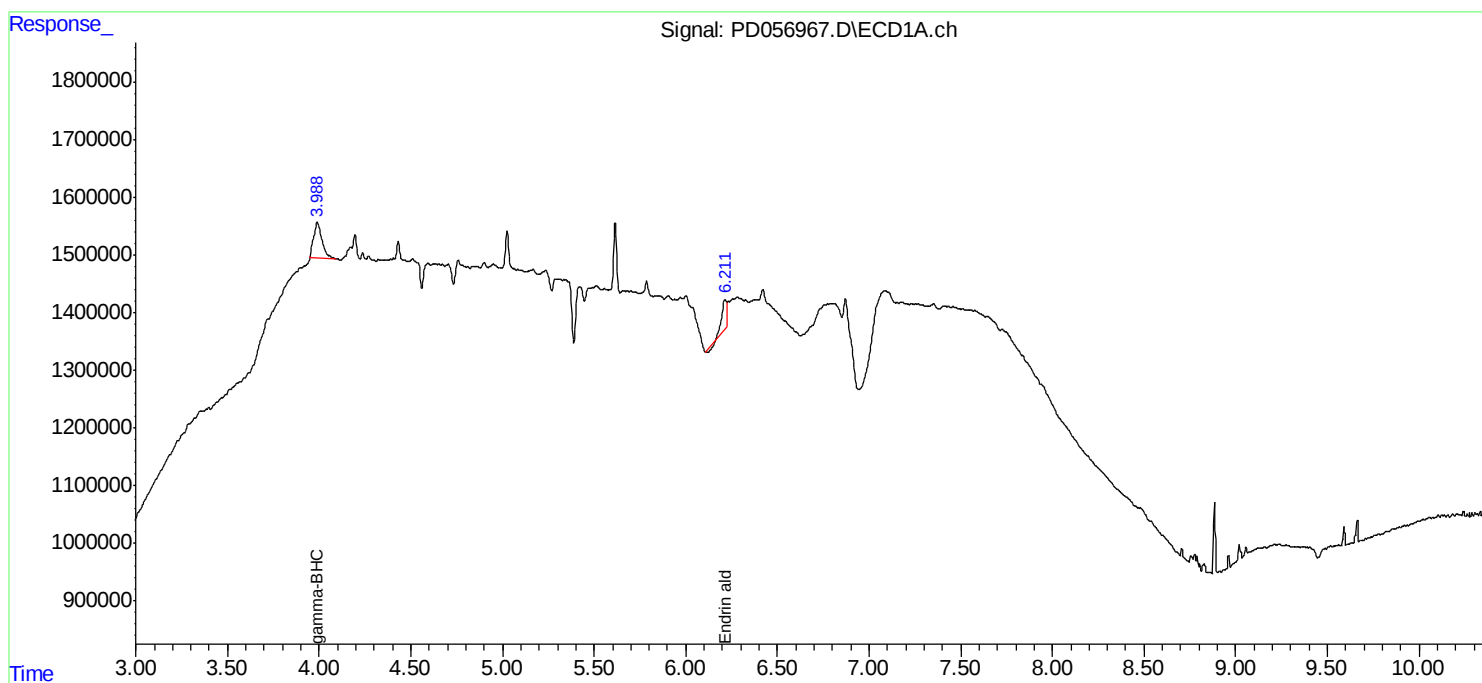


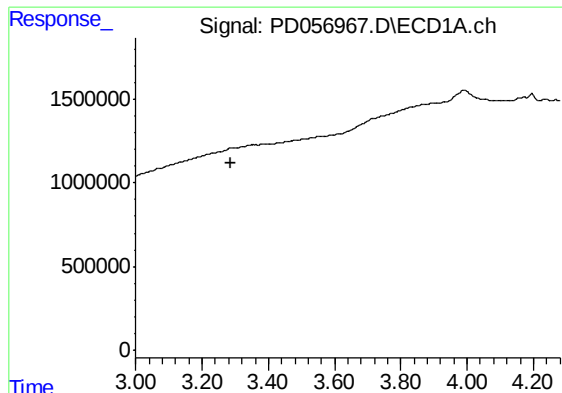

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.285 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

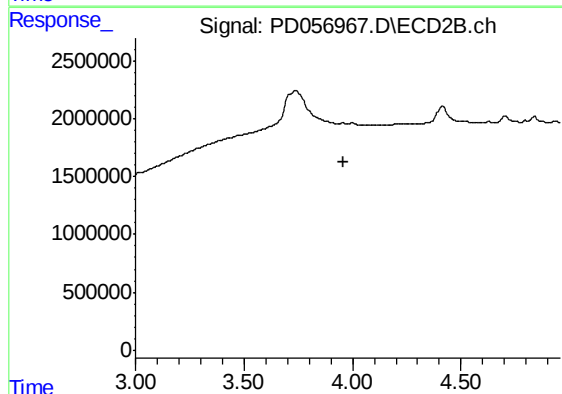


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.959 min
Response: 0
Conc: N.D.

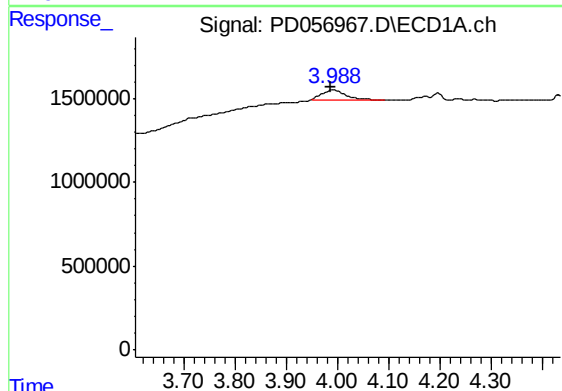


#3 gamma-BHC (Lindane)

R.T.: 3.989 min
Delta R.T.: 0.003 min
Response: 1922393
Conc: 1.44 ng/ml

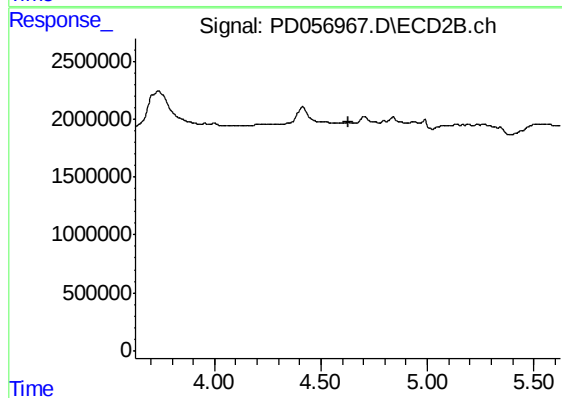

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

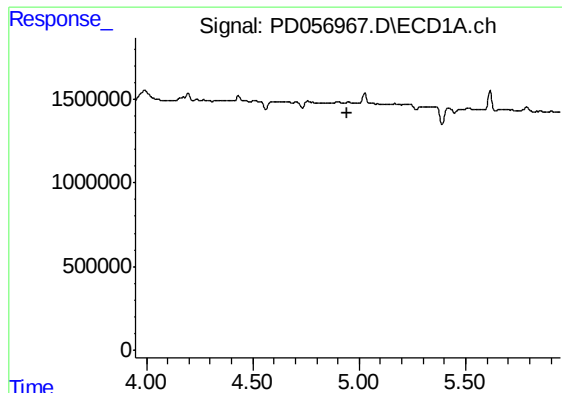

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.947 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

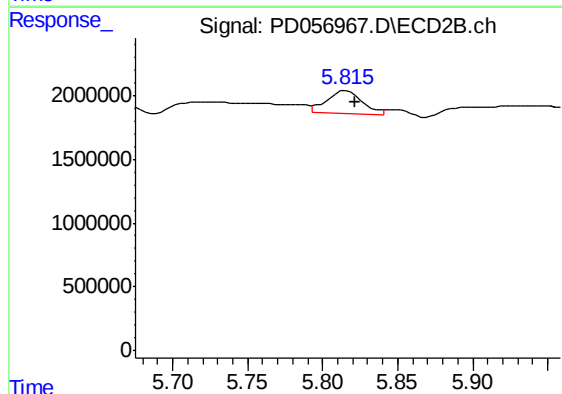


#8 Heptachlor epoxide

R.T.: 5.816 min
Delta R.T.: -0.005 min
Response: 3051881
Conc: 1.41 ng/ml

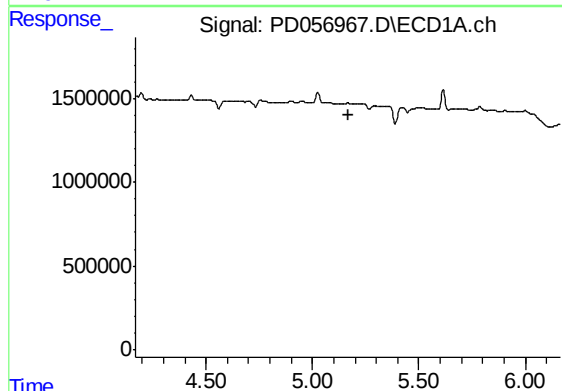


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.168 min
Response: 0
Conc: N.D.

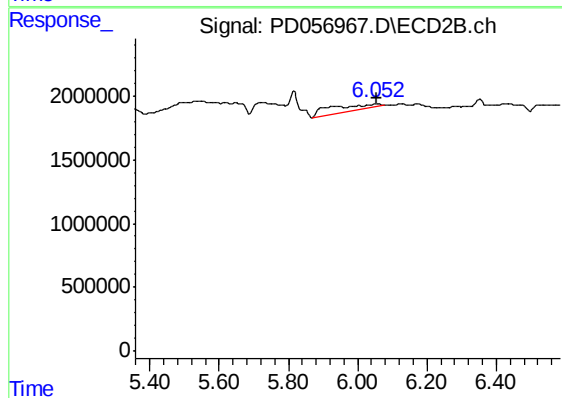

#10 gamma-Chlordane


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 4107279
Conc: 1.84 ng/ml

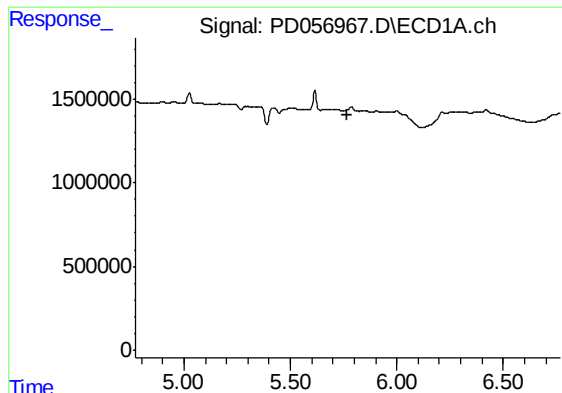

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.770 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

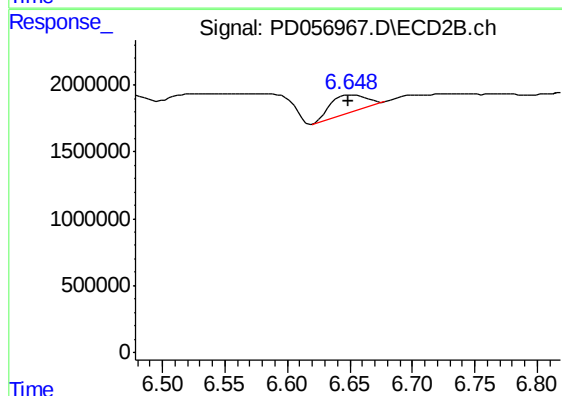


#14 Endrin

R.T.: 6.652 min
Delta R.T.: 0.003 min
Response: 2610966
Conc: 1.52 ng/ml

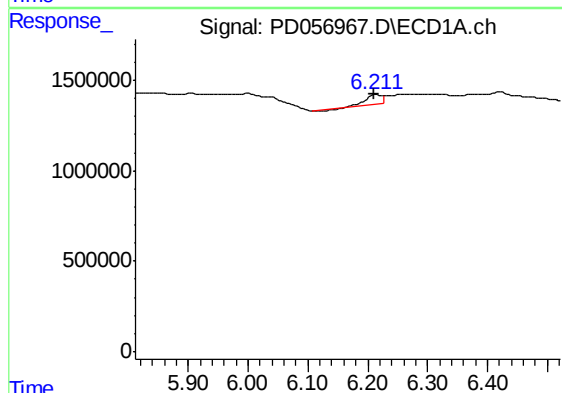


#18 Endrin aldehyde

R.T.: 6.213 min
Delta R.T.: 0.002 min
Response: 869883
Conc: 1.03 ng/ml

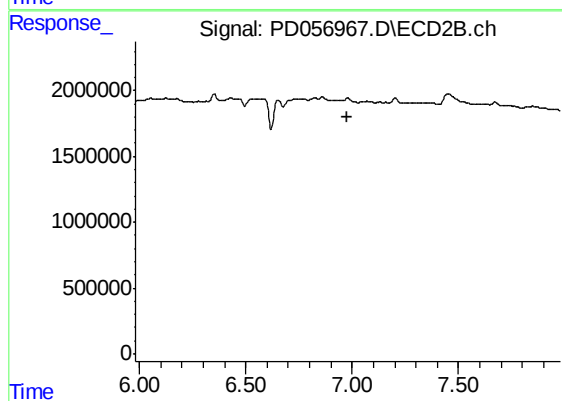

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.980 min
Response: 0
Conc: N.D.

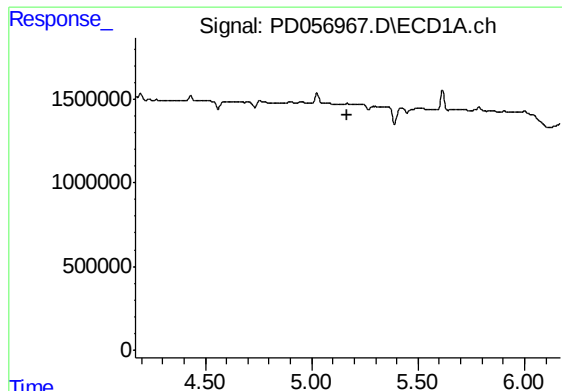

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

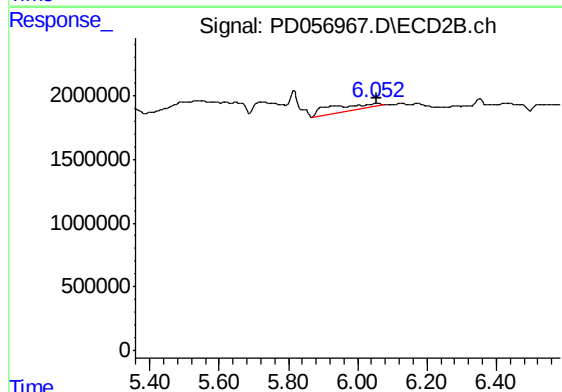


#25 Chlordane-3

R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 4107279
Conc: 14.56 ng/ml

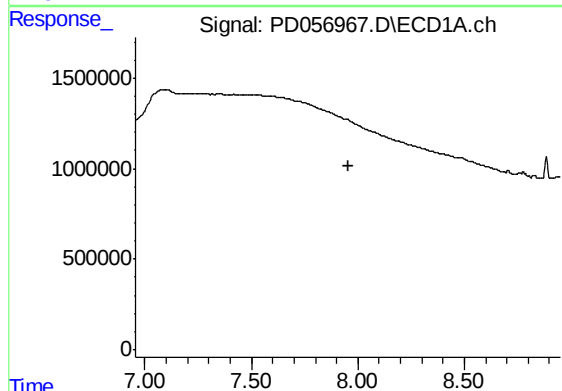

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.955 min
Response: 0
Conc: N.D.

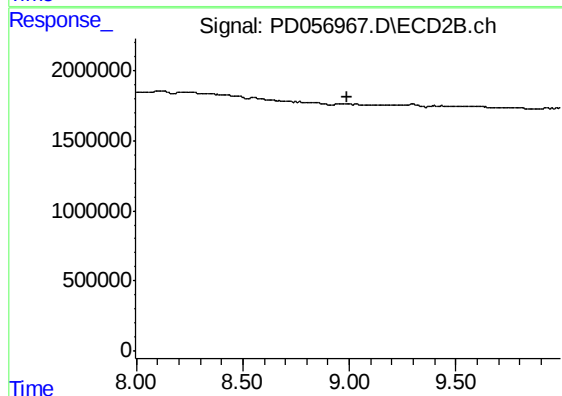

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.992 min
Response: 0
Conc: N.D.