

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 08:22
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 06:29:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	18403377	36228960	22.284	22.140
28)	SA Decachlor...	7.955	8.993	21905137	37826395	22.602	22.695
Target Compounds							
9)	A Endosulfan I	5.278	6.176	10315769	20621469	10.497	10.165
10)	B gamma-Chl...	5.169	6.055	10958670	22143104	10.089	9.946
12)	B 4,4'-DDE	5.394	6.284	21252886	41077590	22.504	20.563
13)	MA Dieldrin	5.517	6.433	22051659	44181926	20.703	20.628
19)	B Endosulfa...	6.422	7.203	18402745	36671272	20.081	20.023
20)	A Methoxychlor	6.687	7.526	44547426	97278038	113.550	110.241
21)	B Endrin ke...	6.906	7.672	21902748	41119413	19.930	20.008
25)	Chlordane-3	5.169	6.055	10958670	22143104	111.909	78.479 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 08:22
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 06:29:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

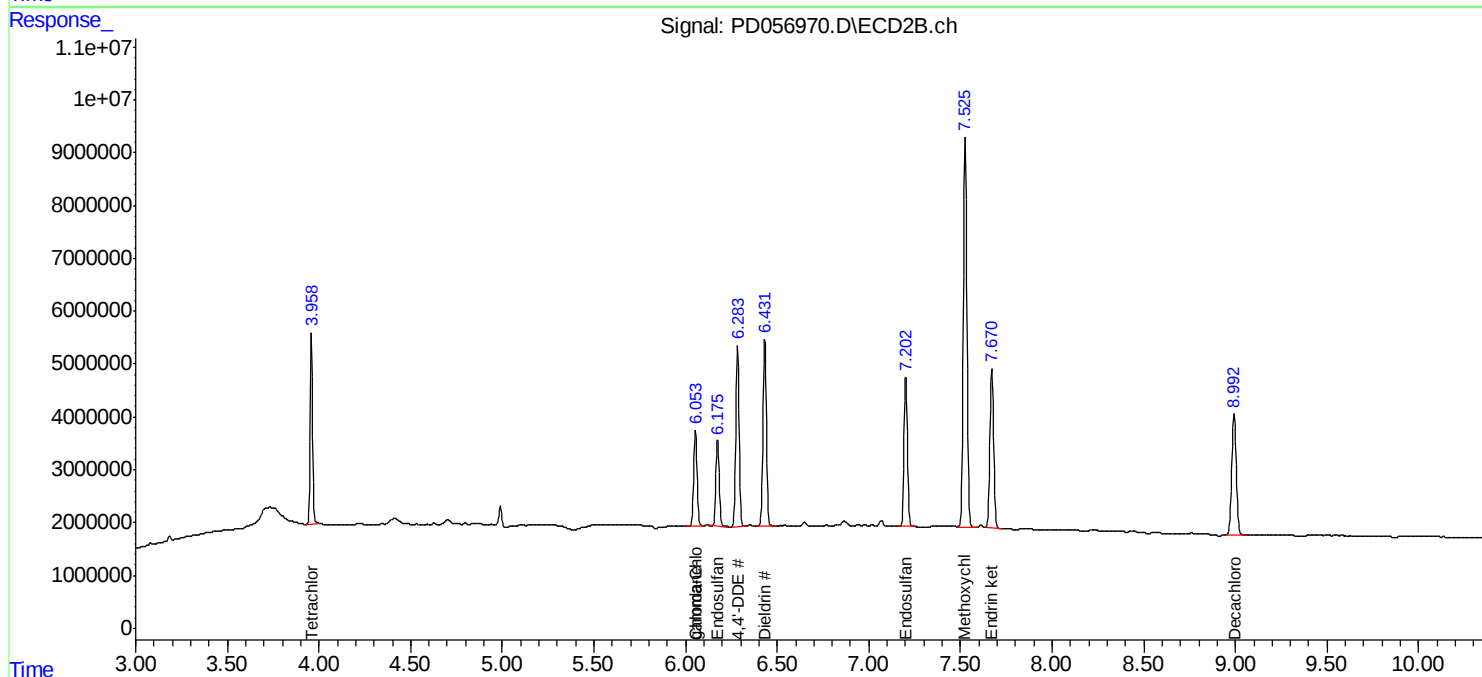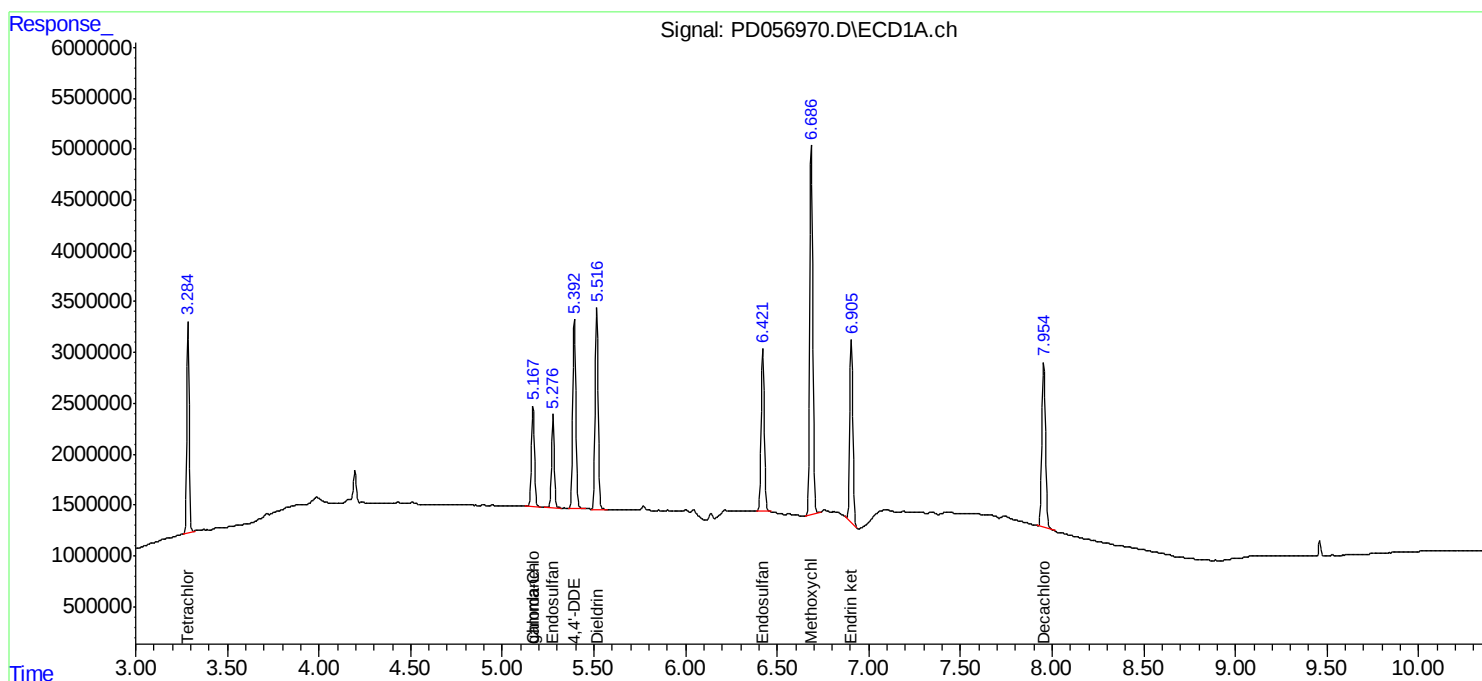


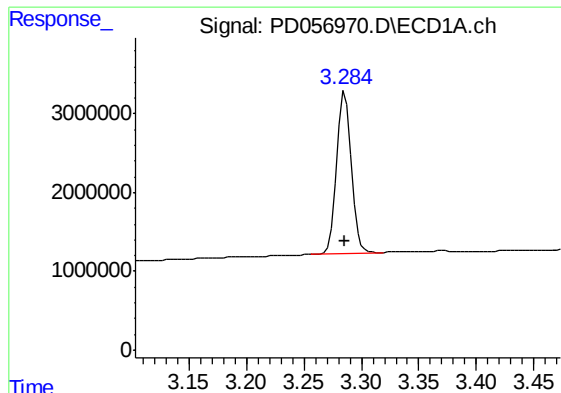

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 18403377
Conc: 22.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

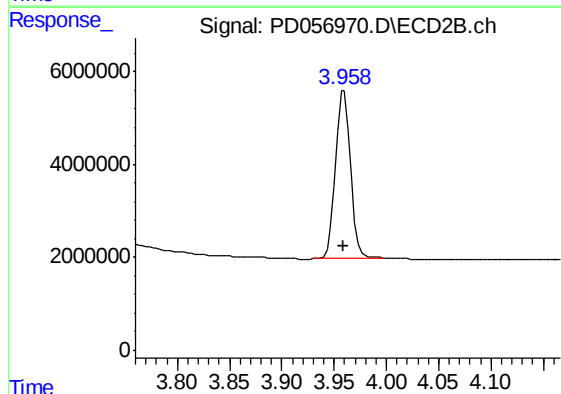


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 36228960
Conc: 22.14 ng/ml

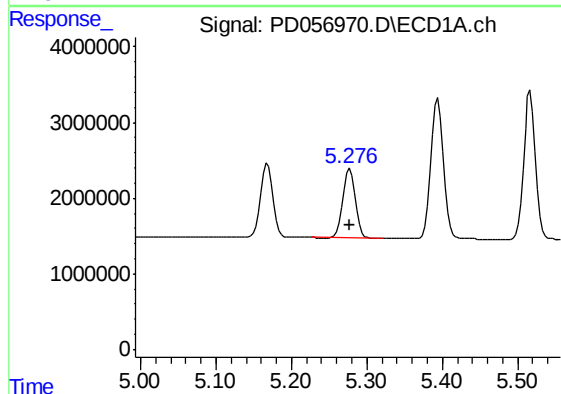


#9 Endosulfan I

R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 10315769
Conc: 10.50 ng/ml

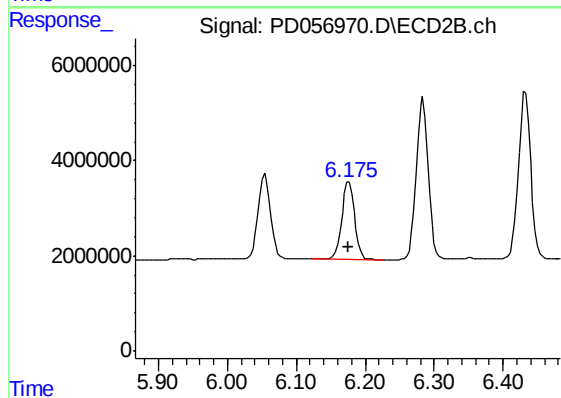

#9 Endosulfan I


R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 20621469
Conc: 10.17 ng/ml

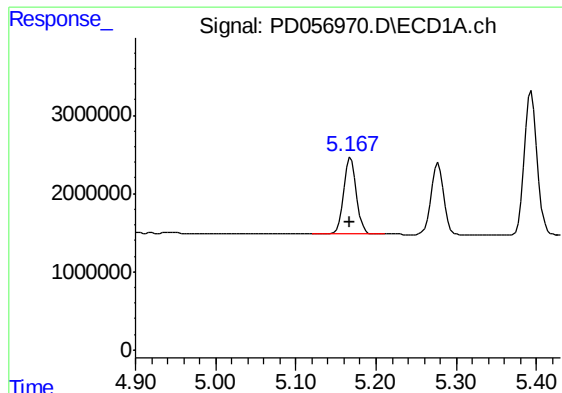

#10 gamma-Chlordane


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 10958670
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

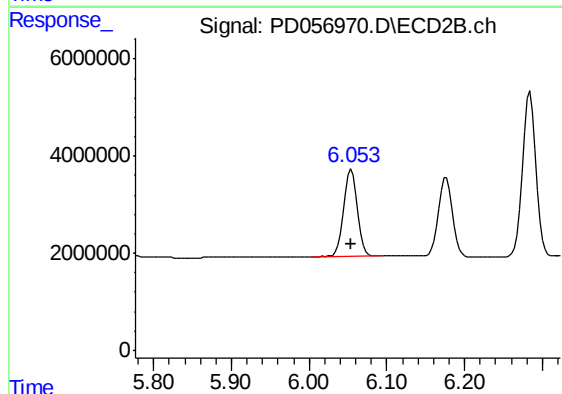


#10 gamma-Chlordane

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 22143104
Conc: 9.95 ng/ml

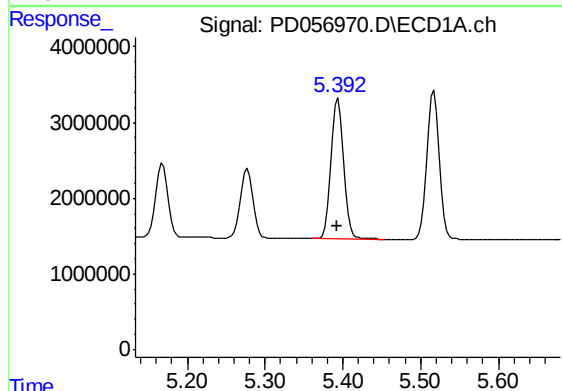


#12 4,4'-DDE

R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 21252886
Conc: 22.50 ng/ml

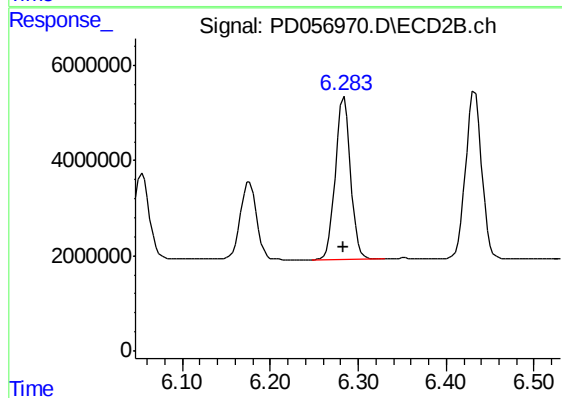

#12 4,4'-DDE


R.T.: 6.284 min
Delta R.T.: 0.000 min
Response: 41077590
Conc: 20.56 ng/ml

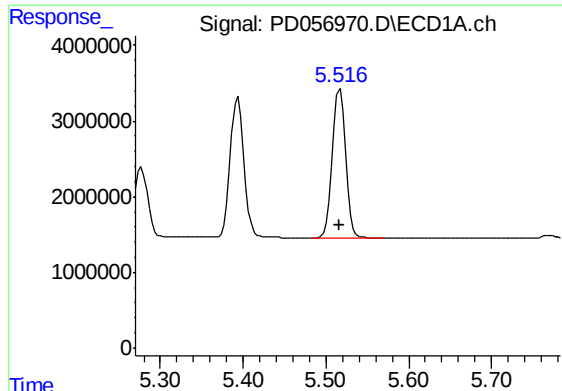

#13 Dielddrin


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 22051659
Conc: 20.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

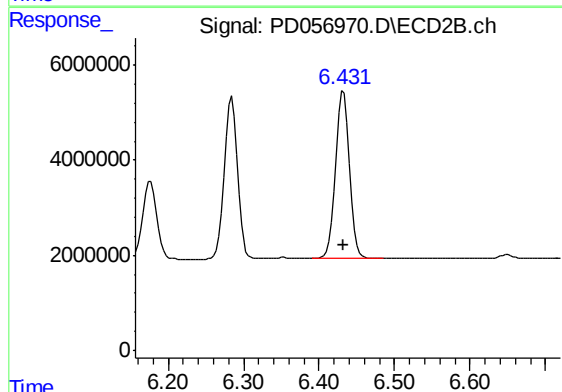


#13 Dielddrin

R.T.: 6.433 min
Delta R.T.: 0.000 min
Response: 44181926
Conc: 20.63 ng/ml

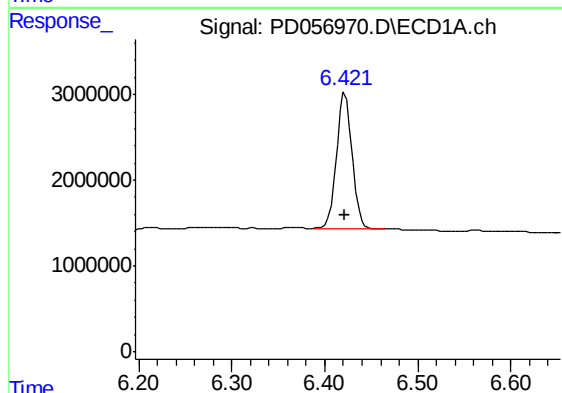


#19 Endosulfan Sulfate

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 18402745
Conc: 20.08 ng/ml

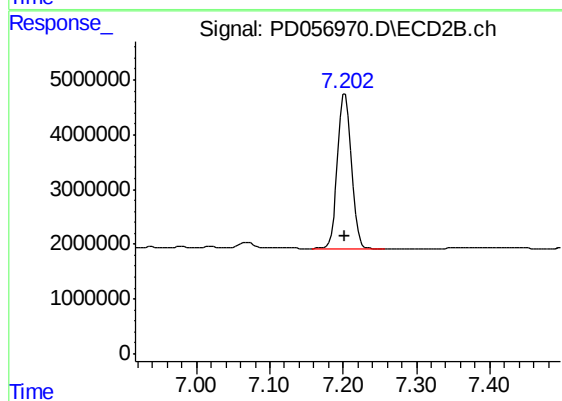

#19 Endosulfan Sulfate


R.T.: 7.203 min
Delta R.T.: 0.000 min
Response: 36671272
Conc: 20.02 ng/ml

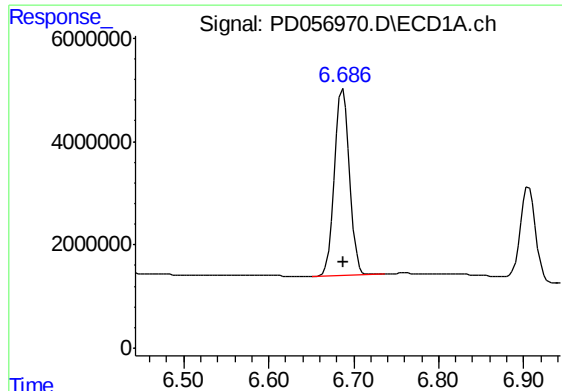

#20 Methoxychlor


R.T.: 6.687 min
Delta R.T.: 0.000 min
Response: 44547426
Conc: 113.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

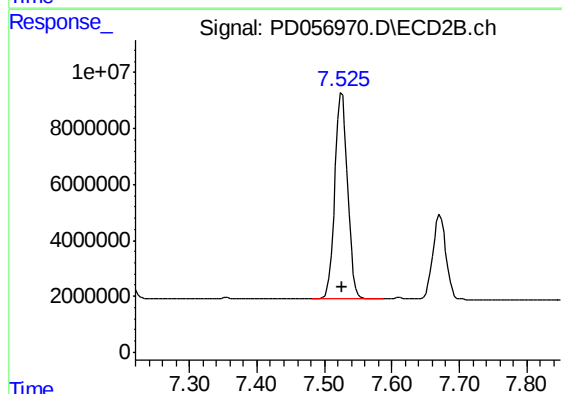


#20 Methoxychlor

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 97278038
Conc: 110.24 ng/ml

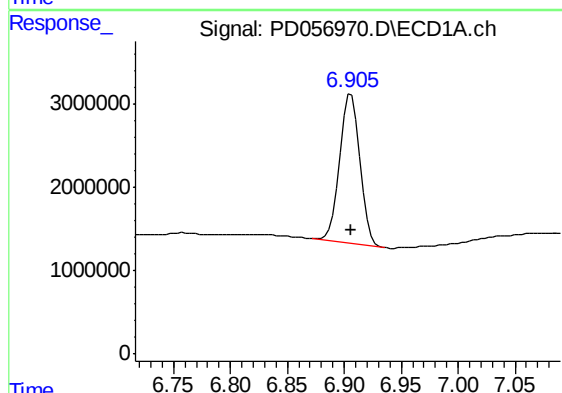


#21 Endrin ketone

R.T.: 6.906 min
Delta R.T.: 0.000 min
Response: 21902748
Conc: 19.93 ng/ml

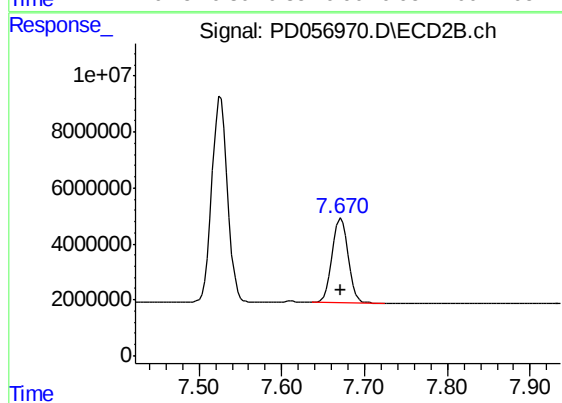

#21 Endrin ketone


R.T.: 7.672 min
Delta R.T.: 0.000 min
Response: 41119413
Conc: 20.01 ng/ml

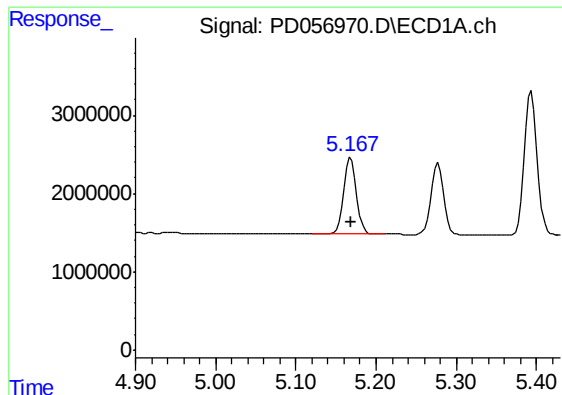

#25 Chlordane-3


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 10958670
Conc: 111.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

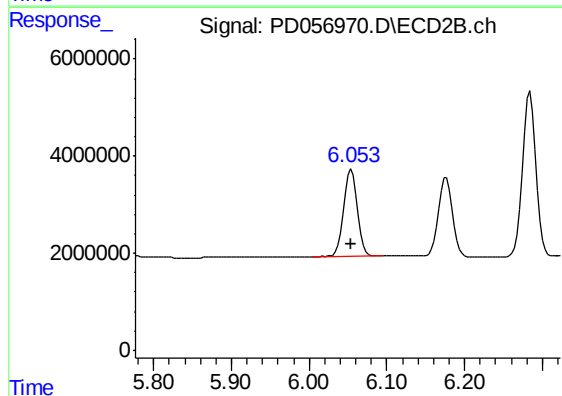


#25 Chlordane-3

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 22143104
Conc: 78.48 ng/ml

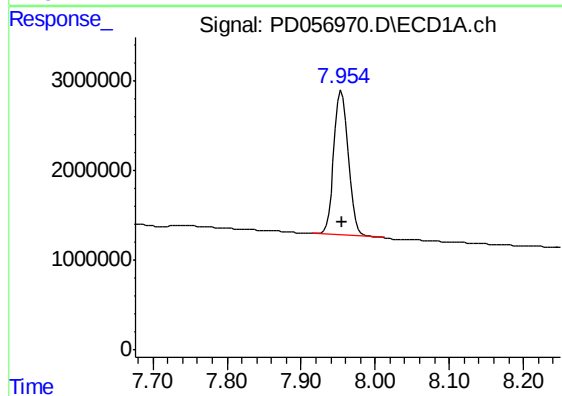

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 21905137
Conc: 22.60 ng/ml

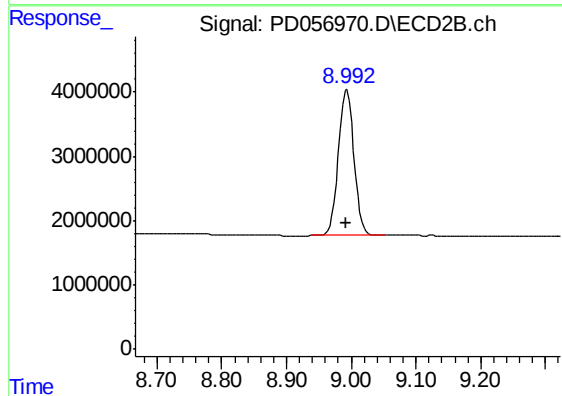

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.001 min
Response: 37826395
Conc: 22.69 ng/ml