

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 09:47
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 04:02:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 04:00:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	92080996	162.9E6	103.530	103.006
28)	SA Decachlor...	7.954	8.993	93011116	154.1E6	95.963	93.741
Target Compounds							
23)	Chlordane-1	4.124	4.947	27513733	64104688	996.370	1013.360
24)	Chlordane-2	4.614	5.412	31759667	67468715	967.282	1012.575
25)	Chlordane-3	5.169	6.055	97314588	285.4E6	1000.547	1031.041
26)	Chlordane-4	5.225	6.129	86739799	337.0E6	1027.493	1029.005
27)	Chlordane-5	6.047	6.930	33858941	56656042	985.778	1001.587



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 09:47
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 04:02:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 04:00:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

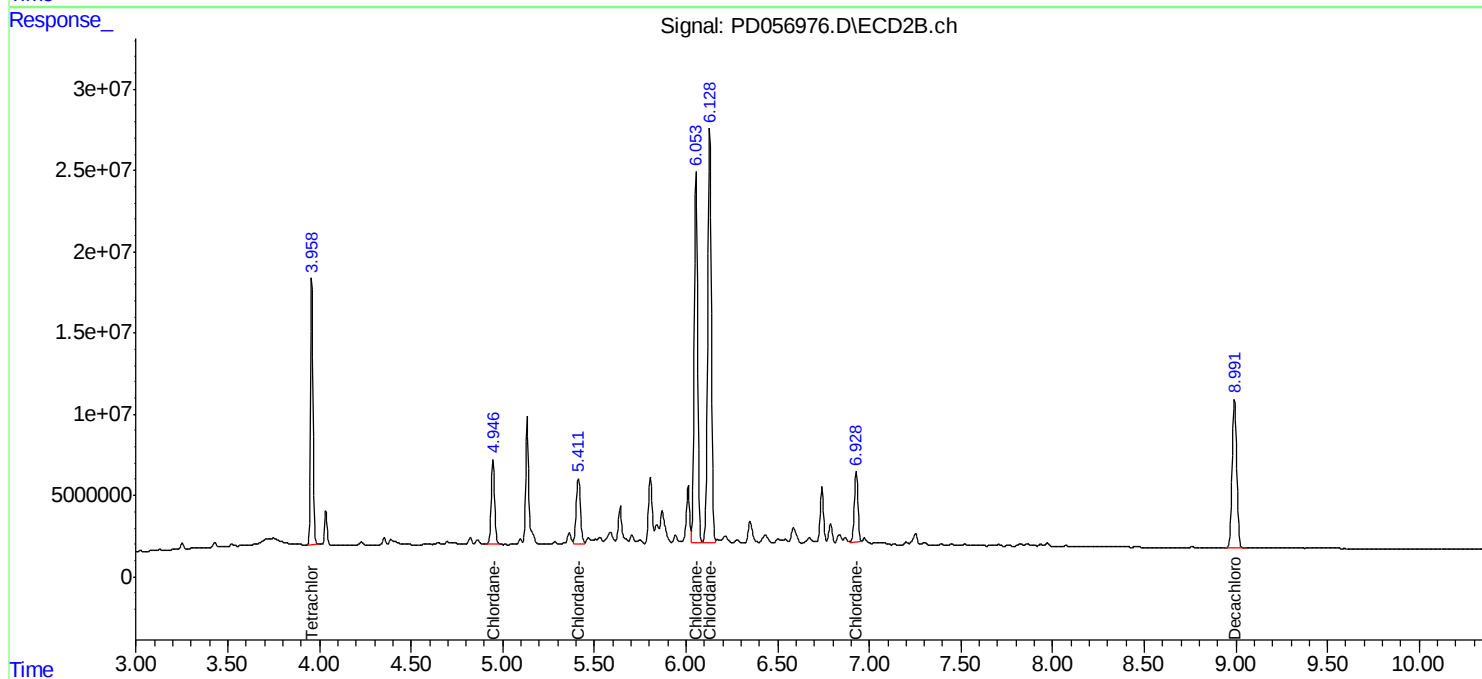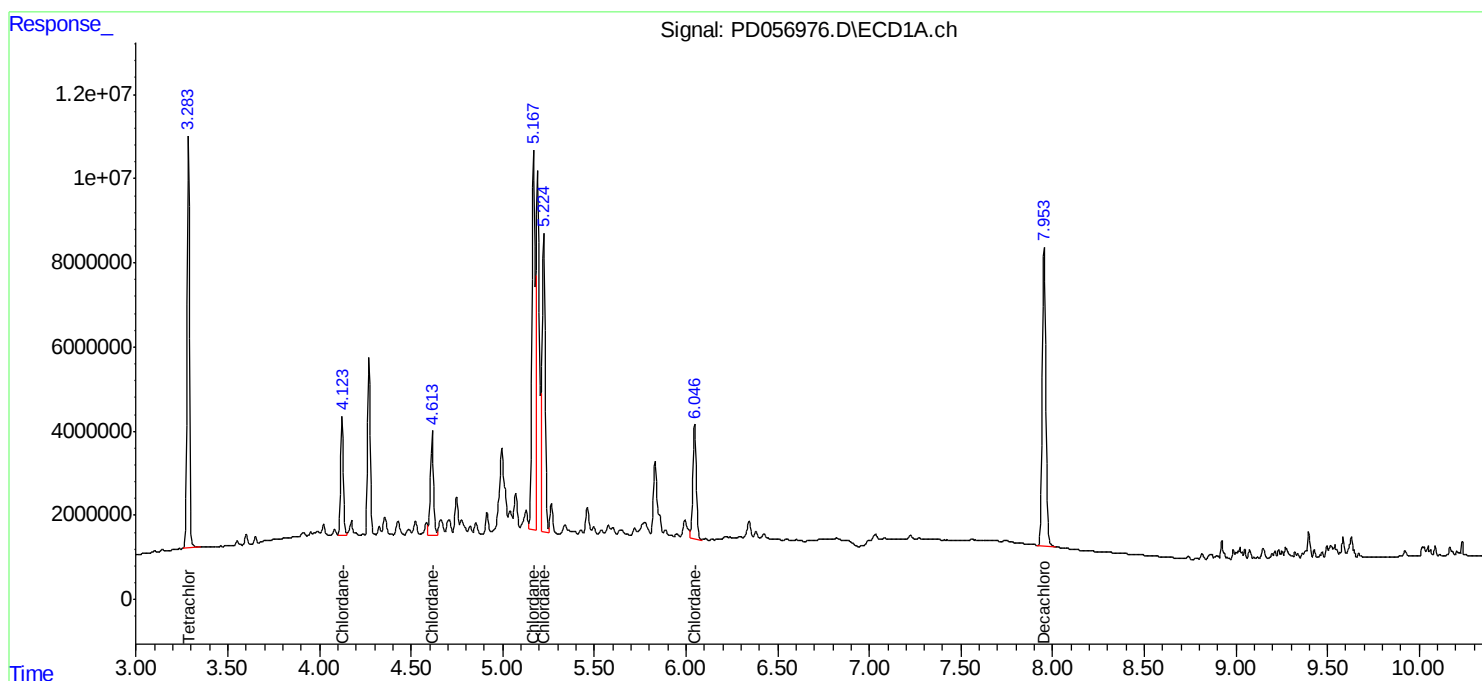


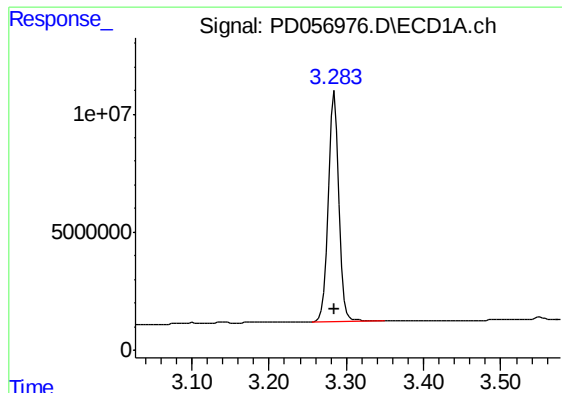

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 92080996
Conc: 103.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

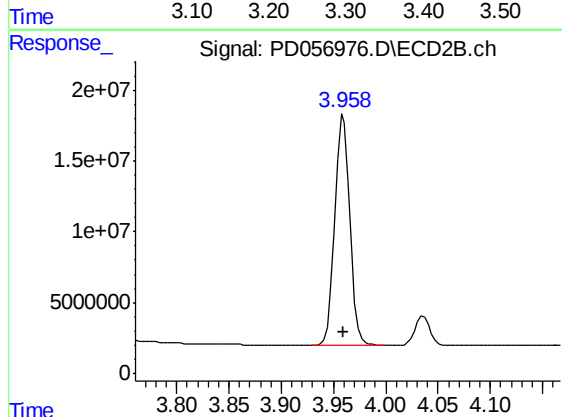


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 162885151
Conc: 103.01 ng/ml

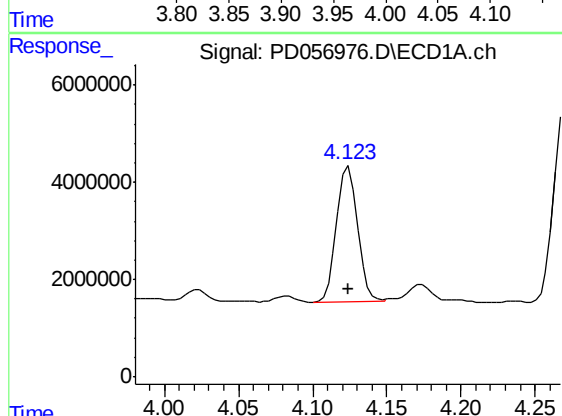


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 27513733
Conc: 996.37 ng/ml

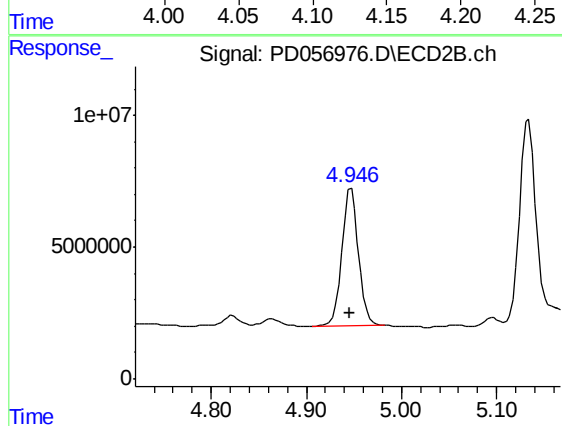

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 64104688
Conc: 1013.36 ng/ml

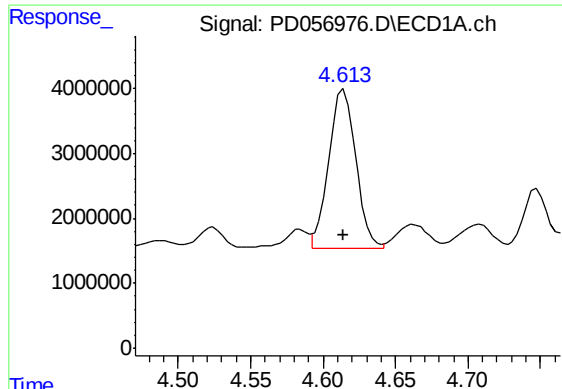

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 31759667
Conc: 967.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

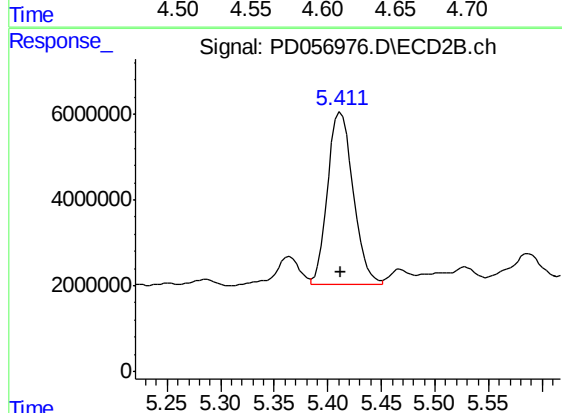


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 67468715
Conc: 1012.57 ng/ml

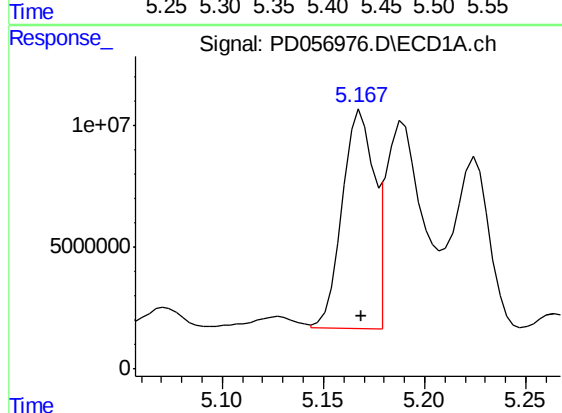


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 97314588
Conc: 1000.55 ng/ml

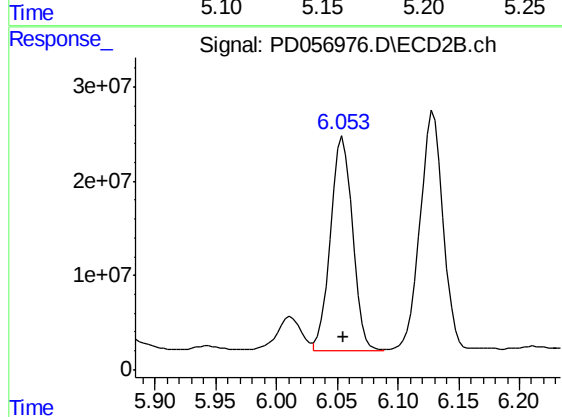

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 285405889
Conc: 1031.04 ng/ml

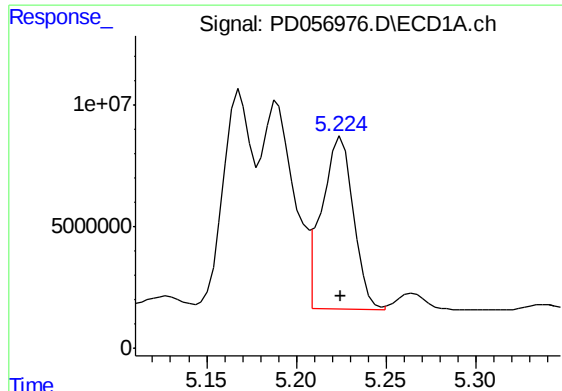

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 86739799
Conc: 1027.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

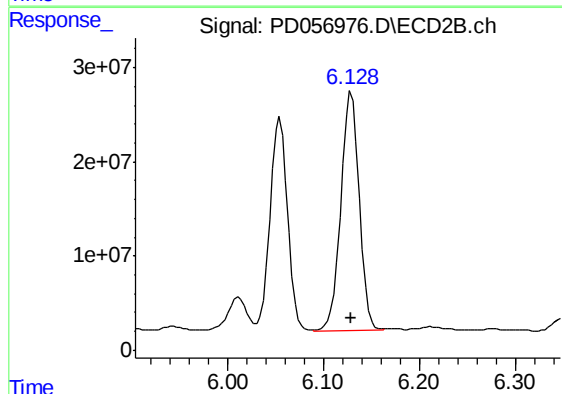


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 337019511
Conc: 1029.01 ng/ml

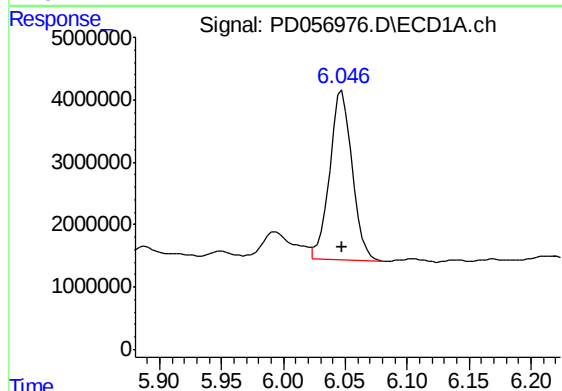


#27 Chlordane-5

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 33858941
Conc: 985.78 ng/ml

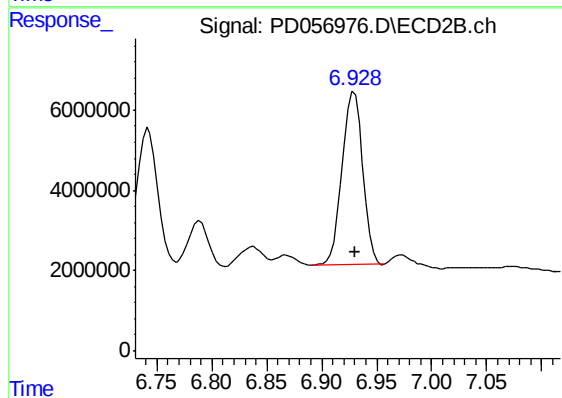

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 56656042
Conc: 1001.59 ng/ml

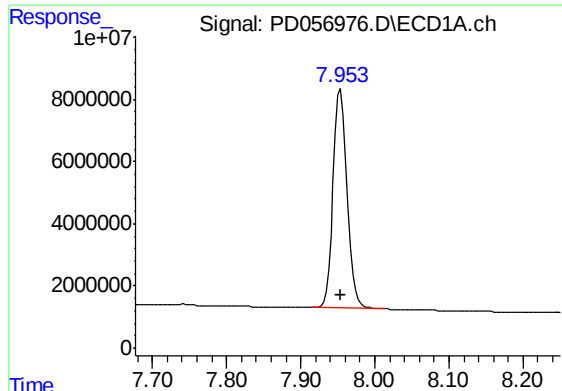

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.000 min
Response: 93011116
Conc: 95.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

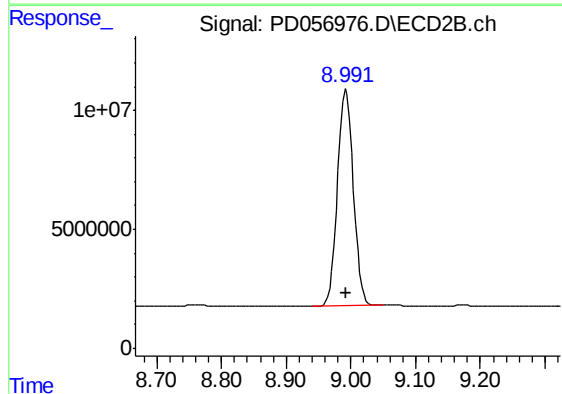

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 154135732
Conc: 93.74 ng/ml