

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 10:01
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 04:02:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 04:00:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	69686491	123.8E6	78.351	78.259
28)	SA Decachlor...	7.955	8.994	71891679	120.4E6	74.173	73.241
Target Compounds							
23)	Chlordane-1	4.124	4.947	21054717	48821016	762.466	771.758
24)	Chlordane-2	4.615	5.412	26976988	51465333	821.619	772.395
25)	Chlordane-3	5.169	6.055	75296996	215.6E6	774.171	778.922
26)	Chlordane-4	5.225	6.129	67043279	252.9E6	794.174	772.302
27)	Chlordane-5	6.048	6.929	25669943	43231249	747.362	764.258



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 10:01
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 04:02:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 04:00:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

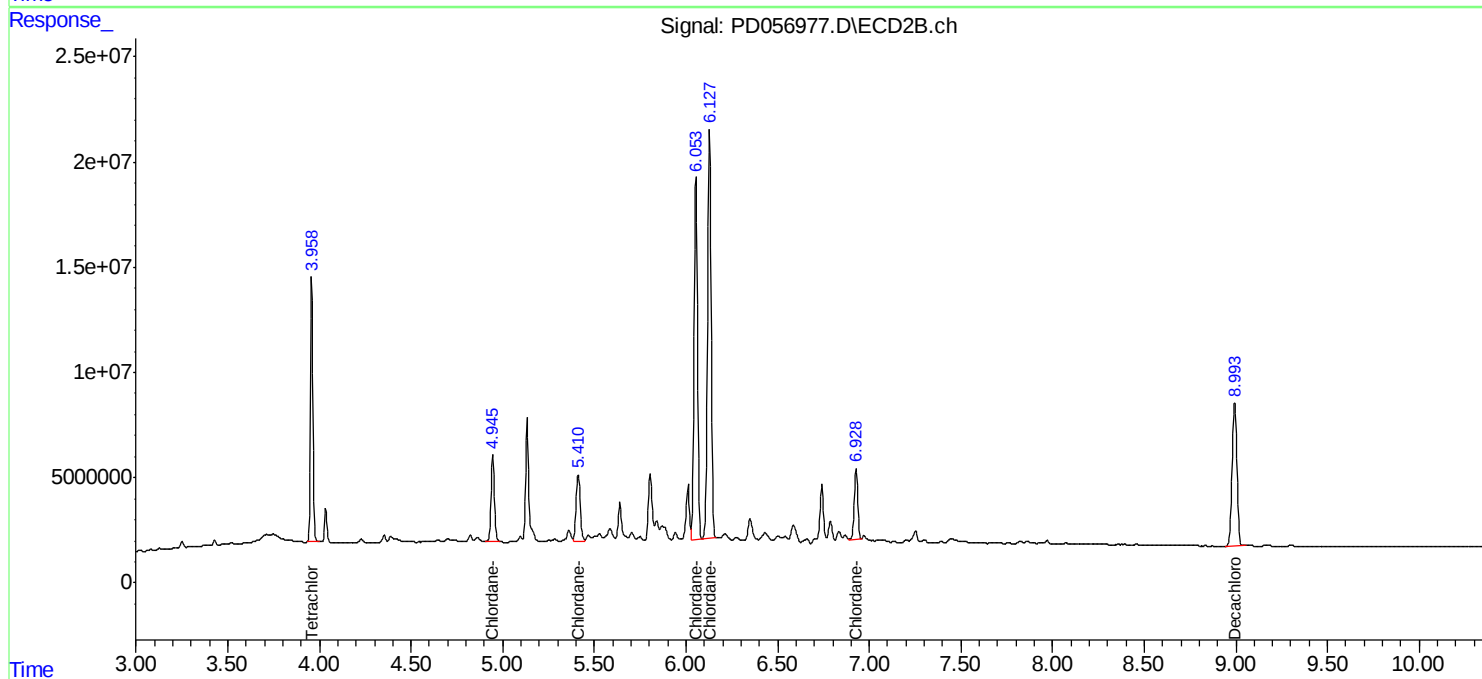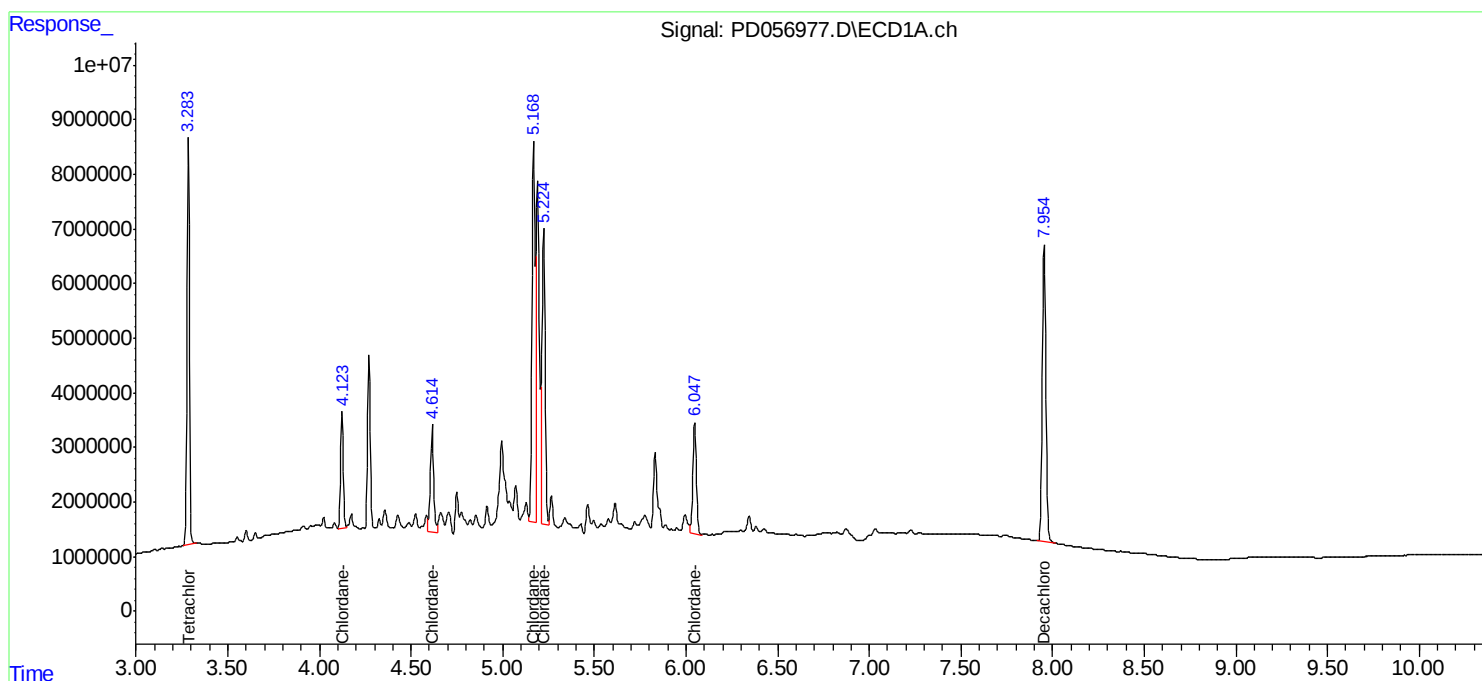


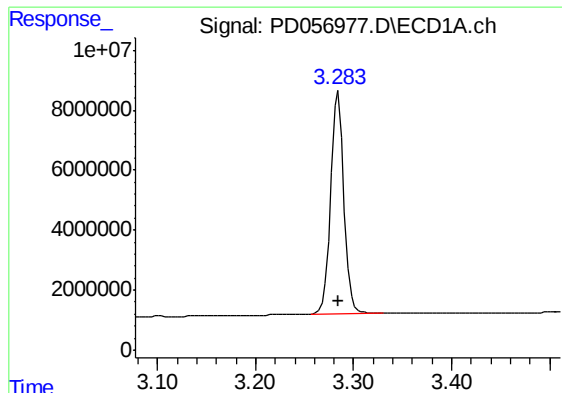

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 69686491
Conc: 78.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

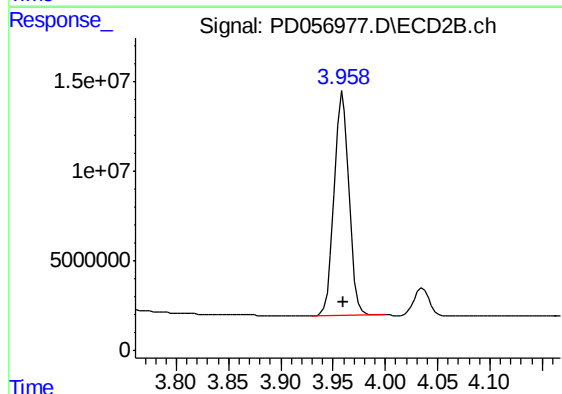


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 123752380
Conc: 78.26 ng/ml

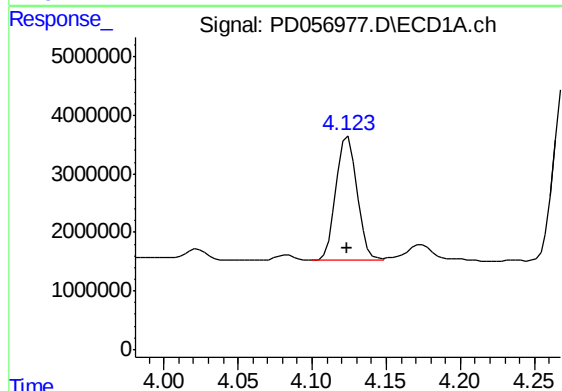


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 21054717
Conc: 762.47 ng/ml

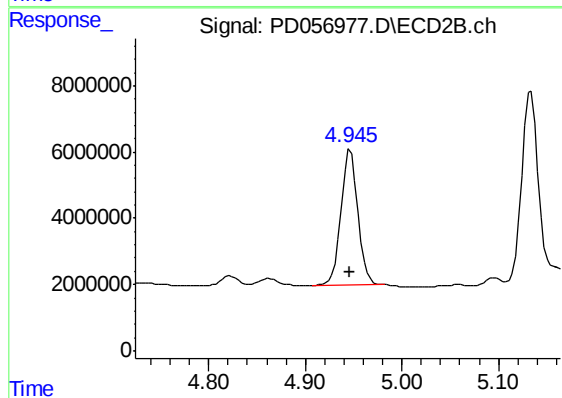

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 48821016
Conc: 771.76 ng/ml

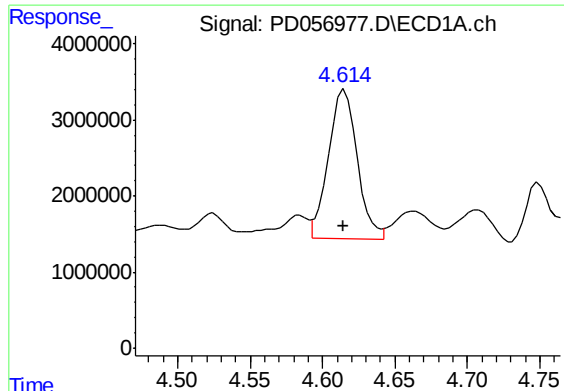

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.001 min
Response: 26976988
Conc: 821.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

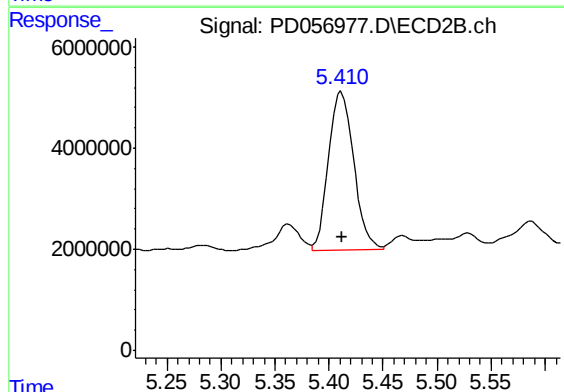


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 51465333
Conc: 772.40 ng/ml

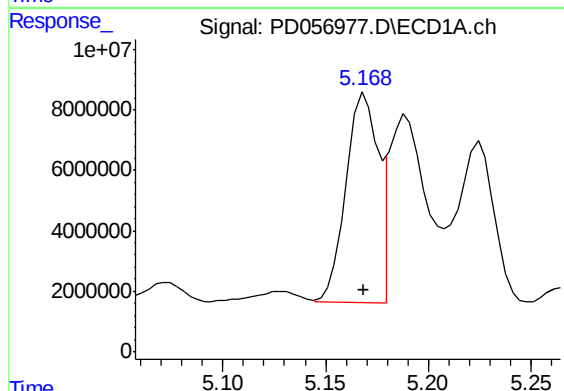


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 75296996
Conc: 774.17 ng/ml

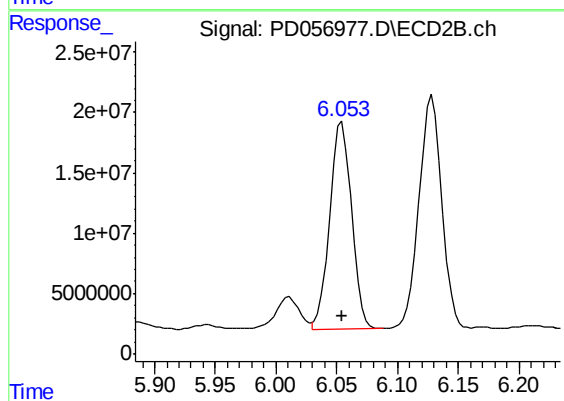

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 215615960
Conc: 778.92 ng/ml

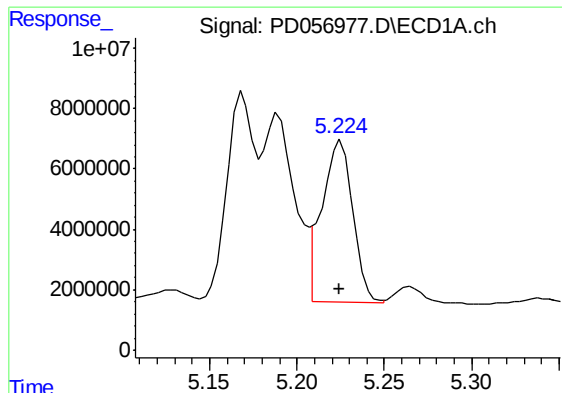

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 67043279
Conc: 794.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

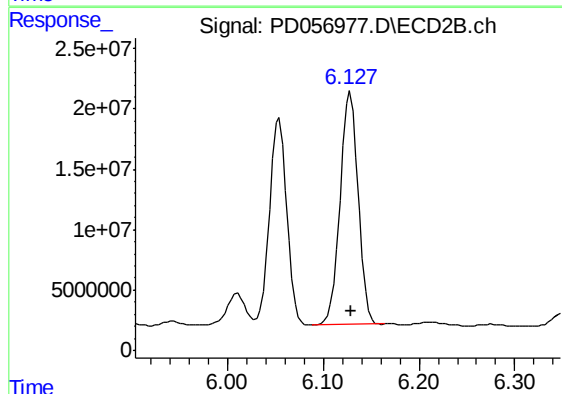


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 252943925
Conc: 772.30 ng/ml

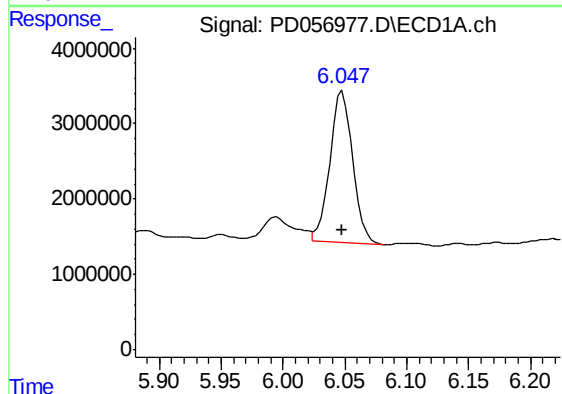


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 25669943
Conc: 747.36 ng/ml

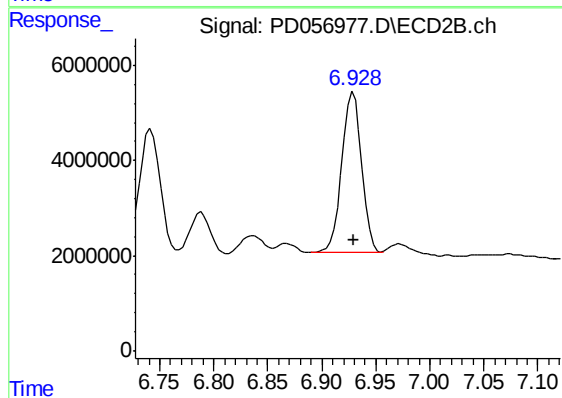

#27 Chlordane-5


R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 43231249
Conc: 764.26 ng/ml

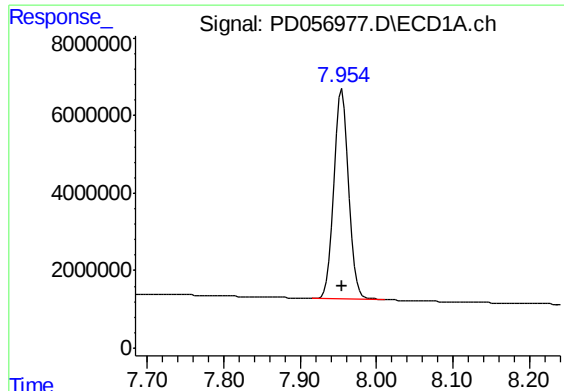

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 71891679
Conc: 74.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

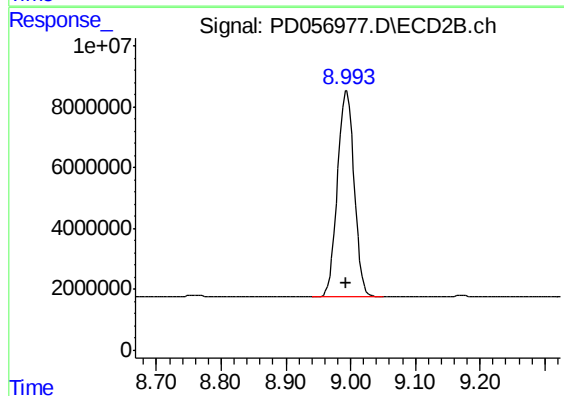

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 120426949
Conc: 73.24 ng/ml