

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 10:15
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 04:02:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 04:00:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	44470605	79066085	50.000	50.000
28)	SA Decachlor...	7.955	8.993	48462190	82213189	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.124	4.946	13806988	31629764	500.000	500.000
24)	Chlordane-2	4.614	5.412	16416964	33315417	500.000	500.000
25)	Chlordane-3	5.169	6.055	48630715	138.4E6	500.000	500.000
26)	Chlordane-4	5.225	6.129	42209449	163.8E6	500.000	500.000
27)	Chlordane-5	6.048	6.930	17173707	28283145	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 10:15
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 04:02:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 04:00:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

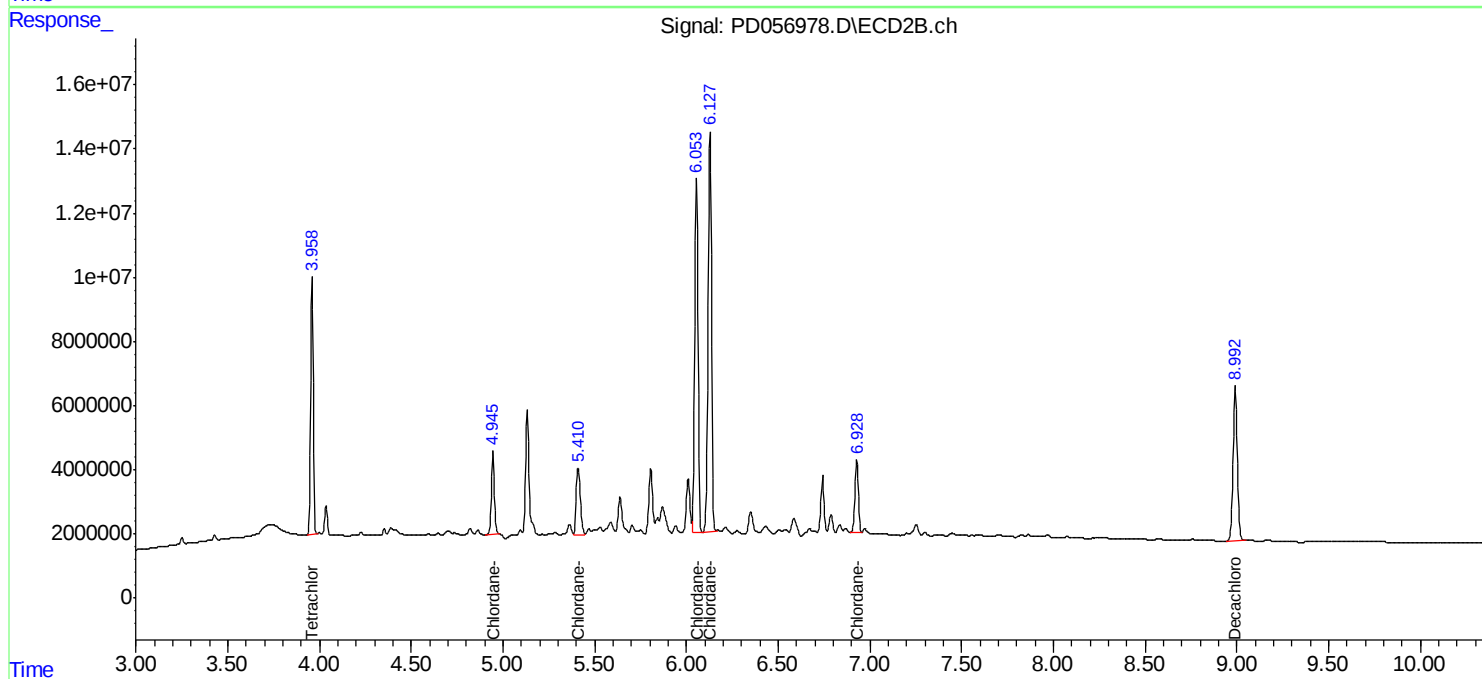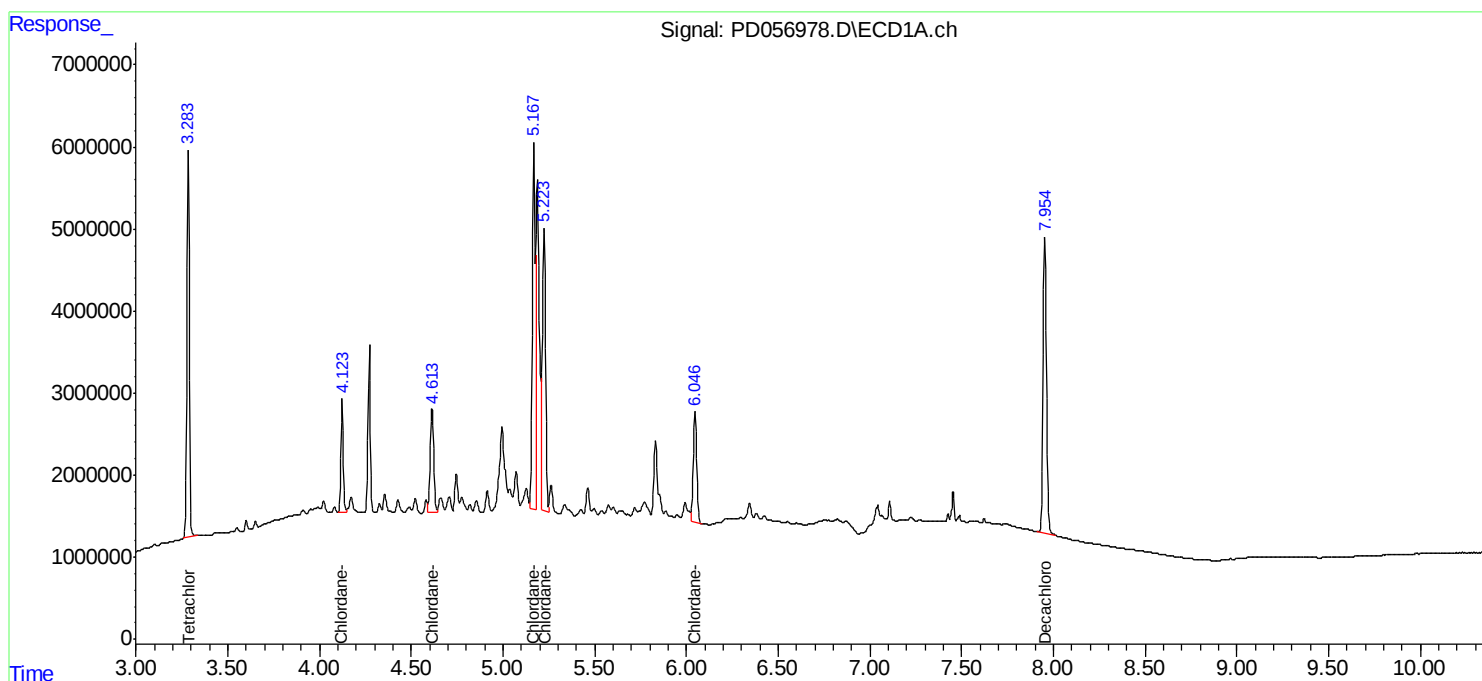


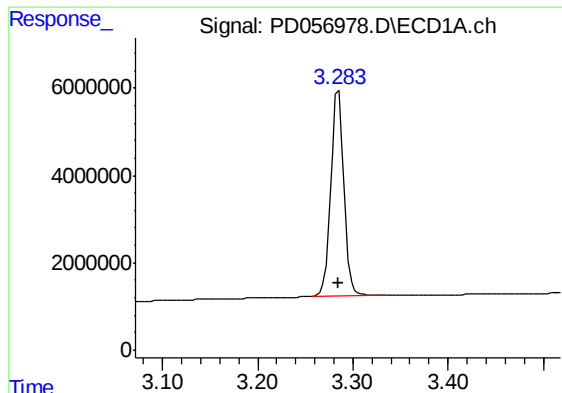

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 44470605
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

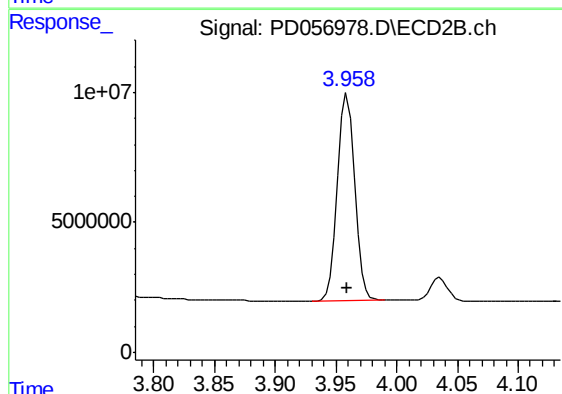


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 79066085
Conc: 50.00 ng/ml

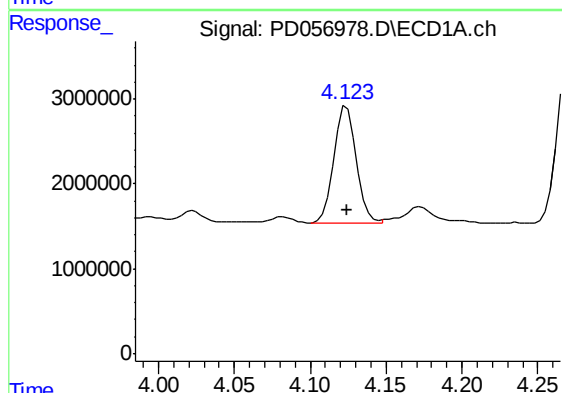


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 13806988
Conc: 500.00 ng/ml

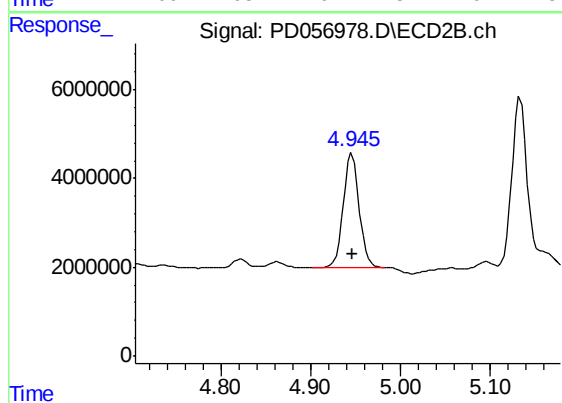

#23 Chlordane-1


R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 31629764
Conc: 500.00 ng/ml

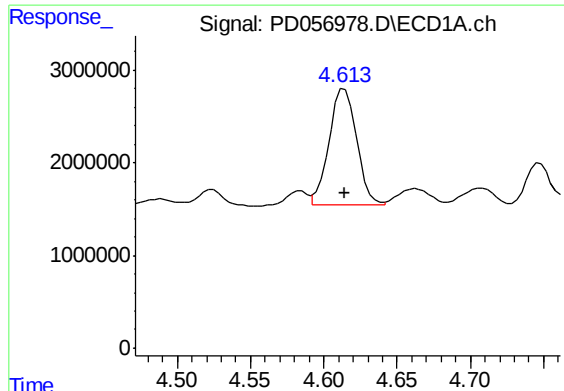

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 16416964
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

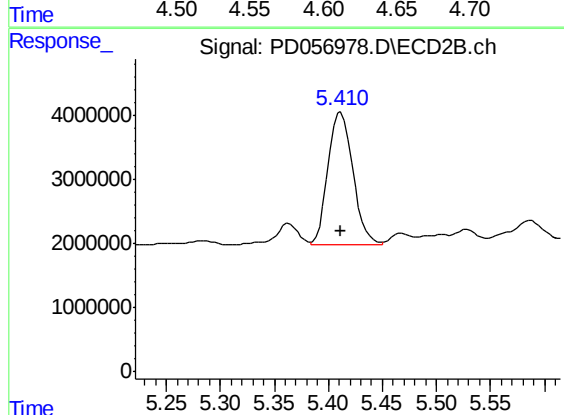


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 33315417
Conc: 500.00 ng/ml

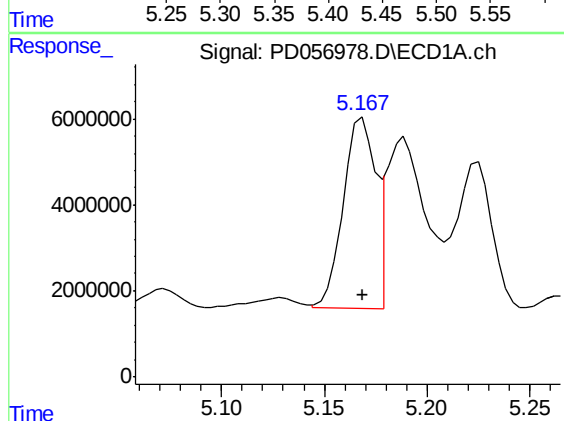


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 48630715
Conc: 500.00 ng/ml

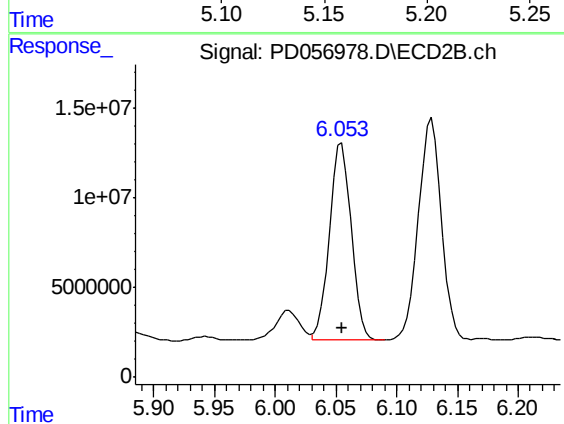

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 138406710
Conc: 500.00 ng/ml

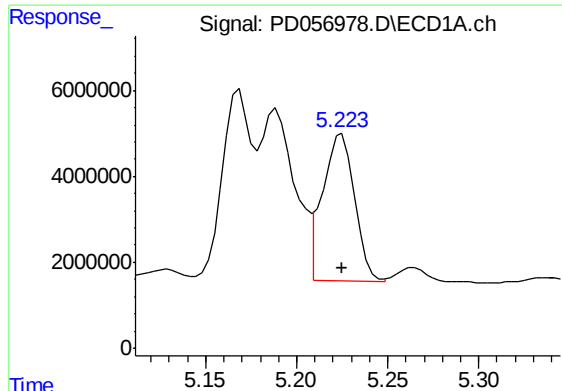

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 42209449
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

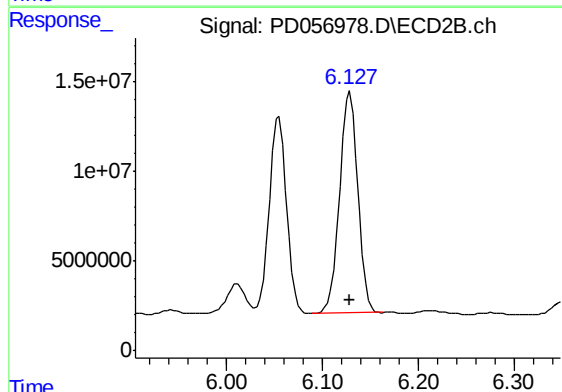


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 163759829
Conc: 500.00 ng/ml

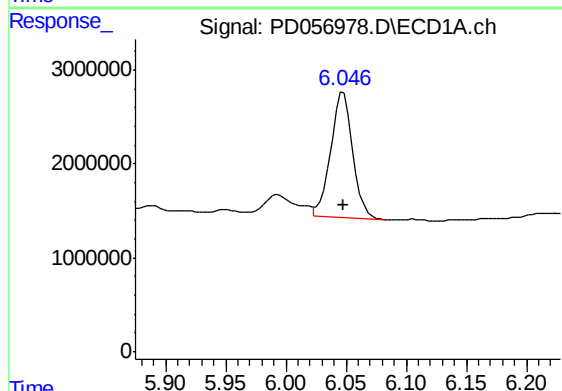


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 17173707
Conc: 500.00 ng/ml

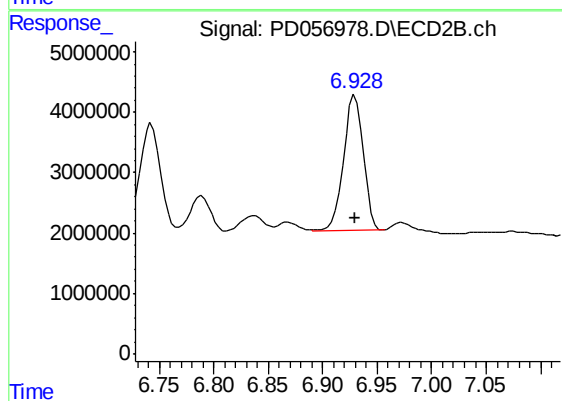

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 28283145
Conc: 500.00 ng/ml

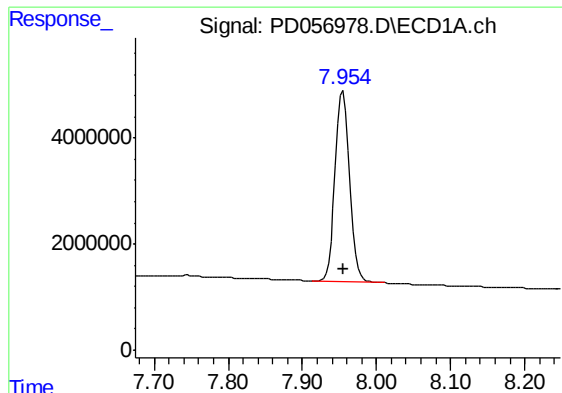

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 48462190
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

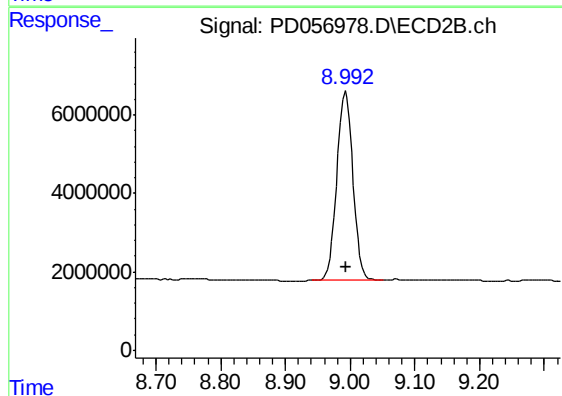

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 82213189
Conc: 50.00 ng/ml