

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 10:29
 Operator : AJ\MA
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 04:03:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 04:00:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	22034070	40273857	24.774	25.468
28)	SA Decachlor...	7.954	8.993	25076419	42846278	25.872	26.058
Target Compounds							
23)	Chlordane-1	4.124	4.947	6844719	15964885	247.872	252.371
24)	Chlordane-2	4.614	5.412	9405529	16576568	286.458	248.782
25)	Chlordane-3	5.168	6.054	23478946	68962149	241.400	249.129
26)	Chlordane-4	5.224	6.128	20958325	83205399	248.266	254.047
27)	Chlordane-5	6.046	6.929	8732925	13759825	254.253	243.251



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 10:29
Operator : AJ\MA
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 04:03:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 04:00:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

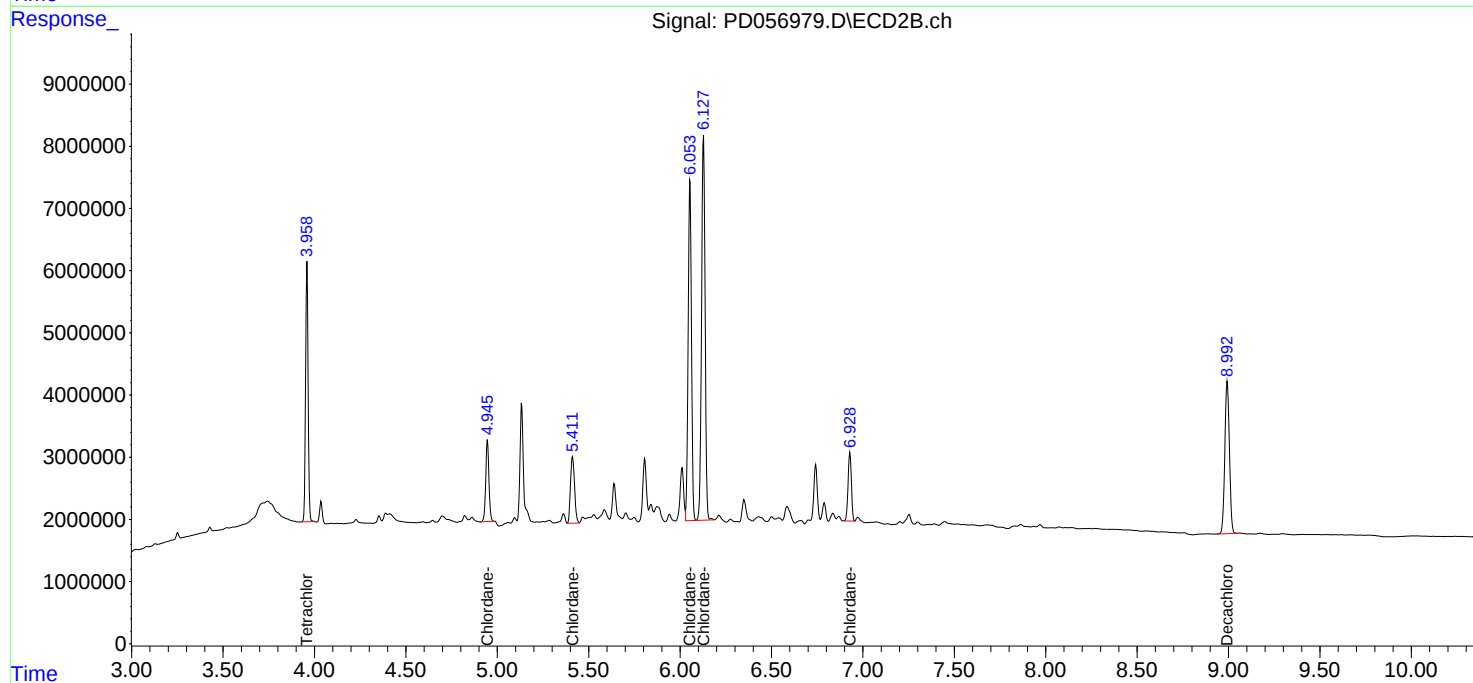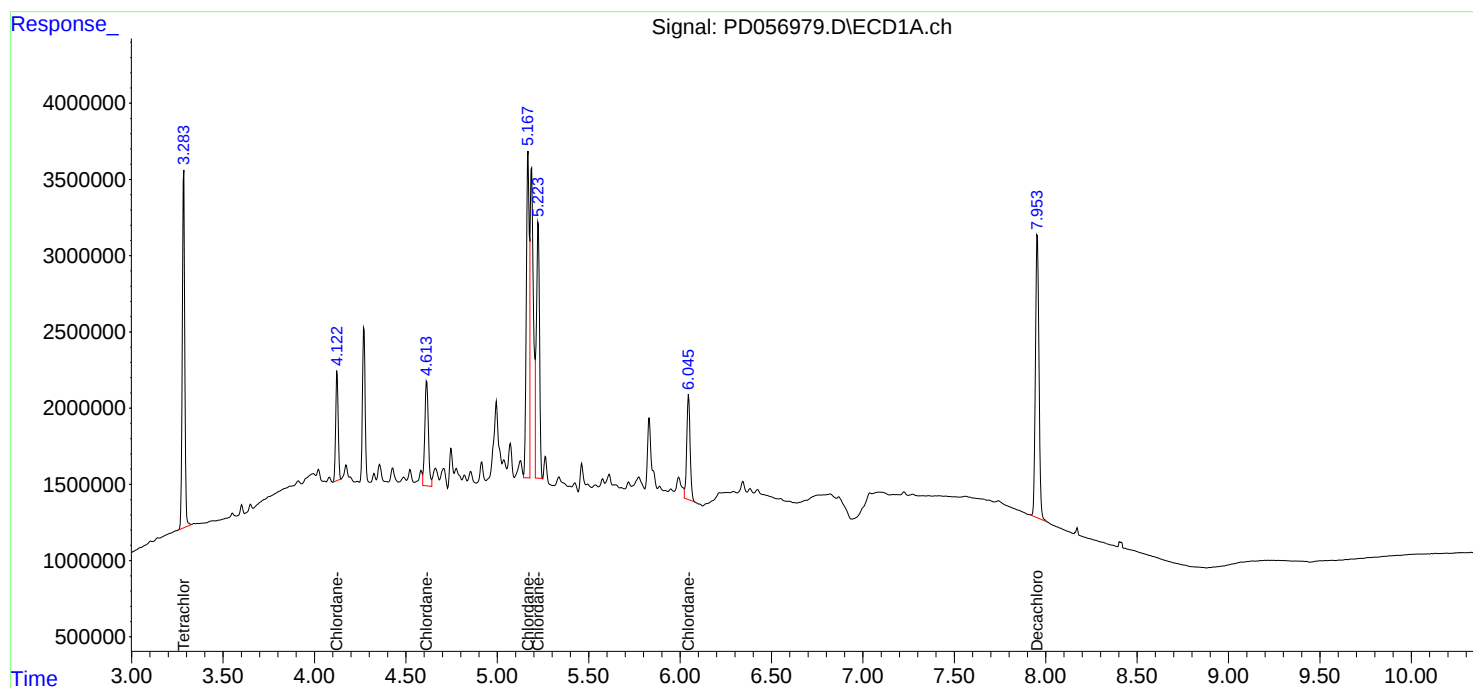


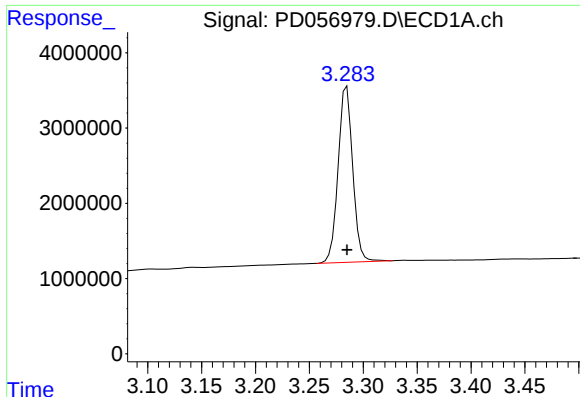

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 22034070
Conc: 24.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

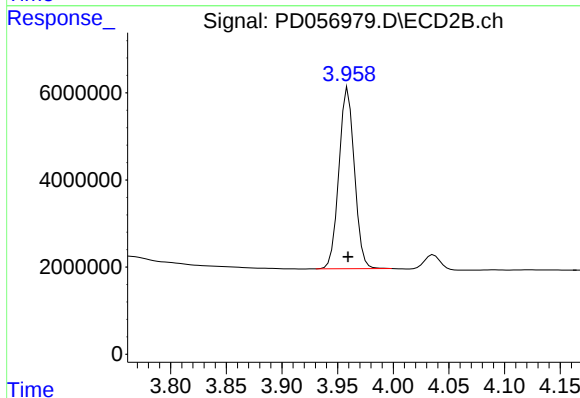


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 40273857
Conc: 25.47 ng/ml

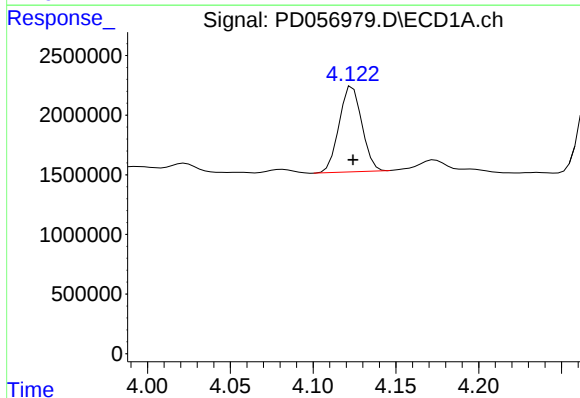


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 6844719
Conc: 247.87 ng/ml

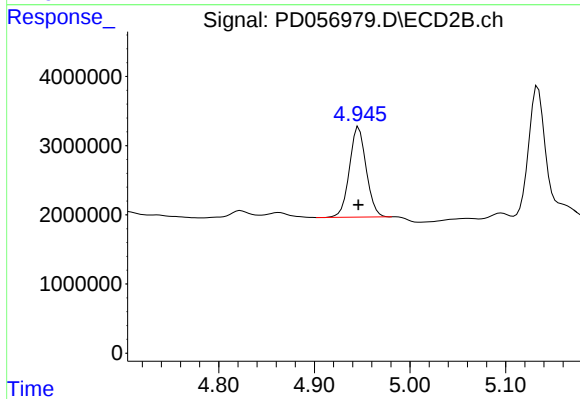

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 15964885
Conc: 252.37 ng/ml

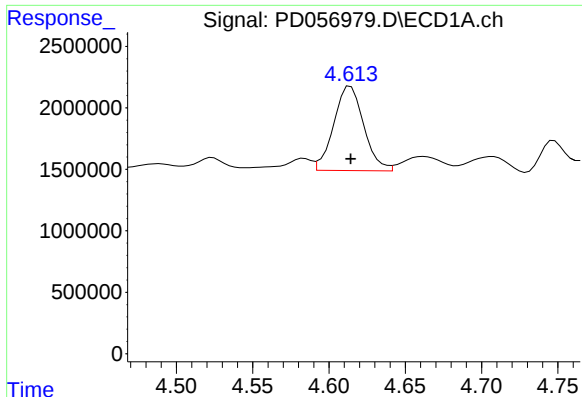

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 9405529
Conc: 286.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

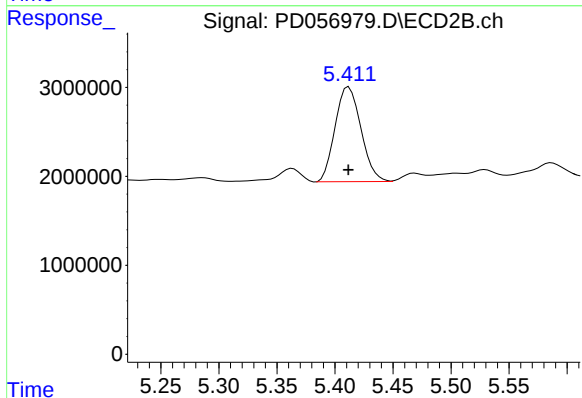


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 16576568
Conc: 248.78 ng/ml

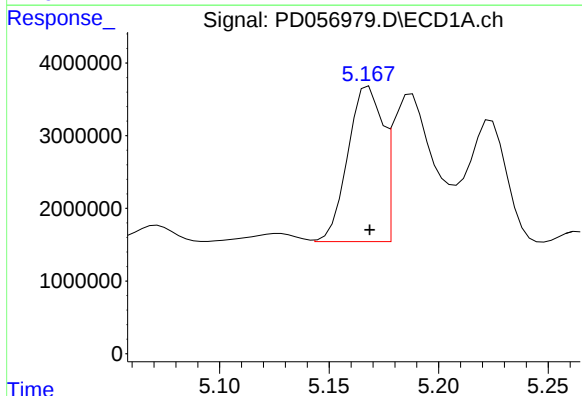


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 23478946
Conc: 241.40 ng/ml

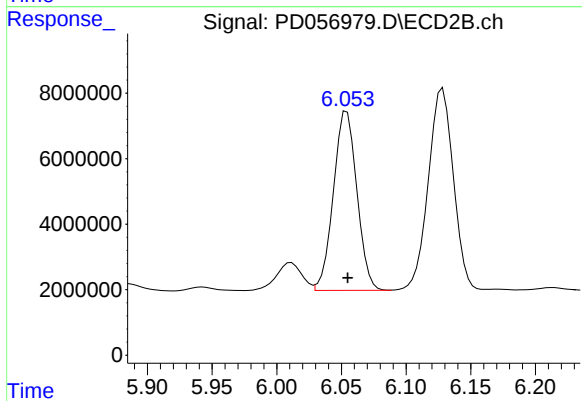

#25 Chlordane-3


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 68962149
Conc: 249.13 ng/ml

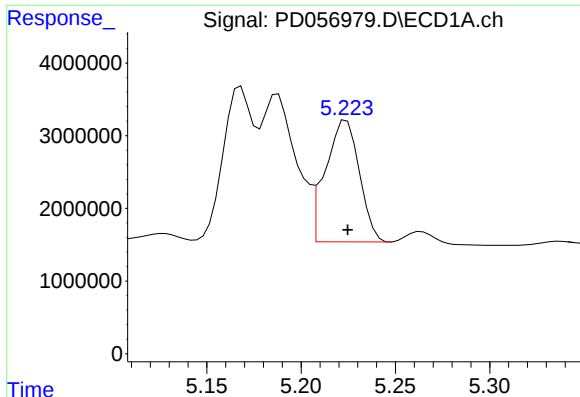

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 20958325
Conc: 248.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

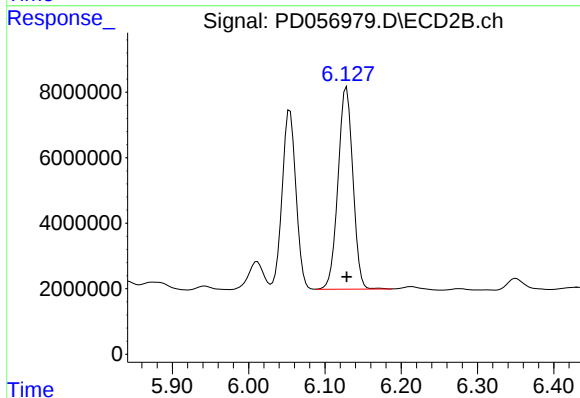


#26 Chlordane-4

R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 83205399
Conc: 254.05 ng/ml

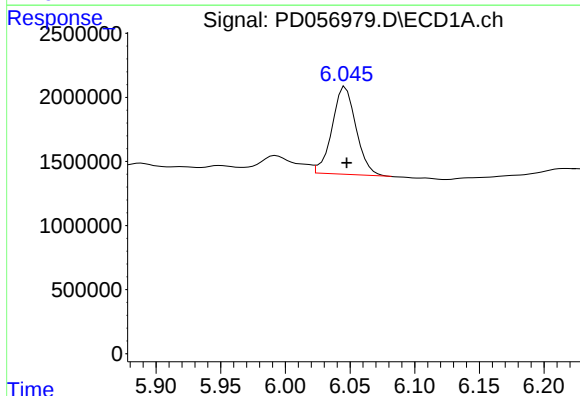


#27 Chlordane-5

R.T.: 6.046 min
Delta R.T.: -0.001 min
Response: 8732925
Conc: 254.25 ng/ml

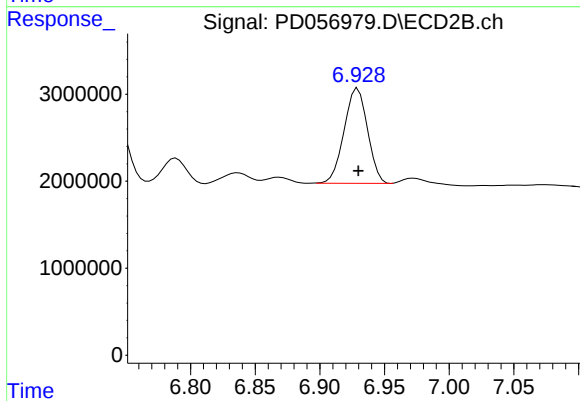

#27 Chlordane-5


R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 13759825
Conc: 243.25 ng/ml

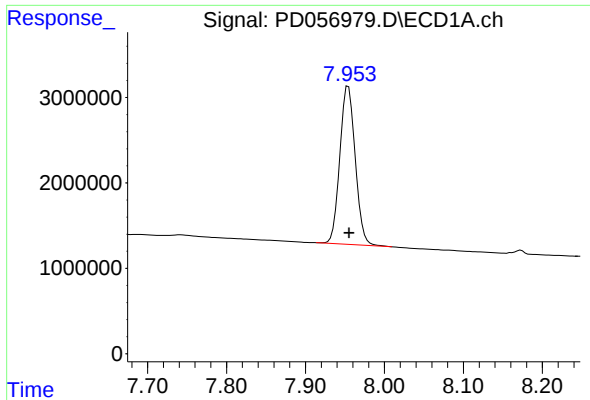

#28 Decachlorobiphenyl

R.T.: 7.954 min
Delta R.T.: 0.000 min
Response: 25076419
Conc: 25.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

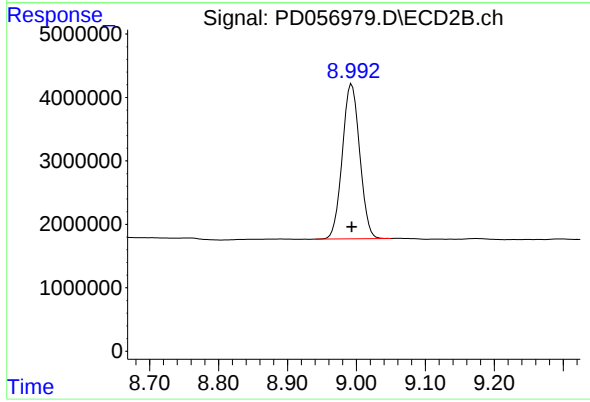

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 42846278
Conc: 26.06 ng/ml